

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
 Data File : VX044275.D
 Acq On : 13 Dec 2024 12:29
 Operator : JC/MD
 Sample : P5252-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F7J19

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
 Title : VOC Analysis

Signal : TIC: VX044275.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.239	22	25	33	rVB3	5242	8797	0.90%	0.117%
2	1.367	43	46	56	rBV	130518	140262	14.29%	1.873%
3	1.648	89	92	100	rBV	93877	129441	13.18%	1.729%
4	2.300	193	199	210	rBV	186100	296119	30.16%	3.955%
5	2.782	275	278	281	rVV4	1045	1628	0.17%	0.022%
6	2.825	284	285	287	rBV2	643	429	0.04%	0.006%
7	3.062	321	324	328	rVB2	658	925	0.09%	0.012%
8	3.160	339	340	343	rVB	686	457	0.05%	0.006%
9	3.239	351	353	355	rVB2	535	422	0.04%	0.006%
10	3.355	370	372	374	rVB2	468	428	0.04%	0.006%
11	3.501	394	396	397	rBV	724	573	0.06%	0.008%
12	3.550	402	404	407	rVB	642	478	0.05%	0.006%
13	3.580	407	409	412	rBV	714	882	0.09%	0.012%
14	3.916	462	464	467	rBV3	622	494	0.05%	0.007%
15	4.068	485	489	491	rBV2	645	770	0.08%	0.010%
16	4.221	510	514	516	rVB2	523	717	0.07%	0.010%
17	4.239	516	517	520	rBV	538	575	0.06%	0.008%
18	4.288	523	525	529	rVB2	472	577	0.06%	0.008%
19	4.355	533	536	538	rBV2	627	809	0.08%	0.011%
20	4.452	544	552	568	rBV	67141	195757	19.94%	2.614%
21	4.702	591	593	595	rVB3	719	488	0.05%	0.007%
22	5.056	638	651	667	rBV2	140179	425037	43.29%	5.677%
23	5.202	673	675	676	rBV2	608	590	0.06%	0.008%
24	5.312	691	693	695	rBV	816	654	0.07%	0.009%
25	5.464	715	718	721	rBV4	972	1461	0.15%	0.020%
26	5.531	727	729	732	rBV3	823	973	0.10%	0.013%
27	5.745	762	764	766	rVB2	590	442	0.05%	0.006%
28	5.964	788	800	818	rBV2	320111	981840	100.00%	13.113%
29	6.104	821	823	828	rVB2	1456	1612	0.16%	0.022%
30	6.300	852	855	856	rBV	423	419	0.04%	0.006%
31	6.623	905	908	909	rVB2	494	430	0.04%	0.006%
32	6.641	909	911	912	rBV	549	430	0.04%	0.006%
33	6.696	917	920	921	rBV2	683	648	0.07%	0.009%
34	6.757	921	930	943	rBV	203446	494360	50.35%	6.603%
35	6.891	951	952	955	rVB2	1297	663	0.07%	0.009%
36	6.964	963	964	968	rVB4	660	848	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
 Data File : VX044275.D
 Acq On : 13 Dec 2024 12:29
 Operator : JC/MD
 Sample : P5252-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F7J19

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

37	7.123	981	990	1004	rBV	296788	651495	66.35%	8.701%
38	7.305	1012	1020	1034	rVB	201539	452415	46.08%	6.042%
39	7.555	1060	1061	1063	rBV2	596	438	0.04%	0.006%
40	7.878	1112	1114	1117	rBV3	649	690	0.07%	0.009%
41	8.019	1133	1137	1140	rBV3	1001	1825	0.19%	0.024%
42	8.080	1144	1147	1151	rVB3	510	805	0.08%	0.011%
43	8.128	1151	1155	1157	rBV3	699	791	0.08%	0.011%
44	8.324	1181	1187	1202	rBV	127609	212448	21.64%	2.837%
45	8.531	1219	1221	1225	rVB2	559	576	0.06%	0.008%
46	8.647	1233	1240	1255	rBV	459528	736415	75.00%	9.835%
47	8.945	1283	1289	1305	rBV	84959	140666	14.33%	1.879%
48	9.159	1322	1324	1326	rBV2	531	568	0.06%	0.008%
49	9.275	1338	1343	1349	rVB3	15843	24614	2.51%	0.329%
50	9.384	1356	1361	1378	rBV	269372	411439	41.90%	5.495%
51	9.774	1423	1425	1427	rVB2	496	435	0.04%	0.006%
52	9.817	1430	1432	1434	rVV2	611	513	0.05%	0.007%
53	9.848	1436	1437	1439	rBV	633	617	0.06%	0.008%
54	9.921	1448	1449	1451	rBV2	724	559	0.06%	0.007%
55	9.963	1454	1456	1464	rVB5	860	1513	0.15%	0.020%
56	10.049	1465	1470	1481	rBV	418346	596068	60.71%	7.961%
57	10.360	1520	1521	1523	rBV2	695	499	0.05%	0.007%
58	10.457	1535	1537	1540	rBV3	427	467	0.05%	0.006%
59	10.591	1556	1559	1560	rBV3	521	546	0.06%	0.007%
60	10.774	1588	1589	1592	rBV2	992	966	0.10%	0.013%
61	10.951	1615	1618	1619	rBV2	634	634	0.06%	0.008%
62	11.012	1626	1628	1632	rBV2	627	536	0.05%	0.007%
63	11.043	1632	1633	1636	rVB2	610	507	0.05%	0.007%
64	11.189	1651	1657	1665	rBV	358843	461506	47.00%	6.164%
65	11.305	1675	1676	1681	rVB3	1828	1992	0.20%	0.027%
66	11.396	1690	1691	1694	rVB2	463	454	0.05%	0.006%
67	11.439	1694	1698	1699	rBV2	919	1073	0.11%	0.014%
68	11.738	1744	1747	1750	rBV4	492	665	0.07%	0.009%
69	11.786	1753	1755	1757	rBV3	386	413	0.04%	0.006%
70	11.835	1761	1763	1766	rVV2	418	456	0.05%	0.006%
71	11.902	1773	1774	1776	rBV2	719	600	0.06%	0.008%
72	11.969	1783	1785	1788	rBV2	729	643	0.07%	0.009%
73	12.018	1788	1793	1806	rBV	389314	479517	48.84%	6.404%
74	12.219	1823	1826	1827	rBV2	786	993	0.10%	0.013%
75	12.317	1837	1842	1852	rVV	464040	591673	60.26%	7.902%
76	12.481	1867	1869	1871	rBV3	564	511	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
 Data File : VX044275.D
 Acq On : 13 Dec 2024 12:29
 Operator : JC/MD
 Sample : P5252-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F7J19

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

77	12.567	1881	1883	1884	rBV2	689	467	0.05%	0.006%
78	12.939	1942	1944	1948	rVB3	560	760	0.08%	0.010%
79	13.731	2071	2074	2075	rBV3	641	664	0.07%	0.009%
80	13.871	2093	2097	2099	rBV	628	696	0.07%	0.009%
81	14.121	2136	2138	2144	rVB3	1262	1980	0.20%	0.026%
82	14.469	2194	2195	2197	rBV2	925	504	0.05%	0.007%
83	14.548	2204	2208	2209	rBV3	782	954	0.10%	0.013%
84	14.707	2233	2234	2236	rBV	669	583	0.06%	0.008%
85	14.767	2242	2244	2246	rBV2	514	424	0.04%	0.006%
86	14.889	2261	2264	2266	rBV4	374	486	0.05%	0.006%
87	15.024	2284	2286	2287	rBV2	627	460	0.05%	0.006%
88	15.066	2290	2293	2294	rBV2	452	588	0.06%	0.008%
89	15.097	2297	2298	2302	rBV3	525	661	0.07%	0.009%
90	15.182	2309	2312	2314	rVB4	681	686	0.07%	0.009%
91	15.206	2314	2316	2319	rVB2	628	658	0.07%	0.009%
92	15.237	2319	2321	2323	rBV2	671	462	0.05%	0.006%
93	15.347	2337	2339	2341	rBV2	648	556	0.06%	0.007%
94	15.438	2353	2354	2357	rVB3	737	544	0.06%	0.007%
95	15.462	2357	2358	2365	rVB3	693	1227	0.12%	0.016%
96	15.615	2382	2383	2385	rBV	723	445	0.05%	0.006%
97	15.743	2401	2404	2407	rBV2	544	811	0.08%	0.011%
98	15.962	2438	2440	2443	rVB3	583	519	0.05%	0.007%
99	16.133	2466	2468	2471	rBV3	619	767	0.08%	0.010%
100	16.670	2555	2556	2558	rVB	854	483	0.05%	0.006%

Sum of corrected areas: 7487361




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
Data File : VX044275.D
Acq On : 13 Dec 2024 12:29
Operator : JC/MD
Sample : P5252-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F7J19

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

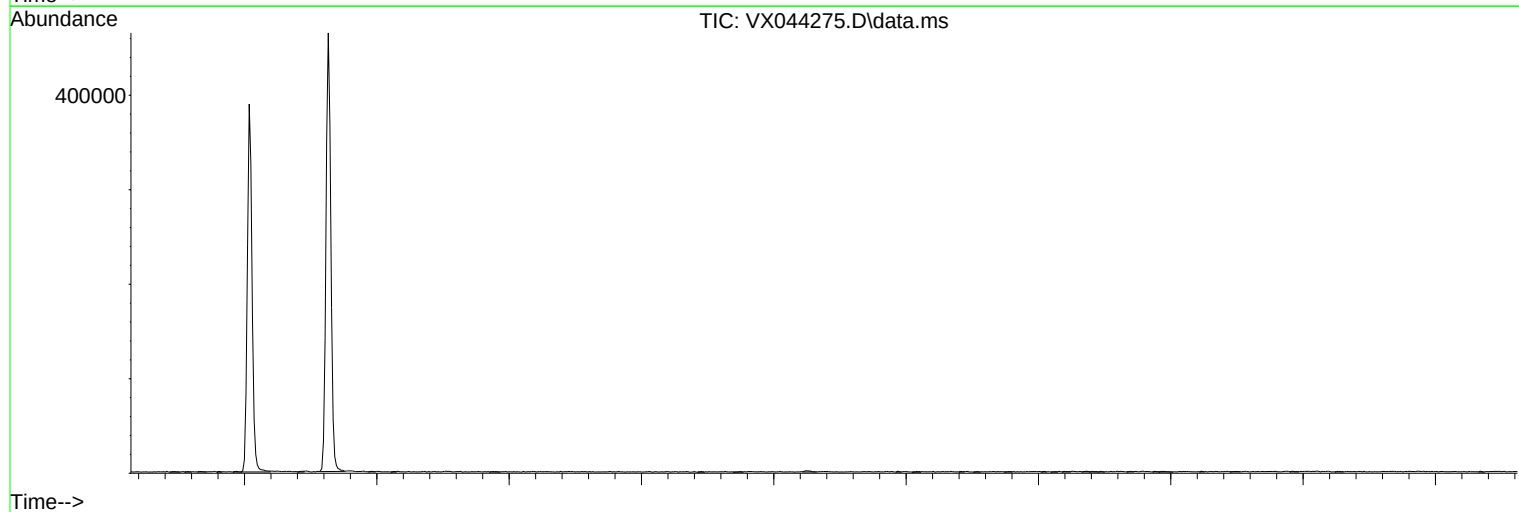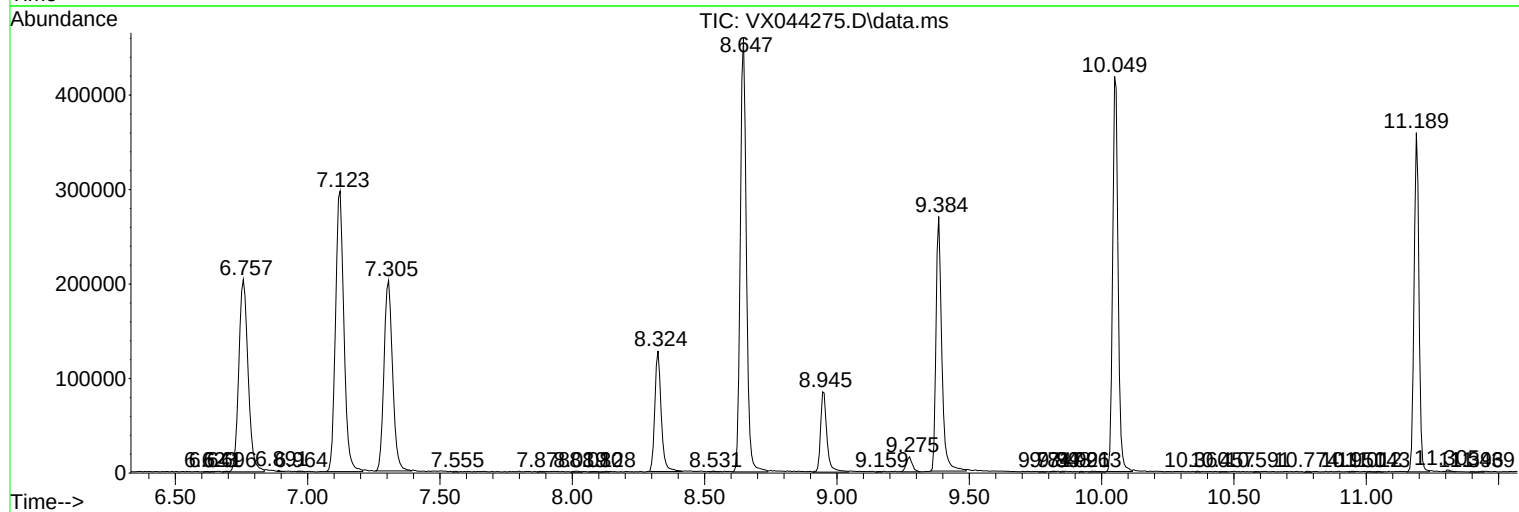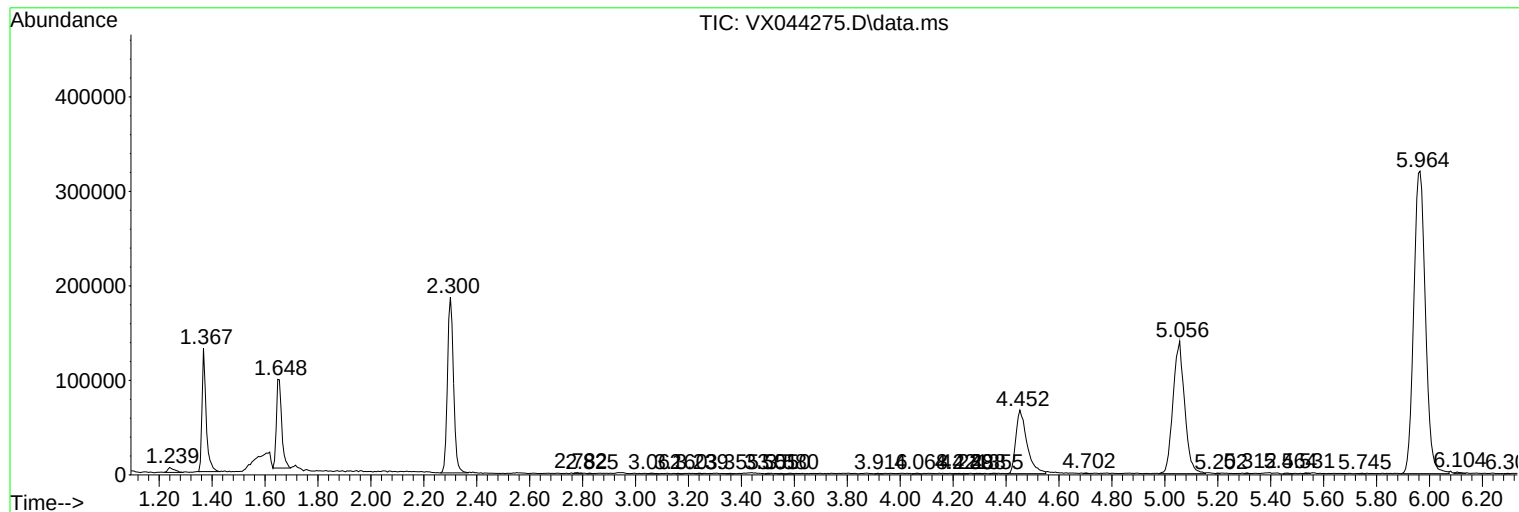

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
Data File : VX044275.D
Acq On : 13 Dec 2024 12:29
Operator : JC/MD
Sample : P5252-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F7J19

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
Data File : VX044275.D
Acq On : 13 Dec 2024 12:29
Operator : JC/MD
Sample : P5252-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F7J19

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
