

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
 Data File : VX044276.D
 Acq On : 13 Dec 2024 12:52
 Operator : JC/MD
 Sample : P5252-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F7J20

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
 Title : VOC Analysis

Signal : TIC: VX044276.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	32	rBV2	5552	8839	0.71%	0.114%
2	1.368	43	46	56	rVB	104228	122542	9.90%	1.576%
3	1.648	88	92	103	rVB	102272	154665	12.50%	1.989%
4	2.294	192	198	209	rBV	172480	276715	22.36%	3.559%
5	2.569	240	243	251	rVB3	3047	5479	0.44%	0.070%
6	2.697	263	264	266	rBV	495	508	0.04%	0.007%
7	2.758	272	274	275	rBV	644	402	0.03%	0.005%
8	2.831	285	286	289	rVB3	486	433	0.03%	0.006%
9	2.935	300	303	304	rVV2	607	579	0.05%	0.007%
10	3.032	317	319	320	rBV	498	391	0.03%	0.005%
11	3.111	330	332	333	rBV	700	606	0.05%	0.008%
12	3.221	345	350	351	rBV2	343	515	0.04%	0.007%
13	3.434	379	385	392	rBV6	2609	6182	0.50%	0.080%
14	3.764	435	439	442	rBV3	1127	1384	0.11%	0.018%
15	4.001	476	478	481	rBV4	630	564	0.05%	0.007%
16	4.068	486	489	490	rBV	686	559	0.05%	0.007%
17	4.196	507	510	512	rVB2	663	646	0.05%	0.008%
18	4.227	512	515	517	rBV4	503	703	0.06%	0.009%
19	4.251	517	519	521	rBV3	558	535	0.04%	0.007%
20	4.361	534	537	538	rVB2	667	586	0.05%	0.008%
21	4.459	544	553	570	rBV	56879	179570	14.51%	2.309%
22	4.770	602	604	605	rBV2	645	406	0.03%	0.005%
23	4.977	636	638	639	rBV	614	485	0.04%	0.006%
24	5.050	639	650	667	rVV2	124783	393040	31.76%	5.055%
25	5.355	699	700	703	rBV	725	671	0.05%	0.009%
26	5.538	727	730	732	rBV2	916	933	0.08%	0.012%
27	5.696	753	756	757	rBV3	460	392	0.03%	0.005%
28	5.715	757	759	762	rVB	561	470	0.04%	0.006%
29	5.830	774	778	781	rBV3	673	874	0.07%	0.011%
30	5.964	788	800	820	rBV2	305472	924139	74.68%	11.885%
31	6.172	833	834	836	rVB2	982	492	0.04%	0.006%
32	6.190	836	837	842	rBV4	653	953	0.08%	0.012%
33	6.300	853	855	857	rVV2	705	527	0.04%	0.007%
34	6.629	908	909	911	rBV2	783	623	0.05%	0.008%
35	6.757	918	930	944	rBV	199053	484101	39.12%	6.226%
36	7.117	980	989	1011	rBV	562324	1237413	100.00%	15.914%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
 Data File : VX044276.D
 Acq On : 13 Dec 2024 12:52
 Operator : JC/MD
 Sample : P5252-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F7J20

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

37	7.306	1012	1020	1035	rVB	187502	420923	34.02%	5.413%
38	7.702	1084	1085	1088	rVB3	713	484	0.04%	0.006%
39	7.769	1095	1096	1099	rVB3	673	420	0.03%	0.005%
40	7.812	1099	1103	1106	rBV3	442	579	0.05%	0.007%
41	7.915	1118	1120	1123	rBV3	666	602	0.05%	0.008%
42	8.123	1151	1154	1156	rBV4	468	394	0.03%	0.005%
43	8.324	1181	1187	1197	rBV	113387	192348	15.54%	2.474%
44	8.647	1234	1240	1256	rVB	410896	668177	54.00%	8.593%
45	8.952	1284	1290	1299	rBV	77585	123553	9.98%	1.589%
46	9.214	1331	1333	1336	rVB2	802	811	0.07%	0.010%
47	9.269	1336	1342	1349	rBV	92658	144625	11.69%	1.860%
48	9.385	1356	1361	1375	rBV	259174	382873	30.94%	4.924%
49	10.049	1465	1470	1479	rBV	392948	564357	45.61%	7.258%
50	10.311	1509	1513	1515	rBV3	528	678	0.05%	0.009%
51	10.384	1522	1525	1529	rVB2	783	1214	0.10%	0.016%
52	10.458	1535	1537	1540	rVB2	704	581	0.05%	0.007%
53	10.555	1551	1553	1555	rVB2	493	387	0.03%	0.005%
54	10.579	1555	1557	1559	rBV2	696	641	0.05%	0.008%
55	10.823	1595	1597	1599	rBV2	521	420	0.03%	0.005%
56	10.951	1616	1618	1620	rBV3	518	513	0.04%	0.007%
57	11.073	1637	1638	1640	rBV	594	451	0.04%	0.006%
58	11.189	1652	1657	1668	rBV	335340	430152	34.76%	5.532%
59	11.311	1672	1677	1680	rBV2	877	1309	0.11%	0.017%
60	11.494	1704	1707	1709	rBV3	627	617	0.05%	0.008%
61	11.585	1719	1722	1723	rBV2	563	648	0.05%	0.008%
62	11.707	1741	1742	1744	rBV2	528	414	0.03%	0.005%
63	11.848	1763	1765	1767	rBV	540	489	0.04%	0.006%
64	12.018	1788	1793	1807	rVB	362229	457294	36.96%	5.881%
65	12.219	1825	1826	1827	rBV	1270	660	0.05%	0.008%
66	12.317	1836	1842	1852	rBV	428048	548342	44.31%	7.052%
67	12.738	1906	1911	1912	rBV3	490	790	0.06%	0.010%
68	12.853	1928	1930	1931	rBV2	654	532	0.04%	0.007%
69	12.884	1933	1935	1936	rVB	664	445	0.04%	0.006%
70	13.061	1961	1964	1965	rBV2	465	474	0.04%	0.006%
71	13.091	1967	1969	1972	rVV2	468	554	0.04%	0.007%
72	13.146	1975	1978	1979	rBV2	626	650	0.05%	0.008%
73	13.353	2010	2012	2014	rBV2	638	611	0.05%	0.008%
74	13.414	2020	2022	2024	rBV3	570	540	0.04%	0.007%
75	13.433	2024	2025	2028	rVB	1061	727	0.06%	0.009%
76	13.475	2028	2032	2033	rBV2	755	906	0.07%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
 Data File : VX044276.D
 Acq On : 13 Dec 2024 12:52
 Operator : JC/MD
 Sample : P5252-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F7J20

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

77	13.573	2045	2048	2051	rBV2	427	632	0.05%	0.008%
78	13.603	2051	2053	2055	rBV2	479	529	0.04%	0.007%
79	13.664	2061	2063	2065	rBV2	627	688	0.06%	0.009%
80	13.780	2081	2082	2085	rVB3	684	595	0.05%	0.008%
81	13.811	2085	2087	2090	rBV2	750	866	0.07%	0.011%
82	13.963	2110	2112	2115	rBV2	641	713	0.06%	0.009%
83	14.134	2134	2140	2143	rVB3	987	1692	0.14%	0.022%
84	14.262	2160	2161	2164	rVB2	490	443	0.04%	0.006%
85	14.298	2164	2167	2168	rBV2	678	533	0.04%	0.007%
86	14.329	2171	2172	2174	rBV	572	481	0.04%	0.006%
87	14.445	2189	2191	2194	rBV3	773	803	0.06%	0.010%
88	14.621	2218	2220	2223	rVV4	422	445	0.04%	0.006%
89	14.877	2259	2262	2264	rBV2	646	828	0.07%	0.011%
90	14.932	2269	2271	2272	rBV2	548	473	0.04%	0.006%
91	14.963	2274	2276	2278	rBV3	871	837	0.07%	0.011%
92	14.987	2278	2280	2283	rVB3	780	677	0.05%	0.009%
93	15.396	2344	2347	2348	rBV2	757	845	0.07%	0.011%
94	15.432	2351	2353	2356	rVB3	722	624	0.05%	0.008%
95	15.579	2375	2377	2382	rBV4	997	831	0.07%	0.011%
96	15.719	2398	2400	2402	rBV3	716	514	0.04%	0.007%
97	15.749	2402	2405	2409	rBV2	659	965	0.08%	0.012%
98	15.780	2409	2410	2412	rBV2	488	403	0.03%	0.005%
99	15.822	2416	2417	2419	rBV2	706	511	0.04%	0.007%
100	15.908	2429	2431	2433	rVB2	763	595	0.05%	0.008%

Sum of corrected areas: 7775630




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
Data File : VX044276.D
Acq On : 13 Dec 2024 12:52
Operator : JC/MD
Sample : P5252-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F7J20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

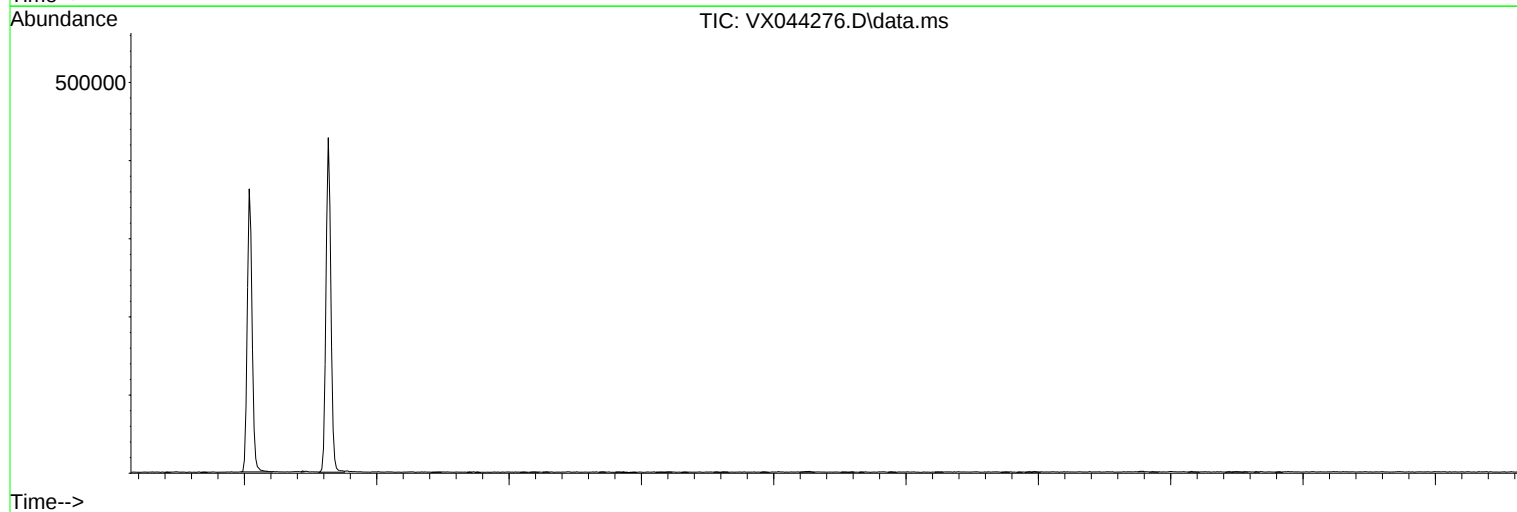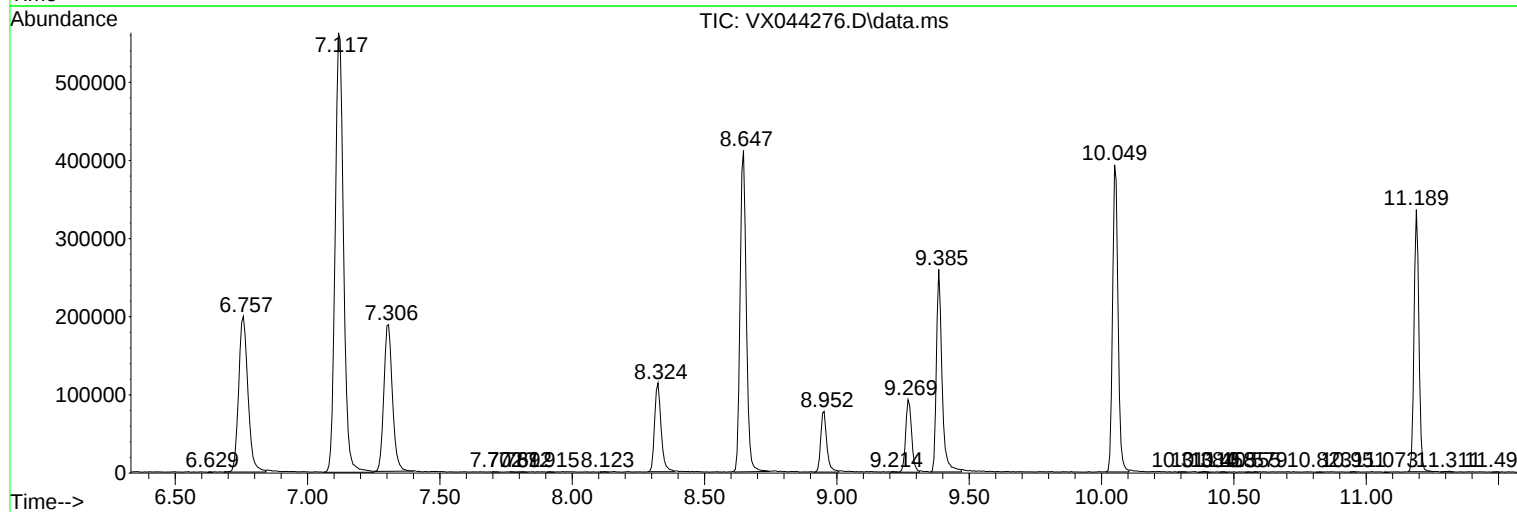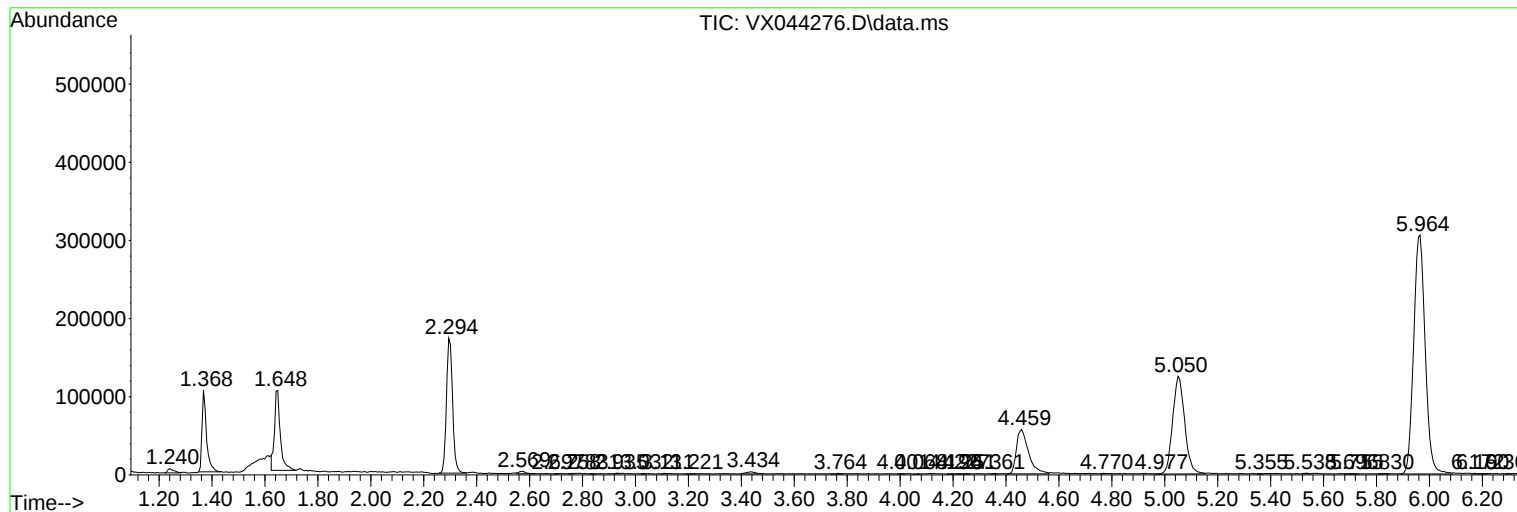

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
Data File : VX044276.D
Acq On : 13 Dec 2024 12:52
Operator : JC/MD
Sample : P5252-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F7J20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
Data File : VX044276.D
Acq On : 13 Dec 2024 12:52
Operator : JC/MD
Sample : P5252-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F7J20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc