

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
 Data File : VX044279.D
 Acq On : 13 Dec 2024 14:01
 Operator : JC/MD
 Sample : P5252-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F7J21

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
 Title : VOC Analysis

Signal : TIC: VX044279.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.239	22	25	28	rBV	6262	6951	0.57%	0.088%
2	1.368	43	46	58	rBV	106975	130576	10.77%	1.661%
3	1.648	89	92	103	rVB	89441	134190	11.07%	1.707%
4	2.294	192	198	210	rBV	181305	288191	23.76%	3.666%
5	2.386	212	213	216	rVB2	1474	731	0.06%	0.009%
6	2.495	229	231	235	rVB3	1427	1385	0.11%	0.018%
7	2.782	272	278	286	rVB5	1496	3962	0.33%	0.050%
8	2.849	286	289	290	rBV	844	733	0.06%	0.009%
9	2.916	297	300	301	rBV3	638	649	0.05%	0.008%
10	3.087	323	328	332	rBV3	1428	2964	0.24%	0.038%
11	3.215	348	349	351	rBV	813	641	0.05%	0.008%
12	3.361	371	373	375	rBV	824	618	0.05%	0.008%
13	3.392	375	378	379	rVV3	586	563	0.05%	0.007%
14	3.440	379	386	394	rVB4	4177	10317	0.85%	0.131%
15	3.507	394	397	400	rBV2	783	819	0.07%	0.010%
16	3.727	430	433	437	rVV4	601	858	0.07%	0.011%
17	3.849	451	453	455	rVB2	647	651	0.05%	0.008%
18	3.940	466	468	470	rBV3	740	590	0.05%	0.008%
19	4.208	510	512	515	rBV3	486	559	0.05%	0.007%
20	4.233	515	516	519	rVB2	950	735	0.06%	0.009%
21	4.306	525	528	529	rBV2	618	672	0.06%	0.009%
22	4.458	546	553	573	rBV	51613	163622	13.49%	2.081%
23	4.721	595	596	599	rBV2	685	633	0.05%	0.008%
24	4.794	607	608	611	rVB	1025	734	0.06%	0.009%
25	4.824	611	613	615	rBV3	738	615	0.05%	0.008%
26	4.934	629	631	634	rVV3	485	616	0.05%	0.008%
27	5.050	639	650	664	rBV	123638	386975	31.91%	4.922%
28	5.257	679	684	687	rBV4	782	1471	0.12%	0.019%
29	5.288	687	689	692	rVB2	759	736	0.06%	0.009%
30	5.355	698	700	702	rVB2	634	643	0.05%	0.008%
31	5.379	702	704	707	rBV3	676	979	0.08%	0.012%
32	5.446	712	715	717	rVV2	557	717	0.06%	0.009%
33	5.464	717	718	722	rVB2	766	734	0.06%	0.009%
34	5.672	750	752	753	rBV	999	605	0.05%	0.008%
35	5.964	788	800	818	rBV3	306572	936271	77.20%	11.909%
36	6.239	843	845	848	rVB2	691	540	0.04%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
 Data File : VX044279.D
 Acq On : 13 Dec 2024 14:01
 Operator : JC/MD
 Sample : P5252-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F7J21

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

37	6.269	848	850	852	rBV	708	610	0.05%	0.008%
38	6.367	864	866	869	rVV2	786	728	0.06%	0.009%
39	6.409	872	873	875	rBV2	685	612	0.05%	0.008%
40	6.757	920	930	944	rBV2	211911	519328	42.82%	6.606%
41	6.952	960	962	963	rVB	1020	547	0.05%	0.007%
42	6.976	963	966	968	rVB4	565	616	0.05%	0.008%
43	7.116	981	989	1006	rBV	556116	1212723	100.00%	15.425%
44	7.305	1012	1020	1031	rBV	188462	417903	34.46%	5.315%
45	7.555	1059	1061	1064	rVB4	530	610	0.05%	0.008%
46	7.610	1068	1070	1072	rBV2	537	655	0.05%	0.008%
47	7.677	1079	1081	1086	rVB3	882	922	0.08%	0.012%
48	7.781	1096	1098	1102	rVB4	647	785	0.06%	0.010%
49	8.007	1132	1135	1137	rVB2	887	946	0.08%	0.012%
50	8.031	1137	1139	1140	rBV2	697	628	0.05%	0.008%
51	8.324	1181	1187	1200	rBV	115208	202608	16.71%	2.577%
52	8.647	1234	1240	1250	rVV	434238	680768	56.14%	8.659%
53	8.860	1274	1275	1280	rBV4	538	788	0.06%	0.010%
54	8.952	1284	1290	1302	rBV	79473	125976	10.39%	1.602%
55	9.269	1336	1342	1352	rBV	107073	166285	13.71%	2.115%
56	9.384	1356	1361	1379	rBV	221765	352774	29.09%	4.487%
57	9.665	1405	1407	1411	rVB4	542	738	0.06%	0.009%
58	9.756	1420	1422	1424	rBV3	553	558	0.05%	0.007%
59	9.964	1454	1456	1457	rBV2	557	571	0.05%	0.007%
60	10.055	1465	1471	1479	rBV	407163	593680	48.95%	7.551%
61	10.195	1492	1494	1500	rVB3	1369	2366	0.20%	0.030%
62	10.311	1509	1513	1516	rBV3	1174	1958	0.16%	0.025%
63	10.415	1528	1530	1533	rBV4	687	751	0.06%	0.010%
64	10.646	1566	1568	1570	rBV3	1416	1413	0.12%	0.018%
65	10.854	1599	1602	1604	rBV	857	932	0.08%	0.012%
66	10.969	1618	1621	1624	rVB	1579	1856	0.15%	0.024%
67	11.097	1640	1642	1644	rBV2	664	631	0.05%	0.008%
68	11.189	1651	1657	1667	rBV	324666	416105	34.31%	5.293%
69	11.305	1673	1676	1683	rVB6	713	1535	0.13%	0.020%
70	11.396	1688	1691	1692	rBV3	662	609	0.05%	0.008%
71	11.451	1698	1700	1705	rVB	1842	1599	0.13%	0.020%
72	11.719	1741	1744	1747	rBV2	409	675	0.06%	0.009%
73	11.762	1747	1751	1756	rVB4	1410	2293	0.19%	0.029%
74	11.975	1780	1786	1788	rBV5	2758	4240	0.35%	0.054%
75	12.018	1788	1793	1803	rVB	367894	478796	39.48%	6.090%
76	12.231	1827	1828	1833	rVB4	875	660	0.05%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
 Data File : VX044279.D
 Acq On : 13 Dec 2024 14:01
 Operator : JC/MD
 Sample : P5252-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F7J21

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

77	12.317	1837	1842	1849	rBV	432053	544536	44.90%	6.926%
78	12.622	1891	1892	1895	rBV2	712	630	0.05%	0.008%
79	12.701	1903	1905	1909	rVB4	656	695	0.06%	0.009%
80	12.768	1909	1916	1919	rVB4	847	1830	0.15%	0.023%
81	12.884	1932	1935	1938	rBV3	874	1055	0.09%	0.013%
82	13.115	1970	1973	1978	rBV3	3000	3474	0.29%	0.044%
83	13.329	2005	2008	2011	rBV4	510	738	0.06%	0.009%
84	13.591	2047	2051	2055	rBV4	2968	4310	0.36%	0.055%
85	13.670	2060	2064	2066	rBV3	415	632	0.05%	0.008%
86	13.780	2078	2082	2086	rBV	5089	7310	0.60%	0.093%
87	13.871	2095	2097	2100	rVB3	862	940	0.08%	0.012%
88	13.908	2100	2103	2105	rBV3	796	796	0.07%	0.010%
89	13.963	2108	2112	2120	rVV6	3384	5493	0.45%	0.070%
90	14.097	2131	2134	2135	rBV2	569	565	0.05%	0.007%
91	14.213	2151	2153	2155	rBV2	674	654	0.05%	0.008%
92	14.329	2171	2172	2176	rBV2	600	551	0.05%	0.007%
93	14.511	2198	2202	2203	rBV2	741	857	0.07%	0.011%
94	15.463	2356	2358	2360	rVB2	865	611	0.05%	0.008%
95	15.493	2360	2363	2364	rBV3	516	678	0.06%	0.009%
96	15.810	2412	2415	2416	rBV	565	688	0.06%	0.009%
97	15.962	2437	2440	2443	rBV4	676	862	0.07%	0.011%
98	16.084	2458	2460	2463	rBV4	683	685	0.06%	0.009%
99	16.139	2467	2469	2472	rBV2	642	706	0.06%	0.009%
100	16.481	2523	2525	2528	rVB2	716	714	0.06%	0.009%

Sum of corrected areas: 7862034




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
Data File : VX044279.D
Acq On : 13 Dec 2024 14:01
Operator : JC/MD
Sample : P5252-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F7J21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

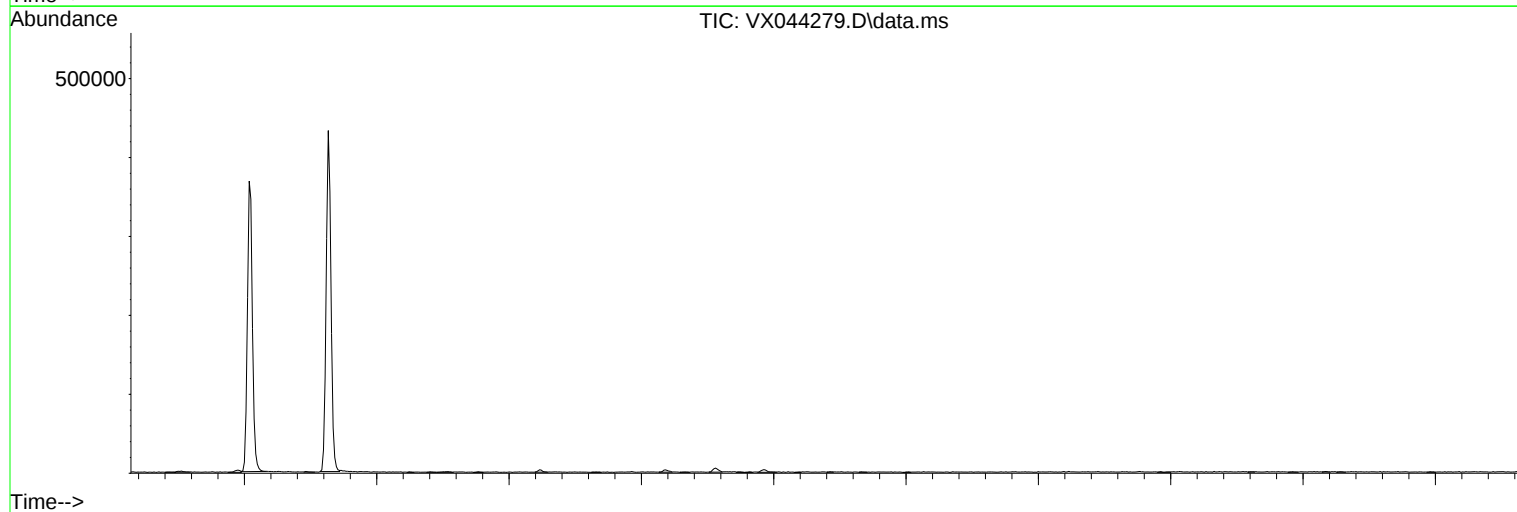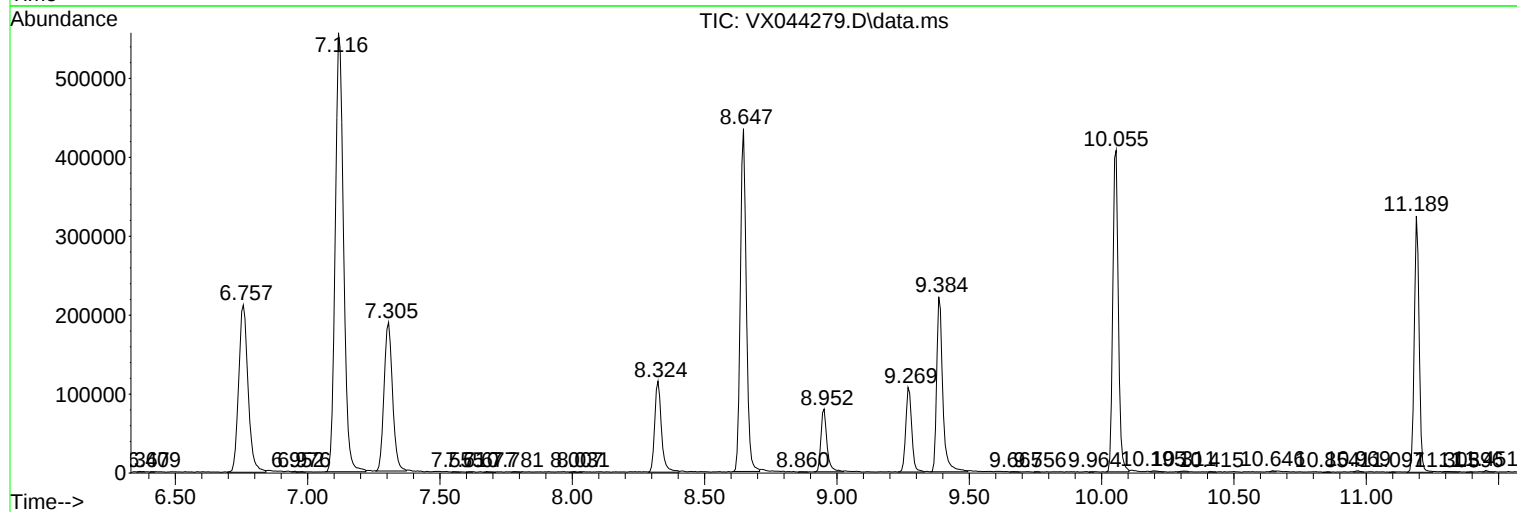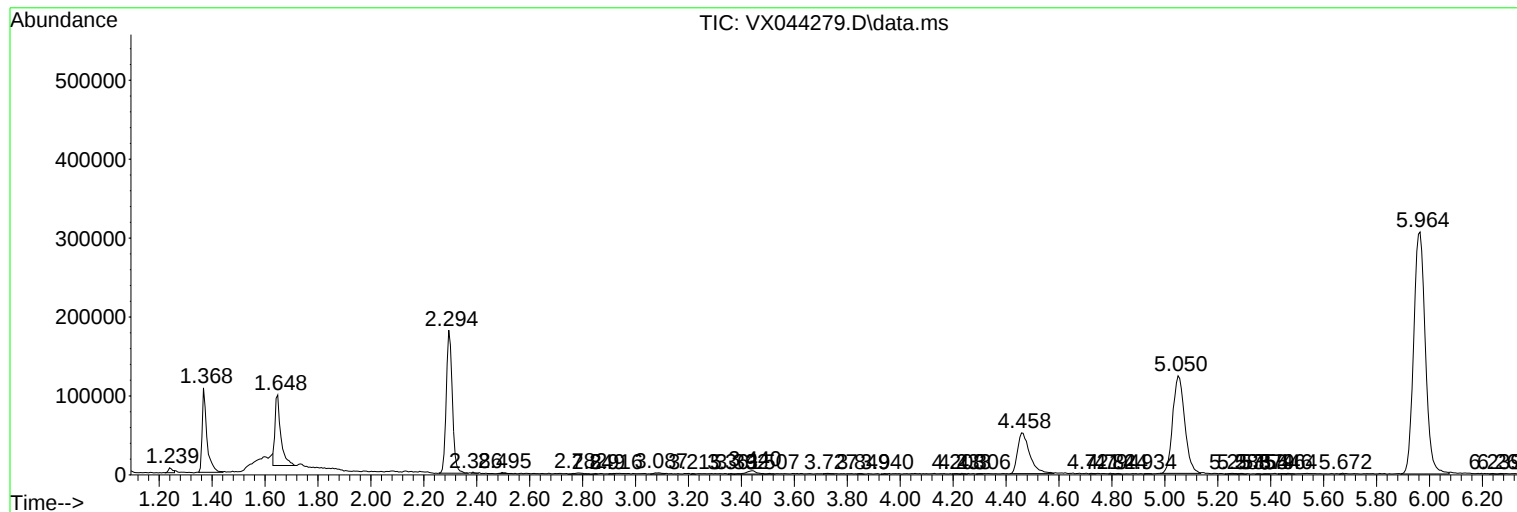

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
Data File : VX044279.D
Acq On : 13 Dec 2024 14:01
Operator : JC/MD
Sample : P5252-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F7J21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
Data File : VX044279.D
Acq On : 13 Dec 2024 14:01
Operator : JC/MD
Sample : P5252-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F7J21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
