

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
 Data File : VX044281.D
 Acq On : 13 Dec 2024 14:47
 Operator : JC/MD
 Sample : P5252-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F7J23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
 Title : VOC Analysis

Signal : TIC: VX044281.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	32	rBV3	6093	9198	1.01%	0.130%
2	1.368	43	46	59	rVB	106149	129605	14.24%	1.834%
3	1.648	88	92	104	rVB	99973	151991	16.70%	2.151%
4	2.300	192	199	209	rBV2	279190	547045	60.12%	7.740%
5	2.483	227	229	232	rBV2	801	907	0.10%	0.013%
6	2.544	237	239	240	rVV	1133	984	0.11%	0.014%
7	2.562	240	242	248	rVB3	2187	3514	0.39%	0.050%
8	2.867	290	292	294	rBV2	887	948	0.10%	0.013%
9	2.928	301	302	305	rBV2	618	715	0.08%	0.010%
10	3.123	332	334	338	rBV2	548	506	0.06%	0.007%
11	3.166	338	341	343	rBV	658	614	0.07%	0.009%
12	3.276	357	359	362	rBV3	442	513	0.06%	0.007%
13	3.386	375	377	379	rVB2	676	529	0.06%	0.007%
14	3.434	379	385	395	rVB3	4066	9592	1.05%	0.136%
15	3.507	395	397	400	rBV3	651	808	0.09%	0.011%
16	3.879	456	458	460	rBV	723	653	0.07%	0.009%
17	4.080	490	491	495	rVB	757	619	0.07%	0.009%
18	4.129	495	499	503	rBV4	806	1656	0.18%	0.023%
19	4.178	503	507	510	rBV5	411	666	0.07%	0.009%
20	4.257	518	520	523	rBV3	652	683	0.08%	0.010%
21	4.288	523	525	527	rBV3	508	512	0.06%	0.007%
22	4.458	545	553	573	rBV2	52804	178604	19.63%	2.527%
23	4.775	601	605	607	rBV3	524	775	0.09%	0.011%
24	5.050	639	650	666	rBV2	126598	383746	42.17%	5.430%
25	5.245	678	682	684	rBV3	562	688	0.08%	0.010%
26	5.342	696	698	701	rVB2	604	526	0.06%	0.007%
27	5.379	701	704	705	rBV2	583	718	0.08%	0.010%
28	5.452	714	716	718	rBV3	554	601	0.07%	0.009%
29	5.733	759	762	765	rBV2	600	927	0.10%	0.013%
30	5.800	772	773	776	rVB3	627	646	0.07%	0.009%
31	5.964	789	800	816	rVV2	305629	909929	100.00%	12.875%
32	6.184	834	836	837	rBV2	1125	1017	0.11%	0.014%
33	6.287	851	853	854	rBV	1127	814	0.09%	0.012%
34	6.330	858	860	862	rVB	913	639	0.07%	0.009%
35	6.525	889	892	893	rBV2	514	541	0.06%	0.008%
36	6.757	920	930	943	rBV	217752	521715	57.34%	7.382%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
 Data File : VX044281.D
 Acq On : 13 Dec 2024 14:47
 Operator : JC/MD
 Sample : P5252-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F7J23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

37	7.123	982	990	1005	rBV	162378	362393	39.83%	5.128%
38	7.306	1011	1020	1032	rBV	196055	423401	46.53%	5.991%
39	7.787	1097	1099	1101	rBV2	505	509	0.06%	0.007%
40	8.007	1134	1135	1138	rBV2	694	538	0.06%	0.008%
41	8.147	1154	1158	1159	rBV3	589	805	0.09%	0.011%
42	8.250	1172	1175	1176	rVB2	830	618	0.07%	0.009%
43	8.324	1181	1187	1198	rBV	108880	188605	20.73%	2.669%
44	8.586	1228	1230	1233	rVB4	605	696	0.08%	0.010%
45	8.647	1233	1240	1256	rBV	424725	683385	75.10%	9.669%
46	8.945	1284	1289	1300	rBV	75784	120407	13.23%	1.704%
47	9.195	1328	1330	1334	rVB2	739	735	0.08%	0.010%
48	9.275	1339	1343	1348	rVB4	1755	2474	0.27%	0.035%
49	9.384	1356	1361	1373	rBV	229753	349352	38.39%	4.943%
50	9.872	1437	1441	1443	rBV3	652	983	0.11%	0.014%
51	9.927	1447	1450	1451	rBV3	682	792	0.09%	0.011%
52	10.000	1459	1462	1465	rBV2	590	736	0.08%	0.010%
53	10.049	1465	1470	1480	rBV	418233	608465	66.87%	8.609%
54	10.195	1492	1494	1498	rBV4	963	1285	0.14%	0.018%
55	10.372	1521	1523	1525	rBV3	686	831	0.09%	0.012%
56	10.451	1532	1536	1537	rBV2	759	831	0.09%	0.012%
57	10.543	1549	1551	1554	rVB2	862	863	0.09%	0.012%
58	10.604	1554	1561	1562	rBV3	640	1044	0.11%	0.015%
59	10.744	1582	1584	1587	rVB3	585	545	0.06%	0.008%
60	10.854	1597	1602	1604	rBV2	730	861	0.09%	0.012%
61	10.896	1607	1609	1611	rVB3	538	477	0.05%	0.007%
62	10.921	1611	1613	1616	rBV2	534	462	0.05%	0.007%
63	11.012	1624	1628	1629	rVV3	438	467	0.05%	0.007%
64	11.030	1629	1631	1634	rVB3	846	601	0.07%	0.009%
65	11.189	1652	1657	1668	rVV	325447	413550	45.45%	5.851%
66	11.299	1673	1675	1678	rBV3	566	668	0.07%	0.009%
67	11.451	1699	1700	1702	rBV	899	495	0.05%	0.007%
68	11.488	1704	1706	1709	rBV2	482	580	0.06%	0.008%
69	11.567	1717	1719	1720	rBV	744	562	0.06%	0.008%
70	11.646	1731	1732	1737	rVV3	557	663	0.07%	0.009%
71	11.756	1748	1750	1751	rBV	805	544	0.06%	0.008%
72	12.018	1788	1793	1802	rBV	392531	485275	53.33%	6.866%
73	12.171	1816	1818	1821	rVB4	717	679	0.07%	0.010%
74	12.317	1837	1842	1851	rBV	413035	529387	58.18%	7.490%
75	12.622	1890	1892	1895	rBV2	498	736	0.08%	0.010%
76	12.677	1900	1901	1904	rBV	644	509	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
 Data File : VX044281.D
 Acq On : 13 Dec 2024 14:47
 Operator : JC/MD
 Sample : P5252-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F7J23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

77	13.128	1971	1975	1979	rVB4	814	1193	0.13%	0.017%
78	13.158	1979	1980	1983	rBV3	487	552	0.06%	0.008%
79	13.237	1991	1993	1997	rVV3	728	708	0.08%	0.010%
80	13.274	1997	1999	2002	rVV	480	516	0.06%	0.007%
81	13.372	2012	2015	2017	rVB3	598	497	0.05%	0.007%
82	13.396	2017	2019	2022	rBV2	435	491	0.05%	0.007%
83	13.652	2058	2061	2062	rBV3	688	603	0.07%	0.009%
84	13.701	2067	2069	2071	rBV2	345	474	0.05%	0.007%
85	13.810	2084	2087	2089	rBV3	730	552	0.06%	0.008%
86	14.176	2143	2147	2148	rBV3	491	669	0.07%	0.009%
87	14.225	2154	2155	2158	rVB3	653	591	0.06%	0.008%
88	14.524	2203	2204	2207	rBV2	533	530	0.06%	0.007%
89	14.597	2214	2216	2218	rVB2	630	475	0.05%	0.007%
90	15.085	2293	2296	2298	rBV2	759	991	0.11%	0.014%
91	15.121	2300	2302	2307	rVB5	829	1061	0.12%	0.015%
92	15.158	2307	2308	2310	rBV2	519	498	0.05%	0.007%
93	15.426	2350	2352	2354	rBV3	712	746	0.08%	0.011%
94	15.578	2375	2377	2380	rBV2	993	871	0.10%	0.012%
95	15.609	2380	2382	2385	rBV3	658	796	0.09%	0.011%
96	15.737	2400	2403	2406	rVB3	643	837	0.09%	0.012%
97	15.767	2406	2408	2410	rBV	695	541	0.06%	0.008%
98	16.078	2456	2459	2462	rBV3	651	1039	0.11%	0.015%
99	16.389	2508	2510	2513	rVB2	599	473	0.05%	0.007%
100	16.633	2548	2550	2555	rBV4	719	977	0.11%	0.014%

Sum of corrected areas: 7067634




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
Data File : VX044281.D
Acq On : 13 Dec 2024 14:47
Operator : JC/MD
Sample : P5252-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F7J23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

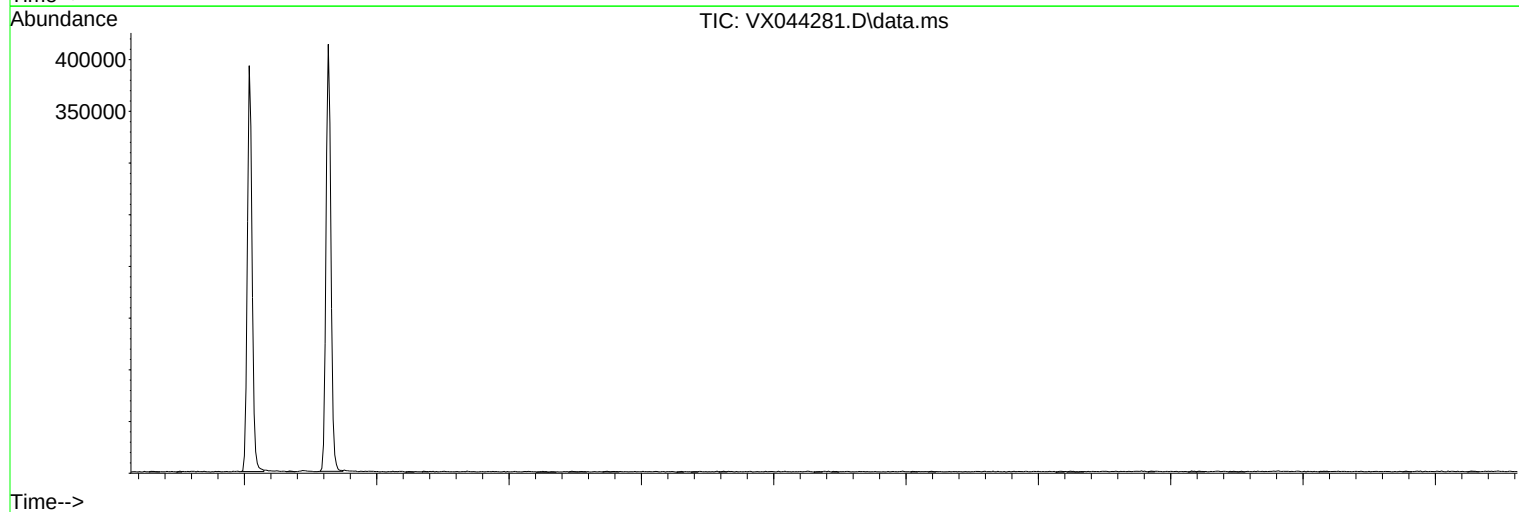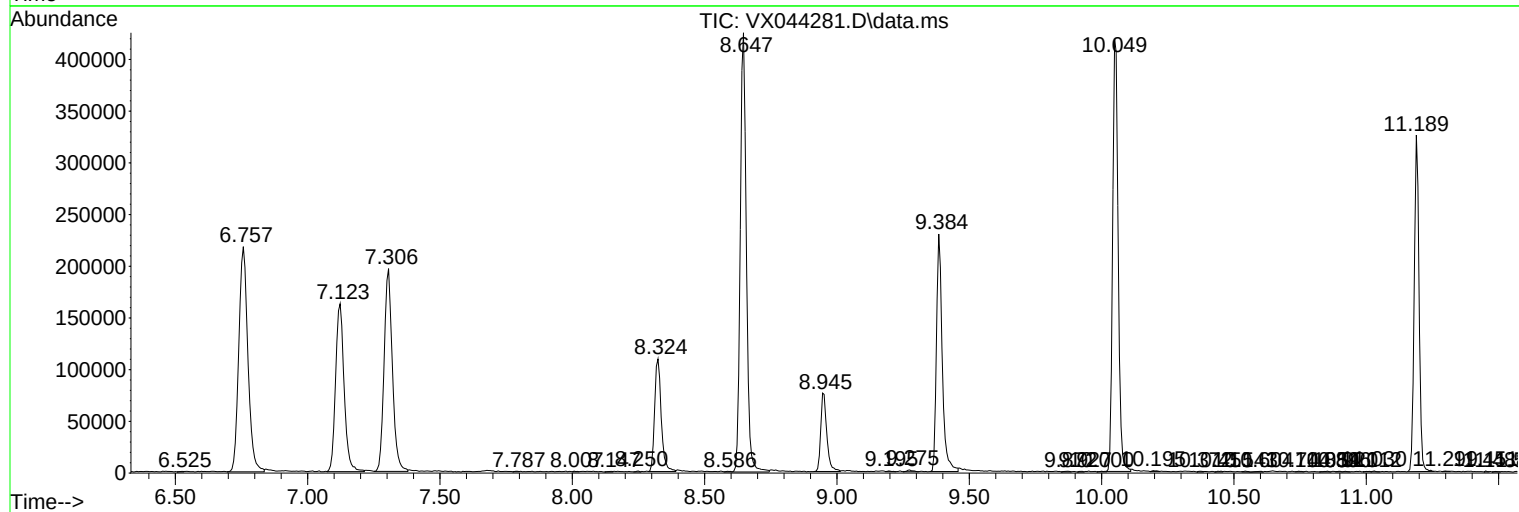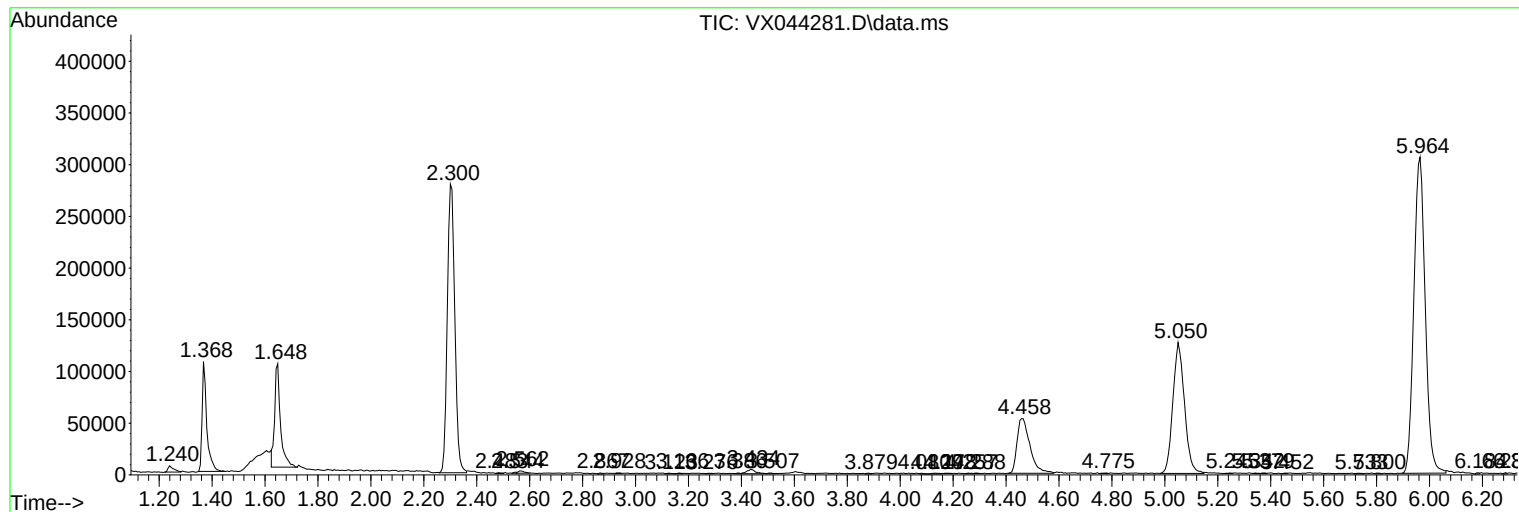

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
Data File : VX044281.D
Acq On : 13 Dec 2024 14:47
Operator : JC/MD
Sample : P5252-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F7J23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
Data File : VX044281.D
Acq On : 13 Dec 2024 14:47
Operator : JC/MD
Sample : P5252-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F7J23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------