
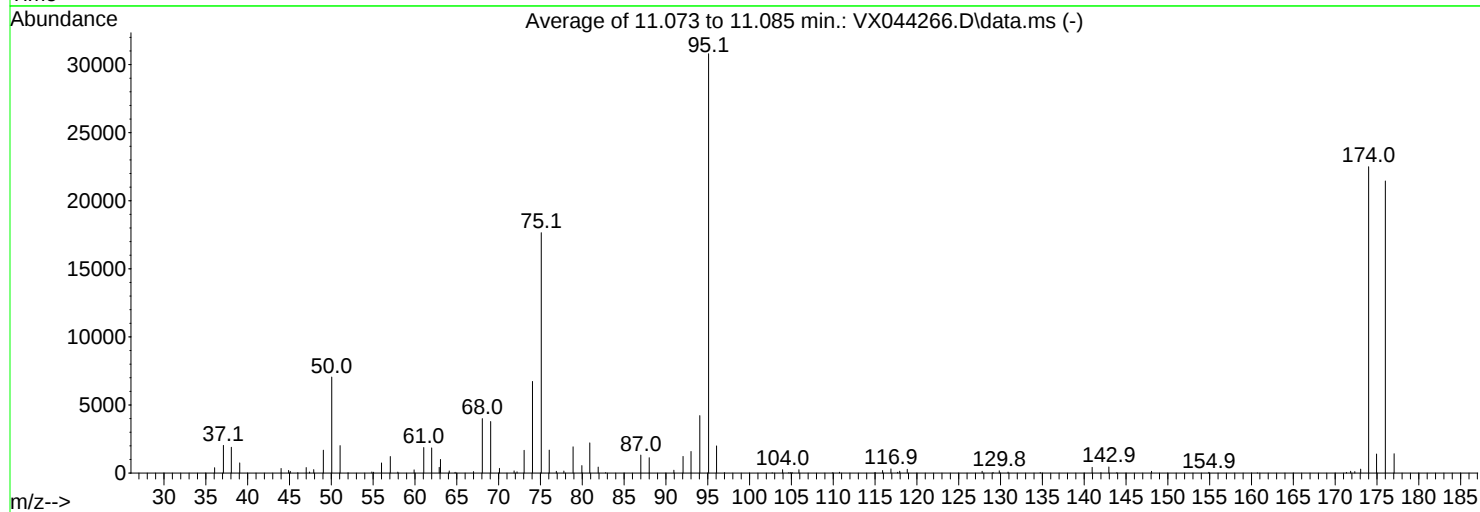


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121324\
Data File : VX044266.D
Acq On : 13 Dec 2024 08:09
Operator : JC/MD
Sample : BFB705
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB705

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Title : VOC Analysis
Last Update : Sat Dec 07 03:56:15 2024

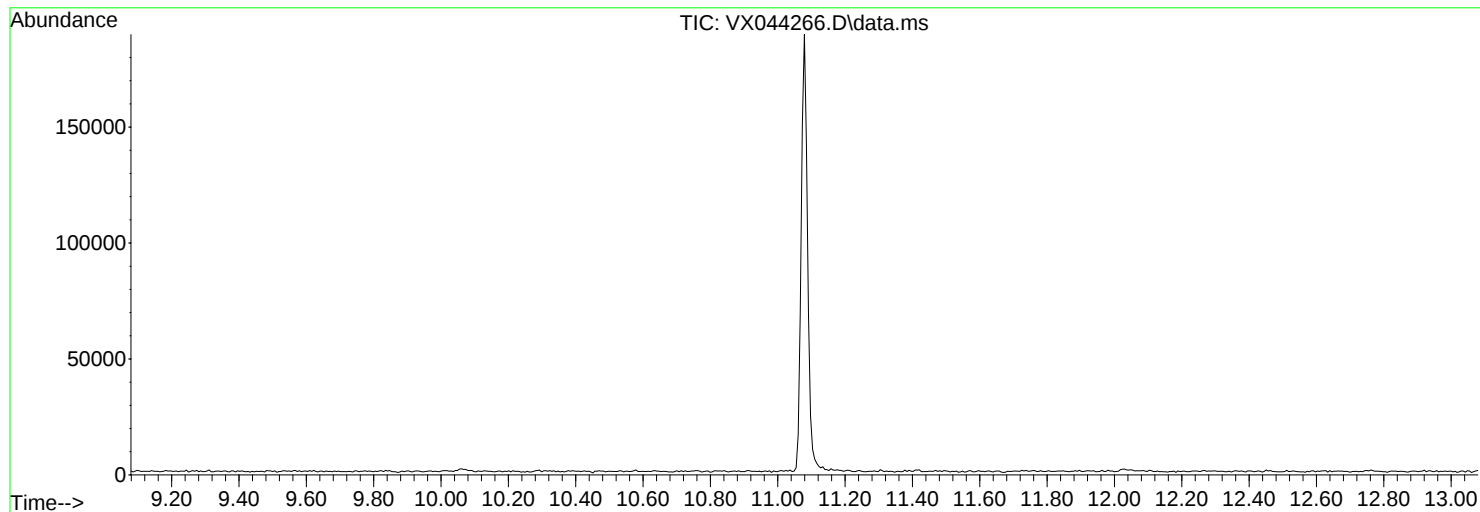

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.9	7049	PASS
75	95	30	80	57.3	17653	PASS
95	95	100	100	100.0	30797	PASS
96	95	5	9	6.5	1994	PASS
173	174	0.00	2	1.3	288	PASS
174	95	50	120	73.1	22499	PASS
175	174	5	9	6.2	1400	PASS
176	174	95	101	95.3	21451	PASS
177	176	5	9	6.6	1422	PASS

Scan 1633 (11.042 min): VX044266.D\data.ms
BFB705

m/z	Abundance
38.40	197.0
39.10	462.0
40.00	577.0
41.10	84.0
44.10	166.0

Instrument :
MSVOA_X
ClientSampleId :
BFB705

m/z	Abundance
36.00	447.0
37.10	2406.0
38.10	1944.0
39.00	1106.0
40.00	489.0
44.00	739.0
44.90	315.0
46.90	462.0
47.40	233.0
47.90	281.0
49.10	1983.0
50.10	6947.0
51.00	1882.0
52.00	52.0
54.80	105.0
55.10	84.0
56.00	705.0
57.00	1157.0
58.00	75.0
59.90	199.0
61.00	1875.0
62.00	1912.0
62.90	1255.0
64.10	221.0
67.00	128.0
68.00	3997.0
69.00	3981.0
70.10	420.0
71.90	115.0
72.20	131.0
73.10	1646.0
74.00	6606.0
75.10	17560.0
76.10	1642.0
77.80	213.0
78.90	2101.0
80.00	538.0
80.90	2402.0
81.90	260.0
82.80	102.0
87.00	1211.0
88.10	1082.0
90.90	183.0
92.00	1164.0
93.10	1611.0
94.00	4473.0
95.10	28064.0
96.00	1835.0
104.10	268.0
104.70	123.0
105.90	200.0
110.90	54.0
115.00	139.0
115.90	160.0
117.00	209.0
117.90	169.0
118.90	267.0
127.70	88.0
129.90	111.0
130.90	64.0
134.70	59.0
140.90	249.0
143.00	393.0
148.00	86.0
160.70	56.0
171.30	78.0
171.90	80.0
172.40	127.0
173.10	283.0
174.00	17688.0
174.90	1196.0
176.00	18768.0
177.10	1324.0

Instrument :
MSVOA_X
ClientSampleId :
BFB705

m/z	Abundance
36.00	388.0
37.10	2444.0
38.10	2283.0
39.00	1333.0
39.90	610.0
44.00	458.0
45.10	375.0
46.00	74.0
47.00	347.0
47.90	233.0
49.00	1758.0
50.10	8200.0
51.10	2485.0
54.90	135.0
56.00	1138.0
57.10	1519.0
58.00	65.0
60.00	333.0
61.10	2438.0
62.00	2344.0
63.10	1781.0
64.10	165.0
64.80	104.0
67.00	139.0
68.10	4482.0
69.10	4474.0
70.10	331.0
71.80	160.0
72.20	146.0
73.00	1804.0
74.00	8258.0
75.10	20496.0
76.00	2037.0
76.90	222.0
77.80	184.0
78.90	2245.0
79.90	582.0
80.90	2390.0
82.00	578.0
87.00	1692.0
87.90	1339.0
91.00	260.0
92.00	1539.0
92.90	1587.0
94.10	4563.0
95.10	36824.0
96.10	2170.0
102.70	75.0
103.90	259.0
104.90	94.0
105.90	262.0
109.90	76.0
110.70	137.0
115.90	192.0
116.80	399.0
118.00	245.0
118.80	338.0
127.80	217.0
129.10	76.0
129.80	166.0
130.90	80.0
134.80	82.0
140.90	500.0
143.00	602.0
143.90	96.0
148.10	159.0
154.90	175.0
171.40	67.0
171.90	180.0
172.40	117.0
173.00	387.0
174.00	27256.0
175.00	1700.0
176.00	24800.0
177.00	1642.0

Instrument :
MSVOA_X
ClientSampleId :
BFB705

m/z	Abundance
36.10	346.0
37.10	1250.0
38.00	1464.0
39.10	1185.0
40.10	382.0
44.10	313.0
44.90	271.0
47.10	411.0
47.90	244.0
49.00	1301.0
50.00	6000.0
51.10	1687.0
55.00	101.0
56.00	388.0
57.10	976.0
57.90	85.0
59.80	180.0
61.00	1317.0
62.10	1281.0
63.00	1222.0
64.00	90.0
64.80	60.0
67.00	63.0
68.00	3521.0
69.00	2907.0
70.10	288.0
71.90	211.0
73.00	1562.0
74.10	5326.0
75.10	14904.0
76.10	1389.0
76.90	164.0
77.80	63.0
78.90	1436.0
80.00	534.0
80.90	1857.0
81.80	486.0
87.00	1062.0
88.00	962.0
90.90	190.0
92.10	971.0
93.00	1561.0
94.10	3626.0
95.10	27504.0
96.10	1978.0
97.00	77.0
103.90	225.0
105.10	85.0
105.90	280.0
115.90	212.0
117.00	314.0
117.70	171.0
118.80	217.0
127.90	95.0
129.10	76.0
129.90	234.0
130.90	75.0
141.00	512.0
142.00	67.0
142.80	349.0
148.00	145.0
171.70	144.0
172.20	86.0
173.00	193.0
174.00	22552.0
175.00	1304.0
176.00	20784.0
177.00	1300.0

Instrument :
MSVOA_X
ClientSampleId :
BFB705