

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX121418\
 Data File : VX006550.D
 Acq On : 15 Dec 2018 07:54
 Operator : JC/MD
 Sample : J6398-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C-MW-05-121118

Quant Time: Dec 17 12:26:16 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112918W.M
 Quant Title : SW846 8260
 QLast Update : Fri Nov 30 03:55:33 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	660942	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	1055565	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	968561	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	456663	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.07	65	359324	53.26	ug/l	0.00
Spiked Amount	50.000		Recovery	=	106.52%	
35) Dibromofluoromethane	5.51	113	309528	45.29	ug/l	0.00
Spiked Amount	50.000		Recovery	=	90.58%	
50) Toluene-d8	8.71	98	1239529	49.86	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.72%	
62) 4-Bromofluorobenzene	11.13	95	452600	48.31	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.62%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX121418\
Data File : VX006550.D
Acq On : 15 Dec 2018 07:54
Operator : JC/MD
Sample : J6398-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C-MW-05-121118

Quant Time: Dec 17 12:26:16 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X112918W.M
Quant Title : SW846 8260
QLast Update : Fri Nov 30 03:55:33 2018
Response via : Initial Calibration

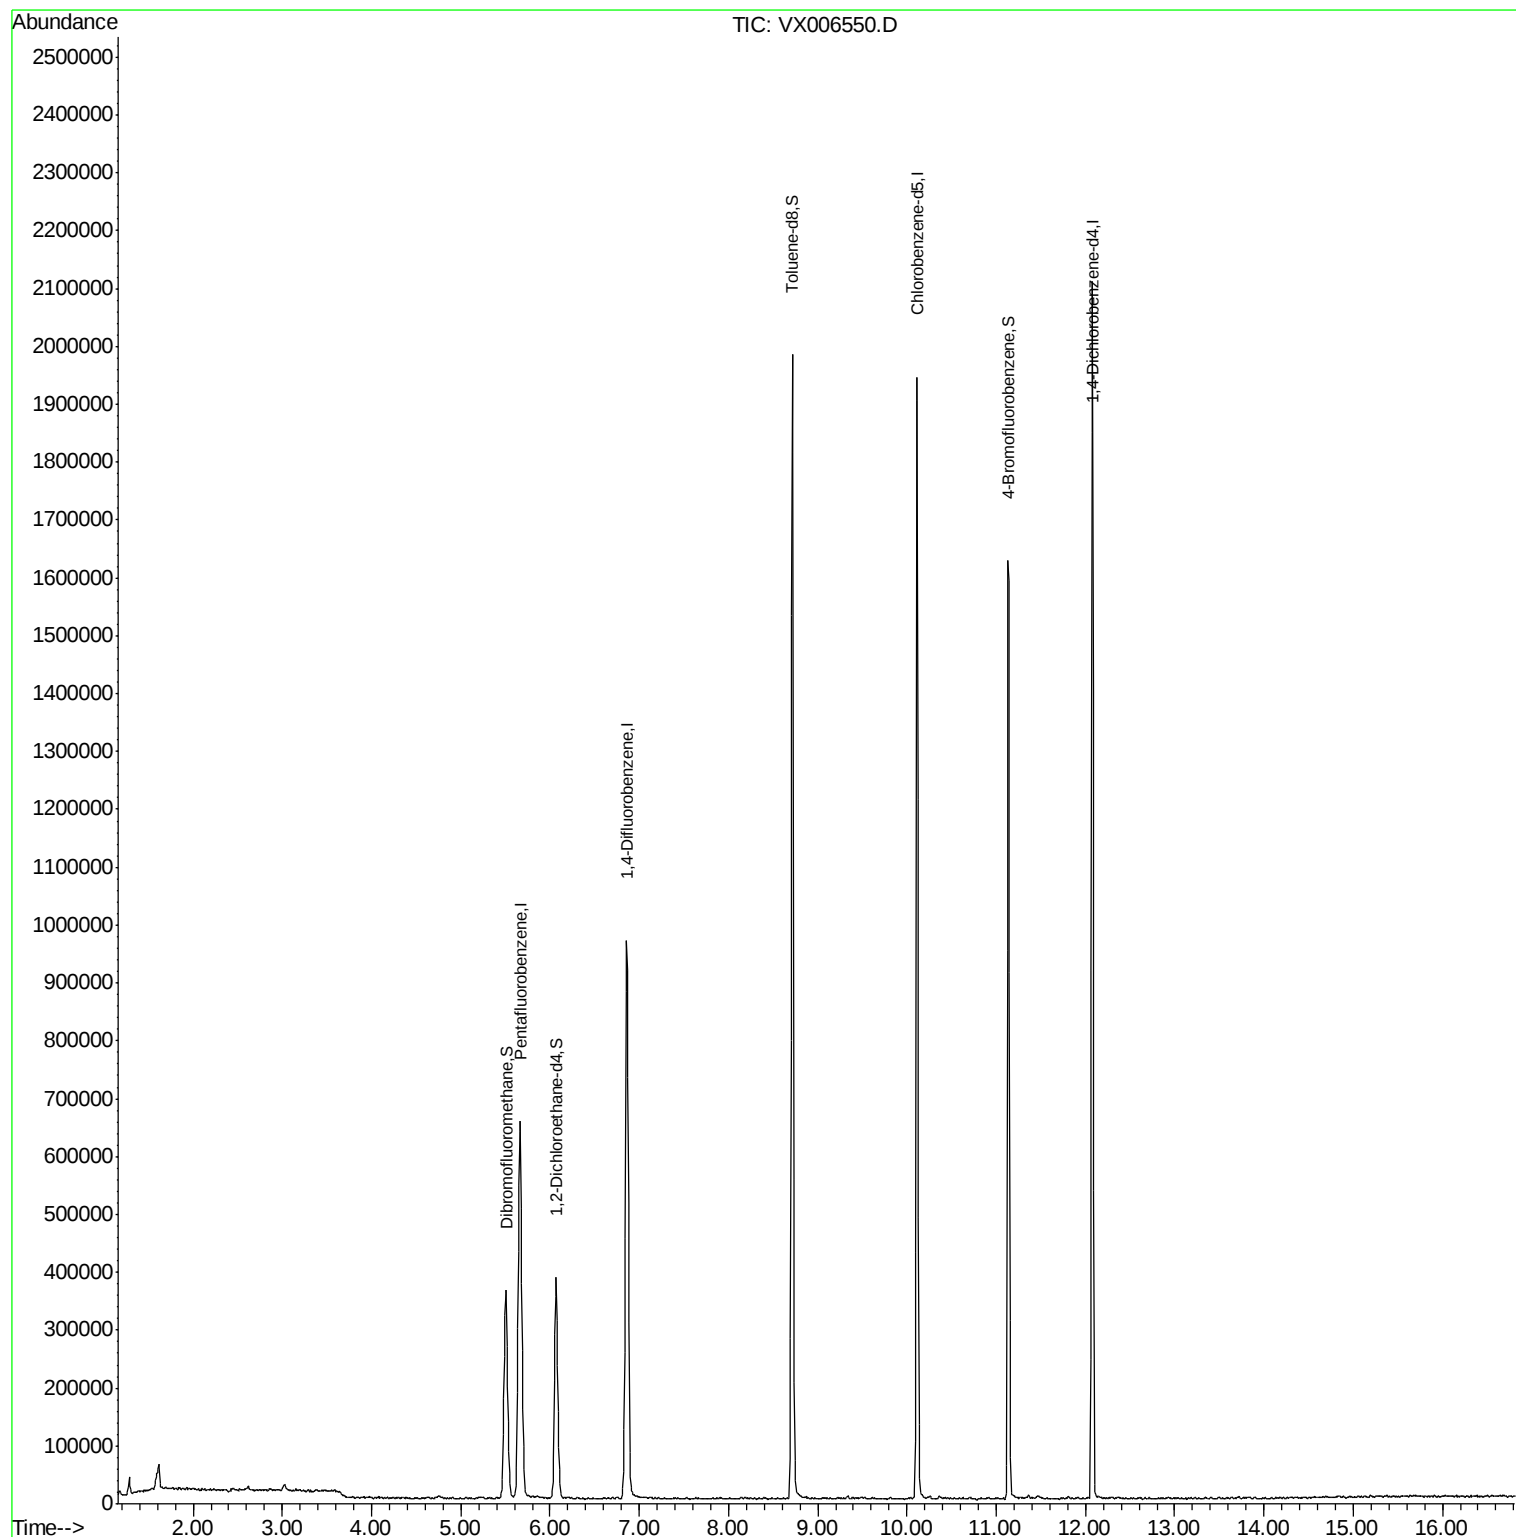

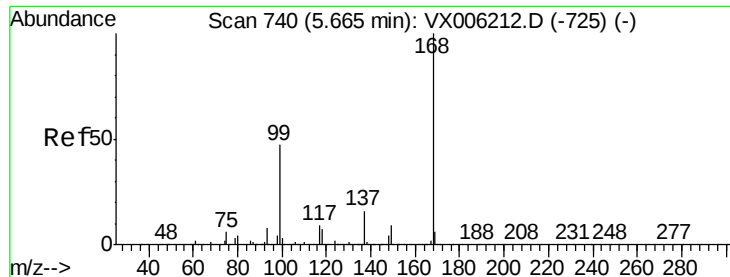

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. 0.00 min

Lab File: VX006550.D

Acq: 15 Dec 2018 07:54

Instrument :

MSVOA_X

ClientSampleId :


C-MW-05-121118

Tgt Ion:168 Resp: 660942

Ion Ratio Lower Upper




168 100

99 52.0 37.8 56.8

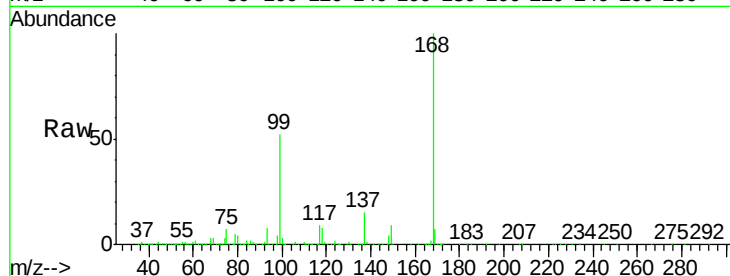

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

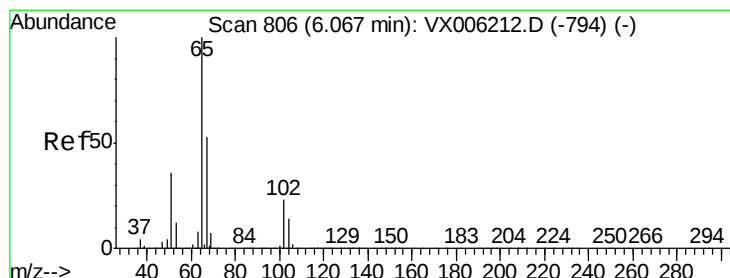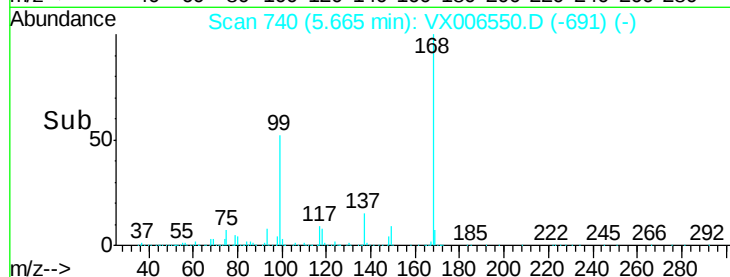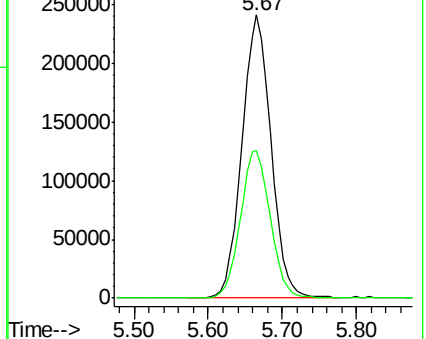

#33

1,2-Dichloroethane-d4

Concen: 53.256 ug/l

RT: 6.07 min Scan# 806

Delta R.T. 0.00 min

Lab File: VX006550.D


Acq: 15 Dec 2018 07:54

Tgt Ion: 65 Resp: 359324

Ion Ratio Lower Upper



65 100

67 53.2 0.0 107.2

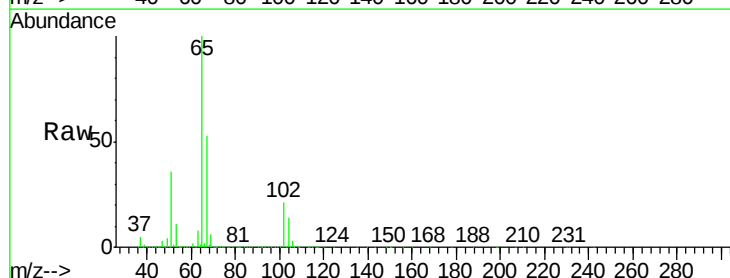

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

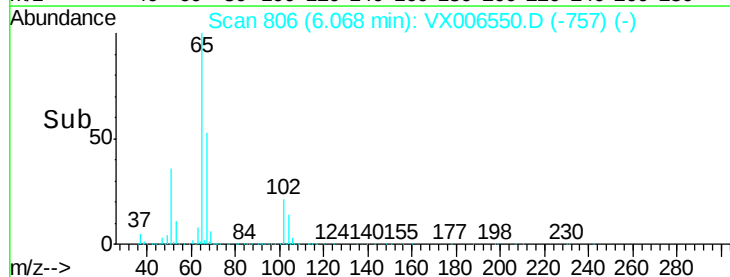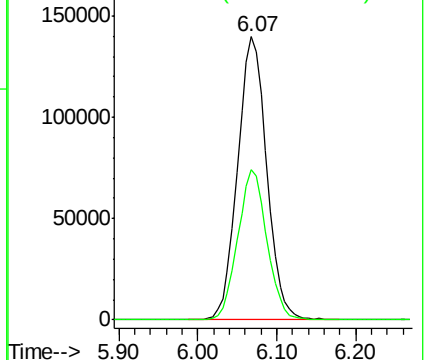



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.86 min Scan# 936

Delta R.T. 0.00 min

Lab File: VX006550.D

Acq: 15 Dec 2018 07:54

Instrument :

MSVOA_X

ClientSampleId :

C-MW-05-121118


Tgt Ion:114 Resp: 1055565

Ion Ratio Lower Upper

114 100

63 18.2 0.0 36.6




88 15.6 0.0 29.0

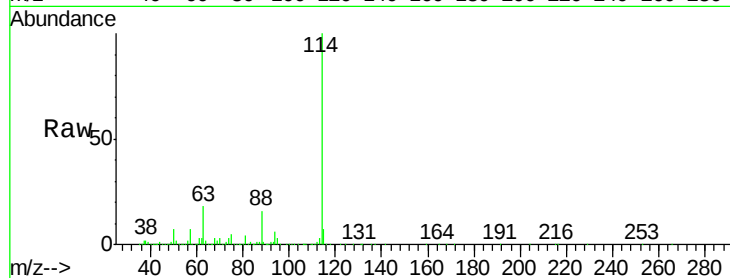

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

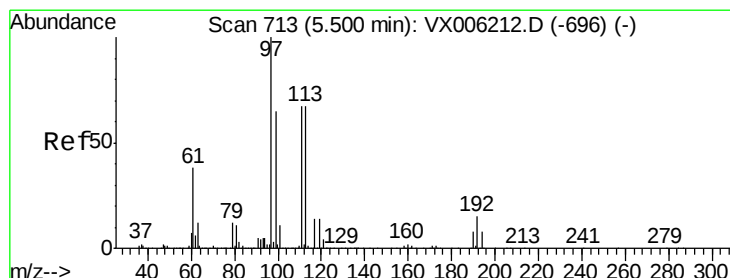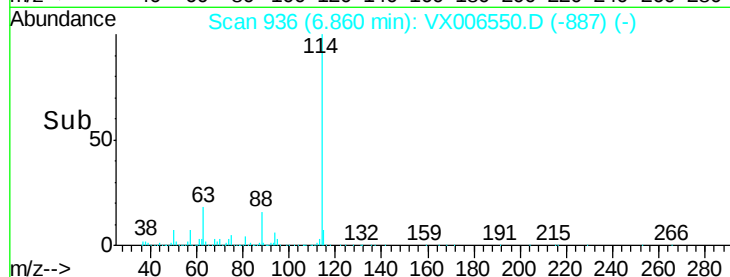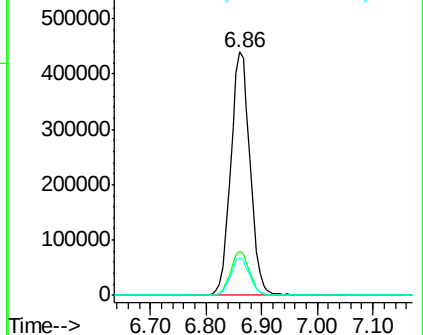

#35

Dibromofluoromethane

Concen: 45.290 ug/l

RT: 5.51 min Scan# 714

Delta R.T. 0.01 min

Lab File: VX006550.D

Acq: 15 Dec 2018 07:54


Tgt Ion:113 Resp: 309528

Ion Ratio Lower Upper

113 100

111 101.1 81.1 121.7



192 20.7 18.2 27.2

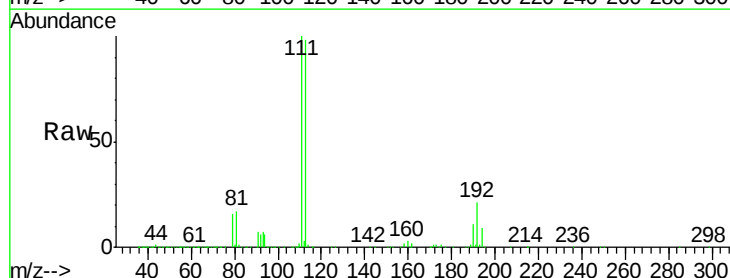

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

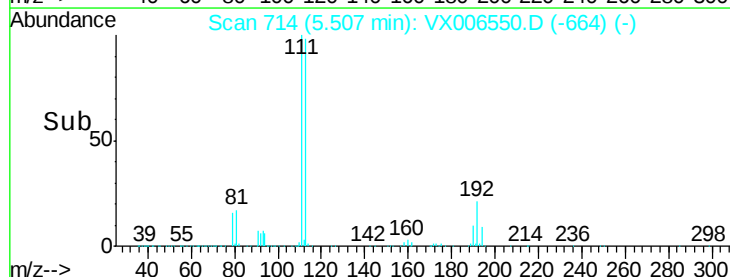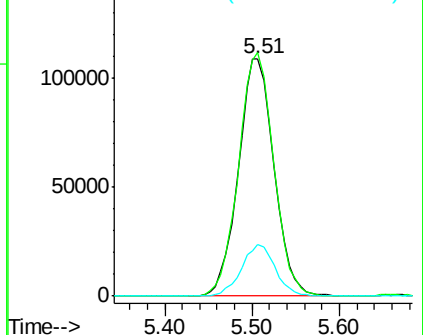



#50

Toluene-d8

Concen: 49.861 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. 0.00 min

Lab File: VX006550.D

Acq: 15 Dec 2018 07:54

Instrument :

MSVOA_X

ClientSampleId :


C-MW-05-121118

Tgt Ion: 98 Resp: 1239529

Ion Ratio Lower Upper




98 100

100 64.7 52.2 78.2

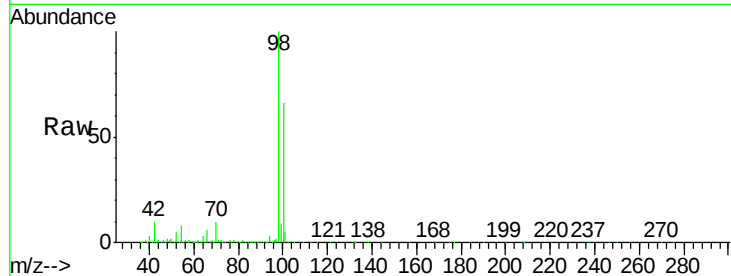

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX

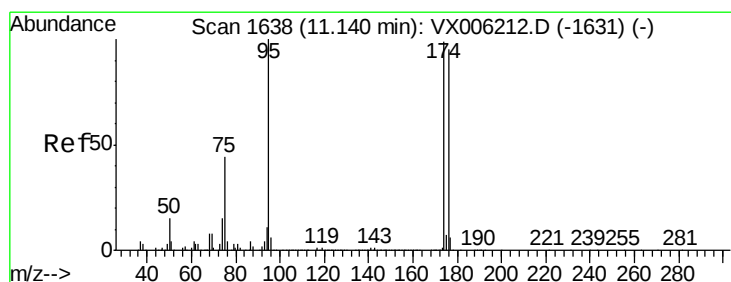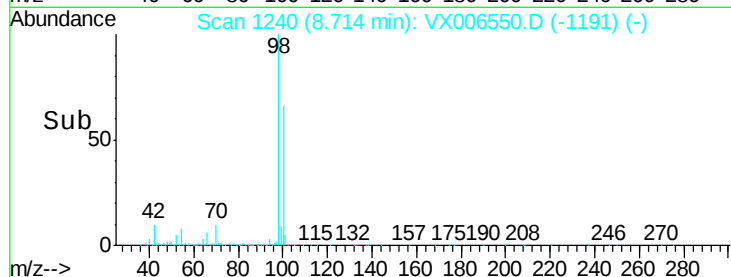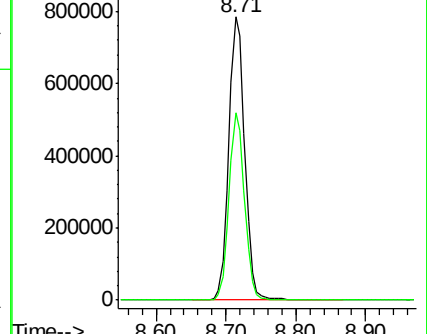

#62

4-Bromofluorobenzene

Concen: 48.315 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. -0.01 min

Lab File: VX006550.D

Acq: 15 Dec 2018 07:54


Tgt Ion: 95 Resp: 452600

Ion Ratio Lower Upper

95 100

174 85.2 0.0 187.0



176 83.8 0.0 181.8

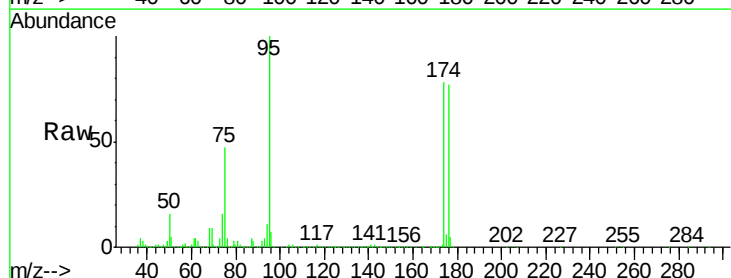


Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V



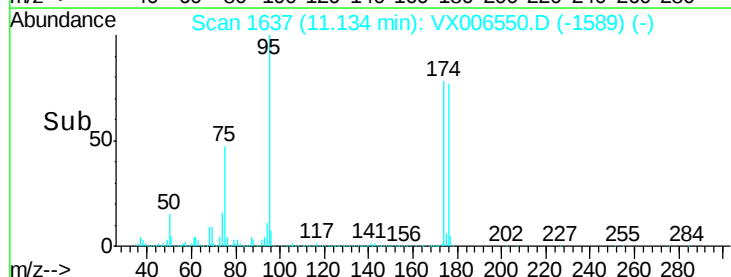
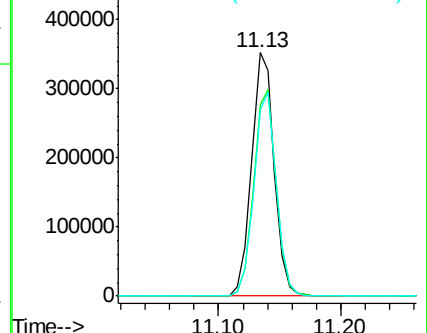


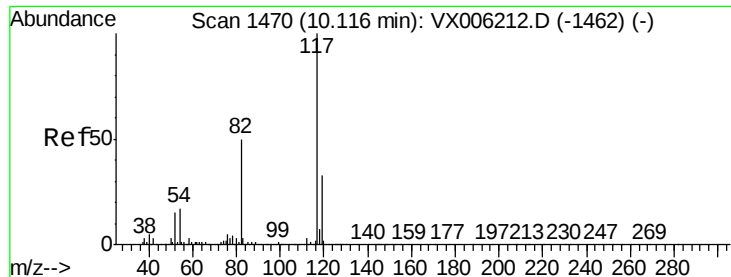

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.12 min Scan# 1470
Delta R.T. 0.00 min
Lab File: VX006550.D
Acq: 15 Dec 2018 07:54

Instrument :
MSVOA_X
ClientSampleId :
C-MW-05-121118

Tgt Ion	Ratio	Lower	Upper
117	100		
82	50.8	39.6	59.4
119	32.6	26.3	39.5

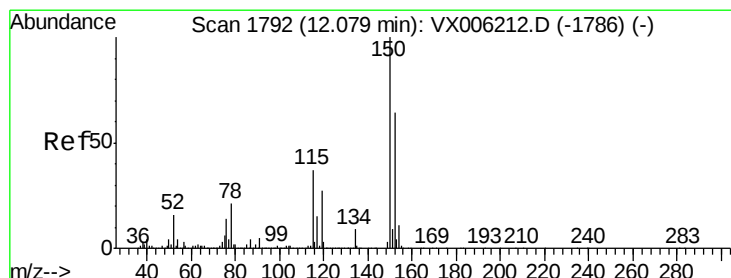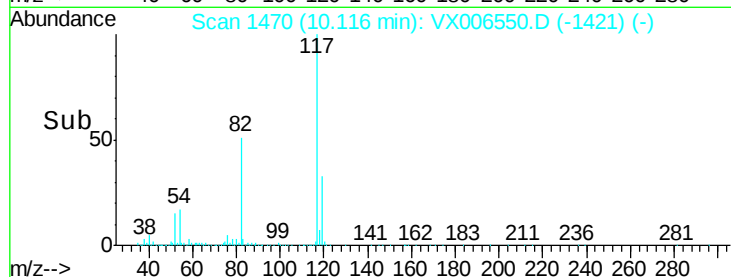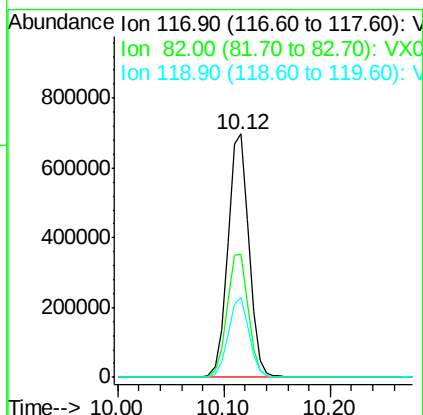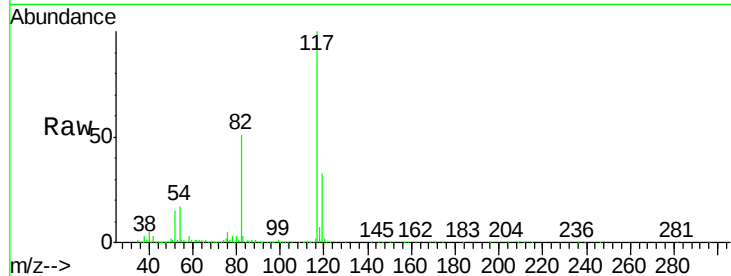

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.08 min Scan# 1792
Delta R.T. 0.00 min
Lab File: VX006550.D
Acq: 15 Dec 2018 07:54

Tgt Ion	Ratio	Lower	Upper
152	100		
115	57.1	39.0	116.9
150	158.4	0.0	345.8

