


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX121418\
Data File : VX006509.D
Acq On : 14 Dec 2018 11:03
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112918W.M
Title : SW846 8260
Last Update : Fri Nov 30 03:55:33 2018

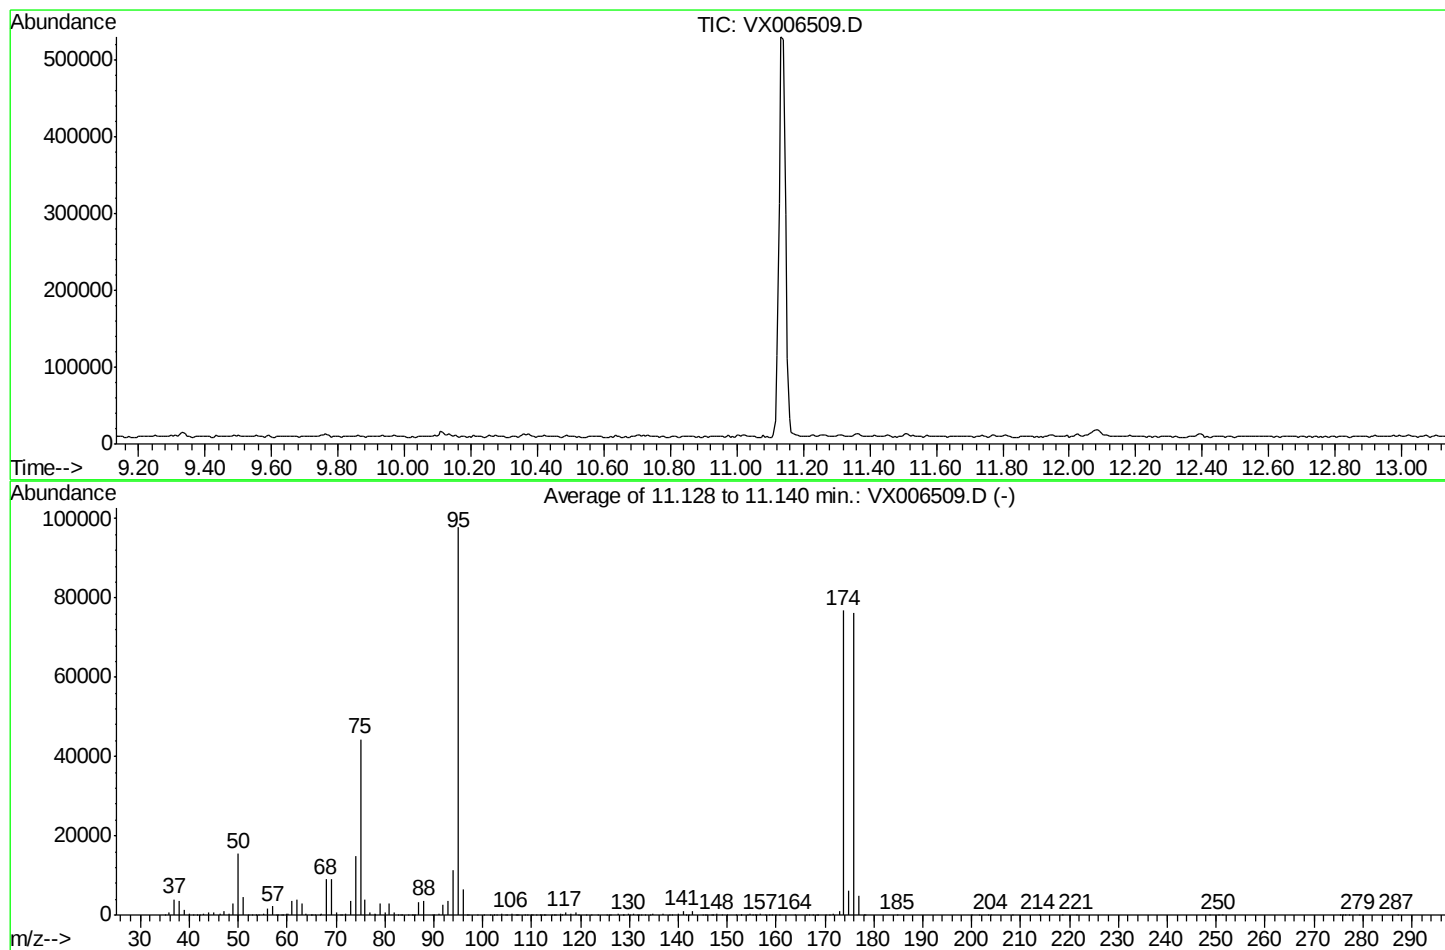

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	15451	PASS
75	95	30	60	45.3	44341	PASS
95	95	100	100	100.0	97842	PASS
96	95	5	9	6.6	6410	PASS
173	174	0.00	2	1.1	837	PASS
174	95	50	100	78.5	76850	PASS
175	174	5	9	8.1	6209	PASS
176	174	95	101	99.1	76173	PASS
177	176	5	9	6.5	4918	PASS