


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX121418\
Data File : VX006535.D
Acq On : 14 Dec 2018 23:38
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X112918W.M
Title : SW846 8260
Last Update : Fri Nov 30 03:55:33 2018

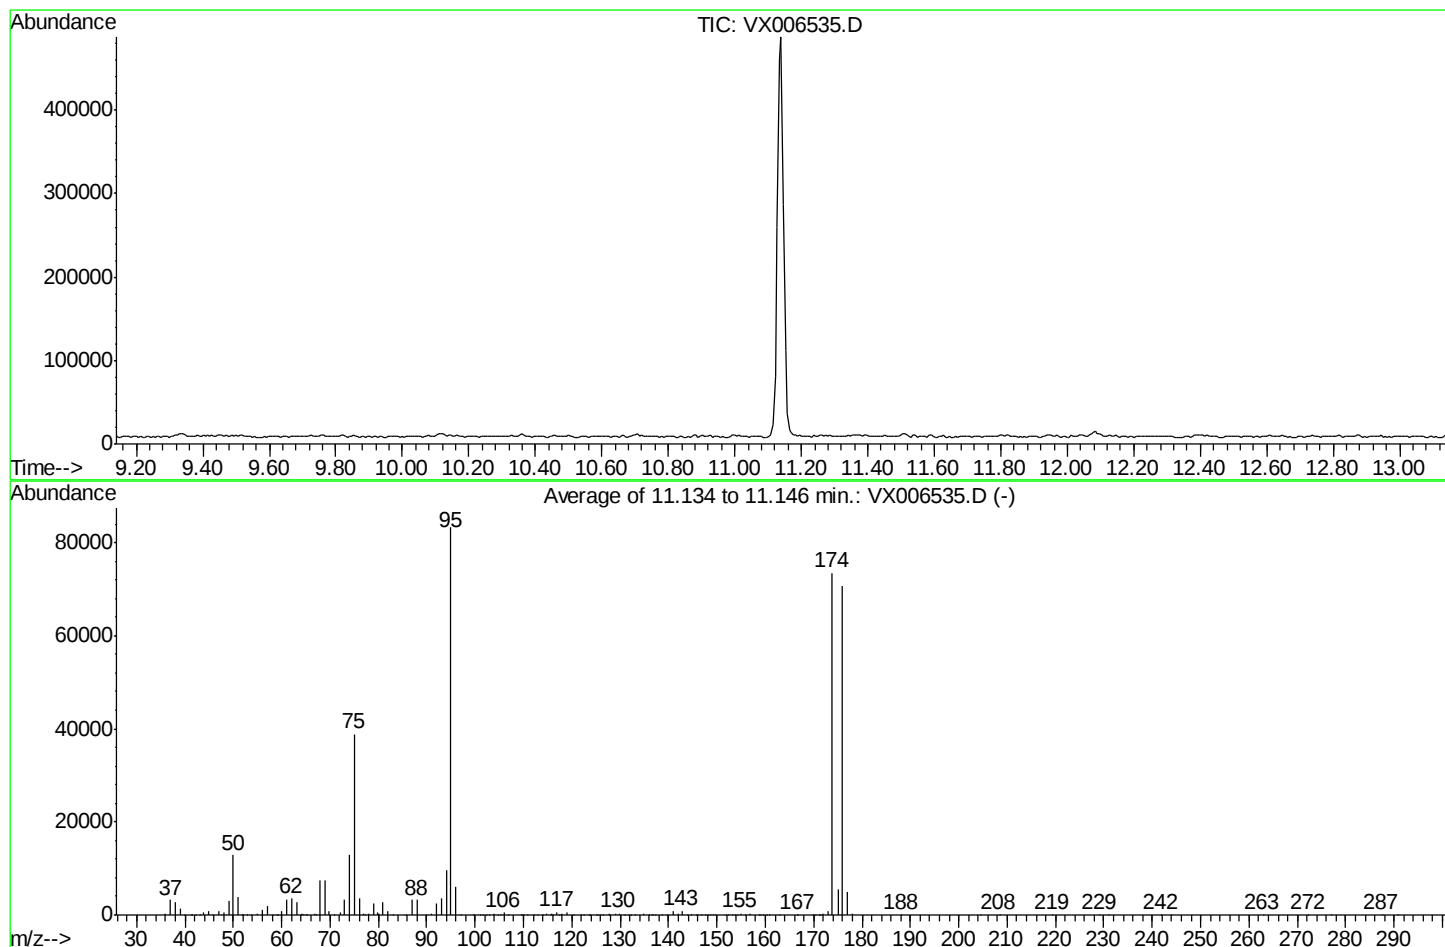

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1628

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.4	12839	PASS
75	95	30	60	46.6	38842	PASS
95	95	100	100	100.0	83282	PASS
96	95	5	9	7.4	6167	PASS
173	174	0.00	2	1.2	877	PASS
174	95	50	100	88.3	73549	PASS
175	174	5	9	7.6	5567	PASS
176	174	95	101	96.1	70696	PASS
177	176	5	9	6.9	4862	PASS