

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX121420\
 Data File : VX019979.D
 Acq On : 14 Dec 2020 12:22
 Operator : JC/MD
 Sample : L5052-15
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TU032-32-TB-121020

Quant Time: Dec 15 00:39:22 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X120420W.M
 Quant Title : SW846 8260
 QLast Update : Fri Dec 04 15:32:53 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	318079	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	519379	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.09	117	476885	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	208593	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.03	65	196852	47.09	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	94.18%		
35) Dibromofluoromethane	5.46	113	160373	47.78	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	95.56%		
50) Toluene-d8	8.70	98	634597	49.52	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	99.04%		
62) 4-Bromofluorobenzene	11.12	95	221693	45.45	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	90.90%		


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX121420\
Data File : VX019979.D
Acq On : 14 Dec 2020 12:22
Operator : JC/MD
Sample : L5052-15
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TU032-32-TB-121020

Quant Time: Dec 15 00:39:22 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X120420W.M
Quant Title : SW846 8260
QLast Update : Fri Dec 04 15:32:53 2020
Response via : Initial Calibration

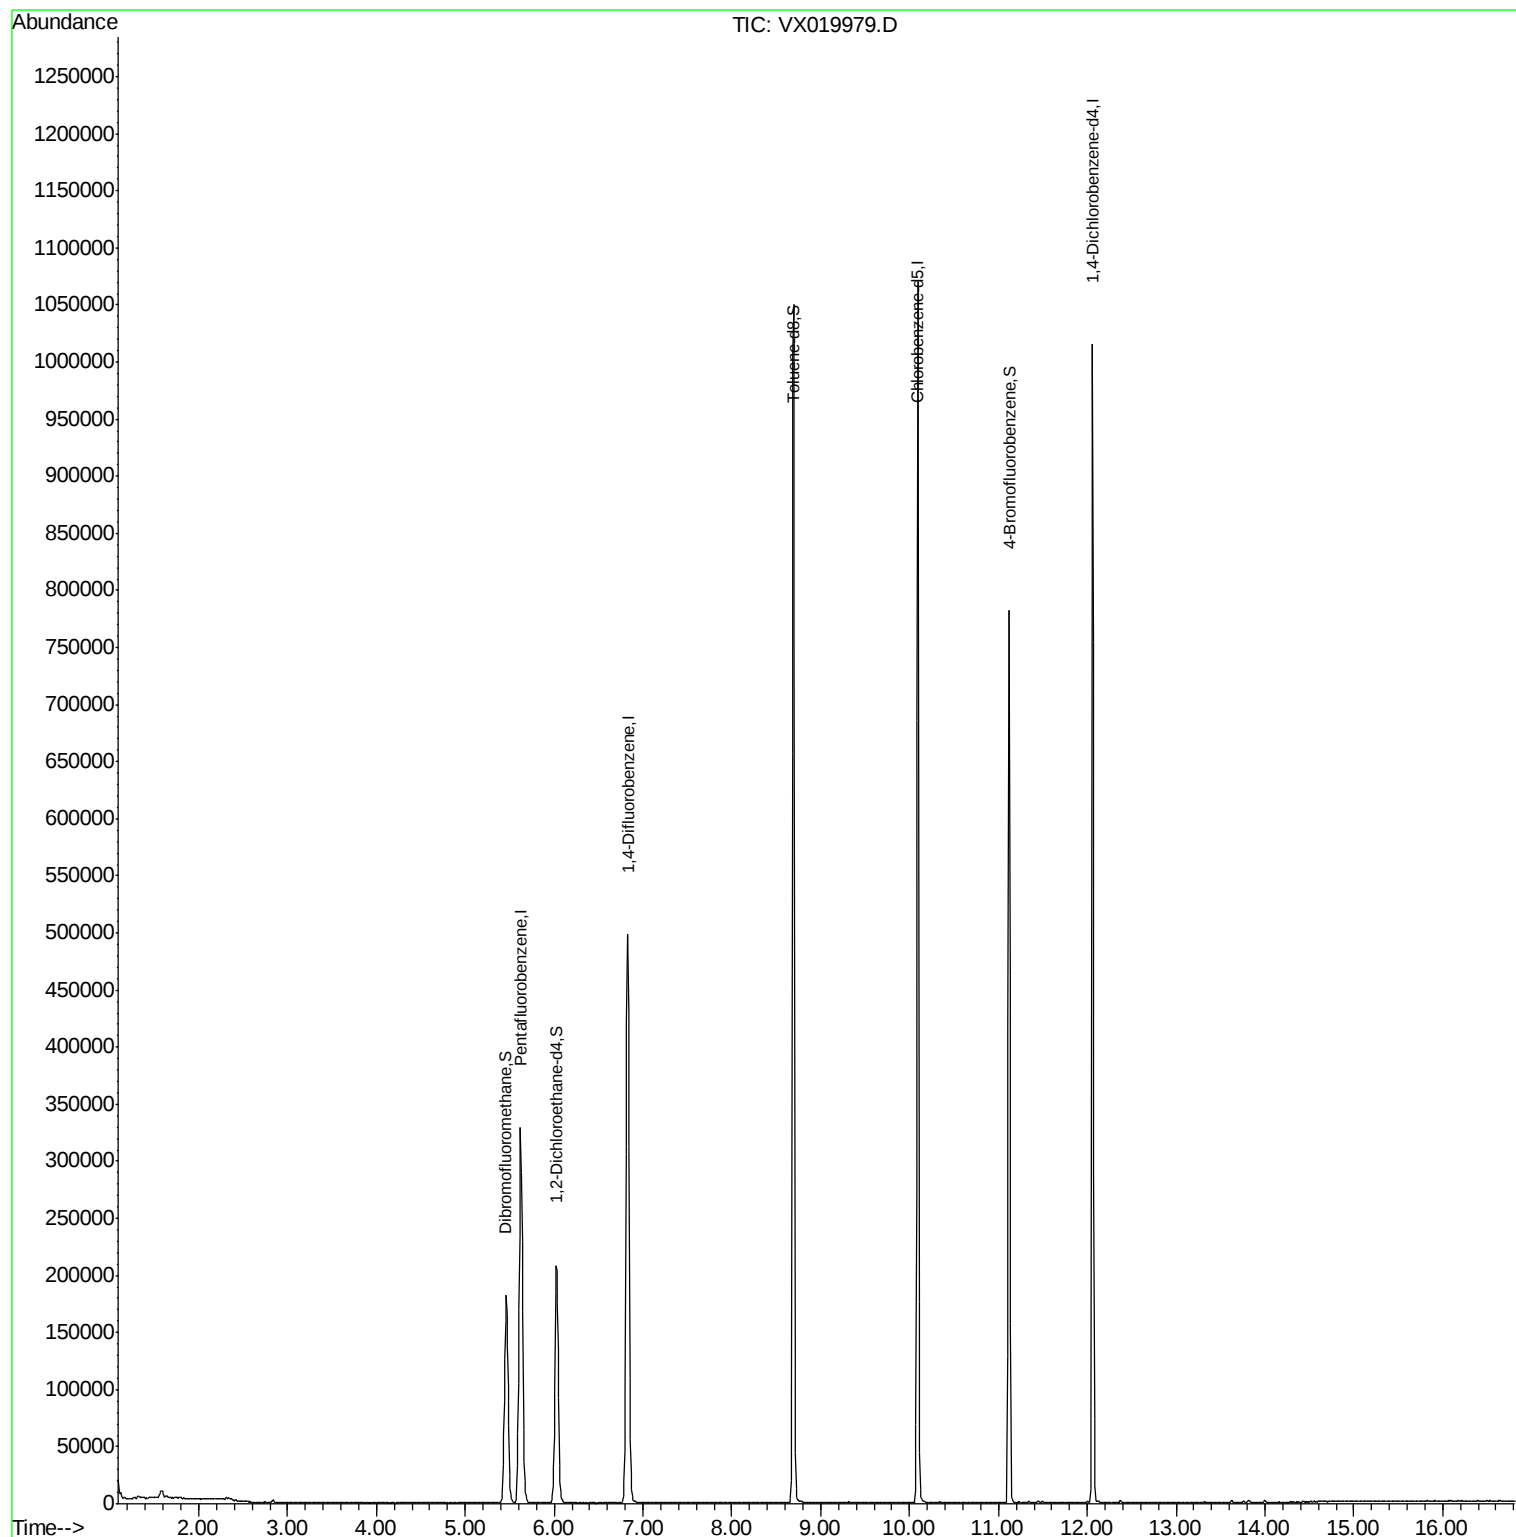

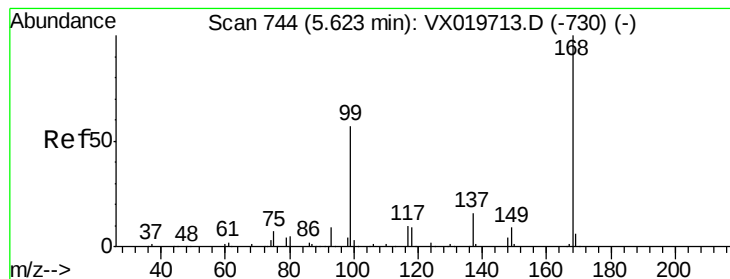

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.63 min Scan# 745

Delta R.T. 0.01 min

Lab File: VX019979.D

Acq: 14 Dec 2020 12:22

Instrument :

MSVOA_X

ClientSampleId :


TU032-32-TB-121020

Tot Ion:168 Resp: 318079

Ion Ratio Lower Upper

168 100

99 53.6 45.8 68.6

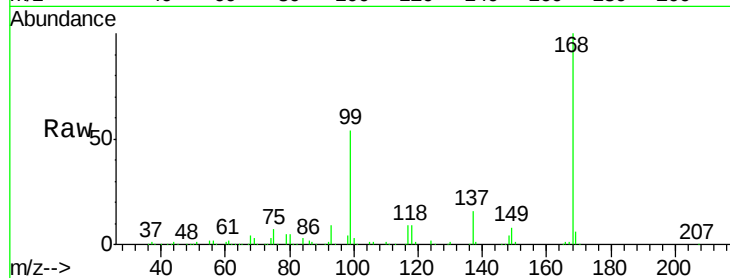

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.63



100000

50000

0

Time-->

5.50 5.60 5.70 5.80

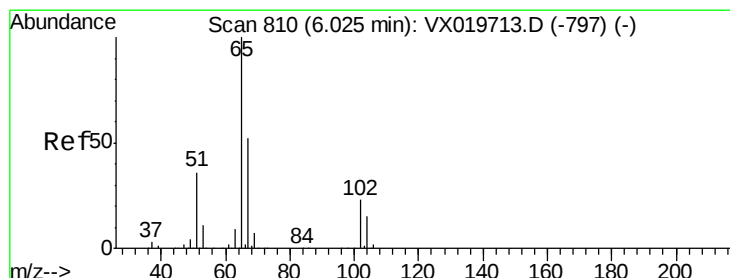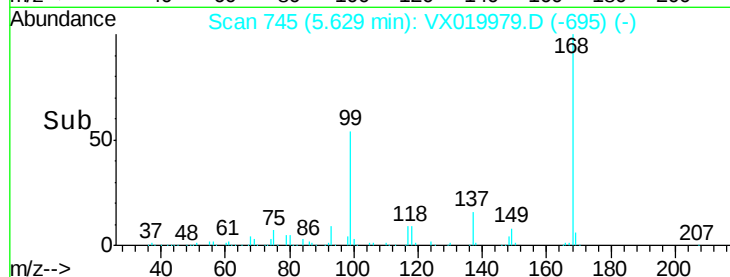

#33

1,2-Dichloroethane-d4

Concen: 47.088 ug/l

RT: 6.03 min Scan# 810

Delta R.T. 0.00 min

Lab File: VX019979.D


Acq: 14 Dec 2020 12:22

Tgt Ion: 65 Resp: 196852

Ion Ratio Lower Upper

65 100

67 53.4 0.0 105.4

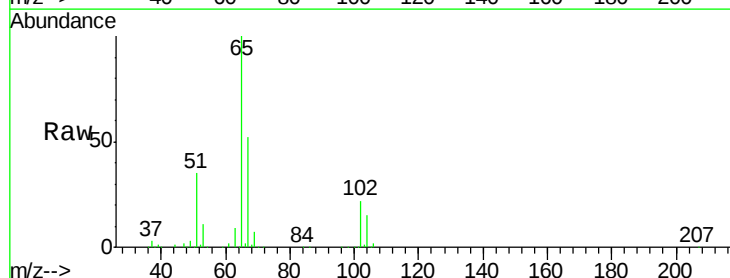

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.03

80000

60000


40000


20000

0

Time-->

5.90 6.00 6.10

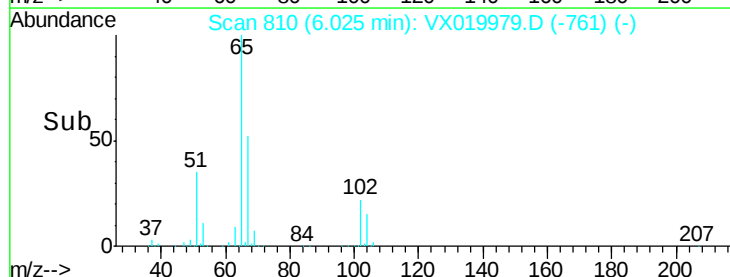

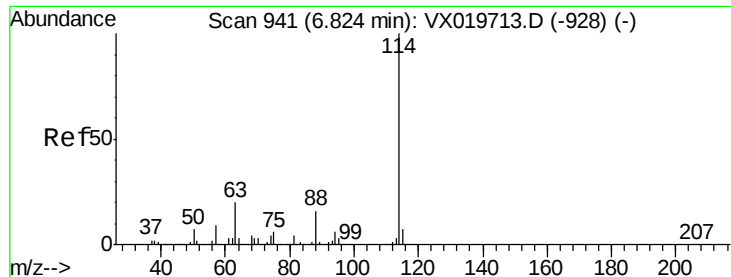

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.83 min Scan# 942

Delta R.T. 0.01 min

Lab File: VX019979.D

Acq: 14 Dec 2020 12:22

Instrument :

MSVOA_X

ClientSampleId :

TU032-32-TB-121020


Tot Ion:114 Resp: 519379

Ion Ratio Lower Upper

114 100

63 20.6 0.0 40.8




88 16.3 0.0 32.8

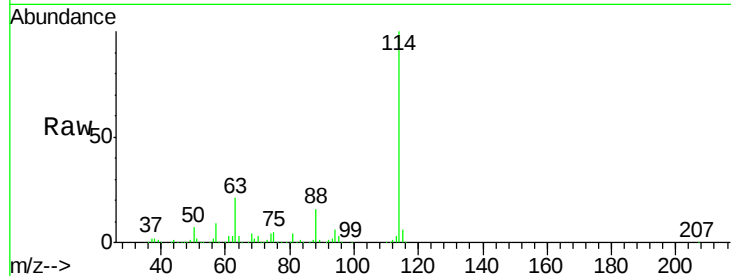

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

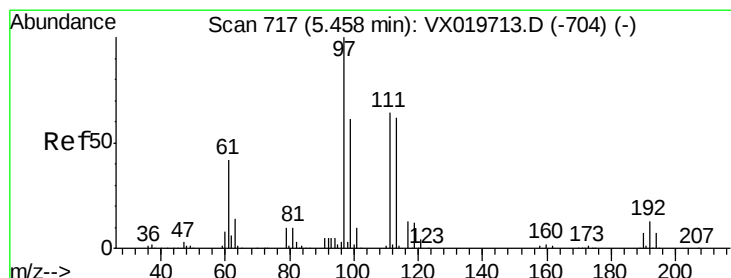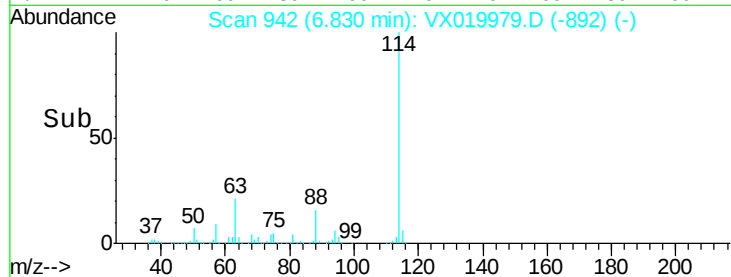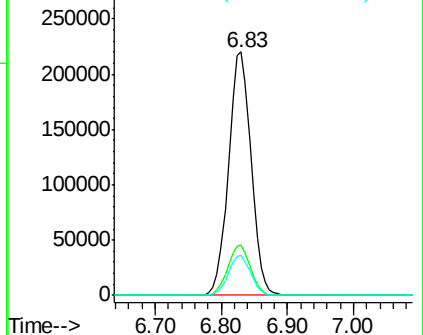

#35

Dibromofluoromethane

Concen: 47.777 ug/l

RT: 5.46 min Scan# 717

Delta R.T. 0.00 min

Lab File: VX019979.D

Acq: 14 Dec 2020 12:22


Tgt Ion:113 Resp: 160373

Ion Ratio Lower Upper

113 100

111 103.0 81.9 122.9



192 20.6 16.7 25.1

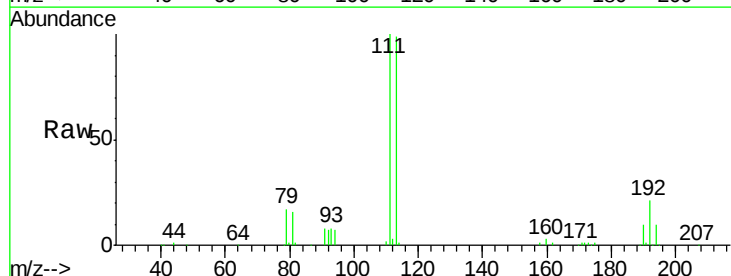


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

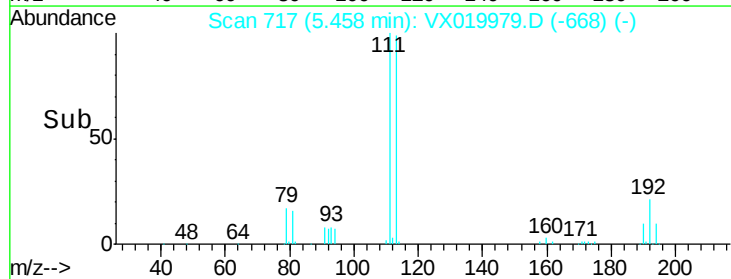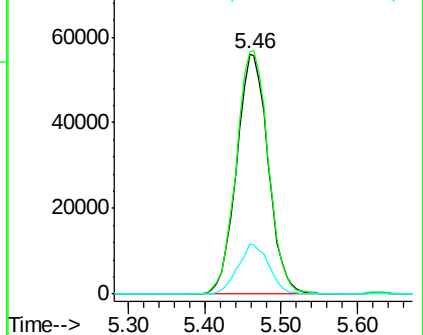

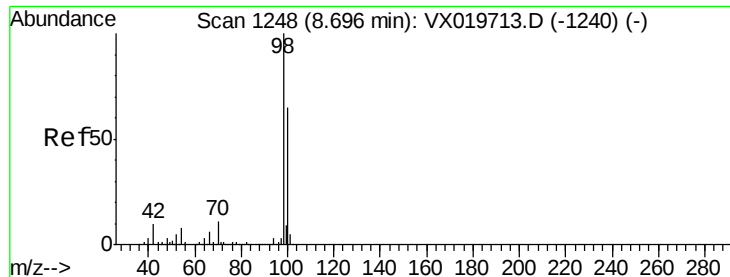

#50

Toluene-d8

Concen: 49.520 ug/l

RT: 8.70 min Scan# 1248

Delta R.T. 0.00 min

Lab File: VX019979.D

Acq: 14 Dec 2020 12:22

Instrument :

MSVOA_X

ClientSampleId :


TU032-32-TB-121020

Tot Ion: 98 Resp: 634597

Ion Ratio Lower Upper




98 100

100 65.8 51.9 77.9

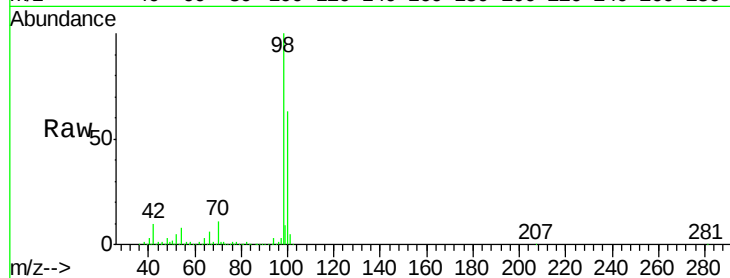

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX

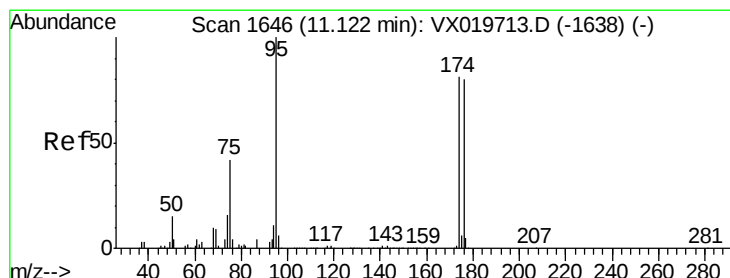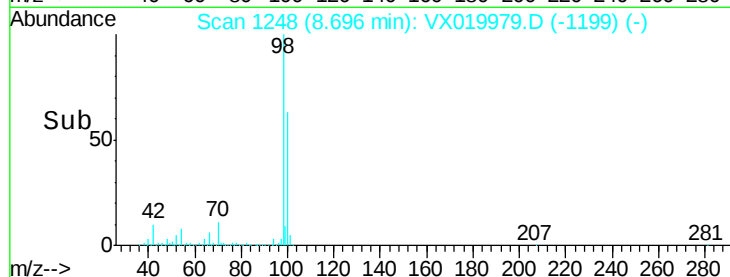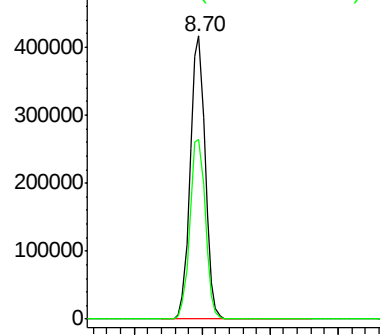

#62

4-Bromofluorobenzene

Concen: 45.452 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. 0.00 min

Lab File: VX019979.D

Acq: 14 Dec 2020 12:22


Tgt Ion: 95 Resp: 221693

Ion Ratio Lower Upper

95 100

174 77.0 0.0 154.6



176 75.2 0.0 155.8

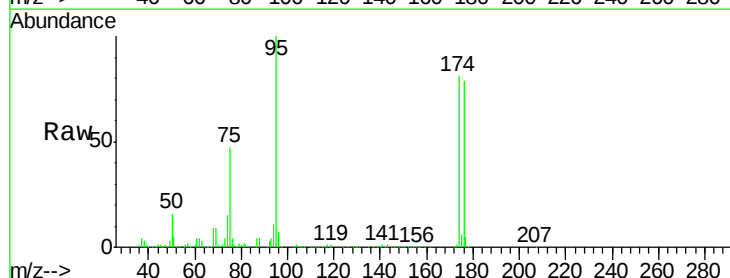


Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V



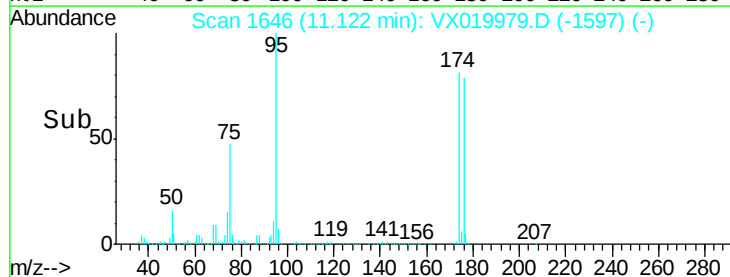
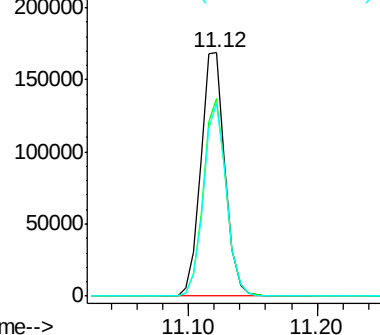


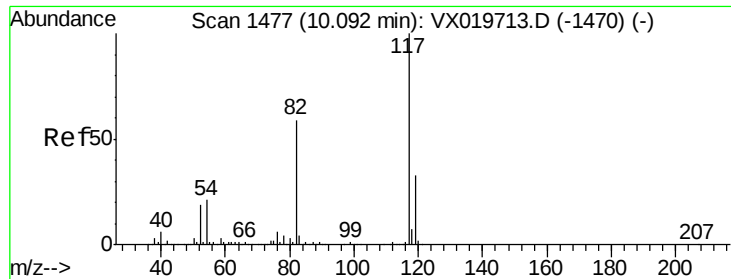

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.09 min Scan# 1477
Delta R.T. 0.00 min
Lab File: VX019979.D
Acq: 14 Dec 2020 12:22

Instrument :
MSVOA_X
ClientSampleId :
TU032-32-TB-121020

Tot Ion:117 Resp: 476885
Ion Ratio Lower Upper
117 100
82 59.8 47.4 71.2
119 32.8 26.6 39.8

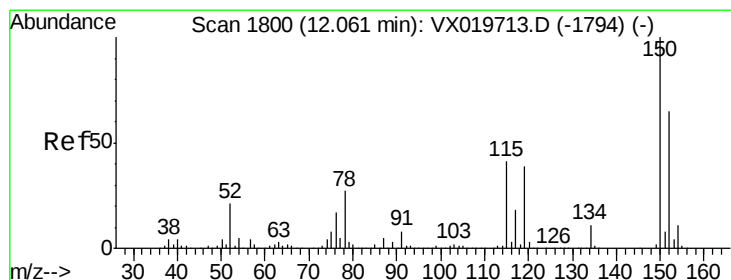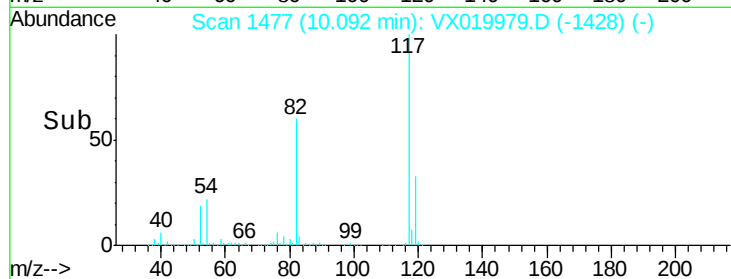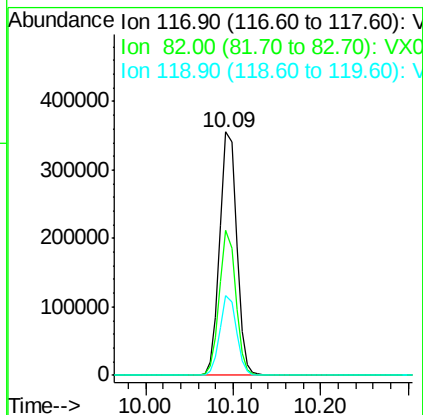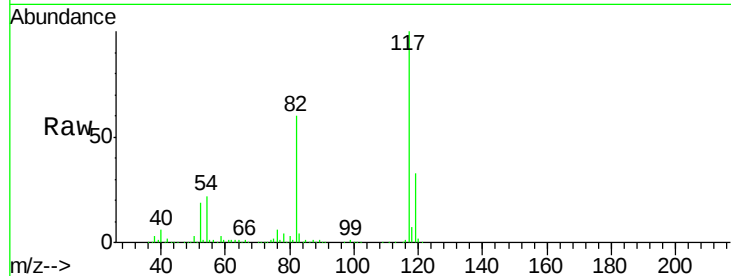

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.06 min Scan# 1800
Delta R.T. 0.00 min
Lab File: VX019979.D
Acq: 14 Dec 2020 12:22

Tgt Ion:152 Resp: 208593
Ion Ratio Lower Upper
152 100
115 60.2 41.1 123.3
150 157.3 0.0 349.0

