

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121422\
 Data File : VX033416.D
 Acq On : 14 Dec 2022 13:58
 Operator : JC/MD
 Sample : N6049-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB-01-121322

Quant Time: Dec 14 22:49:16 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
 Quant Title : SW846 8260
 QLast Update : Wed Dec 07 12:43:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	126325	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	199969	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	177287	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	81682	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	37993	46.881	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	93.760%
35) Dibromofluoromethane	5.379	113	42278	47.006	ug/l	-0.01
Spiked Amount	50.000	Range	75 - 124	Recovery	=	94.020%
50) Toluene-d8	8.647	98	88848	47.221	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	94.440%
62) 4-Bromofluorobenzene	11.079	95	67625	47.006	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	94.020%


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121422\
Data File : VX033416.D
Acq On : 14 Dec 2022 13:58
Operator : JC/MD
Sample : N6049-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-01-121322

Quant Time: Dec 14 22:49:16 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260
QLast Update : Wed Dec 07 12:43:54 2022
Response via : Initial Calibration




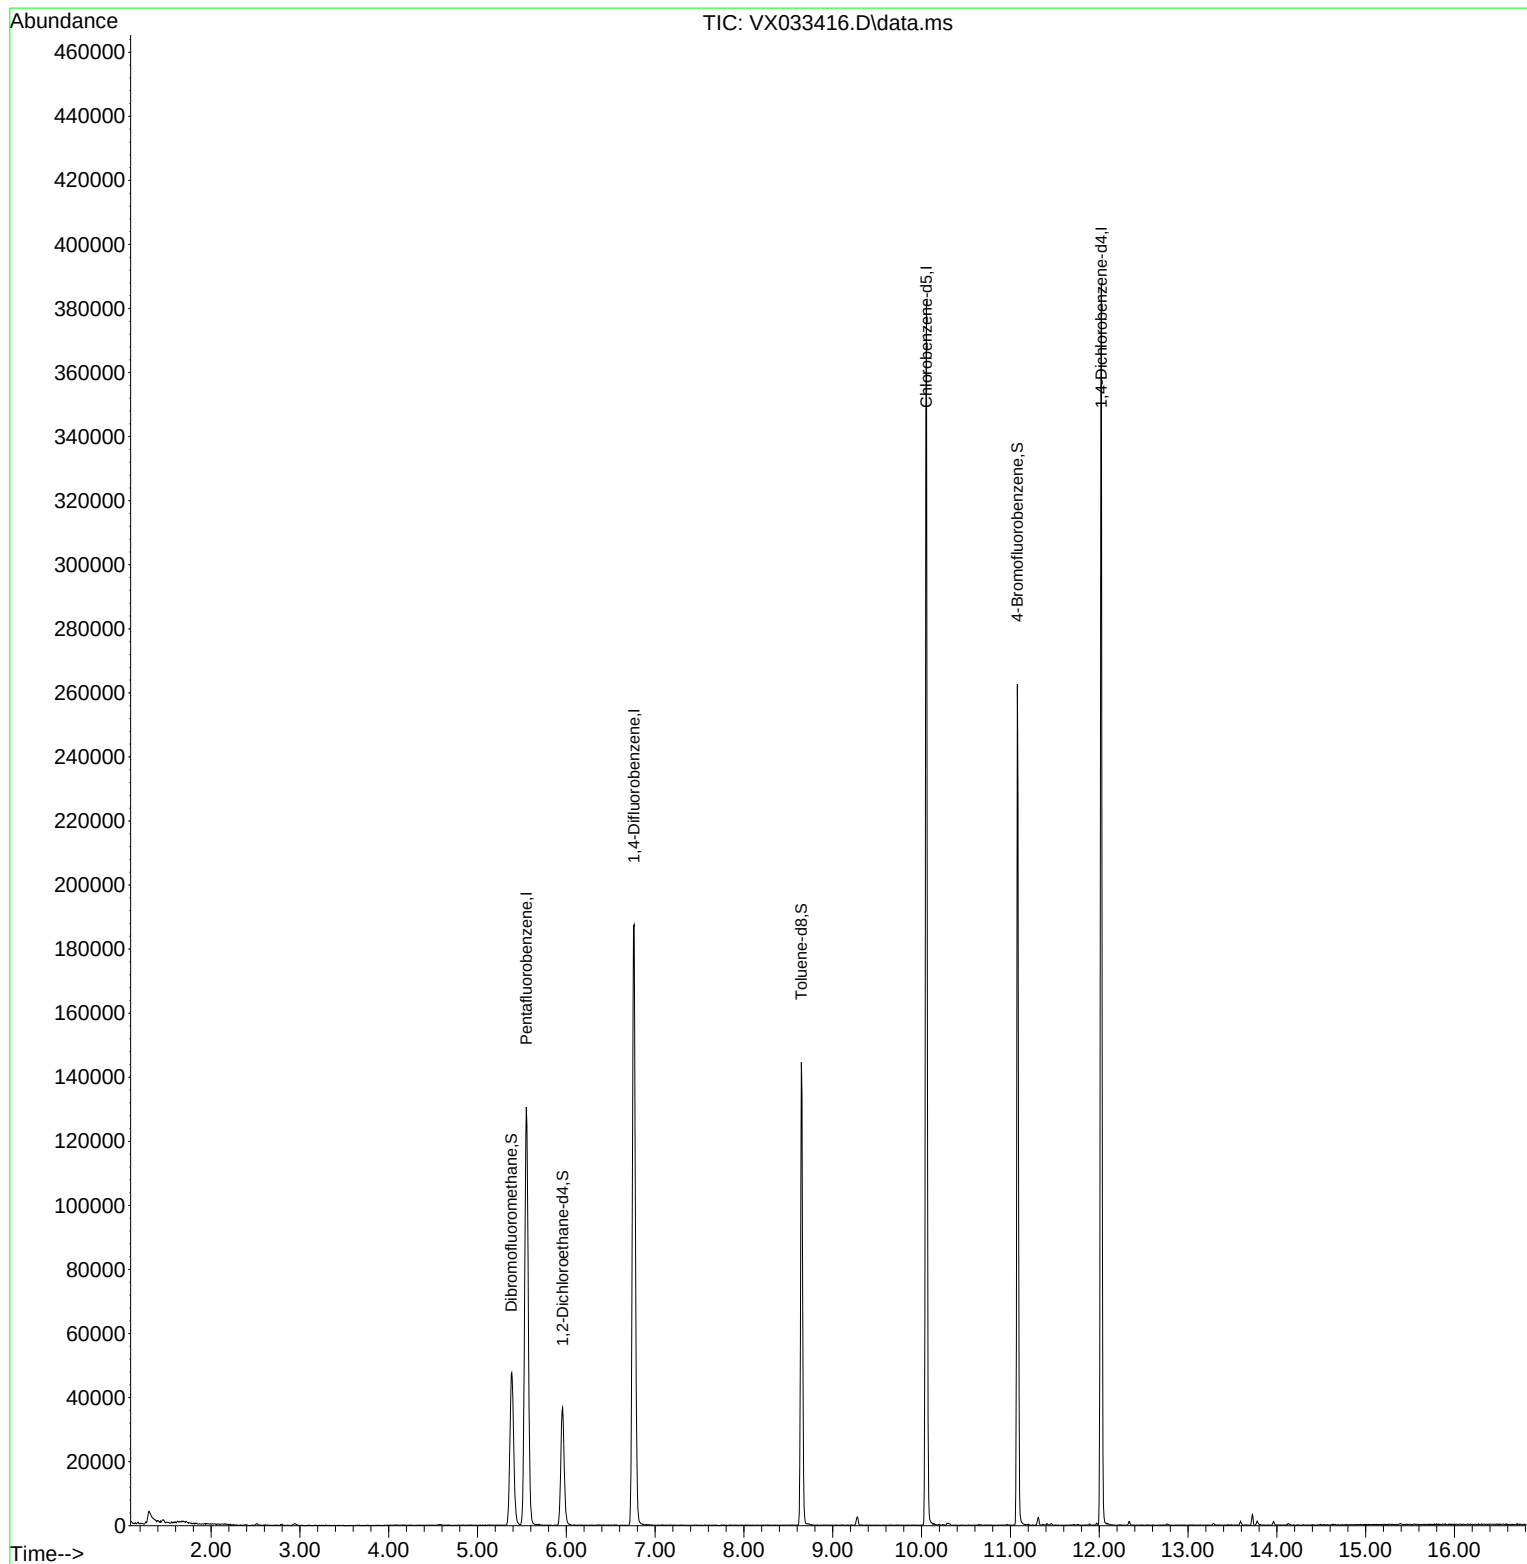


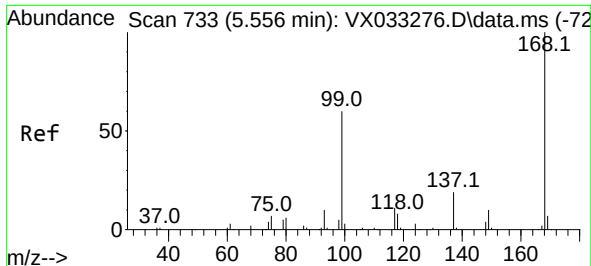

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 711
Delta R.T. -0.006 min
Lab File: VX033416.D
Acq: 14 Dec 2022 13:58




Instrument :
MSVOA_X
ClientSampleId :
TB-01-121322


Tgt Ion:168 Resp: 126325
Ion Ratio Lower Upper
168 100
99 57.3 46.1 69.1

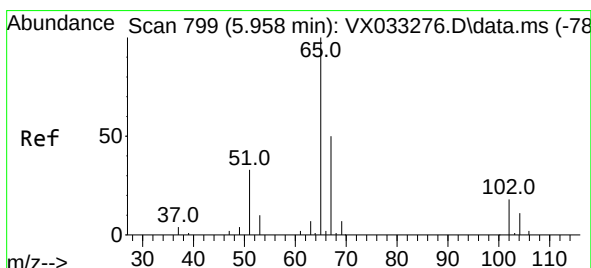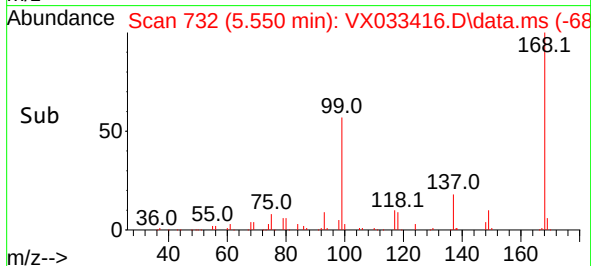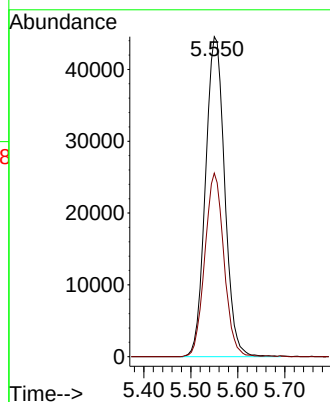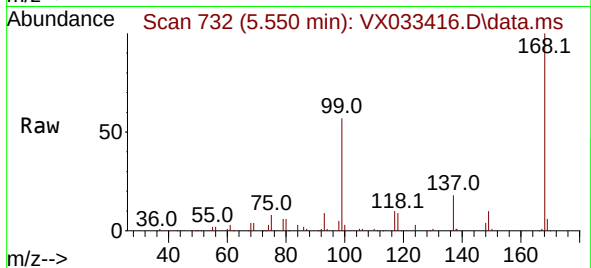

#33
1,2-Dichloroethane-d4
Concen: 46.881 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX033416.D
Acq: 14 Dec 2022 13:58

Tgt Ion: 65 Resp: 37993
Ion Ratio Lower Upper
65 100
67 50.7 0.0 101.8


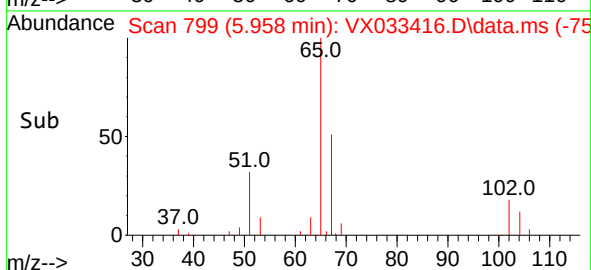
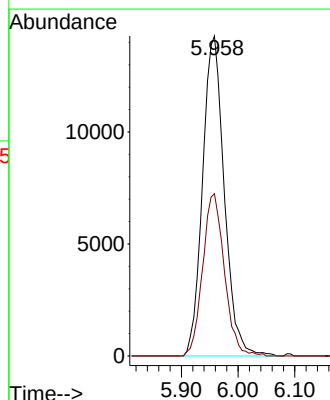
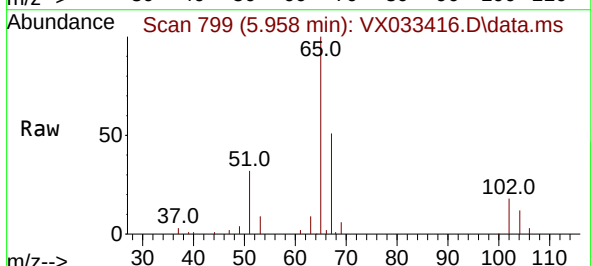


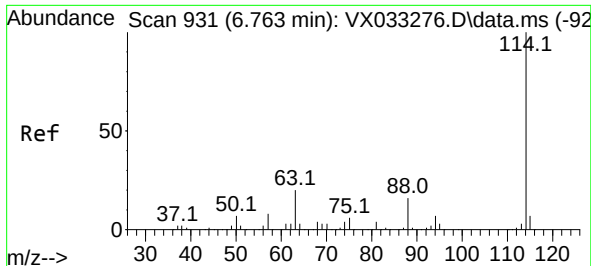

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX033416.D
Acq: 14 Dec 2022 13:58




Instrument :
MSVOA_X
ClientSampleId :
TB-01-121322


Tgt Ion:114 Resp: 199969
Ion Ratio Lower Upper
114 100
63 18.4 0.0 41.6
88 15.3 0.0 33.4

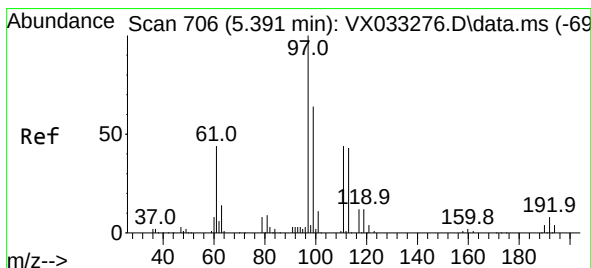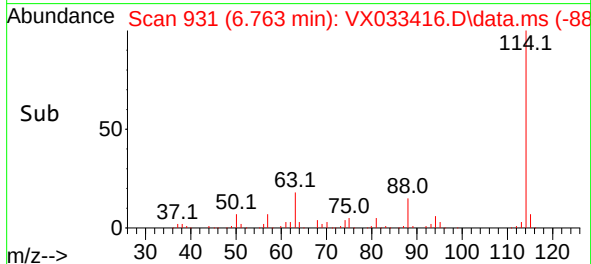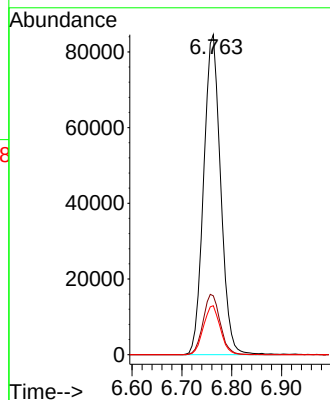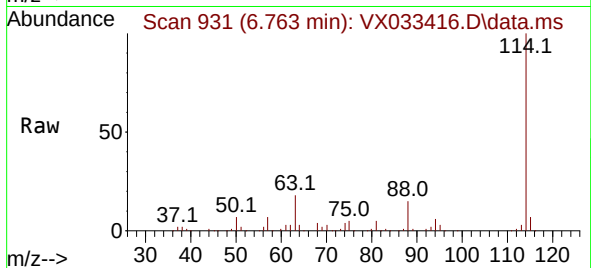

#35
Dibromofluoromethane
Concen: 47.006 ug/l
RT: 5.379 min Scan# 704
Delta R.T. -0.012 min
Lab File: VX033416.D
Acq: 14 Dec 2022 13:58

Tgt Ion:113 Resp: 42278
Ion Ratio Lower Upper
113 100
111 103.5 82.4 123.6
192 20.3 15.4 23.2


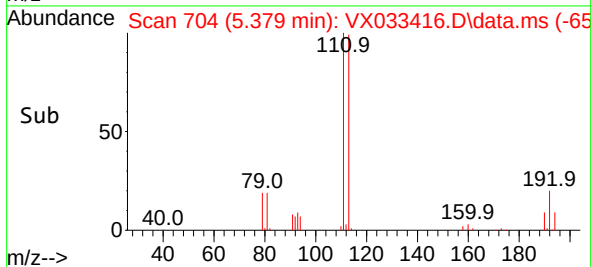
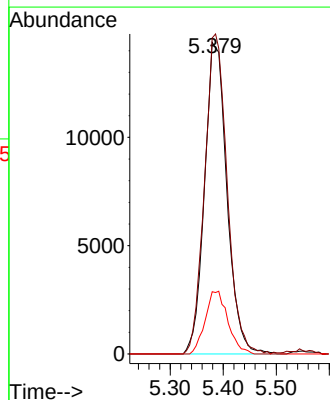
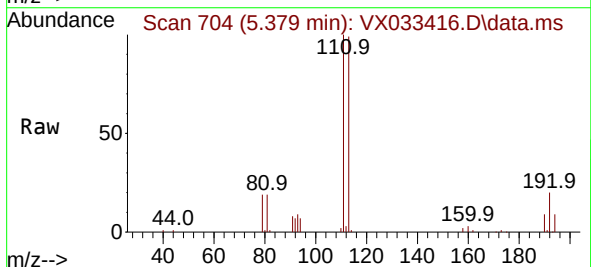


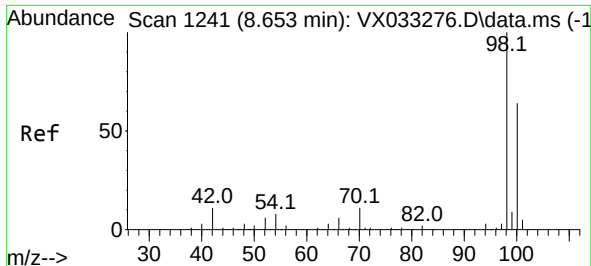

#50
Toluene-d8
Concen: 47.221 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX033416.D
Acq: 14 Dec 2022 13:58




Instrument :
MSVOA_X
ClientSampleId :
TB-01-121322


Tgt Ion: 98 Resp: 88848
Ion Ratio Lower Upper
98 100
100 65.2 50.9 76.3

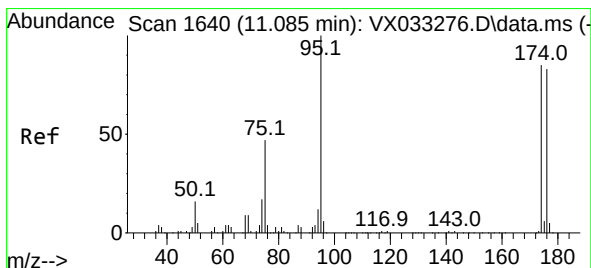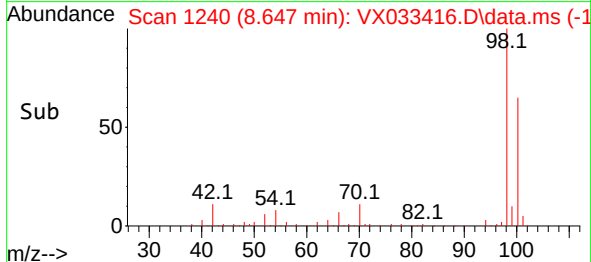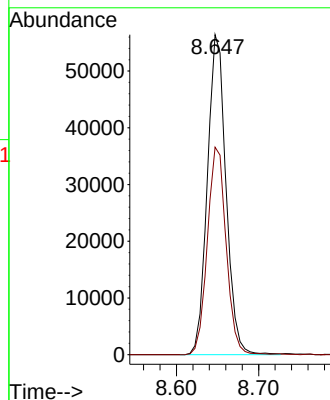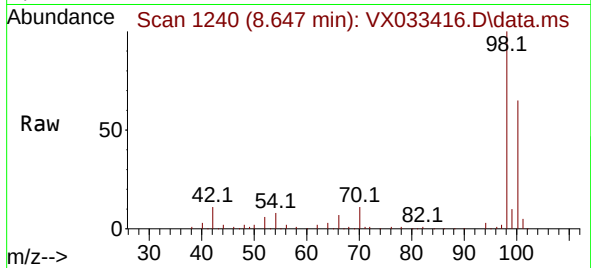

#62
4-Bromofluorobenzene
Concen: 47.006 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.006 min
Lab File: VX033416.D
Acq: 14 Dec 2022 13:58

Tgt Ion: 95 Resp: 67625
Ion Ratio Lower Upper
95 100
174 83.7 0.0 164.0
176 81.0 0.0 154.4


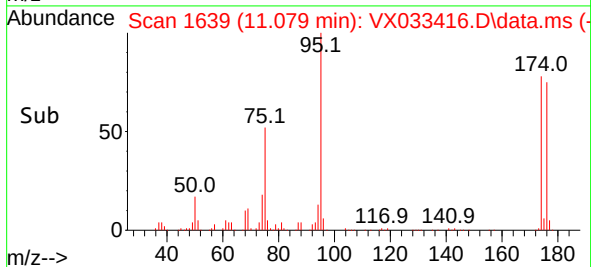
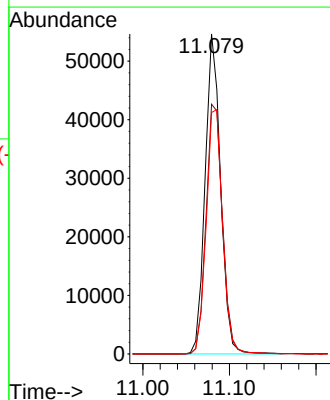
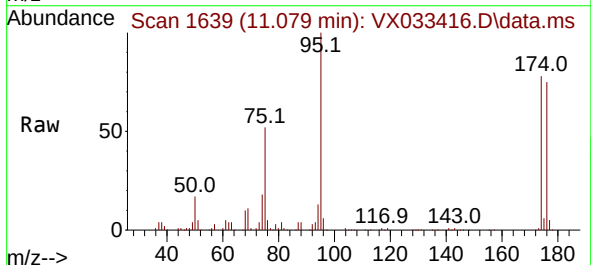


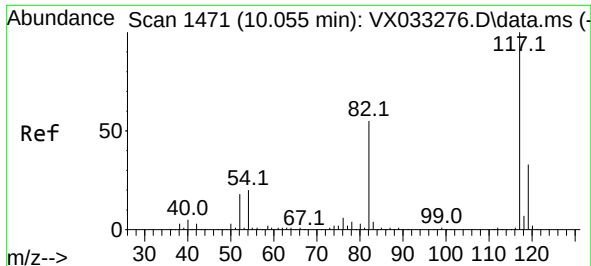

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX033416.D
Acq: 14 Dec 2022 13:58

Instrument :
MSVOA_X
ClientSampleId :
TB-01-121322

Tgt Ion:117 Resp: 177287
Ion Ratio Lower Upper
117 100
82 54.1 44.3 66.5
119 32.8 25.7 38.5

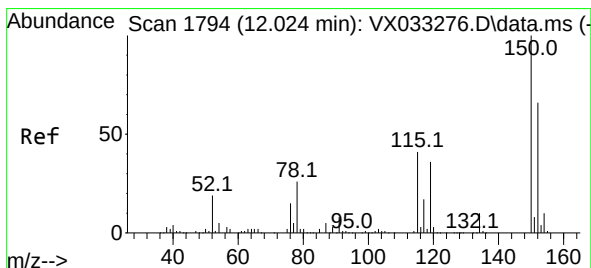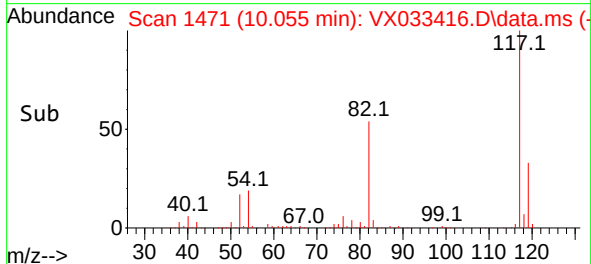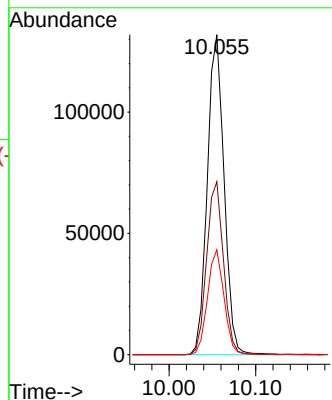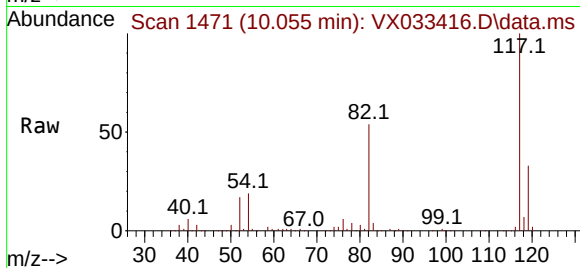

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX033416.D
Acq: 14 Dec 2022 13:58

Tgt Ion:152 Resp: 81682
Ion Ratio Lower Upper
152 100
115 60.2 44.0 132.0
150 158.1 0.0 351.8

