



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX121422\  
Data File : VX033409.D  
Acq On : 14 Dec 2022 08:29  
Operator : JC/MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X120722W.M  
Title : SW846 8260  
Last Update : Wed Dec 07 12:43:54 2022

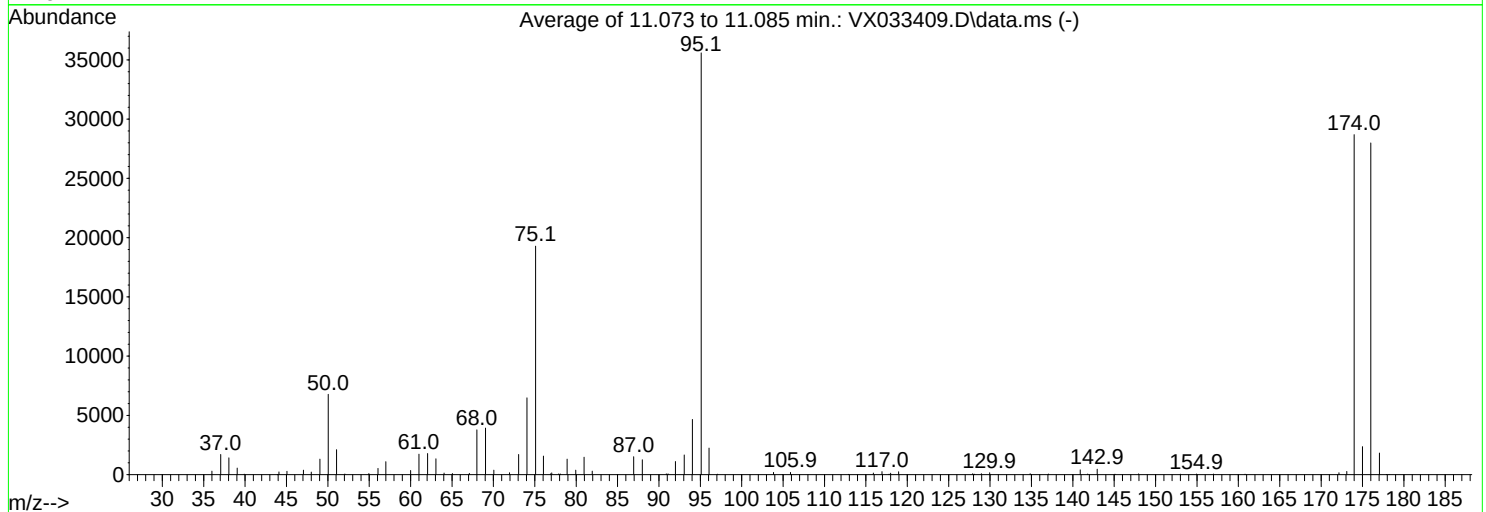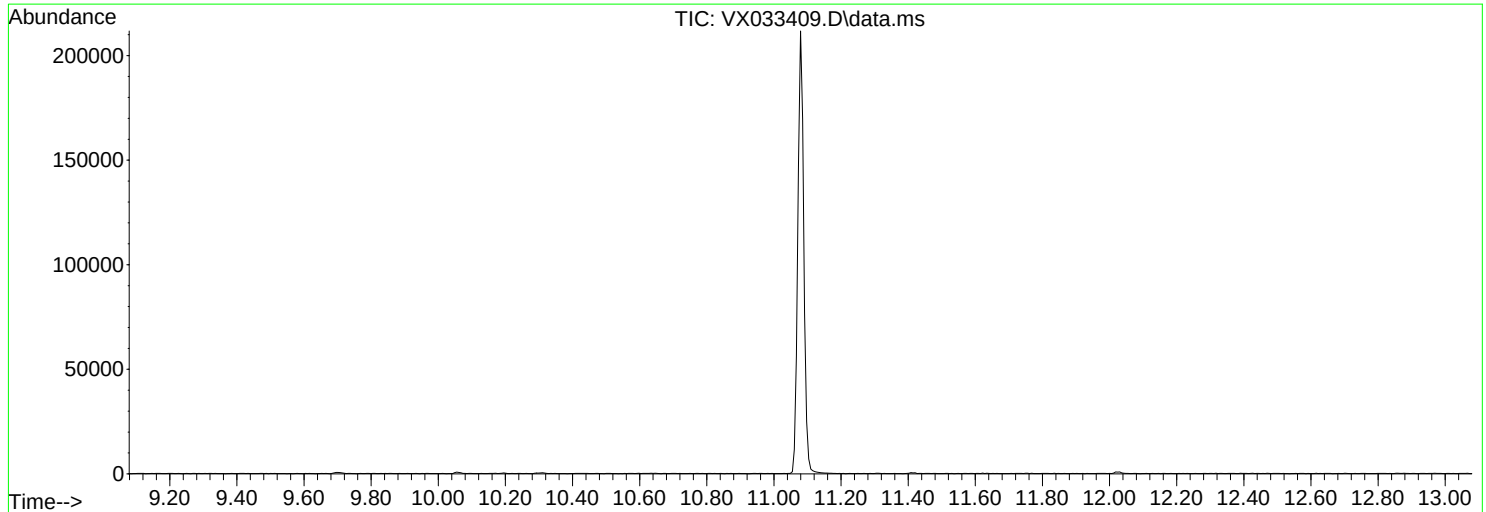

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 19.0         | 6772       | PASS                |
| 75             | 95              | 30              | 60              | 54.2         | 19280      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 35592      | PASS                |
| 96             | 95              | 5               | 9               | 6.3          | 2245       | PASS                |
| 173            | 174             | 0.00            | 2               | 0.9          | 270        | PASS                |
| 174            | 95              | 50              | 100             | 80.6         | 28693      | PASS                |
| 175            | 174             | 5               | 9               | 8.3          | 2369       | PASS                |
| 176            | 174             | 95              | 101             | 97.5         | 27989      | PASS                |
| 177            | 176             | 5               | 9               | 6.5          | 1820       | PASS                |