

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121423\
 Data File : VX039200.D
 Acq On : 14 Dec 2023 11:44
 Operator : JC/MD
 Sample : 05719-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-TT-RW10A-MW01I-GW-20231205

Quant Time: Dec 15 02:58:20 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121323W.M
 Quant Title : SW846 8260
 QLast Update : Thu Dec 14 01:28:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	98327	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	199550	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	205602	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	105399	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	86091	47.794	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	95.580%
35) Dibromofluoromethane	5.385	113	66002	47.877	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	95.760%
50) Toluene-d8	8.647	98	250121	48.870	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	97.740%
62) 4-Bromofluorobenzene	11.079	95	114618	54.278	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	108.560%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121423\
Data File : VX039200.D
Acq On : 14 Dec 2023 11:44
Operator : JC/MD
Sample : 05719-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-TT-RW10A-MW01I-GW-20231205

Quant Time: Dec 15 02:58:20 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121323W.M
Quant Title : SW846 8260
QLast Update : Thu Dec 14 01:28:15 2023
Response via : Initial Calibration




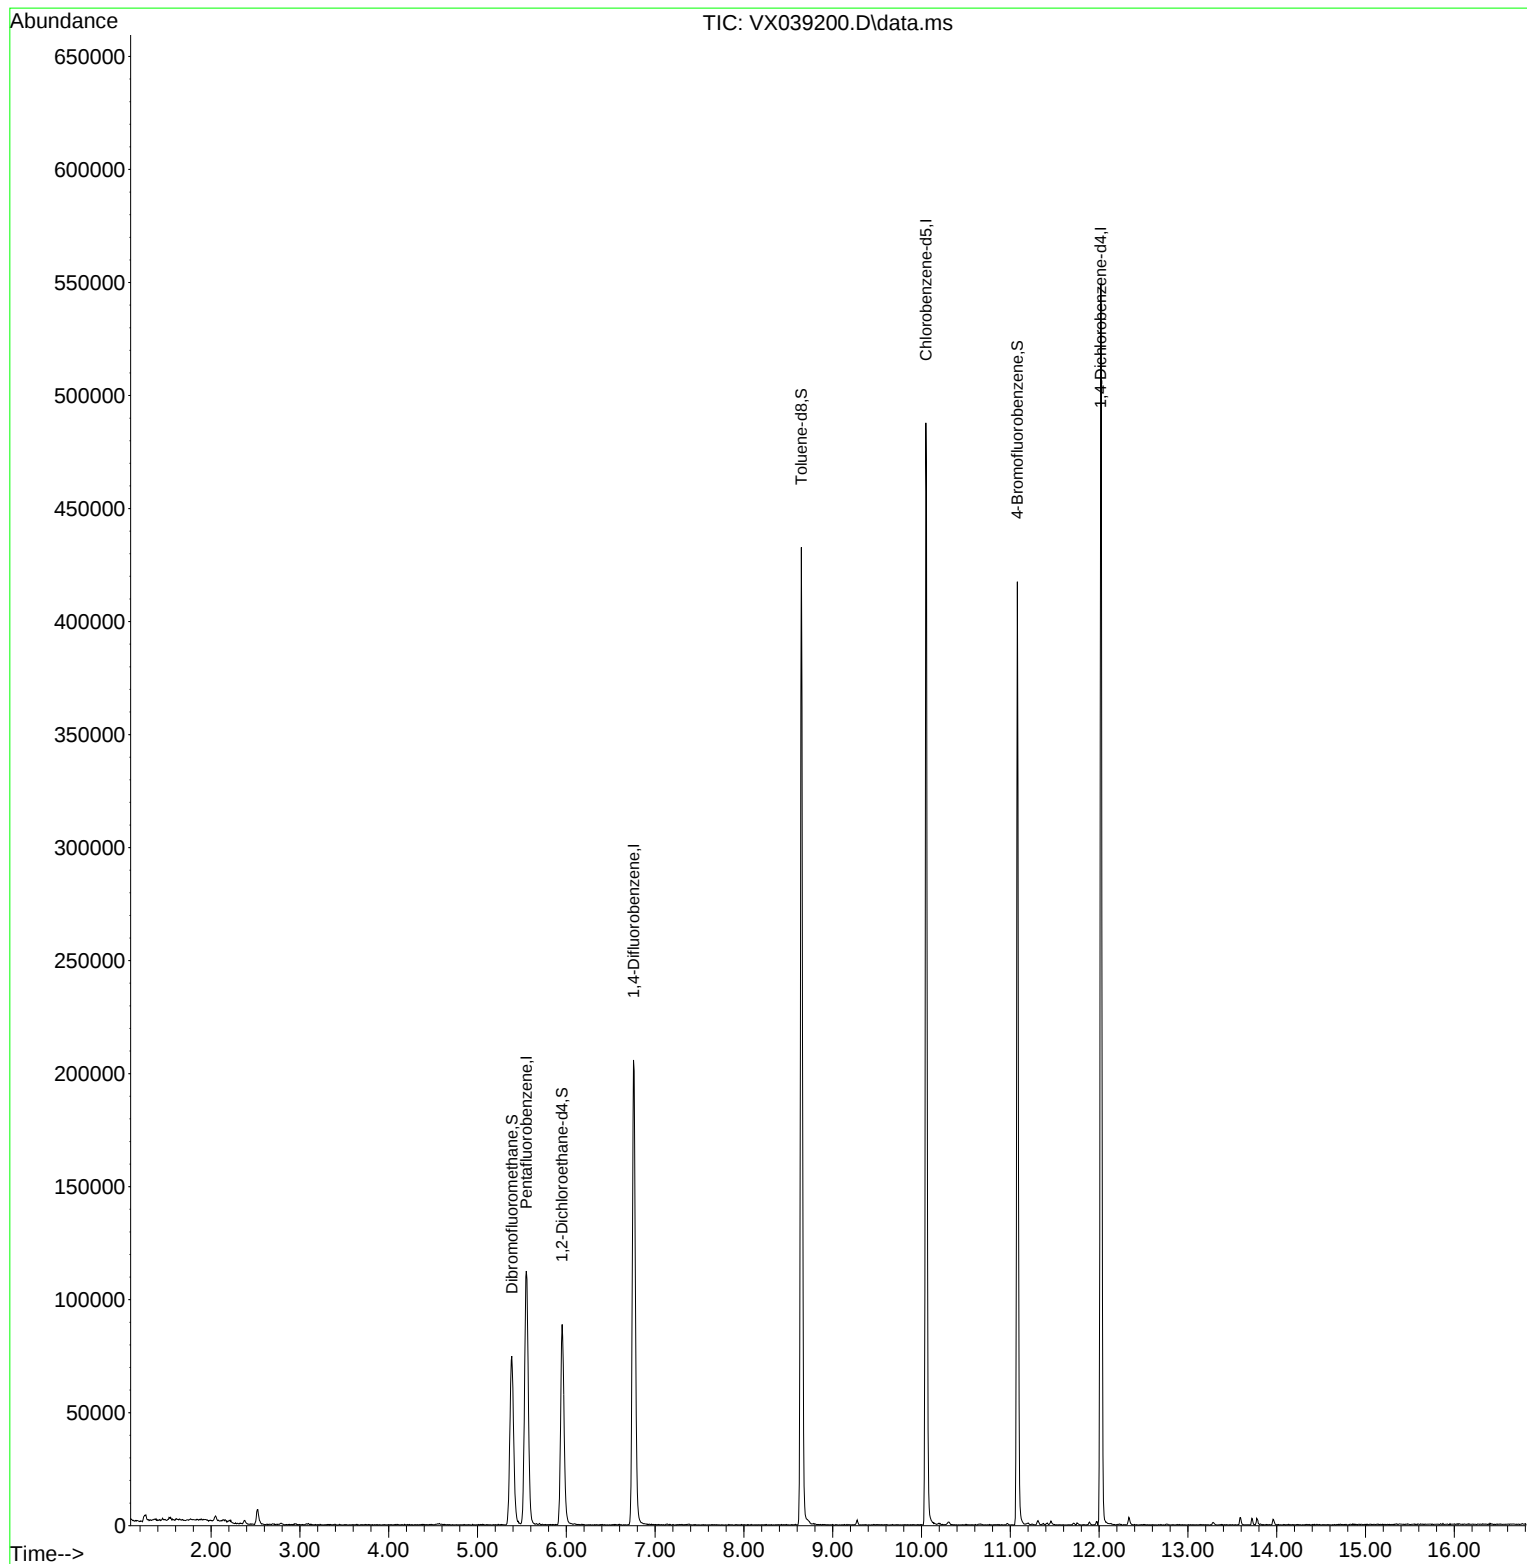


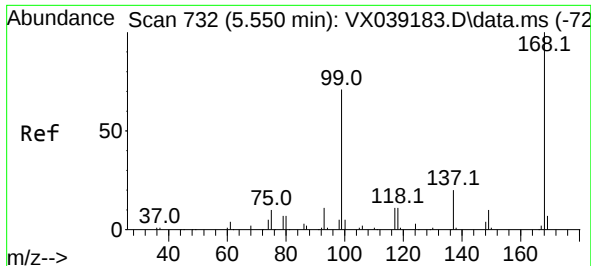

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 712
Delta R.T. -0.000 min
Lab File: VX039200.D
Acq: 14 Dec 2023 11:44




Instrument :
MSVOA_X
ClientSampleId :
BP-TT-RW10A-MW01I-GW-20231205

Tgt Ion:168 Resp: 98327
Ion Ratio Lower Upper
168 100
99 67.3 56.6 85.0

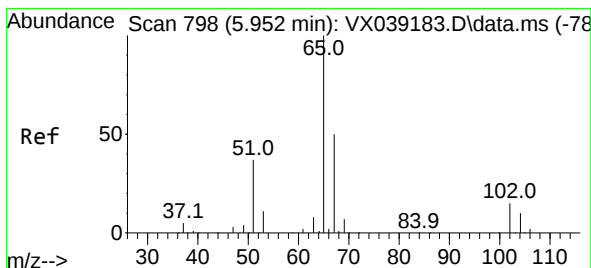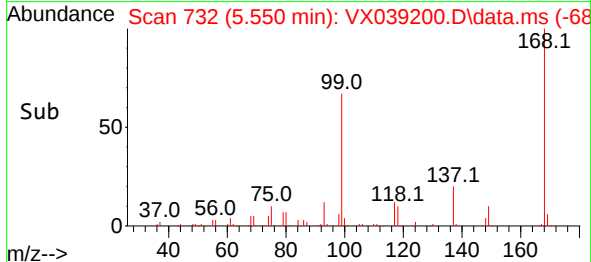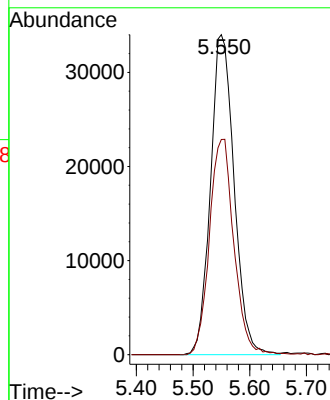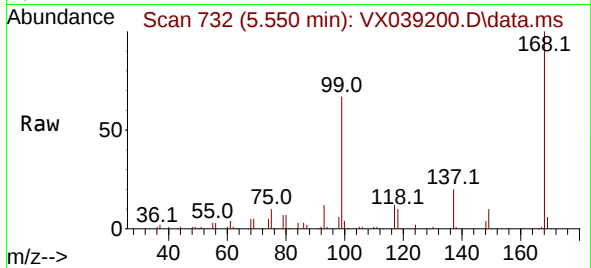

#33
1,2-Dichloroethane-d4
Concen: 47.794 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.000 min
Lab File: VX039200.D
Acq: 14 Dec 2023 11:44

Tgt Ion: 65 Resp: 86091
Ion Ratio Lower Upper
65 100
67 51.8 0.0 100.2


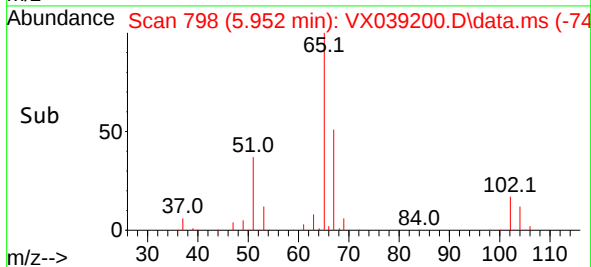
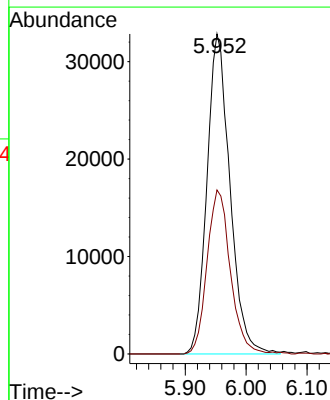
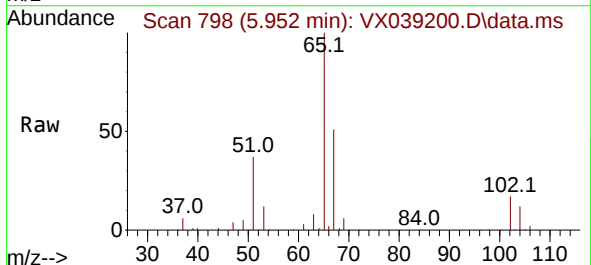




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. -0.006 min
Lab File: VX039200.D
Acq: 14 Dec 2023 11:44




Instrument :
MSVOA_X
ClientSampleId :
BP-TT-RW10A-MW01I-GW-20231205

Tgt Ion:114 Resp: 199550
Ion Ratio Lower Upper
114 100
63 23.9 0.0 45.0
88 18.0 0.0 36.6

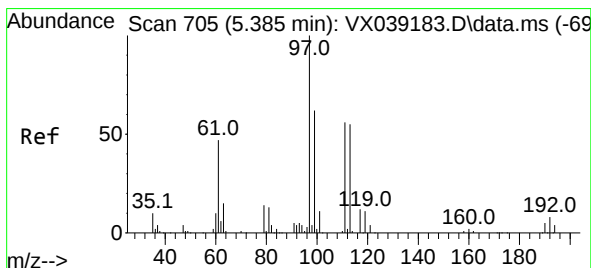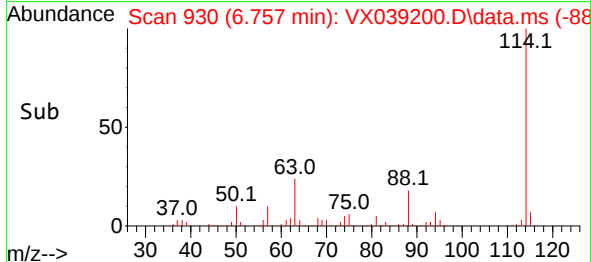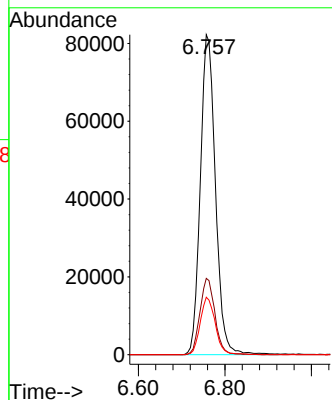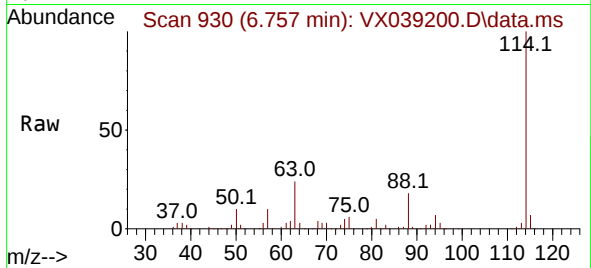

#35
Dibromofluoromethane
Concen: 47.877 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX039200.D
Acq: 14 Dec 2023 11:44

Tgt Ion:113 Resp: 66002
Ion Ratio Lower Upper
113 100
111 103.6 82.9 124.3
192 15.9 13.3 19.9


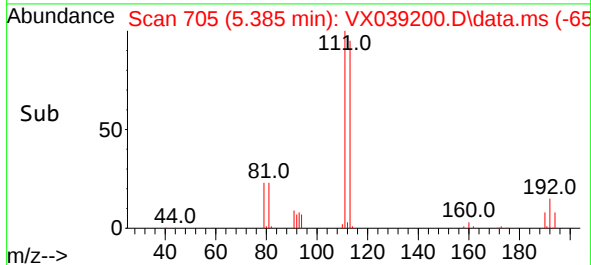
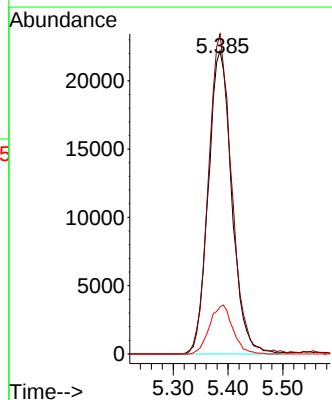
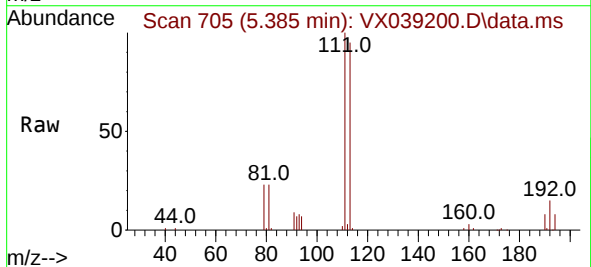




#50
Toluene-d8
Concen: 48.870 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX039200.D
Acq: 14 Dec 2023 11:44




Instrument :
MSVOA_X
ClientSampleId :
BP-TT-RW10A-MW01I-GW-20231205


Tgt Ion: 98 Resp: 250121
Ion Ratio Lower Upper
98 100
100 64.0 53.1 79.7

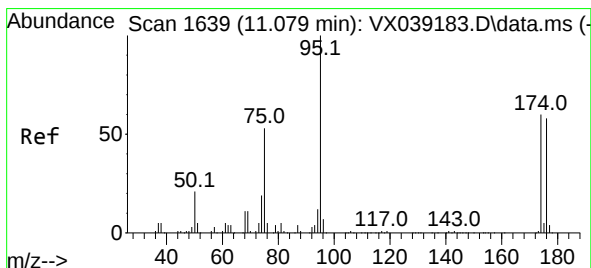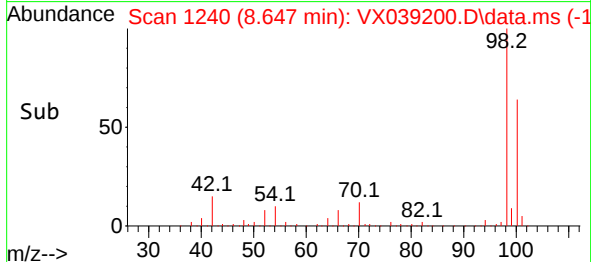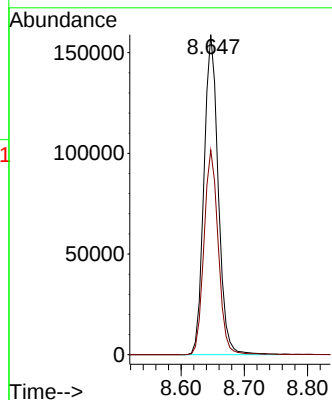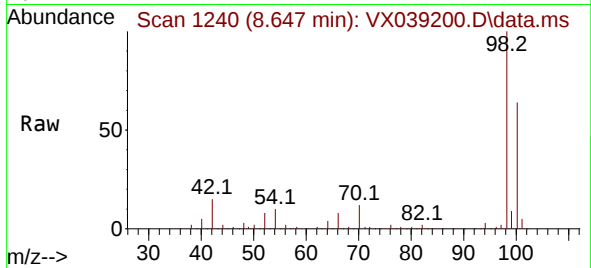

#62
4-Bromofluorobenzene
Concen: 54.278 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX039200.D
Acq: 14 Dec 2023 11:44

Tgt Ion: 95 Resp: 114618
Ion Ratio Lower Upper
95 100
174 62.8 0.0 135.6
176 60.4 0.0 131.0

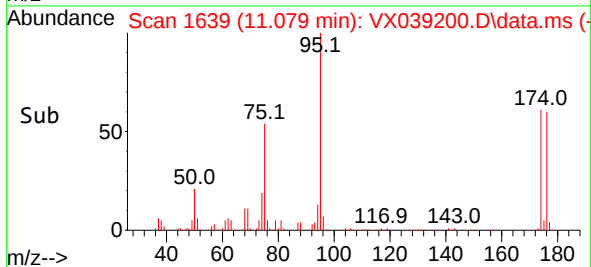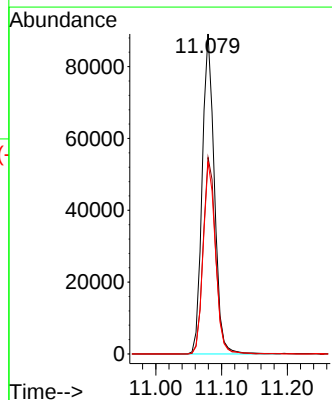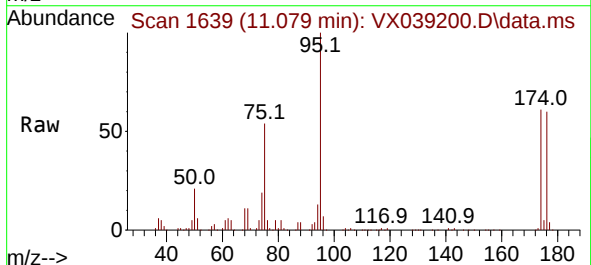

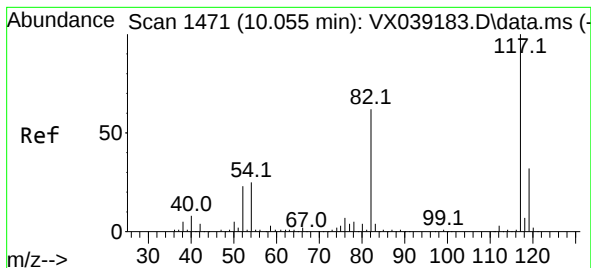

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.049 min Scan# 1471

Delta R.T. -0.006 min

Lab File: VX039200.D

Acq: 14 Dec 2023 11:44

Instrument :

MSVOA_X

ClientSampleId :

BP-TT-RW10A-MW01I-GW-20231205





Tgt Ion:117 Resp: 205602

Ion Ratio Lower Upper

117 100

82 65.4 46.2 69.4

119 32.4 25.5 38.3

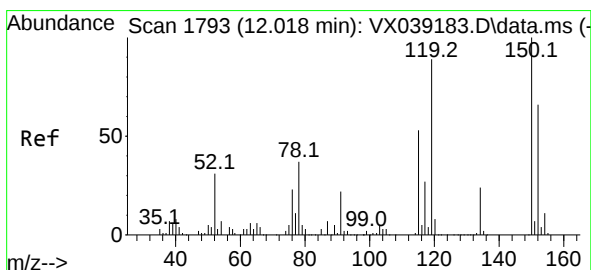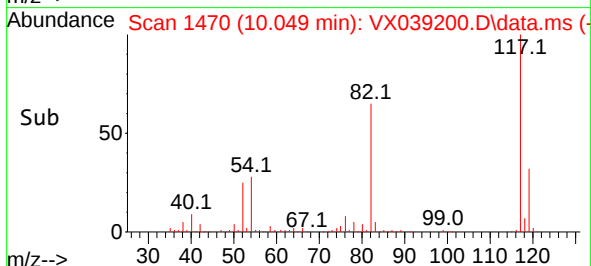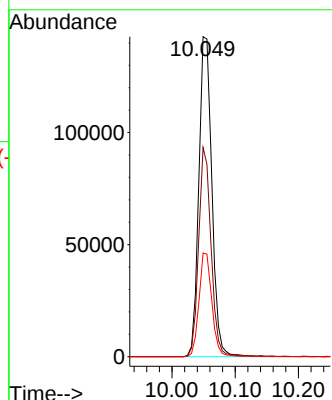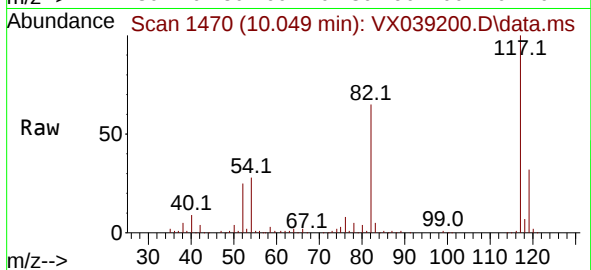

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.018 min Scan# 1793

Delta R.T. 0.000 min

Lab File: VX039200.D

Acq: 14 Dec 2023 11:44

Tgt Ion:152 Resp: 105399

Ion Ratio Lower Upper

152 100

115 67.7 43.3 129.9

150 155.9 0.0 345.0

