

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX121520\
 Data File : VX020011.D
 Acq On : 15 Dec 2020 15:02
 Operator : JC/MD
 Sample : L5052-01DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TU032-32-5229-121020DL

Quant Time: Dec 16 00:24:46 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X120420W.M
 Quant Title : SW846 8260
 QLast Update : Fri Dec 04 15:32:53 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	320422	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	522320	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	485880	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	228024	50.00	ug/l	0.00

System Monitoring Compounds		R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4		6.03	65	198311	47.09	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	94.18%	
35) Dibromofluoromethane		5.46	113	161261	47.77	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	95.54%	
50) Toluene-d8		8.70	98	639606	49.63	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	99.26%	
62) 4-Bromofluorobenzene		11.12	95	232641	47.43	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	94.86%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	1.31	50	744	0.216	ug/l	99
4) Vinyl Chloride	1.39	62	52787	14.511	ug/l	98
5) Bromomethane	1.63	94	807	0.668	ug/l	90
10) Methyl Iodide	2.49	142	1281	0.299	ug/l	98
11) Tert butyl alcohol	2.99	59	5441	3.710	ug/l #	75
12) 1,1-Dichloroethene	2.35	96	5843	1.990	ug/l	93
13) Acrolein	2.27	56	118	0.254	ug/l	99
16) Acetone	2.42	43	5546	3.504	ug/l	99
18) Methyl Acetate	2.76	43	1091	0.282	ug/l #	78
20) Methylene Chloride	2.83	84	1208	Below Cal		94
21) trans-1,2-Dichloroethene	3.14	96	157404	45.989	ug/l	99
25) 2-Butanone	4.63	43	11076	4.554	ug/l	98
27) cis-1,2-Dichloroethene	4.56	96	2006892	501.045	ug/l	89
29) Tetrahydrofuran	5.09	42	1632	1.041	ug/l #	88
31) Cyclohexane	5.62	56	6172	1.178	ug/l #	1
36) 1,1-Dichloropropene	5.63	75	24542	5.200	ug/l #	48
37) Ethyl Acetate	4.79	43	996	0.209	ug/l #	64
38) Carbon Tetrachloride	5.62	117	31286	6.769	ug/l #	16
41) Methacrylonitrile	5.09	41	2106	0.805	ug/l #	41
44) Trichloroethene	7.19	130	21739	5.747	ug/l	99
59) 2-Hexanone	9.47	43	838	0.229	ug/l	75
74) N-amyl acetate	10.91	43	2244	0.359	ug/l #	40
76) 1,2,3-Trichloropropane	11.12	75	113106	22.116	ug/l #	39
81) trans-1,4-Dichloro-2-buten	11.12	75	113106	63.934	ug/l #	12


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX121520\
Data File : VX020011.D
Acq On : 15 Dec 2020 15:02
Operator : JC/MD
Sample : L5052-01DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TU032-32-5229-121020DL

Quant Time: Dec 16 00:24:46 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X120420W.M
Quant Title : SW846 8260
QLast Update : Fri Dec 04 15:32:53 2020
Response via : Initial Calibration

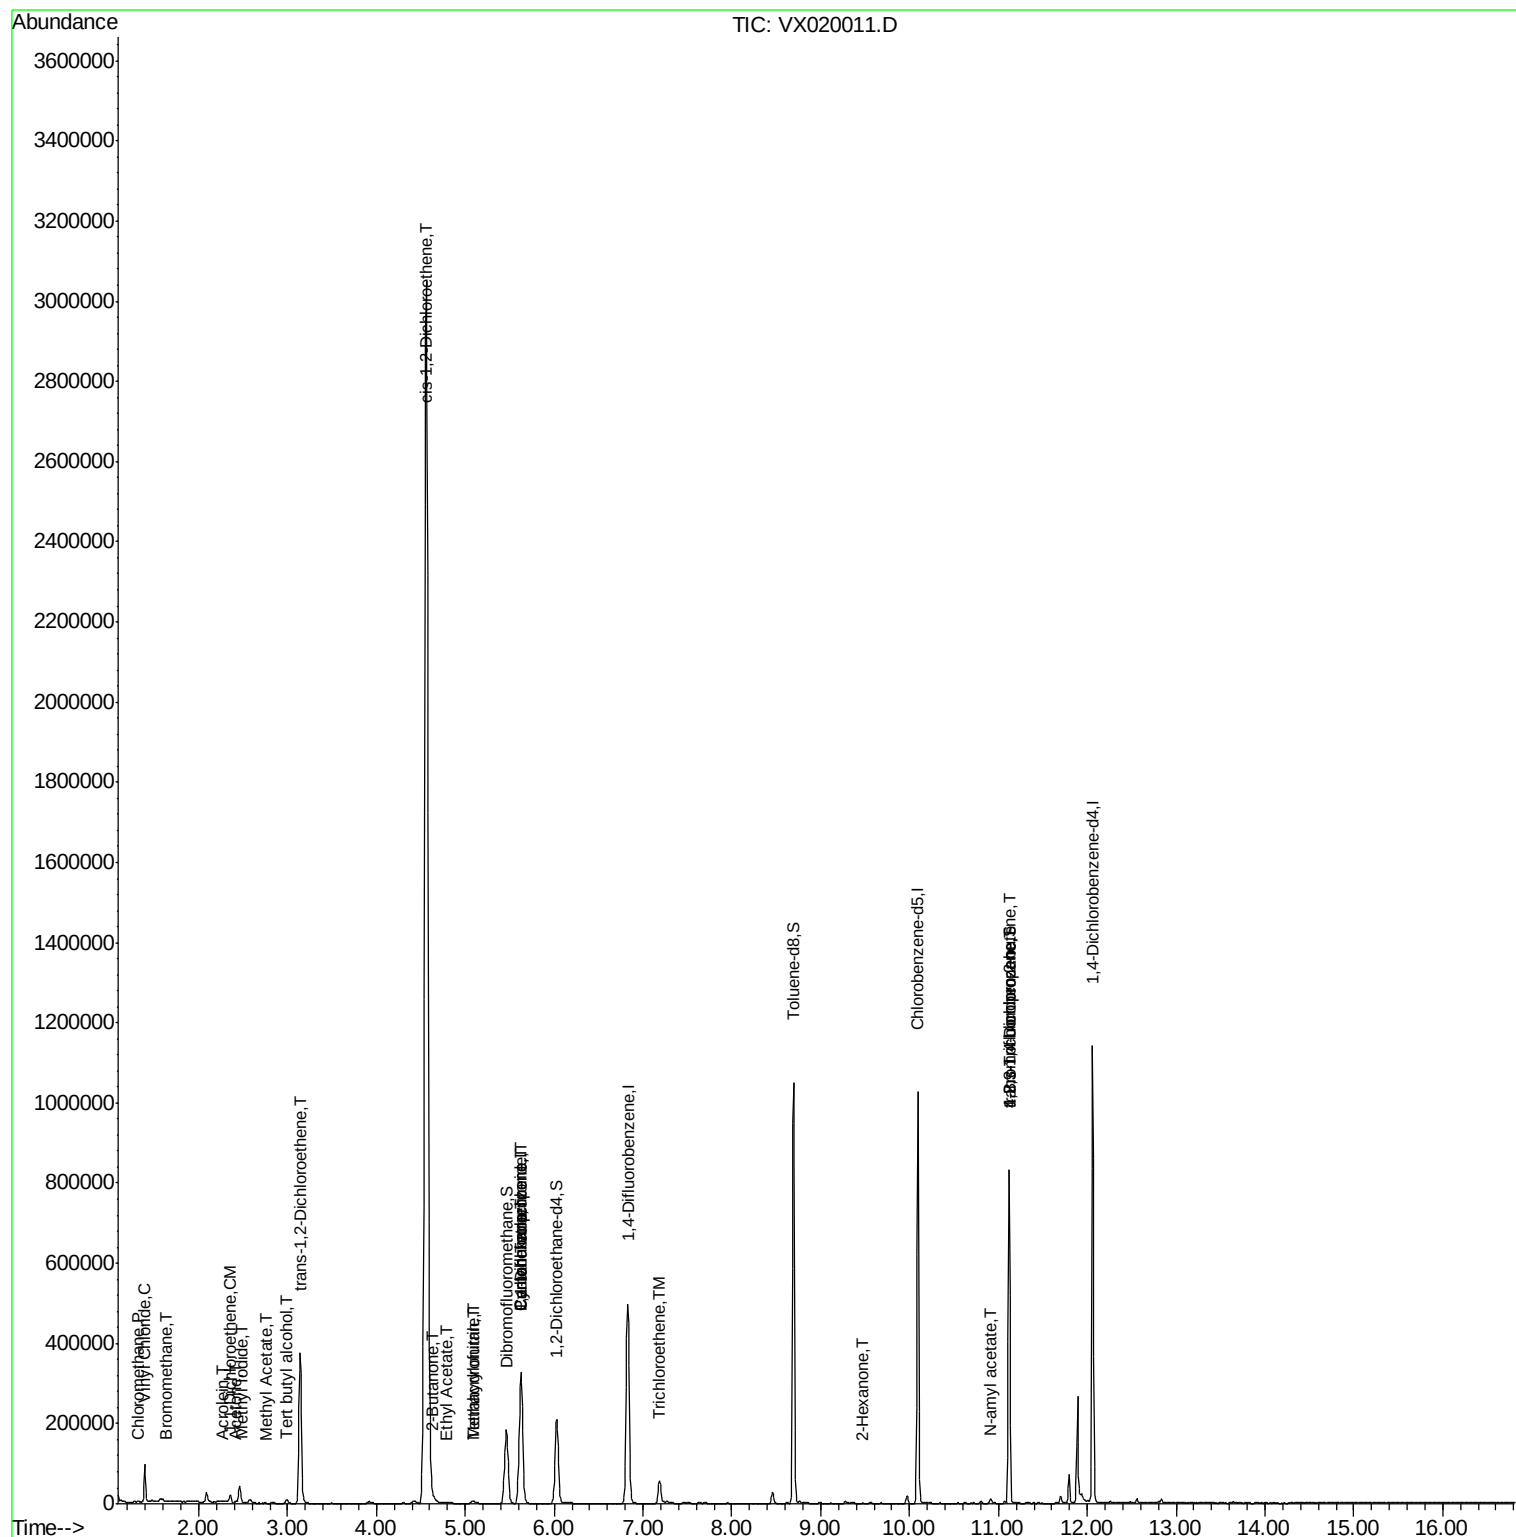

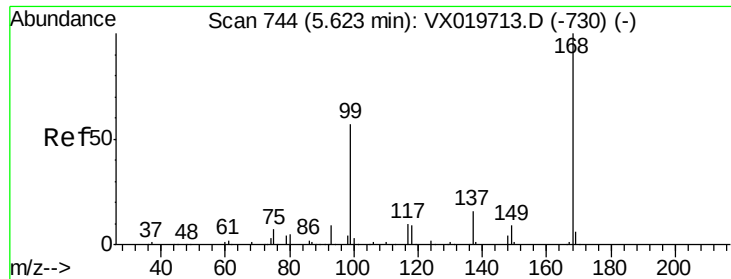

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.63 min Scan# 745

Delta R.T. 0.01 min

Lab File: VX020011.D

Acq: 15 Dec 2020 15:02

Instrument :

MSVOA_X

ClientSampleId :


TU032-32-5229-121020DL

Tgt Ion:168 Resp: 320422

Ion Ratio Lower Upper

168 100

99 56.7 45.8 68.6



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.63

120000

100000

80000



60000

40000

20000

0

Time-->



#3

Chloromethane

Concen: 0.216 ug/l

RT: 1.31 min Scan# 37

Delta R.T. -0.00 min

Lab File: VX020011.D


Acq: 15 Dec 2020 15:02

Tgt Ion: 50 Resp: 744

Ion Ratio Lower Upper

50 100

52 33.8 26.4 39.6



Abundance Ion 49.90 (49.60 to 50.60): VX0

Ion 51.90 (51.60 to 52.60): VX0

1.31

800


600


400

200

0

Time-->



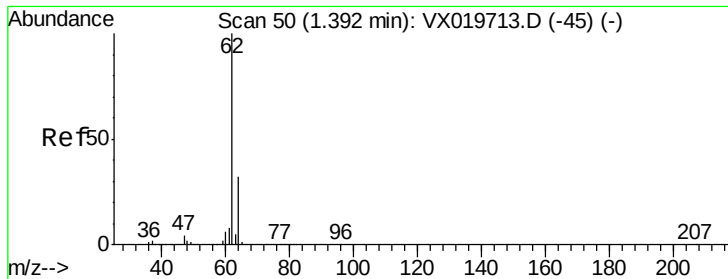

#4

Vinyl Chloride

Concen: 14.511 ug/l

RT: 1.39 min Scan# 50

Delta R.T. -0.00 min

Lab File: VX020011.D

Acq: 15 Dec 2020 15:02

Instrument :

MSVOA_X

ClientSampleId :





TU032-32-5229-121020DL

Tgt Ion: 62 Resp: 52787

Ion Ratio Lower Upper

62 100

64 31.2 25.7 38.5

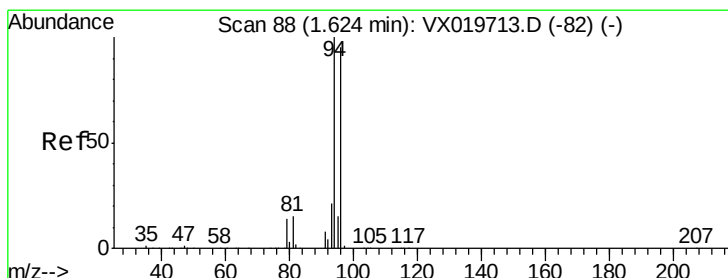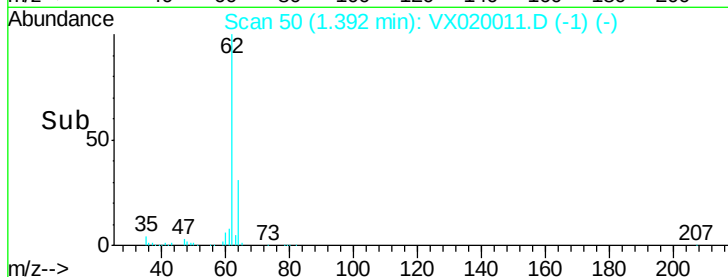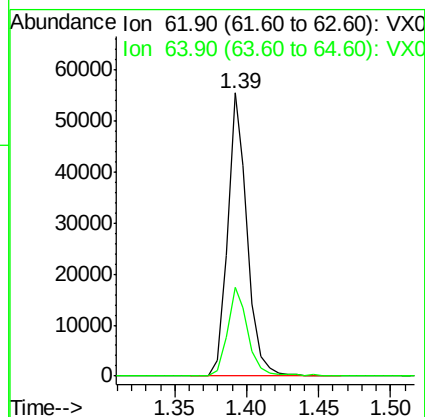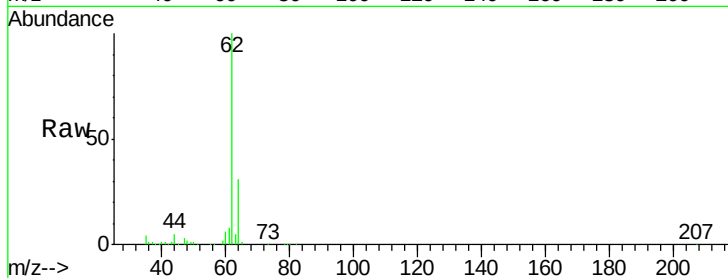

#5

Bromomethane

Concen: 0.668 ug/l

RT: 1.63 min Scan# 89

Delta R.T. 0.01 min

Lab File: VX020011.D




Acq: 15 Dec 2020 15:02


Tgt Ion: 94 Resp: 807

Ion Ratio Lower Upper

94 100

96 85.4 76.4 114.6

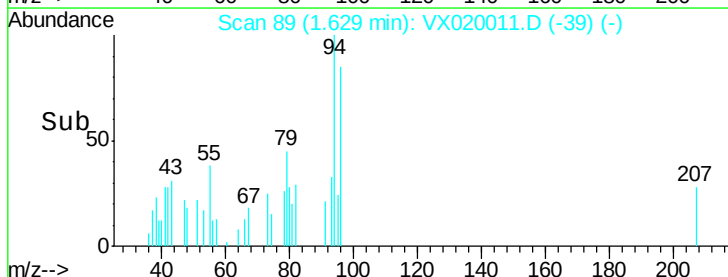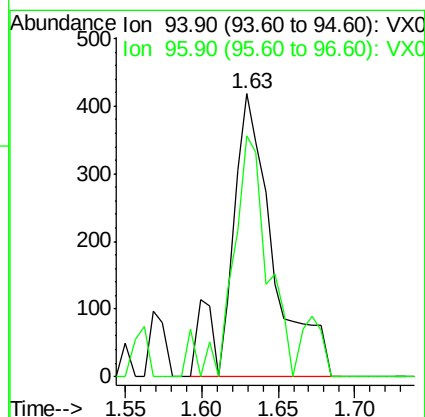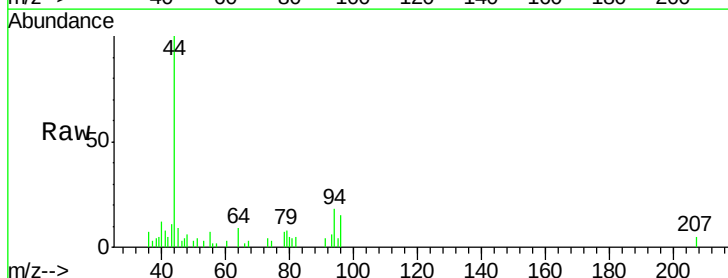

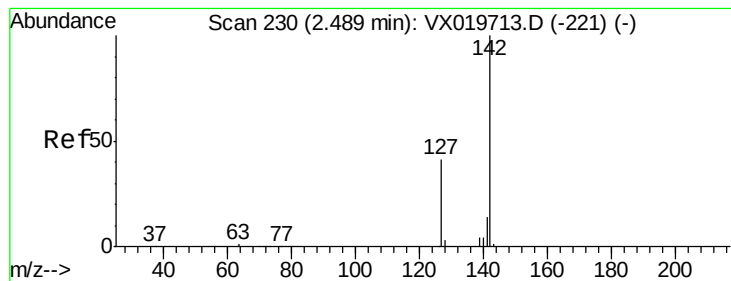

#10

Methyl Iodide

Concen: 0.299 ug/l

RT: 2.49 min Scan# 230

Delta R.T. -0.00 min

Lab File: VX020011.D

Acq: 15 Dec 2020 15:02

Instrument :

MSVOA_X

ClientSampleId :

TU032-32-5229-121020DL


Tgt Ion: 142 Resp: 1281

Ion Ratio Lower Upper

142 100

127 43.1 33.3 49.9


141 13.3 11.4 17.0





Abundance Ion 141.80 (141.50 to 142.50): V

Ion 126.80 (126.50 to 127.50): V

Ion 140.80 (140.50 to 141.50): V

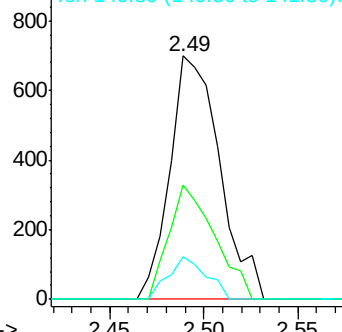

Time-->

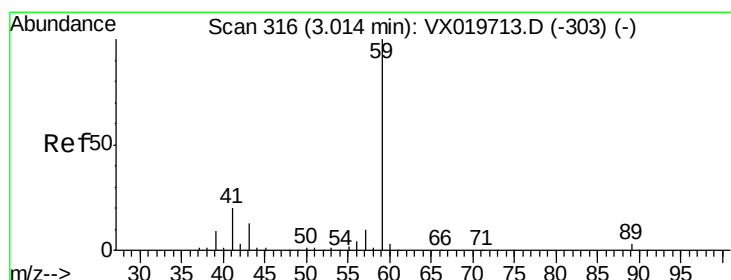

#11

Tert butyl alcohol

Concen: 3.710 ug/l

RT: 2.99 min Scan# 312

Delta R.T. -0.02 min

Lab File: VX020011.D


Acq: 15 Dec 2020 15:02

Tgt Ion: 59 Resp: 5441

Ion Ratio Lower Upper


59 100

57 0.6 7.8 11.8#





Abundance Ion 59.00 (58.70 to 59.70): VX0

Ion 57.00 (56.70 to 57.70): VX0

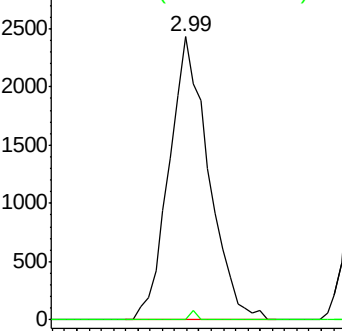

Time-->









#12
 1,1-Dichloroethene
 Concen: 1.990 ug/l
 RT: 2.35 min Scan# 208
 Delta R.T. -0.00 min
 Lab File: VX020011.D
 Acq: 15 Dec 2020 15:02




Instrument :
 MSVOA_X
 ClientSampleId :
 TU032-32-5229-121020DL


Tgt Ion: 96 Resp: 5843
 Ion Ratio Lower Upper
 96 100
 61 166.1 124.6 187.0
 98 66.2 50.6 76.0

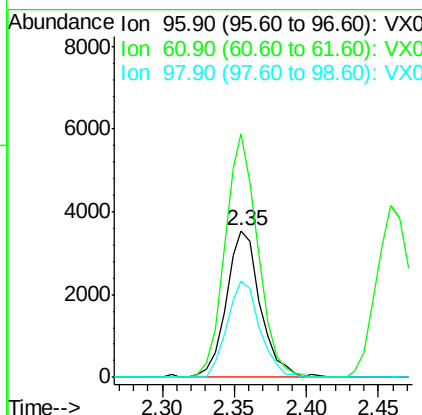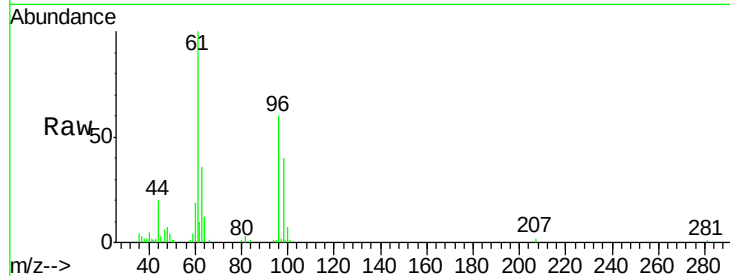

#13
 Acrolein
 Concen: 0.254 ug/l
 RT: 2.27 min Scan# 194
 Delta R.T. -0.00 min
 Lab File: VX020011.D
 Acq: 15 Dec 2020 15:02

Tgt Ion: 56 Resp: 118
 Ion Ratio Lower Upper
 56 100
 55 69.5 56.4 84.6

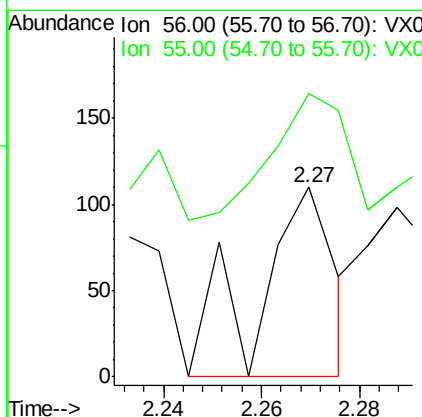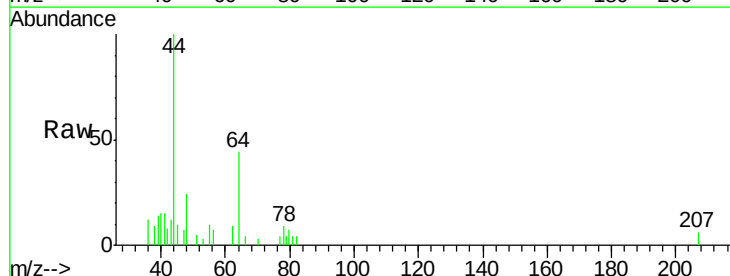



#16

Acetone

Concen: 3.504 ug/l

RT: 2.42 min Scan# 218

Delta R.T. -0.00 min

Lab File: VX020011.D

Acq: 15 Dec 2020 15:02

Instrument :

MSVOA_X

ClientSampleId :


TU032-32-5229-121020DL

Tgt Ion: 43 Resp: 5546

Ion Ratio Lower Upper




43 100

58 33.9 27.8 41.8

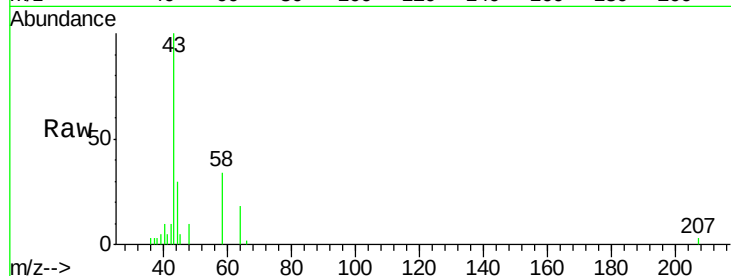

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

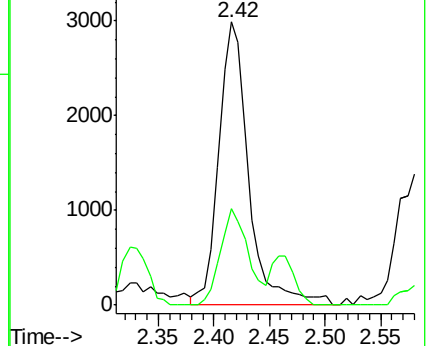

#18

Methyl Acetate

Concen: 0.282 ug/l

RT: 2.76 min Scan# 274

Delta R.T. 0.01 min

Lab File: VX020011.D


Acq: 15 Dec 2020 15:02

Tgt Ion: 43 Resp: 1091

Ion Ratio Lower Upper



43 100


74 15.8 21.9 32.9#



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 74.00 (73.70 to 74.70): VX0

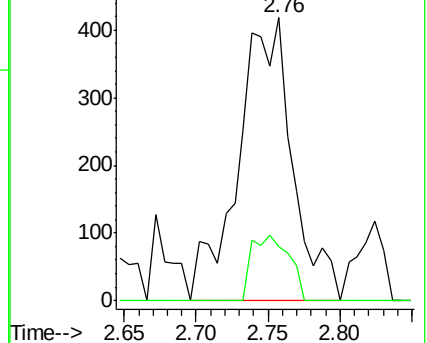

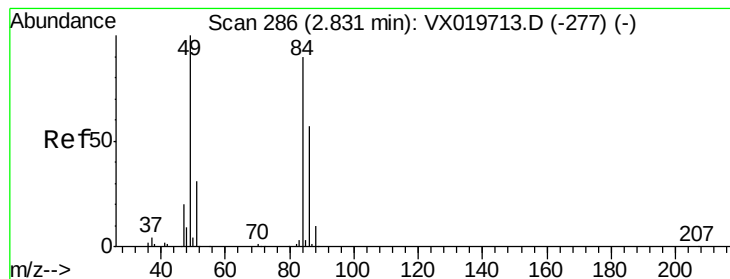

#20

Methylene Chloride

Concen: Below Cal

RT: 2.83 min Scan# 286

Delta R.T. 0.00 min

Lab File: VX020011.D

Acq: 15 Dec 2020 15:02

Instrument :

MSVOA_X

ClientSampleId :

TU032-32-5229-121020DL

Tgt Ion: 84 Resp: 1208


Ion Ratio Lower Upper

84 100

49 105.1 88.6 132.8

51 38.3 27.0 40.6

86 57.3 50.3 75.5






Abundance Ion 83.90 (83.60 to 84.60): VX0

Ion 48.90 (48.60 to 49.60): VX0

Ion 50.90 (50.60 to 51.60): VX0

Ion 85.90 (85.60 to 86.60): VX0

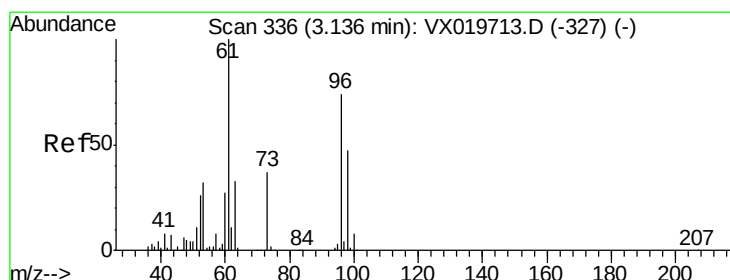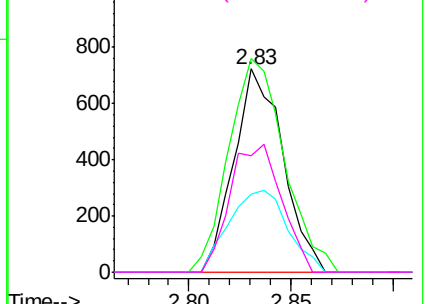

#21

trans-1,2-Dichloroethene

Concen: 45.989 ug/l

RT: 3.14 min Scan# 337

Delta R.T. 0.01 min

Lab File: VX020011.D

Acq: 15 Dec 2020 15:02


Tgt Ion: 96 Resp: 157404

Ion Ratio Lower Upper

96 100

61 132.4 107.7 161.5



98 63.0 50.4 75.6




Abundance Ion 95.90 (95.60 to 96.60): VX0

Ion 60.90 (60.60 to 61.60): VX0

Ion 97.90 (97.60 to 98.60): VX0

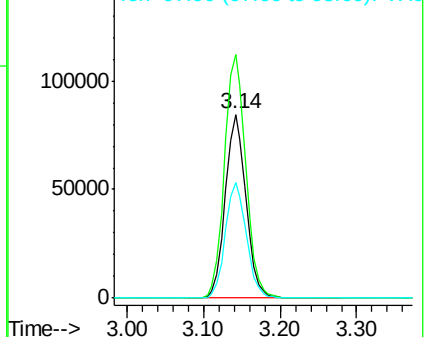



#25

2-Butanone

Concen: 4.554 ug/l

RT: 4.63 min Scan# 582

Delta R.T. 0.01 min

Lab File: VX020011.D

Acq: 15 Dec 2020 15:02

Instrument :

MSVOA_X

ClientSampleId :





TU032-32-5229-121020DL

Tgt Ion: 43 Resp: 11076

Ion Ratio Lower Upper

43 100

72 30.8 23.7 35.5

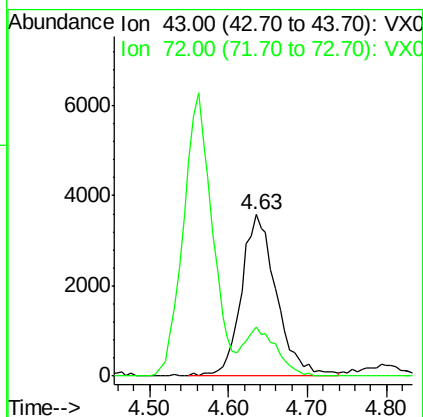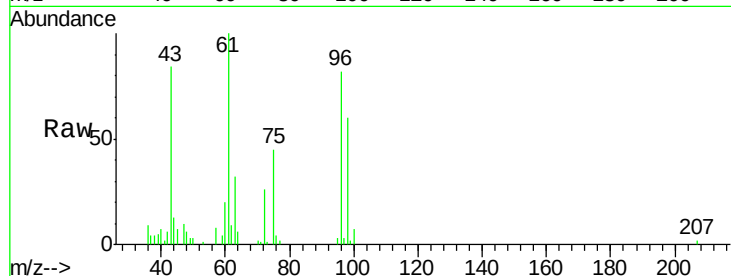

#27

cis-1,2-Dichloroethene

Concen: 501.045 ug/l

RT: 4.56 min Scan# 570

Delta R.T. 0.01 min

Lab File: VX020011.D

Acq: 15 Dec 2020 15:02




Tgt Ion: 96 Resp: 2006892


Ion Ratio Lower Upper

96 100

61 124.0 0.0 285.6

98 63.9 0.0 129.6

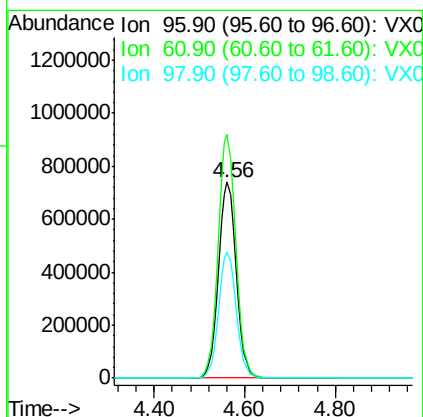



#29

Tetrahydrofuran

Concen: 1.041 ug/l

RT: 5.09 min Scan# 657

Delta R.T. 0.01 min

Lab File: VX020011.D

Acq: 15 Dec 2020 15:02

Instrument :

MSVOA_X

ClientSampleId :

TU032-32-5229-121020DL


Tgt Ion: 42 Resp: 1632

Ion Ratio Lower Upper

42 100

72 49.5 41.7 62.5




71 33.5 38.4 57.6#



Abundance Ion 42.00 (41.70 to 42.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

Ion 71.00 (70.70 to 71.70): VX0

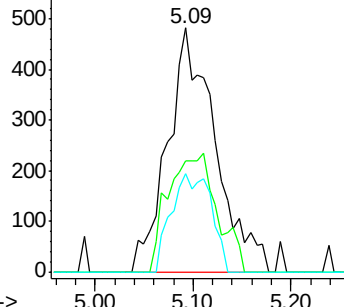

#31

Cyclohexane

Concen: 1.178 ug/l

RT: 5.62 min Scan# 744

Delta R.T. 0.08 min

Lab File: VX020011.D

Acq: 15 Dec 2020 15:02


Tgt Ion: 56 Resp: 6172

Ion Ratio Lower Upper

56 100

69 180.5 25.3 37.9#



84 157.5 71.4 107.0#




Abundance Ion 56.00 (55.70 to 56.70): VX0

Ion 69.00 (68.70 to 69.70): VX0

Ion 84.00 (83.70 to 84.70): VX0




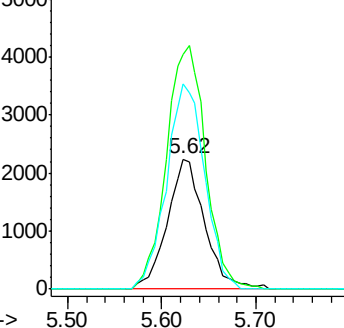


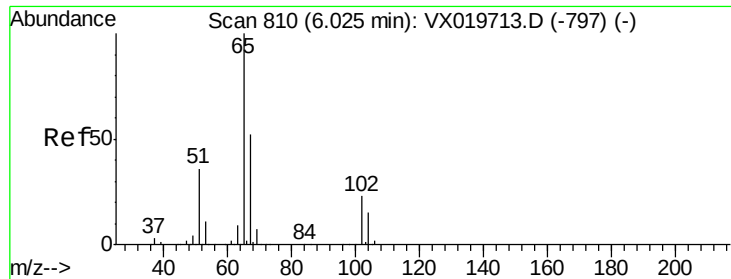

#33
 1,2-Dichloroethane-d4
 Concen: 47.090 ug/l
 RT: 6.03 min Scan# 811
 Delta R.T. 0.01 min
 Lab File: VX020011.D
 Acq: 15 Dec 2020 15:02




Instrument :
 MSVOA_X
 ClientSampleId :
 TU032-32-5229-121020DL


Tgt Ion: 65 Resp: 198311
 Ion Ratio Lower Upper
 65 100
 67 53.2 0.0 105.4

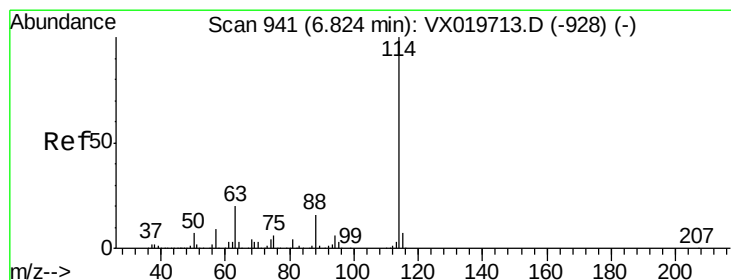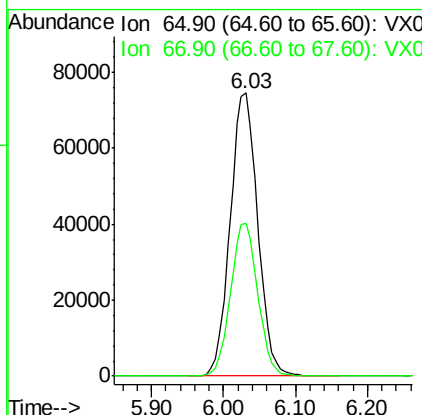

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.83 min Scan# 942
 Delta R.T. 0.01 min
 Lab File: VX020011.D
 Acq: 15 Dec 2020 15:02

Tgt Ion: 114 Resp: 522320
 Ion Ratio Lower Upper
 114 100
 63 20.7 0.0 40.8
 88 16.4 0.0 32.8


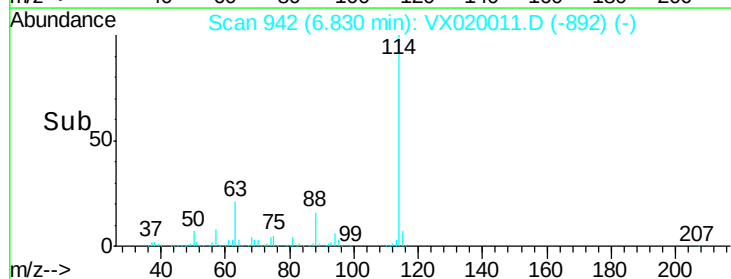
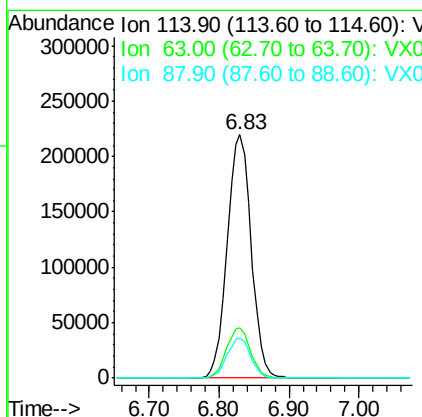
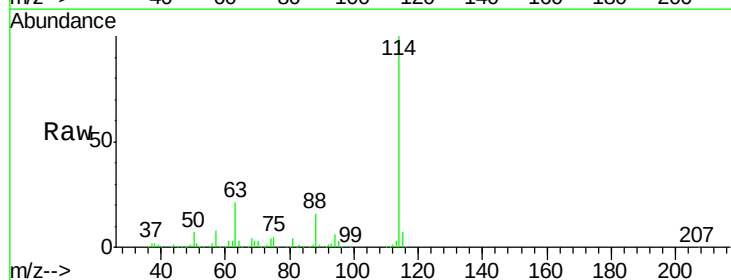




#35
 Dibromofluoromethane
 Concen: 47.771 ug/l
 RT: 5.46 min Scan# 718
 Delta R.T. 0.01 min
 Lab File: VX020011.D
 Acq: 15 Dec 2020 15:02




Instrument :
 MSVOA_X
 ClientSampleId :
 TU032-32-5229-121020DL


Tgt Ion	Ratio	Lower	Upper
113	100		
111	102.4	81.9	122.9
192	20.2	16.7	25.1

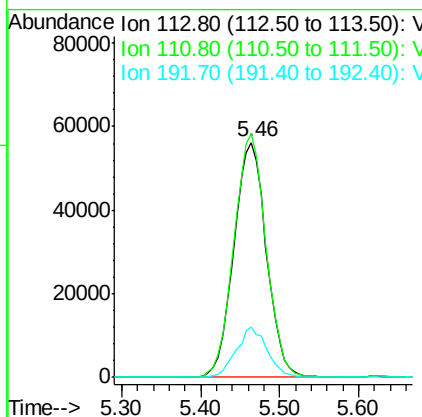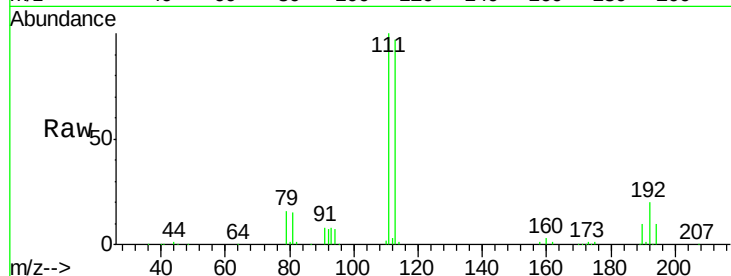

#36
 1,1-Dichloropropene
 Concen: 5.200 ug/l
 RT: 5.63 min Scan# 745
 Delta R.T. -0.13 min
 Lab File: VX020011.D
 Acq: 15 Dec 2020 15:02

Tgt Ion	Ratio	Lower	Upper
75	100		
110	8.6	18.1	54.4#
77	0.0	25.3	37.9#

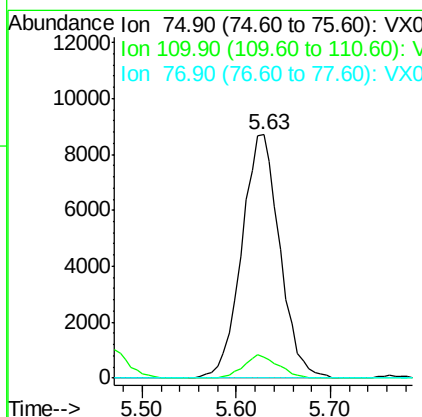

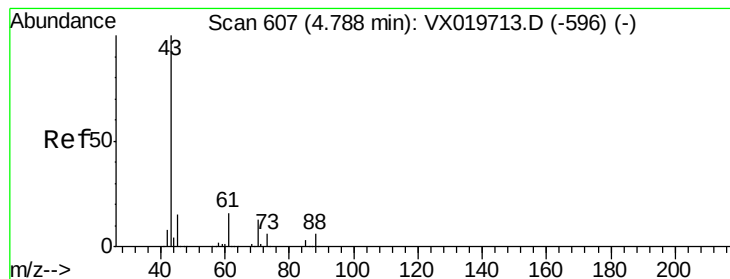

#37

Ethyl Acetate

Concen: 0.209 ug/l

RT: 4.79 min Scan# 608

Delta R.T. 0.01 min

Lab File: VX020011.D

Acq: 15 Dec 2020 15:02

Instrument :

MSVOA_X

ClientSampleId :

TU032-32-5229-121020DL


Tgt Ion: 43 Resp: 996

Ion Ratio Lower Upper

43 100

61 0.0 12.8 19.2#




70 0.0 10.5 15.7#



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 60.90 (60.60 to 61.60): VX0

Ion 70.00 (69.70 to 70.70): VX0

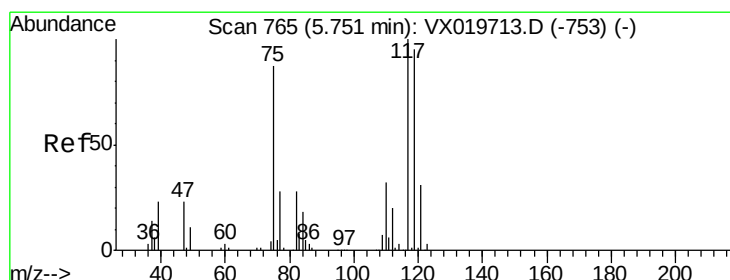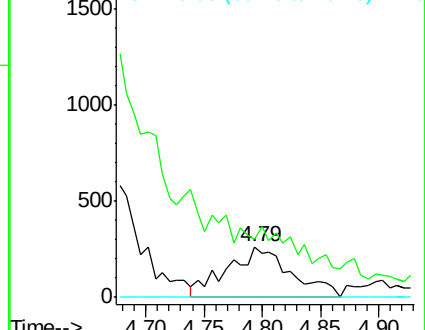

#38

Carbon Tetrachloride

Concen: 6.769 ug/l

RT: 5.62 min Scan# 744

Delta R.T. -0.13 min

Lab File: VX020011.D

Acq: 15 Dec 2020 15:02


Tgt Ion: 117 Resp: 31286

Ion Ratio Lower Upper

117 100

119 4.8 76.2 114.2#



121 0.0 24.8 37.2#




Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V




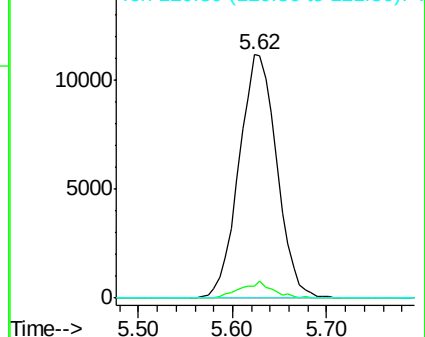




#41
Methacrylonitrile
Concen: 0.805 ug/l
RT: 5.09 min Scan# 656
Delta R.T. 0.09 min
Lab File: VX020011.D
Acq: 15 Dec 2020 15:02




Instrument :
MSVOA_X
ClientSampleId :
TU032-32-5229-121020DL


Tgt Ion:	41	Resp:	2106
Ion	Ratio	Lower	Upper
41	100		
39	45.3	42.5	63.7
67	0.0	65.0	97.6#
52	0.0	25.3	37.9#

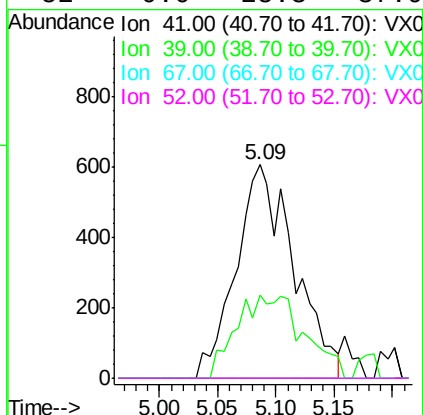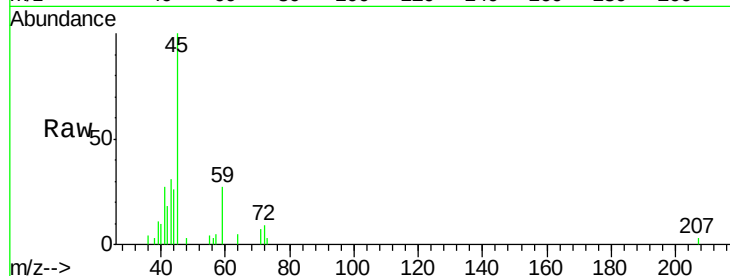

#44
Trichloroethene
Concen: 5.747 ug/l
RT: 7.19 min Scan# 1001
Delta R.T. 0.01 min
Lab File: VX020011.D
Acq: 15 Dec 2020 15:02

Tgt Ion:	130	Resp:	21739
Ion	Ratio	Lower	Upper
130	100		
95	98.2	0.0	198.0


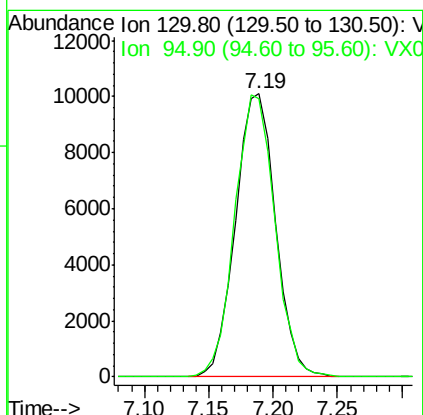




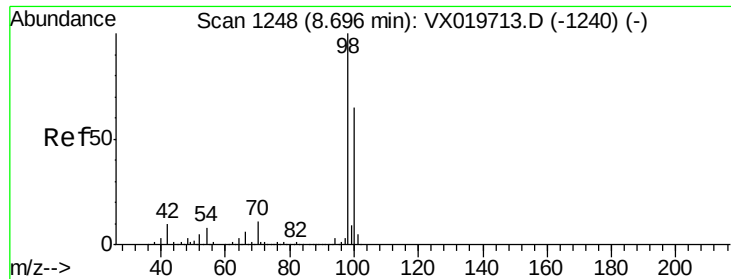

#50
Toluene-d8
Concen: 49.630 ug/l
RT: 8.70 min Scan# 1248
Delta R.T. -0.00 min
Lab File: VX020011.D
Acq: 15 Dec 2020 15:02




Instrument :
MSVOA_X
ClientSampleId :
TU032-32-5229-121020DL


Tgt Ion: 98 Resp: 639606
Ion Ratio Lower Upper
98 100
100 66.0 51.9 77.9

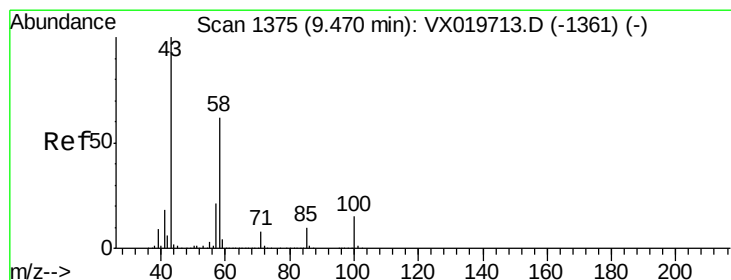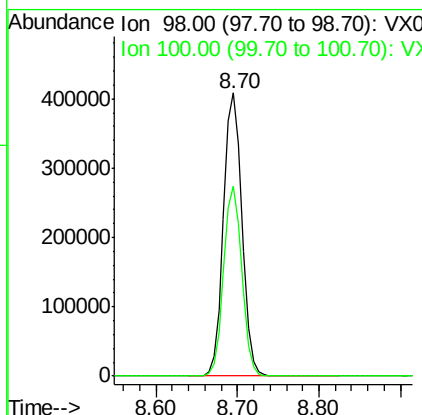

#59
2-Hexanone
Concen: 0.229 ug/l
RT: 9.47 min Scan# 1375
Delta R.T. -0.00 min
Lab File: VX020011.D
Acq: 15 Dec 2020 15:02

Tgt Ion: 43 Resp: 838
Ion Ratio Lower Upper
43 100
58 42.6 30.9 92.8

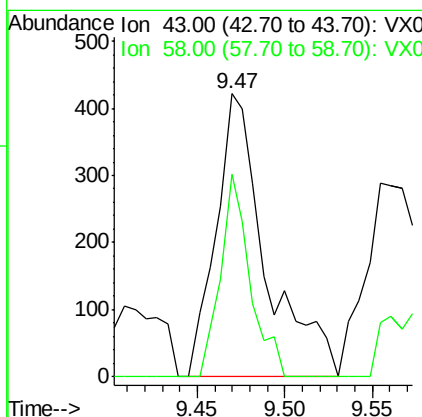



#62

4-Bromofluorobenzene

Concen: 47.428 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.00 min

Lab File: VX020011.D

Acq: 15 Dec 2020 15:02

Instrument :

MSVOA_X

ClientSampleId :

TU032-32-5229-121020DL


Tgt Ion: 95 Resp: 232641

Ion Ratio Lower Upper




95 100

174 78.5 0.0 154.6

176 74.1 0.0 155.8



Abundance Ion 94.90 (94.60 to 95.60): VX0
Ion 173.80 (173.50 to 174.50): V
Ion 175.80 (175.50 to 176.50): V

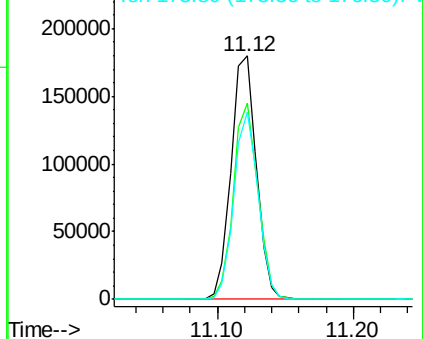

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.10 min Scan# 1478

Delta R.T. 0.01 min

Lab File: VX020011.D

Acq: 15 Dec 2020 15:02


Tgt Ion: 117 Resp: 485880

Ion Ratio Lower Upper



117 100


82 56.9 47.4 71.2

119 32.9 26.6 39.8



Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VX0
Ion 118.90 (118.60 to 119.60): V

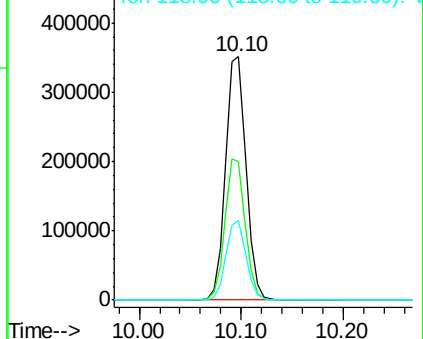

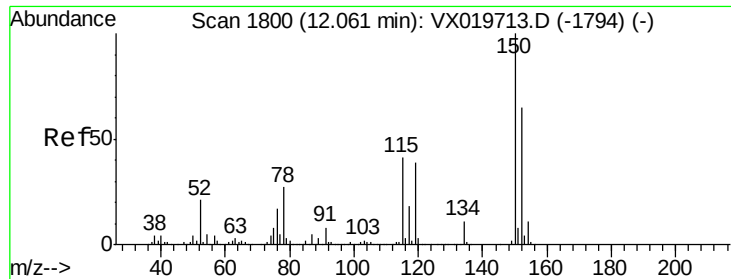

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.06 min Scan# 1800

Delta R.T. -0.00 min

Lab File: VX020011.D

Acq: 15 Dec 2020 15:02

Instrument :

MSVOA_X

ClientSampleId :

TU032-32-5229-121020DL


Tgt Ion:152 Resp: 228024

Ion Ratio Lower Upper

152 100

115 60.8 41.1 123.3




150 158.3 0.0 349.0

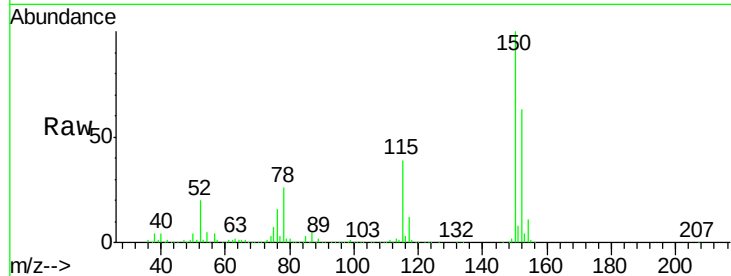

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

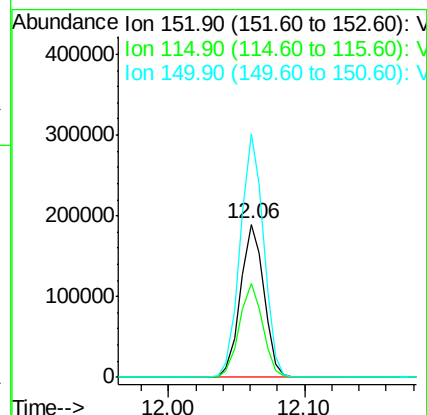

#74

N-ethyl acetate

Concen: 0.359 ug/l

RT: 10.91 min Scan# 1612

Delta R.T. 0.04 min

Lab File: VX020011.D

Acq: 15 Dec 2020 15:02

Tgt Ion: 43 Resp: 2244


Ion Ratio Lower Upper

43 100

70 34.8 39.0 58.6#

55 98.8 21.5 32.3#

61 0.0 22.1 33.1#






Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 70.00 (69.70 to 70.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

Ion 61.00 (60.70 to 61.70): VX0



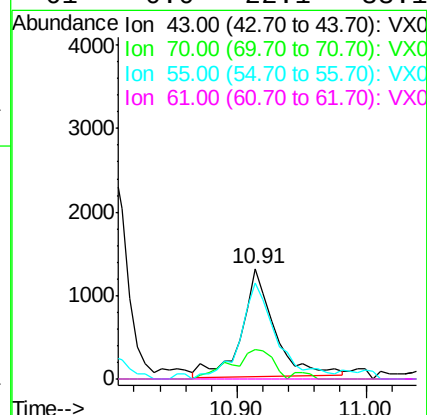





#76
 1,2,3-Trichloropropane
 Concen: 22.116 ug/l
 RT: 11.12 min Scan# 1645
 Delta R.T. -0.16 min
 Lab File: VX020011.D
 Acq: 15 Dec 2020 15:02

Instrument :
 MSVOA_X
 ClientSampleId :
 TU032-32-5229-121020DL

Tgt Ion: 75 Resp: 113106
 Ion Ratio Lower Upper
 75 100
 77 1.2 19.1 57.5#

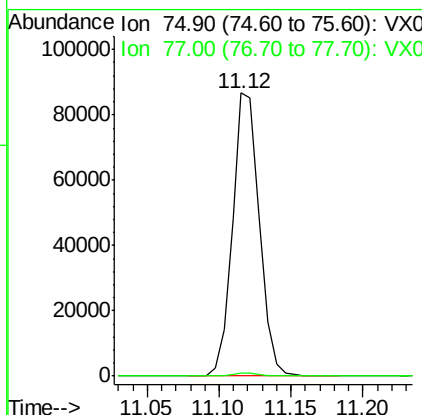

#81
 trans-1,4-Dichloro-2-butene
 Concen: 63.934 ug/l
 RT: 11.12 min Scan# 1645
 Delta R.T. 0.06 min
 Lab File: VX020011.D
 Acq: 15 Dec 2020 15:02

Tgt Ion: 75 Resp: 113106
 Ion Ratio Lower Upper
 75 100
 53 0.1 74.5 111.7#
 89 0.0 37.9 56.9#

