

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX121520\
 Data File : VX020042.D
 Acq On : 16 Dec 2020 03:48
 Operator : JC/MD
 Sample : L5088-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TR1-A-BOTTOM

Quant Time: Dec 16 05:11:16 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X120420W.M
 Quant Title : SW846 8260
 QLast Update : Fri Dec 04 15:32:53 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.62	168	309742	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	512899	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.09	117	481408	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	205581	50.00	ug/l	0.00

System Monitoring Compounds

33) 1,2-Dichloroethane-d4	6.03	65	200357	49.22	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	98.44%
35) Dibromofluoromethane	5.46	113	160713	48.48	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	96.96%
50) Toluene-d8	8.70	98	634145	50.11	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	100.22%
62) 4-Bromofluorobenzene	11.12	95	221379	45.96	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	91.92%

Target Compounds


					Qvalue
5) Bromomethane	1.63	94	635	0.544 ug/l #	73
11) Tert butyl alcohol	2.99	59	1601	Below Cal #	77
13) Acrolein	2.29	56	187	0.416 ug/l #	78
16) Acetone	2.42	43	30108	19.676 ug/l	98
18) Methyl Acetate	2.75	43	2351	0.628 ug/l	94
20) Methylene Chloride	2.83	84	28132	6.825 ug/l	96
25) 2-Butanone	4.64	43	5008	2.130 ug/l	90
29) Tetrahydrofuran	5.10	42	1005	0.663 ug/l #	74
31) Cyclohexane	5.63	56	5854	1.156 ug/l #	1
36) 1,1-Dichloropropene	5.63	75	23892	5.155 ug/l #	49
38) Carbon Tetrachloride	5.62	117	30540	6.729 ug/l #	17
40) Benzene	6.11	78	3376	0.238 ug/l	97
43) Isopropyl Acetate	6.41	43	23549	3.095 ug/l	98
44) Trichloroethene	7.18	130	2463	0.663 ug/l	98
48) Methyl methacrylate	7.65	41	7127	1.905 ug/l #	10
49) 1,4-Dioxane	7.85	88	251	2.769 ug/l #	1
51) 4-Methyl-2-Pentanone	8.59	43	82865	17.840 ug/l #	48
52) Toluene	8.76	92	3405	0.385 ug/l	97
54) cis-1,3-Dichloropropene	8.59	75	43604	7.628 ug/l #	62
57) 1,3-Dichloropropane	9.52	76	23871	3.918 ug/l #	43
59) 2-Hexanone	9.52	43	292538	81.251 ug/l #	46
60) Dibromochloromethane	9.32	129	1234	0.340 ug/l #	11
64) Tetrachloroethene	9.32	164	1371	0.425 ug/l	96
76) 1,2,3-Trichloropropane	11.12	75	106919	23.189 ug/l #	39
81) trans-1,4-Dichloro-2-buten	11.12	75	106919	67.034 ug/l #	12


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX121520\
Data File : VX020042.D
Acq On : 16 Dec 2020 03:48
Operator : JC/MD
Sample : L5088-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TR1-A-BOTTOM

Quant Time: Dec 16 05:11:16 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X120420W.M
Quant Title : SW846 8260
QLast Update : Fri Dec 04 15:32:53 2020
Response via : Initial Calibration

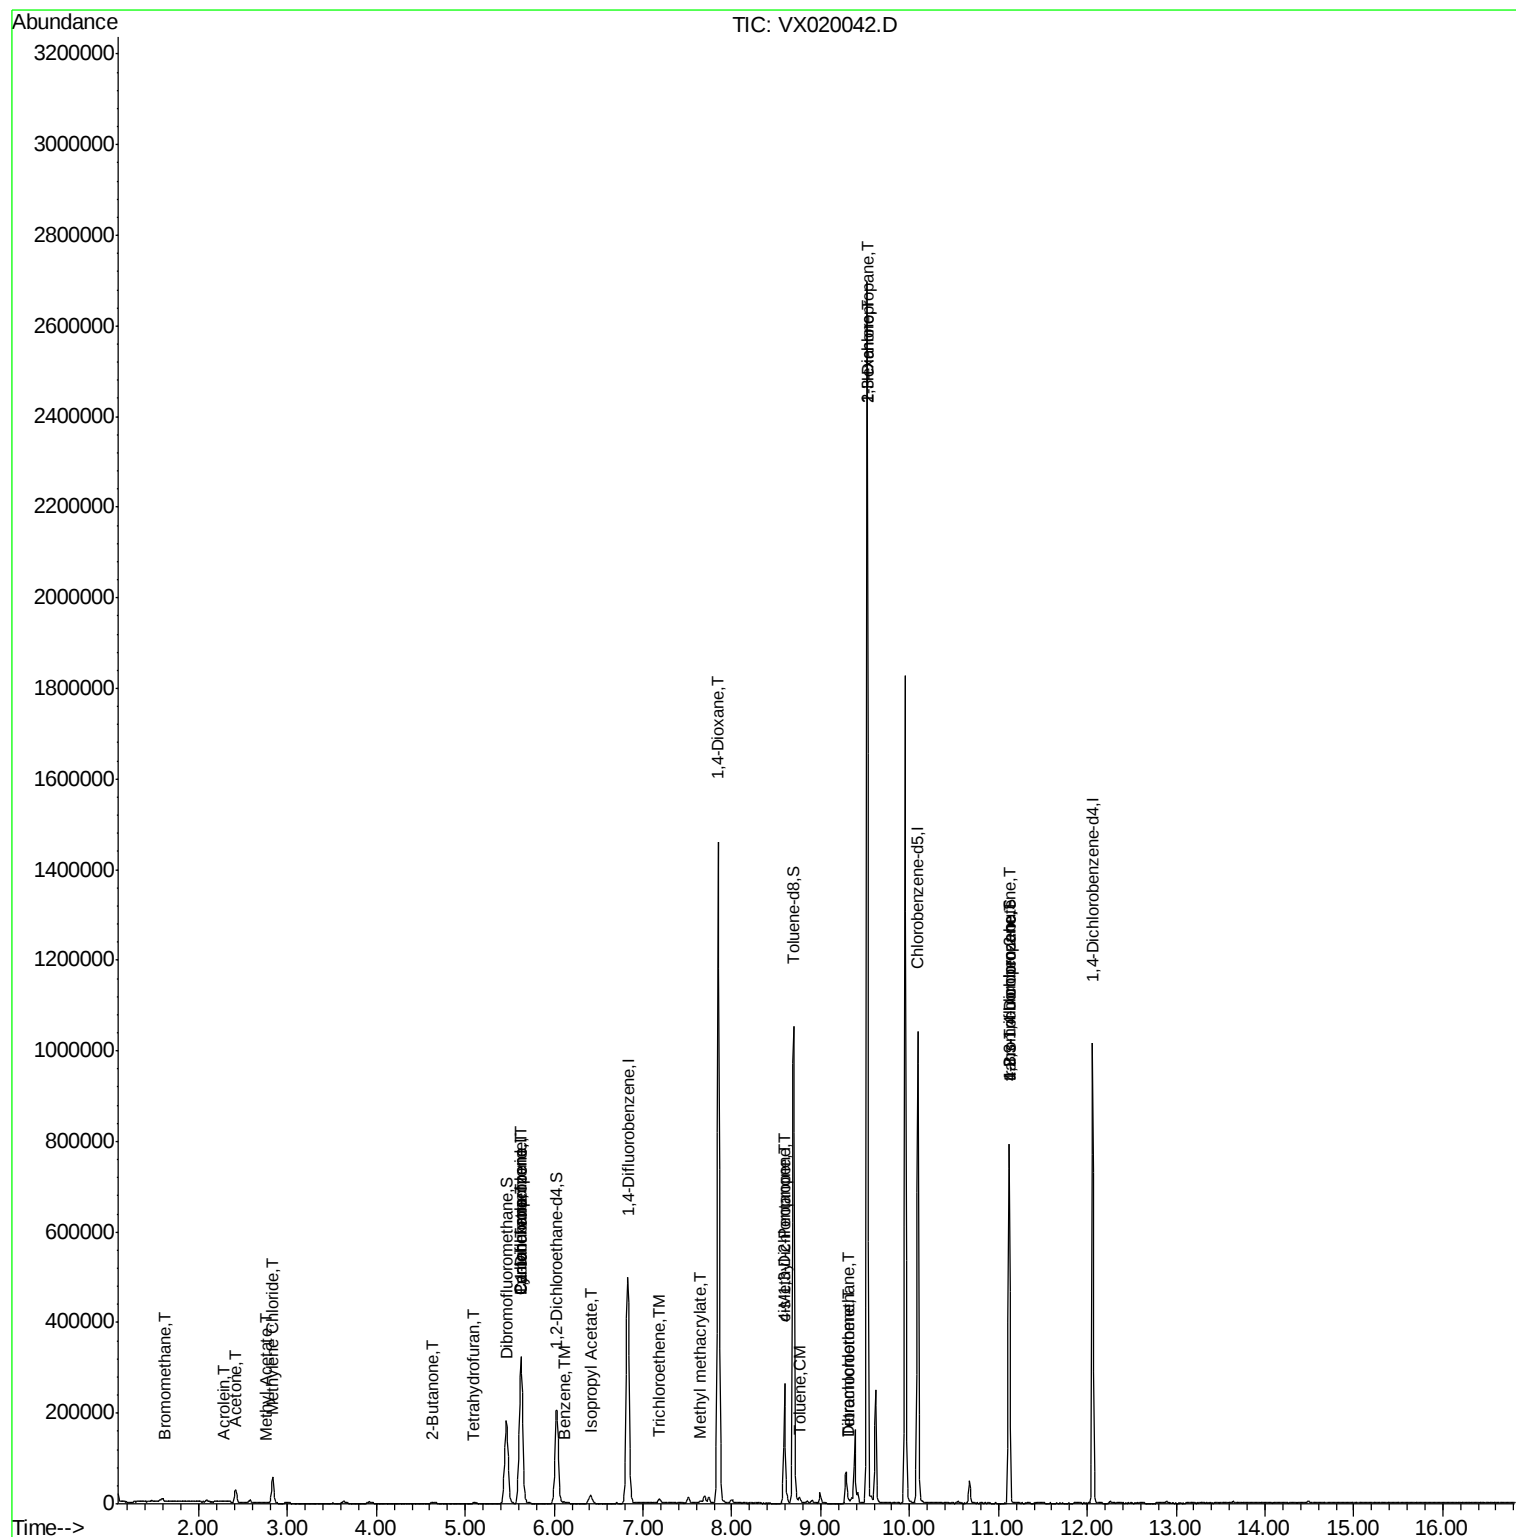

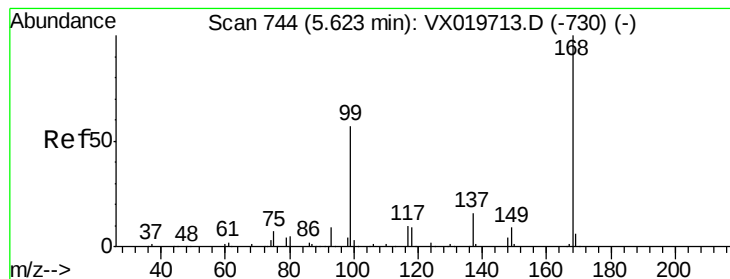

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.62 min Scan# 744

Delta R.T. -0.00 min

Lab File: VX020042.D

Acq: 16 Dec 2020 03:48

Instrument :

MSVOA_X

ClientSampleId :


TR1-A-BOTTOM

Tgt Ion:168 Resp: 309742

Ion Ratio Lower Upper

168 100

99 55.7 45.8 68.6

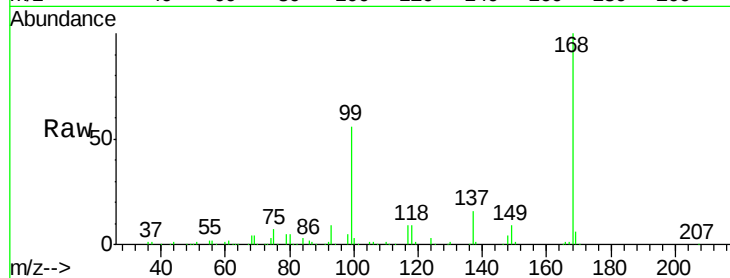

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.62

120000

100000

80000



60000

40000

20000

0

Time-->

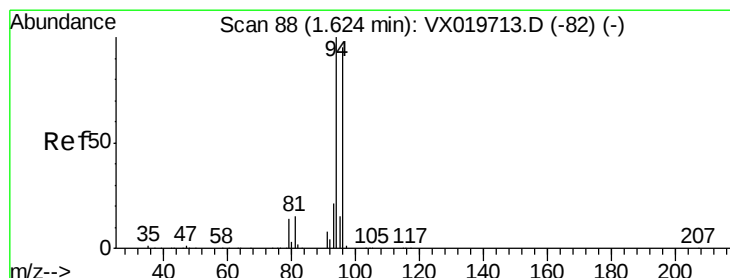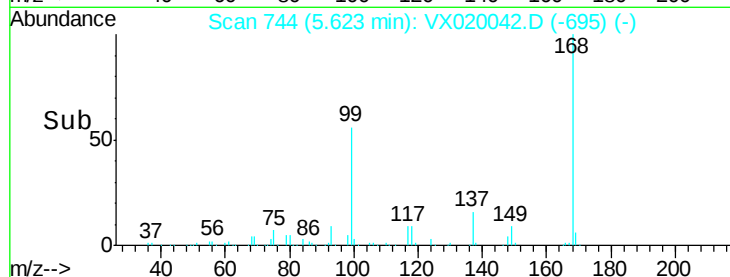

#5

Bromomethane

Concen: 0.544 ug/l

RT: 1.63 min Scan# 89

Delta R.T. 0.01 min

Lab File: VX020042.D


Acq: 16 Dec 2020 03:48

Tgt Ion: 94 Resp: 635

Ion Ratio Lower Upper

94 100

96 68.8 76.4 114.6#

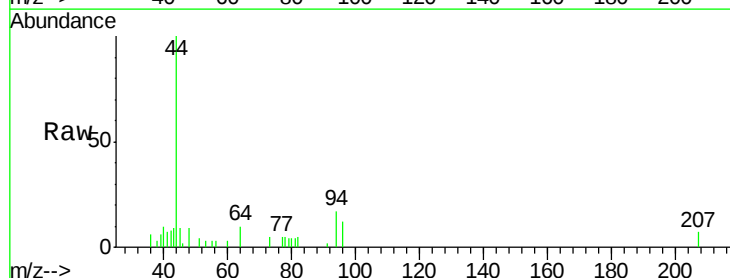

Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0

1.63

400


300


200

100

0

Time-->

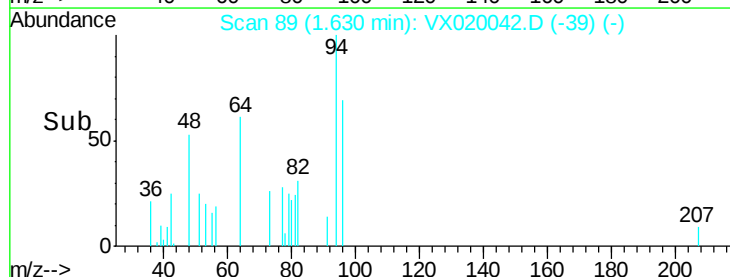

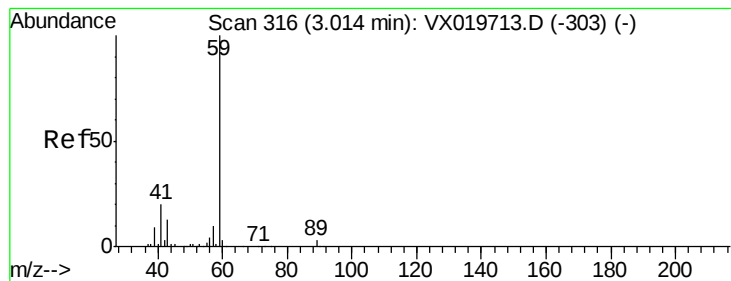

#11

Tert butyl alcohol

Concen: Below Cal

RT: 2.99 min Scan# 312

Delta R.T. -0.02 min

Lab File: VX020042.D

Acq: 16 Dec 2020 03:48

Instrument :

MSVOA_X

ClientSampleId :





TR1-A-BOTTOM

Tgt Ion: 59 Resp: 1601

Ion Ratio Lower Upper

59 100

57 1.2 7.8 11.8#

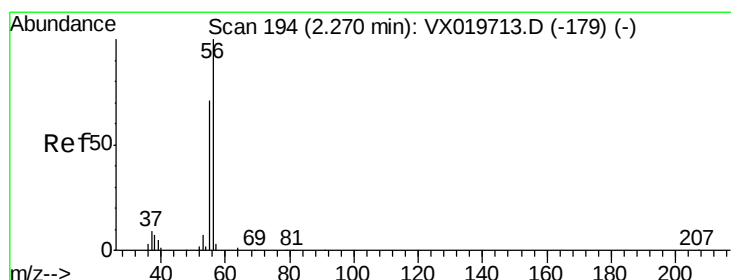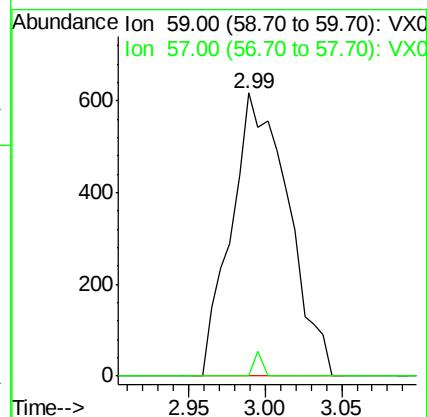

#13

Acrolein

Concen: 0.416 ug/l

RT: 2.29 min Scan# 198

Delta R.T. 0.02 min

Lab File: VX020042.D




Acq: 16 Dec 2020 03:48


Tgt Ion: 56 Resp: 187

Ion Ratio Lower Upper

56 100

55 88.2 56.4 84.6#

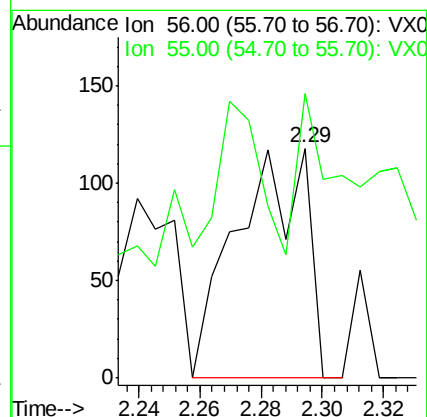



#16

Acetone

Concen: 19.676 ug/l

RT: 2.42 min Scan# 218

Delta R.T. -0.00 min

Lab File: VX020042.D

Acq: 16 Dec 2020 03:48

Instrument :

MSVOA_X

ClientSampleId :


TR1-A-BOTTOM

Tgt Ion: 43 Resp: 30108

Ion Ratio Lower Upper

43 100

58 33.8 27.8 41.8



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

20000

15000



10000

5000

0

2.35 2.40 2.45 2.50

Time-->



#18

Methyl Acetate

Concen: 0.628 ug/l

RT: 2.75 min Scan# 273

Delta R.T. 0.01 min

Lab File: VX020042.D


Acq: 16 Dec 2020 03:48

Tgt Ion: 43 Resp: 2351

Ion Ratio Lower Upper

43 100

74 24.1 21.9 32.9



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 74.00 (73.70 to 74.70): VX0


1000


500

0

2.65 2.70 2.75 2.80 2.85

Time-->







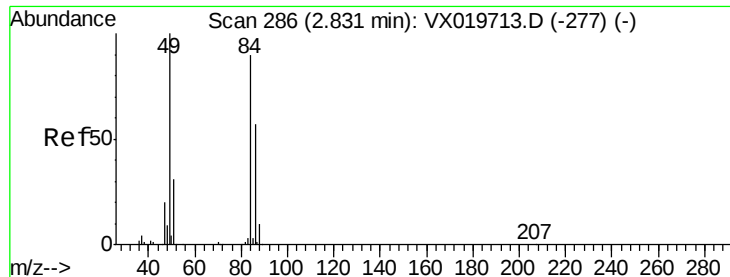

#20
Methylene Chloride
Concen: 6.825 ug/l
RT: 2.83 min Scan# 286
Delta R.T. 0.00 min
Lab File: VX020042.D
Acq: 16 Dec 2020 03:48




Instrument :
MSVOA_X
ClientSampleId :
TR1-A-BOTTOM


Tgt Ion: 84 Resp: 28132
Ion Ratio Lower Upper
84 100
49 116.7 88.6 132.8
51 37.5 27.0 40.6
86 62.5 50.3 75.5

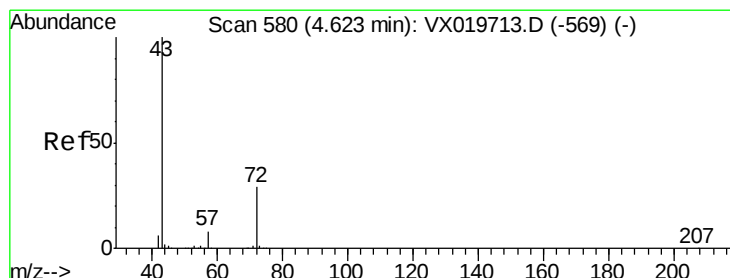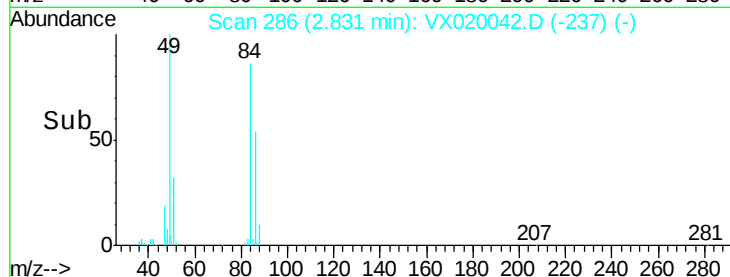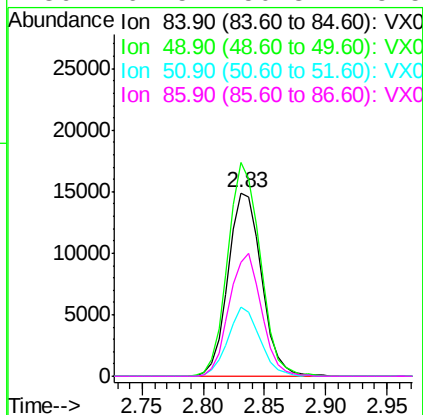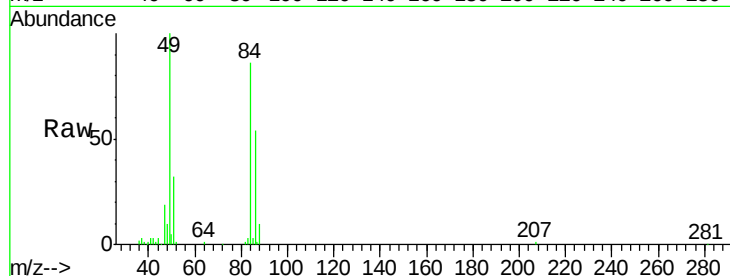

#25
2-Butanone
Concen: 2.130 ug/l
RT: 4.64 min Scan# 582
Delta R.T. 0.01 min
Lab File: VX020042.D
Acq: 16 Dec 2020 03:48

Tgt Ion: 43 Resp: 5008
Ion Ratio Lower Upper
43 100
72 24.2 23.7 35.5


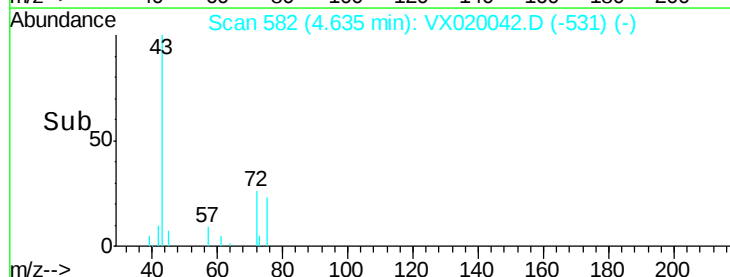
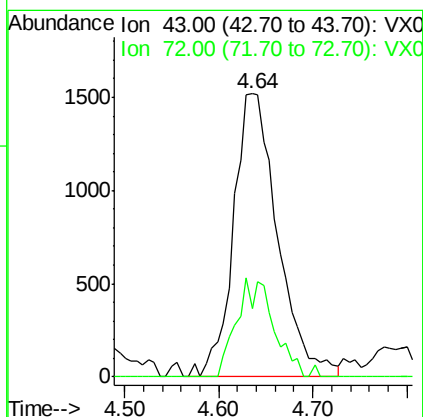
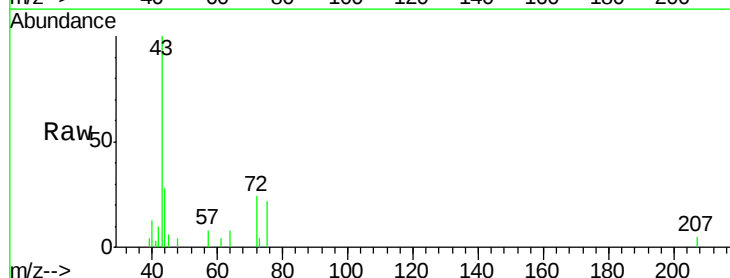




#29
Tetrahydrofuran
Concen: 0.663 ug/l
RT: 5.10 min Scan# 658
Delta R.T. 0.02 min
Lab File: VX020042.D
Acq: 16 Dec 2020 03:48




Instrument :
MSVOA_X
ClientSampleId :
TR1-A-BOTTOM


Tgt Ion: 42 Resp: 1005
Ion Ratio Lower Upper
42 100
72 30.3 41.7 62.5#
71 34.1 38.4 57.6#

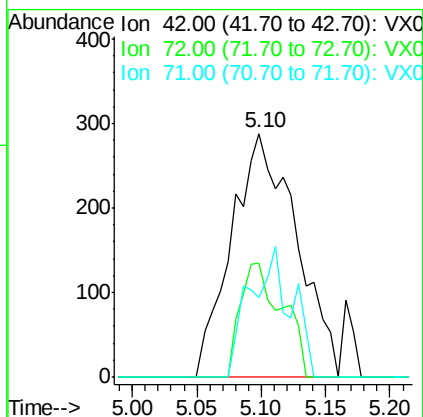

#31
Cyclohexane
Concen: 1.156 ug/l
RT: 5.63 min Scan# 745
Delta R.T. 0.09 min
Lab File: VX020042.D
Acq: 16 Dec 2020 03:48

Tgt Ion: 56 Resp: 5854
Ion Ratio Lower Upper
56 100
69 191.3 25.3 37.9#
84 154.0 71.4 107.0#



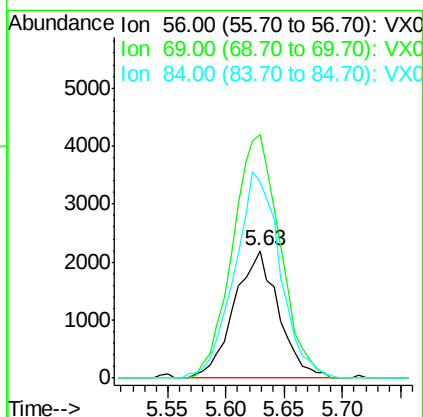





#33
 1,2-Dichloroethane-d4
 Concen: 49.217 ug/l
 RT: 6.03 min Scan# 810
 Delta R.T. -0.00 min
 Lab File: VX020042.D
 Acq: 16 Dec 2020 03:48




Instrument :
 MSVOA_X
 ClientSampleId :
 TR1-A-BOTTOM


Tgt Ion: 65 Resp: 200357
 Ion Ratio Lower Upper
 65 100
 67 53.1 0.0 105.4

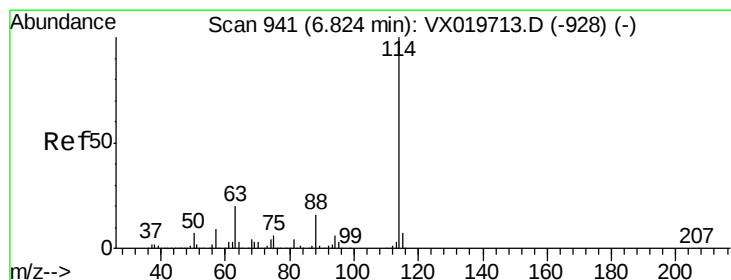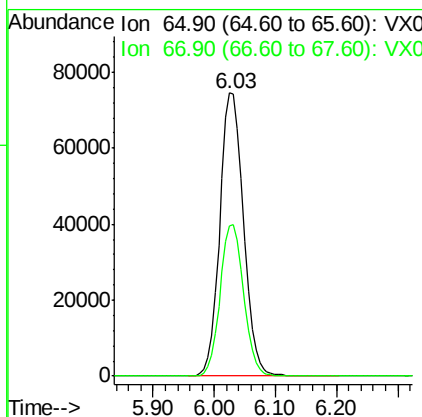

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.83 min Scan# 942
 Delta R.T. 0.01 min
 Lab File: VX020042.D
 Acq: 16 Dec 2020 03:48

Tgt Ion: 114 Resp: 512899
 Ion Ratio Lower Upper
 114 100
 63 20.3 0.0 40.8
 88 17.1 0.0 32.8

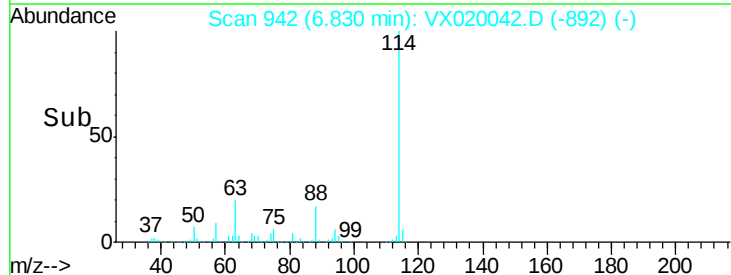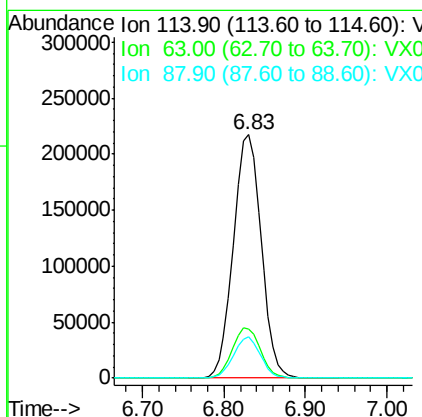







#35
 Dibromofluoromethane
 Concen: 48.484 ug/l
 RT: 5.46 min Scan# 718
 Delta R.T. 0.01 min
 Lab File: VX020042.D
 Acq: 16 Dec 2020 03:48

Instrument :
 MSVOA_X
 ClientSampleId :
 TR1-A-BOTTOM

Tgt Ion	Ratio	Lower	Upper
113	100		
111	102.3	81.9	122.9
192	20.2	16.7	25.1




Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V


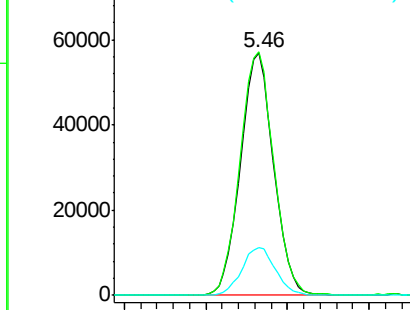



#36
 1,1-Dichloropropene
 Concen: 5.155 ug/l
 RT: 5.63 min Scan# 745
 Delta R.T. -0.13 min
 Lab File: VX020042.D
 Acq: 16 Dec 2020 03:48

Tgt Ion	Ratio	Lower	Upper
75	100		
110	9.0	18.1	54.4#
77	0.0	25.3	37.9#



Abundance Ion 74.90 (74.60 to 75.60): VX0
 Ion 109.90 (109.60 to 110.60): V
 Ion 76.90 (76.60 to 77.60): VX0

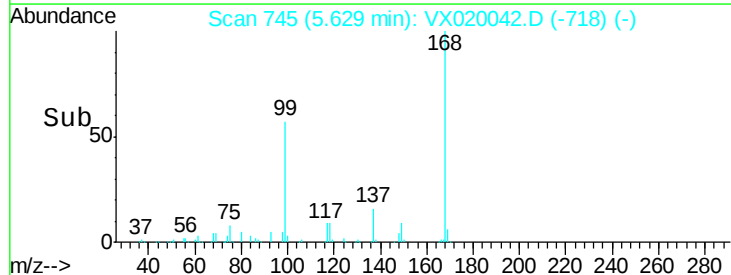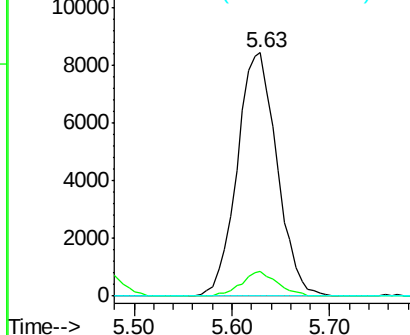



#38

Carbon Tetrachloride

Concen: 6.729 ug/l

RT: 5.62 min Scan# 744

Delta R.T. -0.13 min

Lab File: VX020042.D

Acq: 16 Dec 2020 03:48

Instrument :

MSVOA_X

ClientSampleId :

TR1-A-BOTTOM


Tgt Ion:117 Resp: 30540

Ion Ratio Lower Upper

117 100

119 6.7 76.2 114.2#




121 0.0 24.8 37.2#



Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

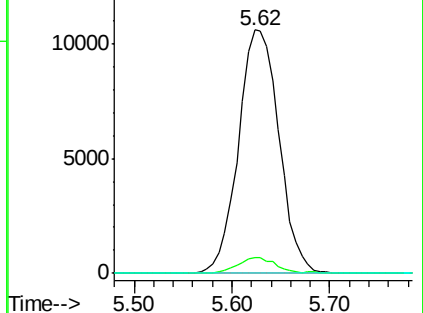

#40

Benzene

Concen: 0.238 ug/l

RT: 6.11 min Scan# 824

Delta R.T. 0.01 min

Lab File: VX020042.D


Acq: 16 Dec 2020 03:48

Tgt Ion: 78 Resp: 3376

Ion Ratio Lower Upper



78 100


77 25.1 18.9 28.3



Abundance Ion 78.00 (77.70 to 78.70): VX0

Ion 77.00 (76.70 to 77.70): VX0

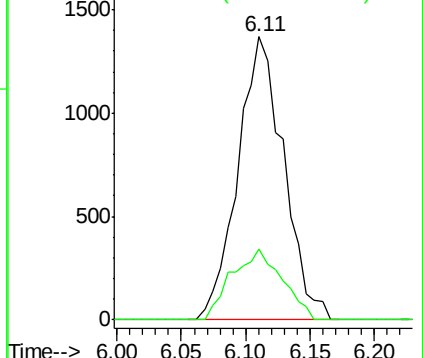



#43

Isopropyl Acetate

Concen: 3.095 ug/l

RT: 6.41 min Scan# 873

Delta R.T. 0.01 min

Lab File: VX020042.D

Acq: 16 Dec 2020 03:48

Instrument :

MSVOA_X

ClientSampleId :

TR1-A-BOTTOM


Tgt Ion: 43 Resp: 23549

Ion Ratio Lower Upper

43 100

61 24.1 18.2 27.4




87 15.1 12.5 18.7



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

Ion 87.00 (86.70 to 87.70): VX0

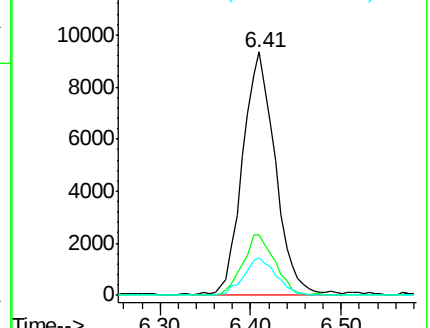

#44

Trichloroethene

Concen: 0.663 ug/l

RT: 7.18 min Scan# 1000

Delta R.T. -0.00 min

Lab File: VX020042.D


Acq: 16 Dec 2020 03:48

Tgt Ion: 130 Resp: 2463

Ion Ratio Lower Upper



130 100


95 101.0 0.0 198.0



Abundance Ion 129.80 (129.50 to 130.50): V

Ion 94.90 (94.60 to 95.60): VX0

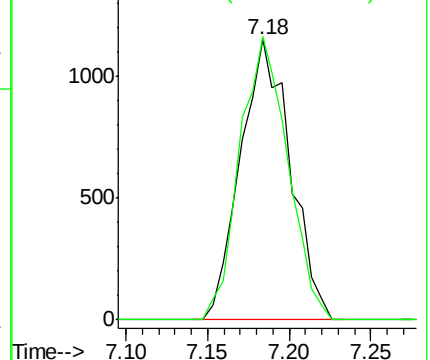



#48

Methyl methacrylate

Concen: 1.905 ug/l

RT: 7.65 min Scan# 1076

Delta R.T. -0.09 min

Lab File: VX020042.D

Acq: 16 Dec 2020 03:48

Instrument :

MSVOA_X

ClientSampleId :

TR1-A-BOTTOM


Tgt Ion: 41 Resp: 7127

Ion Ratio Lower Upper

41 100

69 0.0 76.0 114.0#




39 0.0 44.6 67.0#



Abundance Ion 41.00 (40.70 to 41.70): VX0

Ion 69.00 (68.70 to 69.70): VX0

Ion 39.00 (38.70 to 39.70): VX0

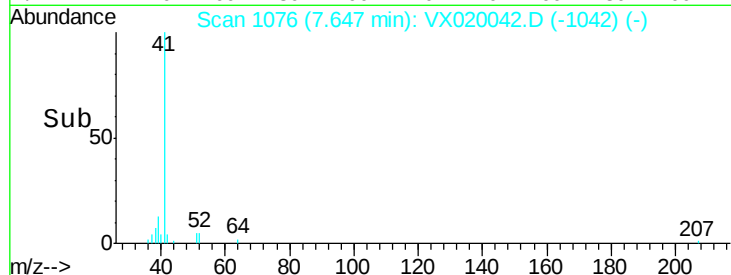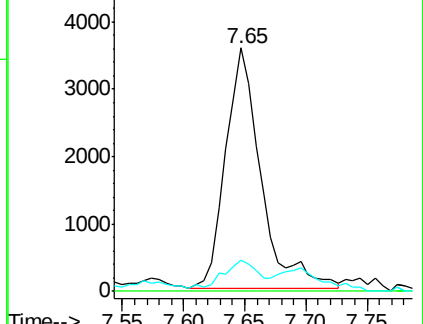

#49

1,4-Dioxane

Concen: 2.769 ug/l

RT: 7.85 min Scan# 1109

Delta R.T. 0.14 min

Lab File: VX020042.D

Acq: 16 Dec 2020 03:48


Tgt Ion: 88 Resp: 251

Ion Ratio Lower Upper

88 100

43 492913.1 23.2 34.8#



58 2592.0 55.0 82.4#




Abundance Ion 88.00 (87.70 to 88.70): VX0

Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0




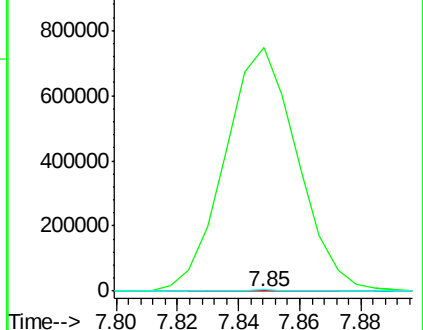




#50
Toluene-d8
Concen: 50.110 ug/l
RT: 8.70 min Scan# 1248
Delta R.T. -0.00 min
Lab File: VX020042.D
Acq: 16 Dec 2020 03:48




Instrument :
MSVOA_X
ClientSampleId :
TR1-A-BOTTOM


Tgt Ion: 98 Resp: 634145
Ion Ratio Lower Upper
98 100
100 66.3 51.9 77.9

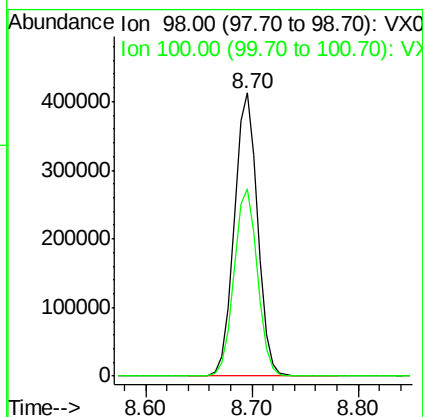

#51
4-Methyl-2-Pentanone
Concen: 17.840 ug/l
RT: 8.59 min Scan# 1231
Delta R.T. -0.02 min
Lab File: VX020042.D
Acq: 16 Dec 2020 03:48

Tgt Ion: 43 Resp: 82865
Ion Ratio Lower Upper
43 100
58 10.4 35.4 53.0#

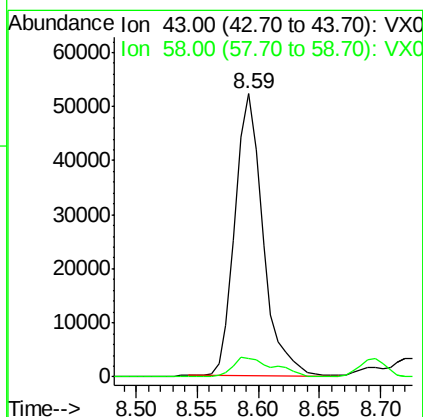

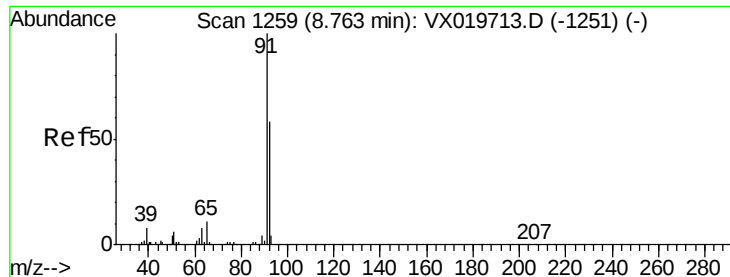

#52

Toluene

Concen: 0.385 ug/l

RT: 8.76 min Scan# 1259

Delta R.T. -0.00 min

Lab File: VX020042.D

Acq: 16 Dec 2020 03:48

Instrument :

MSVOA_X

ClientSampleId :





TR1-A-BOTTOM

Tgt Ion: 92 Resp: 3405

Ion Ratio Lower Upper

92 100

91 174.9 137.1 205.7

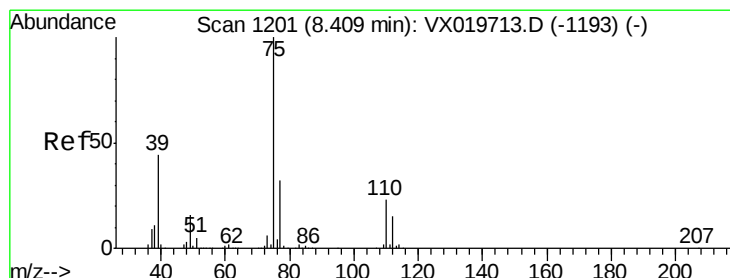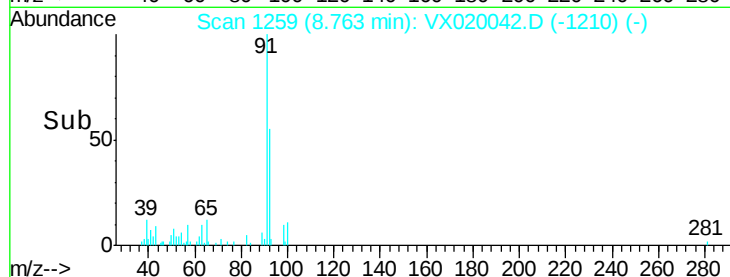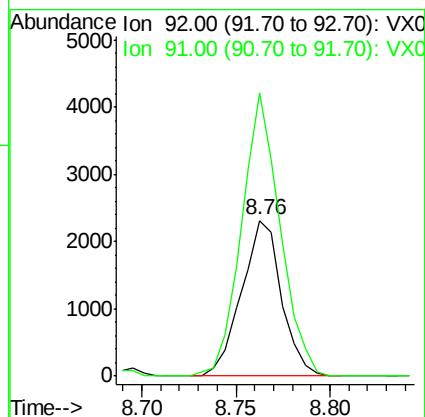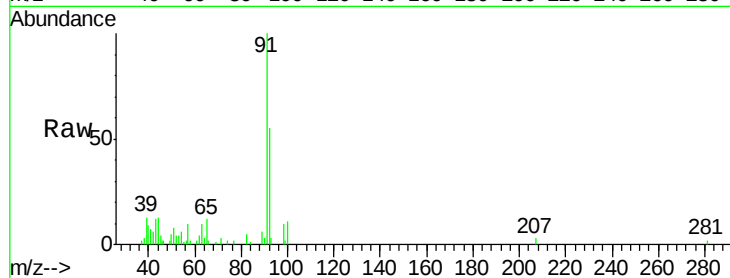

#54

cis-1,3-Dichloropropene

Concen: 7.628 ug/l

RT: 8.59 min Scan# 1231

Delta R.T. 0.18 min

Lab File: VX020042.D

Acq: 16 Dec 2020 03:48




Tgt Ion: 75 Resp: 43604


Ion Ratio Lower Upper

75 100

77 0.6 25.7 38.5#

39 28.5 35.1 52.7#

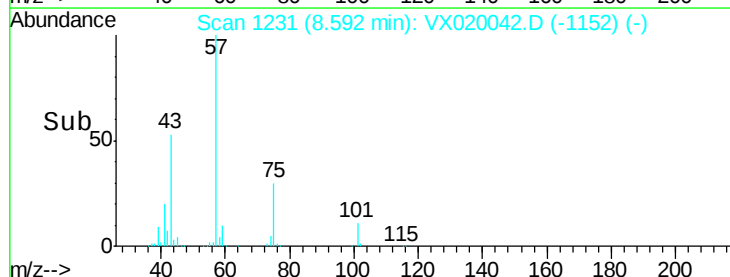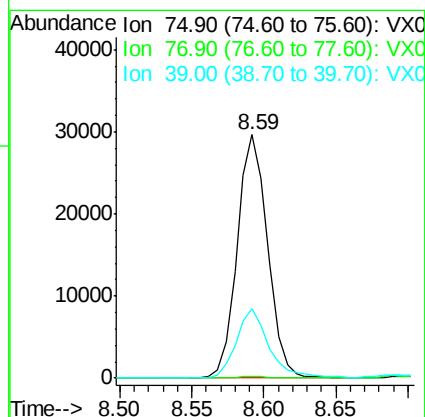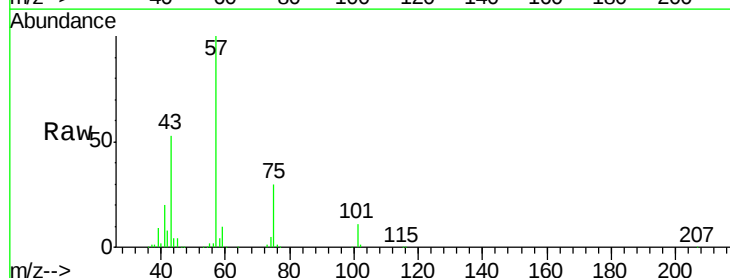



#57

1,3-Dichloropropane

Concen: 3.918 ug/l

RT: 9.52 min Scan# 1384

Delta R.T. 0.18 min

Lab File: VX020042.D

Acq: 16 Dec 2020 03:48

Instrument :

MSVOA_X

ClientSampleId :


TR1-A-BOTTOM

Tgt Ion: 76 Resp: 23871

Ion Ratio Lower Upper

76 100

78 0.7 26.2 39.2#



Abundance Ion 75.90 (75.60 to 76.60): VX0

Ion 77.90 (77.60 to 78.60): VX0

9.52

20000

15000



10000

5000

0

9.45 9.50 9.55 9.60

Time-->



#59

2-Hexanone

Concen: 81.251 ug/l

RT: 9.52 min Scan# 1384

Delta R.T. 0.05 min

Lab File: VX020042.D


Acq: 16 Dec 2020 03:48

Tgt Ion: 43 Resp: 292538

Ion Ratio Lower Upper

43 100

58 20.4 30.9 92.8#



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

9.52

250000

200000

150000


100000


50000

0

9.45 9.50 9.55 9.60

Time-->









#60
Dibromochloromethane
Concen: 0.340 ug/l
RT: 9.32 min Scan# 1350
Delta R.T. -0.24 min
Lab File: VX020042.D
Acq: 16 Dec 2020 03:48




Instrument :
MSVOA_X
ClientSampleId :
TR1-A-BOTTOM


Tgt Ion:129 Resp: 1234
Ion Ratio Lower Upper
129 100
127 0.0 38.4 115.2#

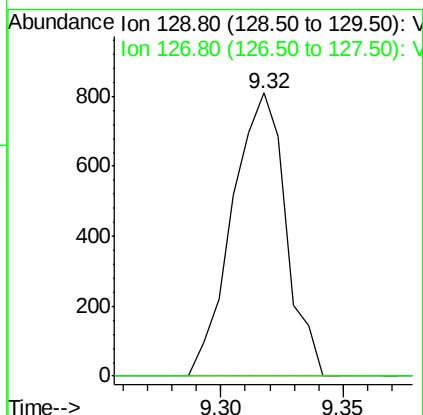

#62
4-Bromofluorobenzene
Concen: 45.961 ug/l
RT: 11.12 min Scan# 1646
Delta R.T. -0.00 min
Lab File: VX020042.D
Acq: 16 Dec 2020 03:48

Tgt Ion: 95 Resp: 221379
Ion Ratio Lower Upper
95 100
174 77.3 0.0 154.6
176 73.2 0.0 155.8



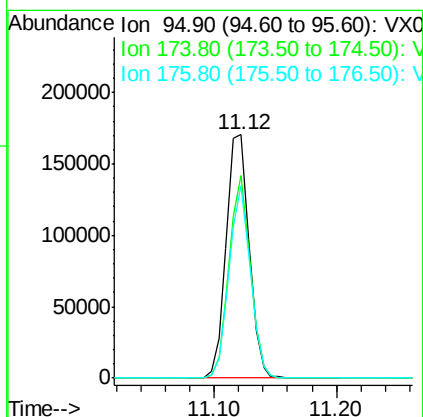





#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.09 min Scan# 1477
Delta R.T. -0.00 min
Lab File: VX020042.D
Acq: 16 Dec 2020 03:48




Instrument :
MSVOA_X
ClientSampleId :
TR1-A-BOTTOM


Tgt Ion:117 Resp: 481408
Ion Ratio Lower Upper
117 100
82 58.4 47.4 71.2
119 32.1 26.6 39.8

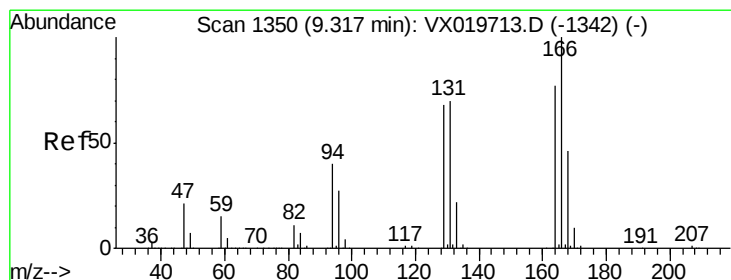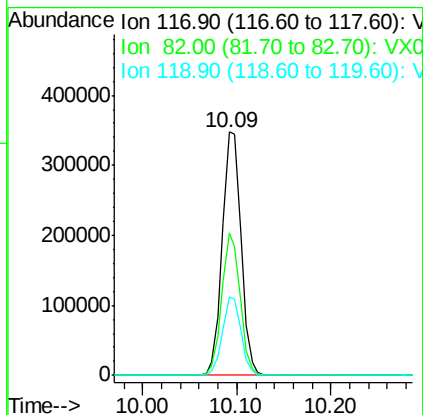

#64
Tetrachloroethene
Concen: 0.425 ug/l
RT: 9.32 min Scan# 1350
Delta R.T. -0.00 min
Lab File: VX020042.D
Acq: 16 Dec 2020 03:48

Tgt Ion:164 Resp: 1371
Ion Ratio Lower Upper
164 100
166 137.1 103.4 155.2
129 87.1 70.8 106.2
131 92.2 72.5 108.7

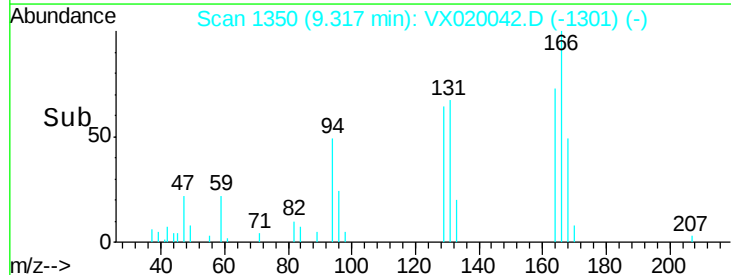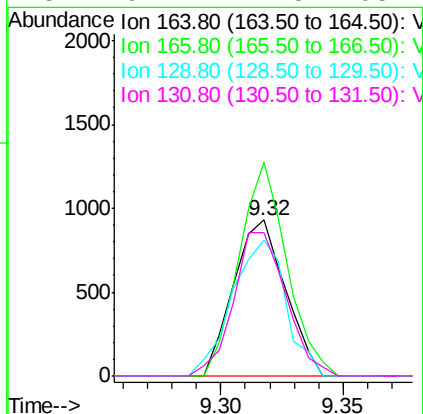



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.06 min Scan# 1800

Delta R.T. -0.00 min

Lab File: VX020042.D

Acq: 16 Dec 2020 03:48

Instrument :

MSVOA_X

ClientSampleId :

TR1-A-BOTTOM


Tgt Ion:152 Resp: 205581

Ion Ratio Lower Upper

152 100

115 59.2 41.1 123.3




150 156.9 0.0 349.0



Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

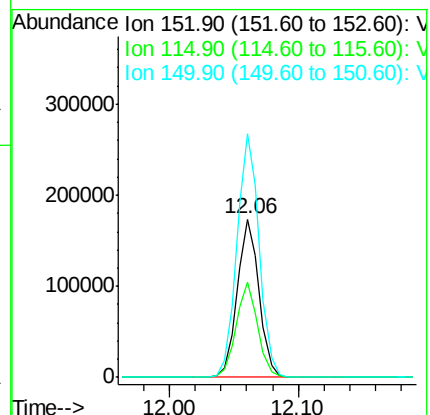

#76

1,2,3-Trichloropropane

Concen: 23.189 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.16 min

Lab File: VX020042.D


Acq: 16 Dec 2020 03:48

Tgt Ion: 75 Resp: 106919

Ion Ratio Lower Upper



75 100


77 1.3 19.1 57.5#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

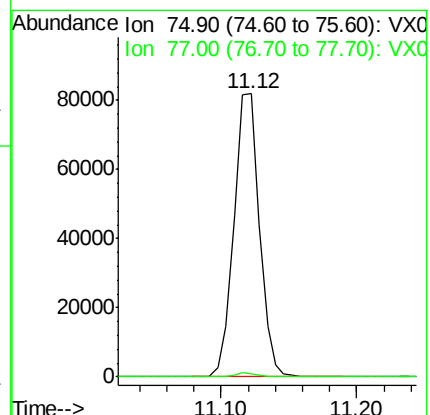



#81

trans-1,4-Dichloro-2-butene

Concen: 67.034 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. 0.07 min

Lab File: VX020042.D

Acq: 16 Dec 2020 03:48

Instrument :

MSVOA_X

ClientSampleId :

TR1-A-BOTTOM

Tgt Ion: 75 Resp: 106919

Ion Ratio Lower Upper

75 100

53 0.1 74.5 111.7#

89 0.0 37.9 56.9#

