
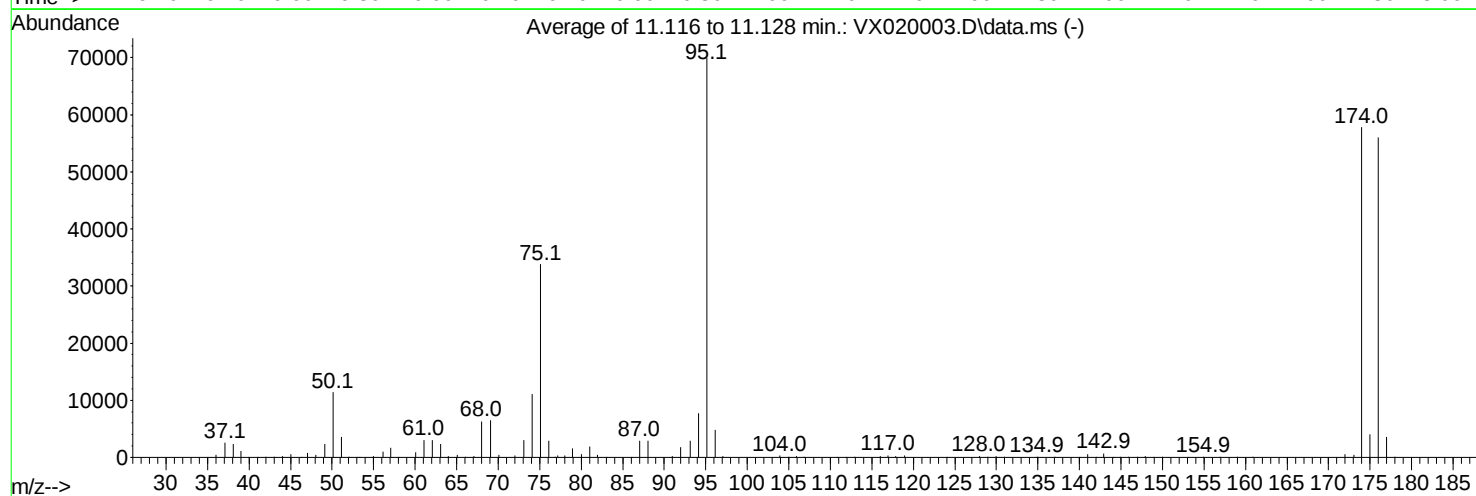


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121520\
 Data File : VX020003.D
 Acq On : 15 Dec 2020 10:52
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X120420W.M
 Title : SW846 8260
 Last Update : Fri Dec 04 15:32:53 2020

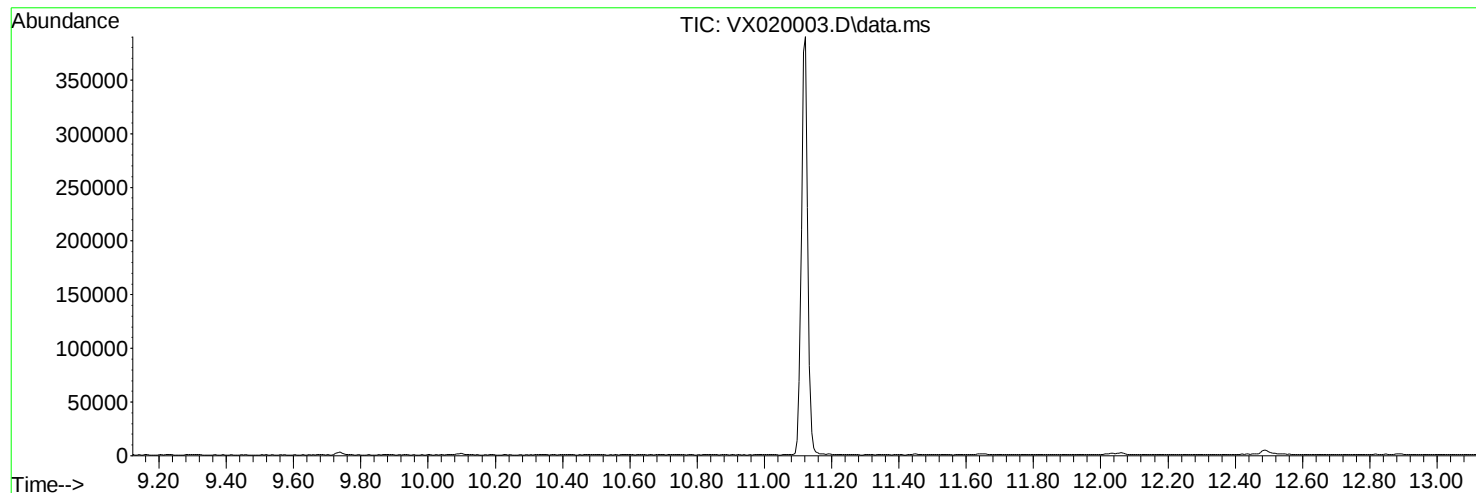

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	11423	PASS
75	95	30	60	48.4	33832	PASS
95	95	100	100	100.0	69896	PASS
96	95	5	9	6.9	4838	PASS
173	174	0.00	2	0.9	504	PASS
174	95	50	100	82.7	57771	PASS
175	174	5	9	6.9	3999	PASS
176	174	95	101	96.9	55973	PASS
177	176	5	9	6.4	3599	PASS