
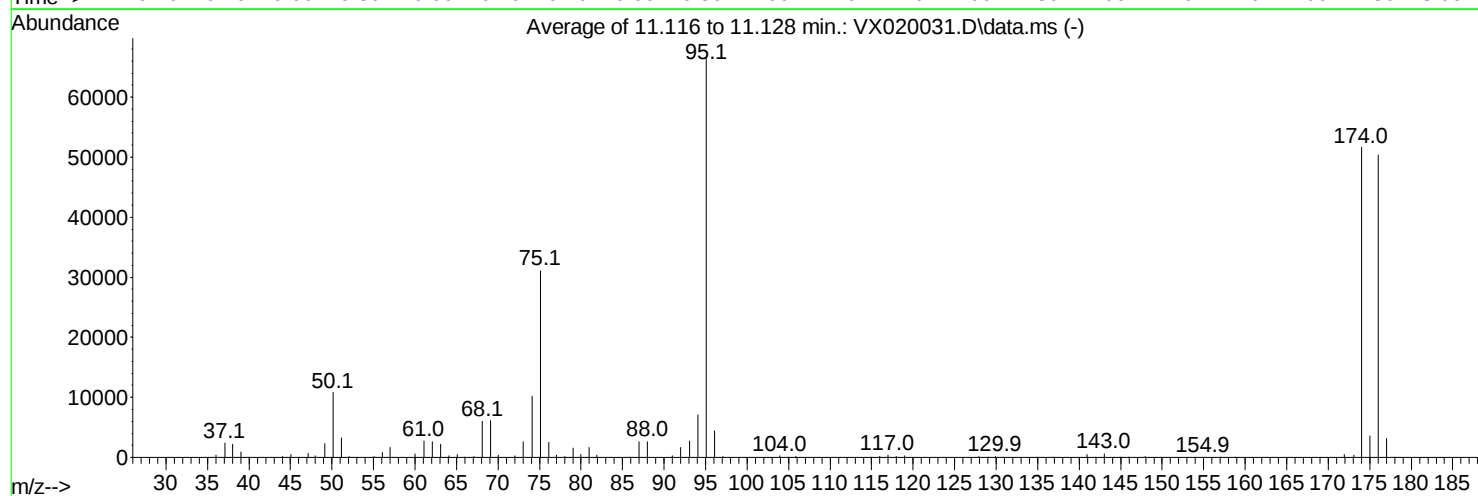


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121520\
 Data File : VX020031.D
 Acq On : 15 Dec 2020 23:09
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X120420W.M
 Title : SW846 8260
 Last Update : Fri Dec 04 15:32:53 2020

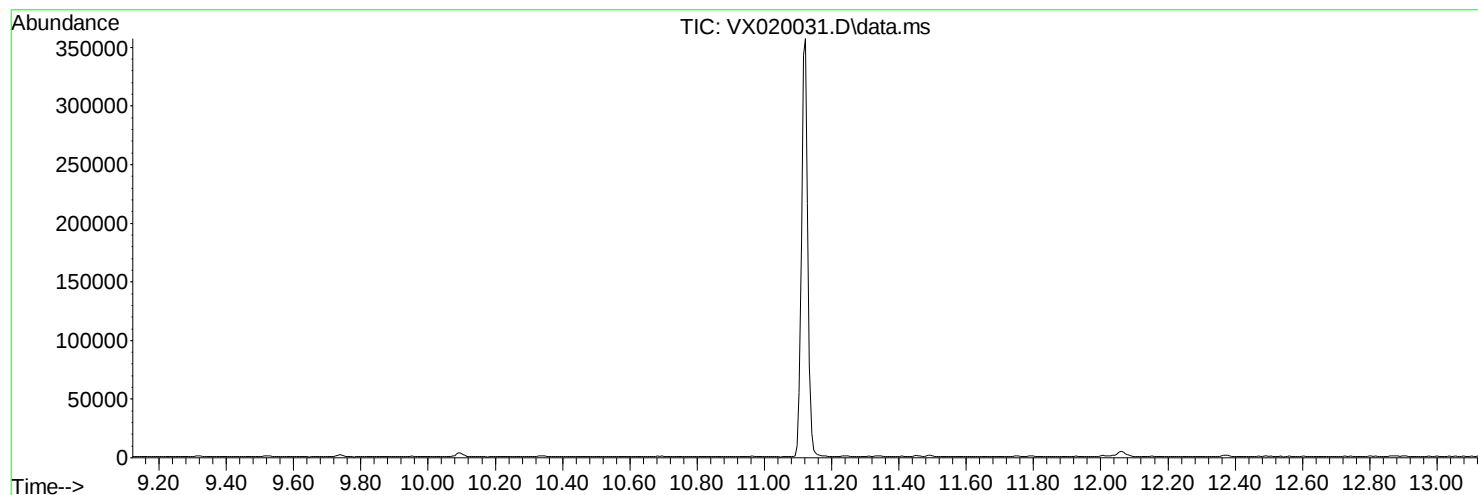

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	10840	PASS
75	95	30	60	46.8	31133	PASS
95	95	100	100	100.0	66491	PASS
96	95	5	9	6.7	4435	PASS
173	174	0.00	2	0.8	430	PASS
174	95	50	100	77.7	51688	PASS
175	174	5	9	7.1	3671	PASS
176	174	95	101	97.6	50467	PASS
177	176	5	9	6.3	3203	PASS