

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121521\
 Data File : VX025806.D
 Acq On : 15 Dec 2021 10:44
 Operator : JC/MD
 Sample : VX1215WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK653

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M

Title : VOC Analysis

Signal : TIC: VX025806.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	56	rVB	84722	81317	12.49%	1.576%
2	1.666	91	95	106	rVB	65617	86040	13.22%	1.667%
3	2.307	194	200	213	rVB	125810	209673	32.21%	4.063%
4	2.441	219	222	226	rVB3	461	642	0.10%	0.012%
5	2.477	226	228	230	rBV2	278	259	0.04%	0.005%
6	2.502	230	232	233	rBV2	452	382	0.06%	0.007%
7	2.672	256	260	262	rBV2	311	459	0.07%	0.009%
8	2.697	262	264	269	rVB3	236	448	0.07%	0.009%
9	2.794	274	280	284	rVB4	1073	1947	0.30%	0.038%
10	2.928	300	302	303	rBV2	408	384	0.06%	0.007%
11	2.947	303	305	311	rVB4	663	952	0.15%	0.018%
12	3.142	334	337	338	rVB	308	238	0.04%	0.005%
13	3.160	338	340	341	rBV2	236	174	0.03%	0.003%
14	3.581	406	409	411	rBV	266	280	0.04%	0.005%
15	3.642	417	419	421	rBV	284	257	0.04%	0.005%
16	3.745	434	436	439	rBV2	213	285	0.04%	0.006%
17	3.800	443	445	448	rBV2	153	199	0.03%	0.004%
18	4.148	501	502	506	rVB2	303	192	0.03%	0.004%
19	4.184	506	508	511	rBV3	172	187	0.03%	0.004%
20	4.251	514	519	521	rBV	327	534	0.08%	0.010%
21	4.453	541	552	572	rBV	53598	154745	23.77%	2.998%
22	4.599	574	576	579	rVB3	379	375	0.06%	0.007%
23	4.678	588	589	591	rBV2	246	184	0.03%	0.004%
24	5.050	639	650	666	rBV2	87831	275066	42.25%	5.330%
25	5.184	670	672	674	rVB3	317	240	0.04%	0.005%
26	5.398	701	707	711	rBV3	430	793	0.12%	0.015%
27	5.538	728	730	732	rBV2	331	379	0.06%	0.007%
28	5.849	777	781	784	rBV	196	353	0.05%	0.007%
29	5.971	789	801	818	rBV2	212843	651006	100.00%	12.614%
30	6.324	858	859	861	rBV2	247	189	0.03%	0.004%
31	6.373	864	867	868	rBV2	219	199	0.03%	0.004%
32	6.763	921	931	946	rVV	178237	427177	65.62%	8.277%
33	7.111	982	988	997	rBV3	2768	6240	0.96%	0.121%
34	7.306	1012	1020	1038	rVB	134207	297377	45.68%	5.762%
35	7.812	1102	1103	1106	rVB2	524	376	0.06%	0.007%
36	7.928	1119	1122	1123	rBV2	421	410	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121521\
 Data File : VX025806.D
 Acq On : 15 Dec 2021 10:44
 Operator : JC/MD
 Sample : VX1215WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK653

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

37	8.324	1181	1187	1197	rVV	91031	144924	22.26%	2.808%
38	8.476	1210	1212	1217	rVB4	522	572	0.09%	0.011%
39	8.531	1219	1221	1224	rVB	225	176	0.03%	0.003%
40	8.647	1233	1240	1248	rBV	321216	512974	78.80%	9.940%
41	8.720	1248	1252	1256	rVB2	4083	6796	1.04%	0.132%
42	8.854	1272	1274	1277	rBV2	342	286	0.04%	0.006%
43	8.952	1283	1290	1298	rBV	62941	88143	13.54%	1.708%
44	9.250	1336	1339	1340	rBV	212	221	0.03%	0.004%
45	9.385	1355	1361	1381	rBV	233682	334937	51.45%	6.490%
46	9.756	1419	1422	1423	rVB2	190	195	0.03%	0.004%
47	9.939	1450	1452	1455	rVB	224	197	0.03%	0.004%
48	10.055	1465	1471	1487	rVB	396656	532732	81.83%	10.323%
49	10.195	1492	1494	1498	rBV	407	374	0.06%	0.007%
50	10.269	1504	1506	1508	rVB2	250	185	0.03%	0.004%
51	10.305	1508	1512	1515	rBV2	1050	1270	0.20%	0.025%
52	10.354	1518	1520	1523	rBV	184	191	0.03%	0.004%
53	10.512	1544	1546	1547	rBV2	298	180	0.03%	0.003%
54	10.610	1560	1562	1564	rBV2	192	204	0.03%	0.004%
55	10.732	1580	1582	1587	rVB2	289	292	0.04%	0.006%
56	10.970	1618	1621	1625	rVV3	498	658	0.10%	0.013%
57	11.018	1627	1629	1632	rBV2	295	335	0.05%	0.006%
58	11.079	1638	1639	1642	rBV3	406	288	0.04%	0.006%
59	11.122	1642	1646	1652	rVB2	1312	1808	0.28%	0.035%
60	11.195	1652	1658	1665	rBV	259231	338434	51.99%	6.558%
61	11.250	1665	1667	1668	rVB	501	269	0.04%	0.005%
62	11.274	1668	1671	1674	rVB3	428	502	0.08%	0.010%
63	11.305	1674	1676	1678	rBV3	477	480	0.07%	0.009%
64	11.579	1718	1721	1722	rBV2	214	236	0.04%	0.005%
65	11.683	1737	1738	1741	rBV	280	279	0.04%	0.005%
66	11.750	1745	1749	1753	rVB3	1534	2199	0.34%	0.043%
67	11.884	1769	1771	1774	rBV2	190	226	0.03%	0.004%
68	11.939	1777	1780	1783	rVB4	608	658	0.10%	0.013%
69	11.976	1783	1786	1789	rBV2	704	831	0.13%	0.016%
70	12.024	1789	1794	1804	rVV	410009	509947	78.33%	9.881%
71	12.323	1837	1843	1850	rBV	346766	466733	71.69%	9.044%
72	12.482	1868	1869	1873	rVB	400	298	0.05%	0.006%
73	12.658	1896	1898	1902	rVB2	302	337	0.05%	0.007%
74	12.994	1949	1953	1957	rBV2	195	293	0.05%	0.006%
75	13.036	1957	1960	1962	rBV2	257	267	0.04%	0.005%
76	13.116	1970	1973	1976	rBV2	664	822	0.13%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121521\
 Data File : VX025806.D
 Acq On : 15 Dec 2021 10:44
 Operator : JC/MD
 Sample : VX1215WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK653

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

77	13.195	1984	1986	1989	rBV	208	227	0.03%	0.004%
78	13.262	1993	1997	1999	rBV	383	551	0.08%	0.011%
79	13.292	1999	2002	2004	rBV2	264	273	0.04%	0.005%
80	13.591	2048	2051	2055	rVV3	1077	1293	0.20%	0.025%
81	13.786	2078	2083	2087	rBV2	807	1251	0.19%	0.024%
82	13.859	2093	2095	2097	rVB2	275	205	0.03%	0.004%
83	13.878	2097	2098	2102	rVB2	315	386	0.06%	0.007%
84	13.914	2102	2104	2106	rBV2	211	262	0.04%	0.005%
85	13.963	2109	2112	2118	rVB4	785	1198	0.18%	0.023%
86	14.085	2129	2132	2133	rBV2	250	211	0.03%	0.004%
87	14.372	2177	2179	2183	rBV	331	348	0.05%	0.007%
88	14.445	2188	2191	2192	rBV	311	296	0.05%	0.006%
89	14.512	2201	2202	2205	rVB	341	291	0.04%	0.006%
90	14.548	2207	2208	2212	rVB	358	313	0.05%	0.006%
91	14.579	2212	2213	2215	rBV	276	201	0.03%	0.004%
92	14.615	2217	2219	2222	rBV	359	433	0.07%	0.008%
93	14.762	2241	2243	2244	rBV	393	252	0.04%	0.005%
94	14.969	2275	2277	2280	rBV2	276	325	0.05%	0.006%
95	15.054	2289	2291	2294	rBV3	206	287	0.04%	0.006%
96	15.530	2367	2369	2371	rBV2	279	221	0.03%	0.004%
97	15.573	2375	2376	2378	rBV2	229	180	0.03%	0.003%
98	16.030	2449	2451	2453	rBV2	279	296	0.05%	0.006%
99	16.072	2456	2458	2462	rBV3	375	542	0.08%	0.011%
100	16.261	2487	2489	2491	rBV2	316	266	0.04%	0.005%




Sum of corrected areas: 5160815

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121521\
Data File : VX025806.D
Acq On : 15 Dec 2021 10:44
Operator : JC/MD
Sample : VX1215WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK653

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

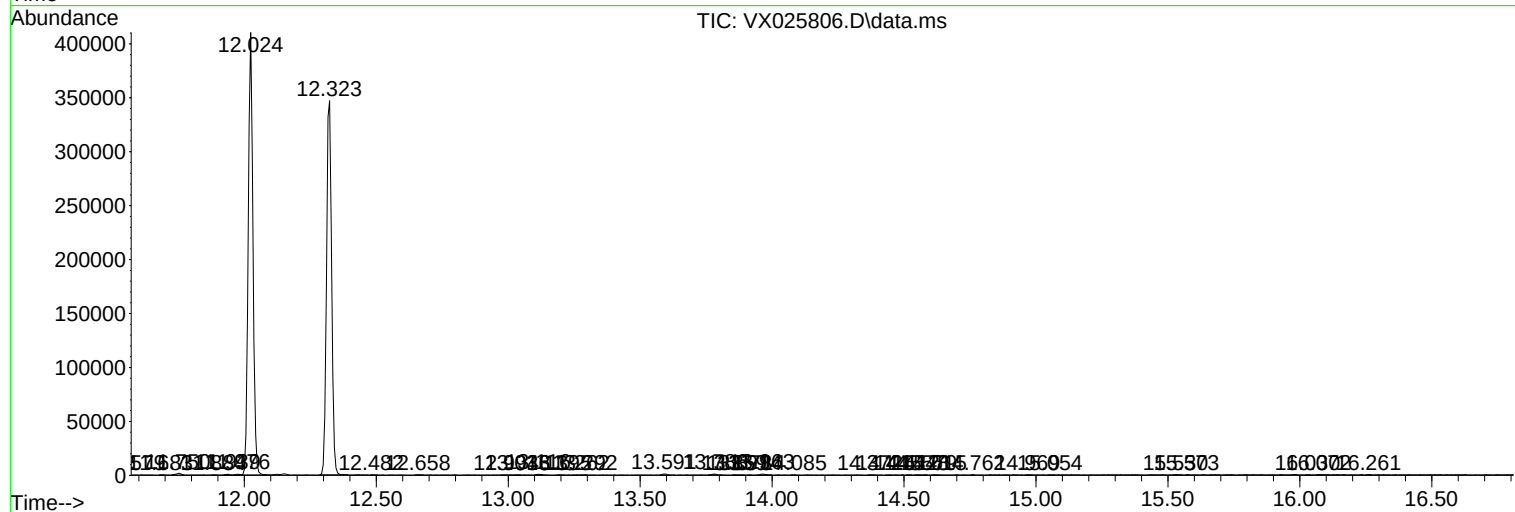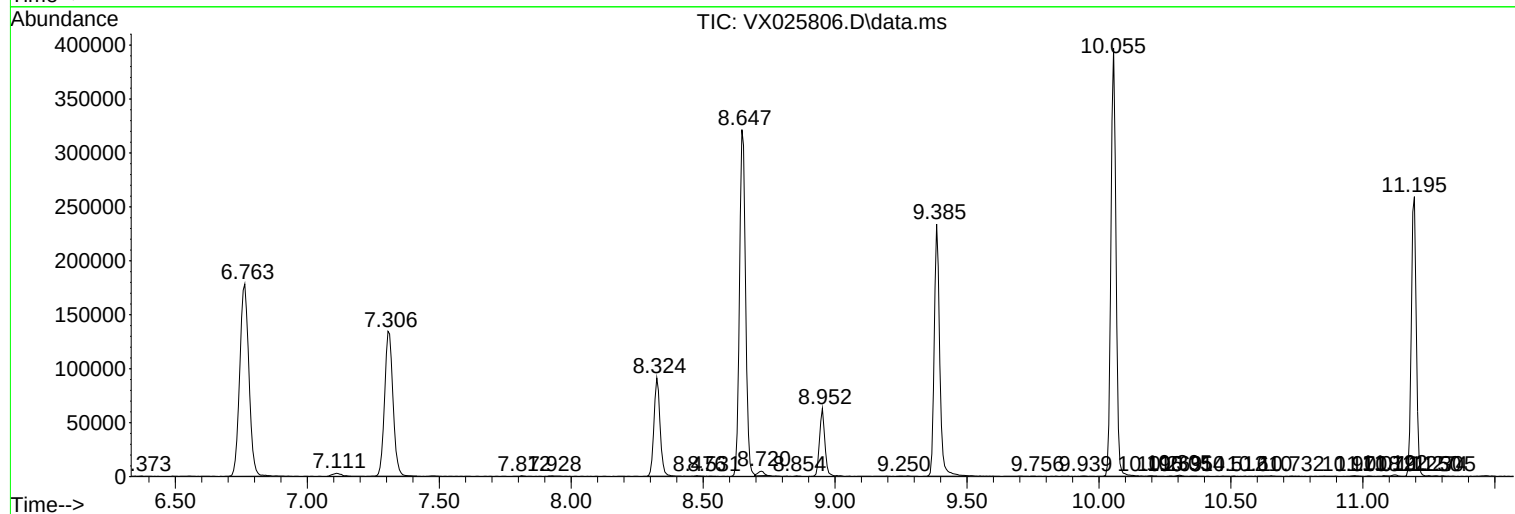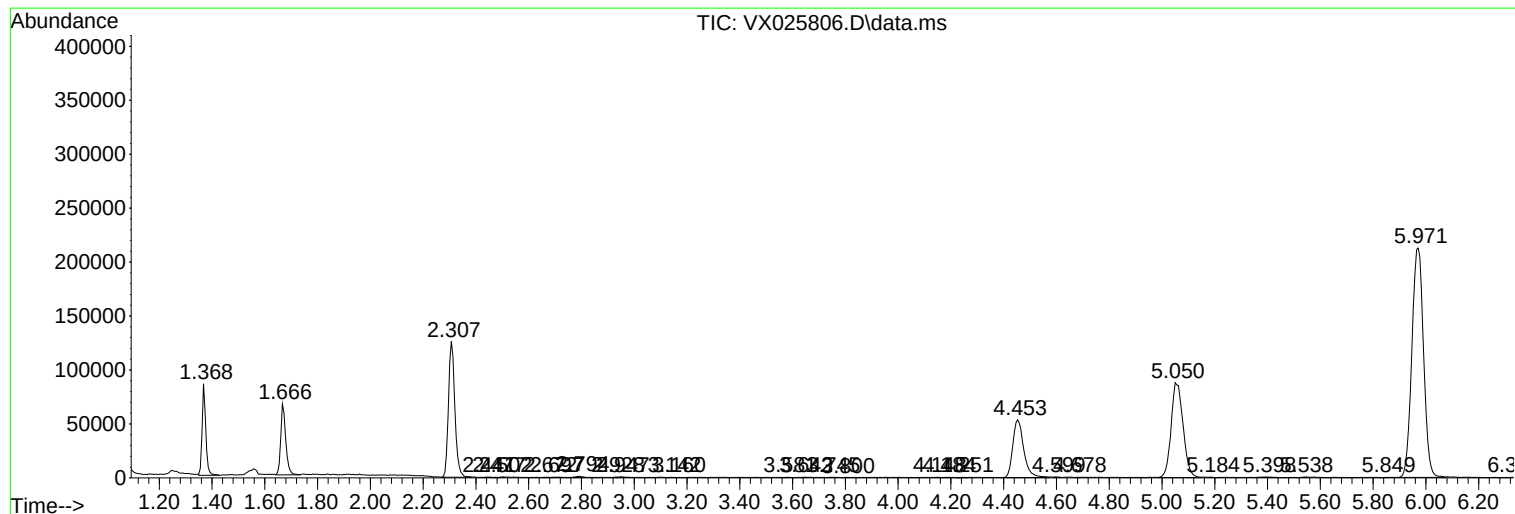

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121521\
Data File : VX025806.D
Acq On : 15 Dec 2021 10:44
Operator : JC/MD
Sample : VX1215WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK653

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121521\
Data File : VX025806.D
Acq On : 15 Dec 2021 10:44
Operator : JC/MD
Sample : VX1215WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK653

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc