

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121521\
 Data File : VX025807.D
 Acq On : 15 Dec 2021 11:09
 Operator : JC/MD
 Sample : M5026-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
 Title : VOC Analysis

Signal : TIC: VX025807.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	55	rVB	74722	76384	12.07%	1.529%
2	1.666	91	95	106	rVB	62493	81942	12.95%	1.640%
3	2.306	194	200	215	rVB	126118	202497	32.00%	4.053%
4	2.520	230	235	239	rBV3	506	877	0.14%	0.018%
5	2.660	256	258	261	rBV2	202	226	0.04%	0.005%
6	2.788	275	279	284	rVB3	1062	1517	0.24%	0.030%
7	2.947	297	305	315	rBV3	1375	3533	0.56%	0.071%
8	3.885	457	459	463	rBV2	167	248	0.04%	0.005%
9	4.062	486	488	490	rVB	258	215	0.03%	0.004%
10	4.129	497	499	502	rBV2	178	243	0.04%	0.005%
11	4.452	543	552	571	rBV	51915	152316	24.07%	3.048%
12	4.635	580	582	586	rVB	401	303	0.05%	0.006%
13	4.769	601	604	607	rBV2	169	199	0.03%	0.004%
14	5.062	638	652	668	rBV	85479	265697	41.98%	5.317%
15	5.190	671	673	674	rBV2	269	223	0.04%	0.004%
16	5.379	702	704	705	rBV2	352	246	0.04%	0.005%
17	5.538	725	730	732	rBV3	359	556	0.09%	0.011%
18	5.727	757	761	763	rBV2	210	274	0.04%	0.005%
19	5.970	788	801	816	rBV2	211622	632863	100.00%	12.665%
20	6.172	832	834	837	rVB2	319	304	0.05%	0.006%
21	6.251	844	847	849	rBV2	262	311	0.05%	0.006%
22	6.342	859	862	867	rVB	207	307	0.05%	0.006%
23	6.482	883	885	888	rBV2	147	228	0.04%	0.005%
24	6.550	892	896	899	rVB2	341	421	0.07%	0.008%
25	6.574	899	900	903	rBV	182	193	0.03%	0.004%
26	6.763	922	931	943	rBV	171217	409787	64.75%	8.201%
27	6.915	954	956	959	rVB2	443	292	0.05%	0.006%
28	6.946	959	961	967	rVB2	433	651	0.10%	0.013%
29	7.013	971	972	976	rBV2	209	259	0.04%	0.005%
30	7.117	982	989	996	rVB3	3251	6644	1.05%	0.133%
31	7.312	1012	1021	1033	rVV	134488	289007	45.67%	5.784%
32	7.409	1035	1037	1040	rVB	329	242	0.04%	0.005%
33	7.671	1079	1080	1084	rBV	139	194	0.03%	0.004%
34	7.805	1101	1102	1105	rVV2	343	226	0.04%	0.005%
35	7.927	1119	1122	1123	rBV2	434	337	0.05%	0.007%
36	8.110	1151	1152	1155	rVB2	296	212	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121521\
 Data File : VX025807.D
 Acq On : 15 Dec 2021 11:09
 Operator : JC/MD
 Sample : M5026-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

37	8.147	1155	1158	1161	rBV2	205	315	0.05%	0.006%
38	8.324	1181	1187	1200	rBV	83932	139929	22.11%	2.800%
39	8.452	1205	1208	1209	rBB	278	240	0.04%	0.005%
40	8.476	1209	1212	1218	rBV2	473	739	0.12%	0.015%
41	8.653	1233	1241	1248	rBV	313258	493538	77.98%	9.877%
42	8.720	1249	1252	1262	rVB2	4440	7761	1.23%	0.155%
43	8.872	1275	1277	1280	rVB2	185	195	0.03%	0.004%
44	8.952	1284	1290	1299	rVV	57897	84546	13.36%	1.692%
45	9.043	1303	1305	1308	rVB	271	211	0.03%	0.004%
46	9.067	1308	1309	1313	rBV2	185	195	0.03%	0.004%
47	9.147	1319	1322	1325	rVB2	306	338	0.05%	0.007%
48	9.171	1325	1326	1329	rBV	234	194	0.03%	0.004%
49	9.250	1336	1339	1340	rBV	194	198	0.03%	0.004%
50	9.281	1340	1344	1346	rBV3	151	195	0.03%	0.004%
51	9.384	1356	1361	1385	rBV	221850	324729	51.31%	6.499%
52	9.836	1432	1435	1437	rVB2	264	233	0.04%	0.005%
53	9.939	1450	1452	1457	rBV3	186	248	0.04%	0.005%
54	10.055	1465	1471	1487	rBV	389166	519020	82.01%	10.387%
55	10.305	1510	1512	1515	rVB2	629	645	0.10%	0.013%
56	10.579	1554	1557	1559	rBV2	247	306	0.05%	0.006%
57	10.646	1566	1568	1570	rBV3	274	293	0.05%	0.006%
58	10.768	1587	1588	1590	rBV2	212	201	0.03%	0.004%
59	10.841	1598	1600	1604	rBV2	169	196	0.03%	0.004%
60	10.915	1610	1612	1616	rVB2	206	252	0.04%	0.005%
61	11.079	1637	1639	1642	rVV3	338	350	0.06%	0.007%
62	11.122	1642	1646	1652	rVV3	1501	1847	0.29%	0.037%
63	11.195	1652	1658	1666	rBV	272890	339085	53.58%	6.786%
64	11.280	1670	1672	1676	rVB	312	297	0.05%	0.006%
65	11.360	1684	1685	1690	rBV2	210	237	0.04%	0.005%
66	11.408	1690	1693	1694	rVB	358	239	0.04%	0.005%
67	11.451	1697	1700	1702	rVB2	307	273	0.04%	0.005%
68	11.476	1702	1704	1709	rBV2	462	655	0.10%	0.013%
69	11.713	1741	1743	1745	rBV2	182	204	0.03%	0.004%
70	11.756	1746	1750	1754	rVB2	1269	1594	0.25%	0.032%
71	11.933	1776	1779	1784	rVB4	780	892	0.14%	0.018%
72	12.024	1788	1794	1804	rBV	392076	487667	77.06%	9.760%
73	12.116	1808	1809	1810	rBV	744	414	0.07%	0.008%
74	12.323	1837	1843	1850	rBV	346714	450036	71.11%	9.007%
75	12.475	1864	1868	1874	rVB2	254	463	0.07%	0.009%
76	12.664	1897	1899	1903	rVV	312	271	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121521\
 Data File : VX025807.D
 Acq On : 15 Dec 2021 11:09
 Operator : JC/MD
 Sample : M5026-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis

77	12.725	1907	1909	1911	rBV2	209	209	0.03%	0.004%
78	13.304	2003	2004	2007	rBV	288	270	0.04%	0.005%
79	13.359	2011	2013	2014	rBV	248	194	0.03%	0.004%
80	13.402	2017	2020	2021	rBV	234	202	0.03%	0.004%
81	13.426	2021	2024	2027	rVB3	266	370	0.06%	0.007%
82	13.573	2045	2048	2050	rVB	236	249	0.04%	0.005%
83	13.597	2050	2052	2054	rBV2	506	400	0.06%	0.008%
84	13.786	2079	2083	2088	rBV3	250	407	0.06%	0.008%
85	14.109	2133	2136	2137	rVV2	162	200	0.03%	0.004%
86	14.127	2137	2139	2142	rVB3	323	302	0.05%	0.006%
87	14.237	2154	2157	2163	rBV3	367	623	0.10%	0.012%
88	14.298	2165	2167	2171	rVB2	200	225	0.04%	0.005%
89	14.341	2171	2174	2179	rBV	241	396	0.06%	0.008%
90	14.457	2190	2193	2194	rBV2	301	336	0.05%	0.007%
91	14.883	2261	2263	2266	rBV2	198	206	0.03%	0.004%
92	14.932	2269	2271	2275	rVV2	187	226	0.04%	0.005%
93	15.066	2290	2293	2294	rBV	364	287	0.05%	0.006%
94	15.511	2364	2366	2370	rBV3	239	384	0.06%	0.008%
95	15.719	2397	2400	2403	rBV3	314	498	0.08%	0.010%
96	16.036	2450	2452	2455	rBV2	301	315	0.05%	0.006%
97	16.310	2495	2497	2500	rVB2	440	313	0.05%	0.006%
98	16.395	2509	2511	2512	rBV	288	213	0.03%	0.004%
99	16.432	2516	2517	2521	rVB2	360	378	0.06%	0.008%
100	16.572	2538	2540	2543	rBV2	270	342	0.05%	0.007%




Sum of corrected areas: 4996760

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121521\
Data File : VX025807.D
Acq On : 15 Dec 2021 11:09
Operator : JC/MD
Sample : M5026-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

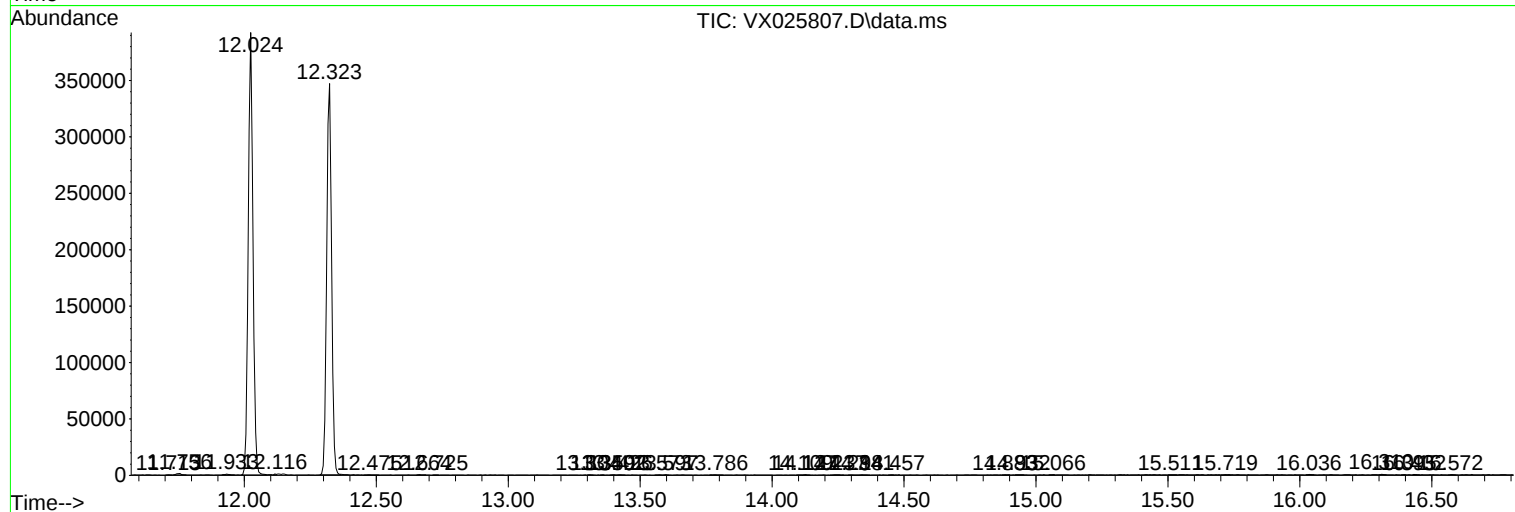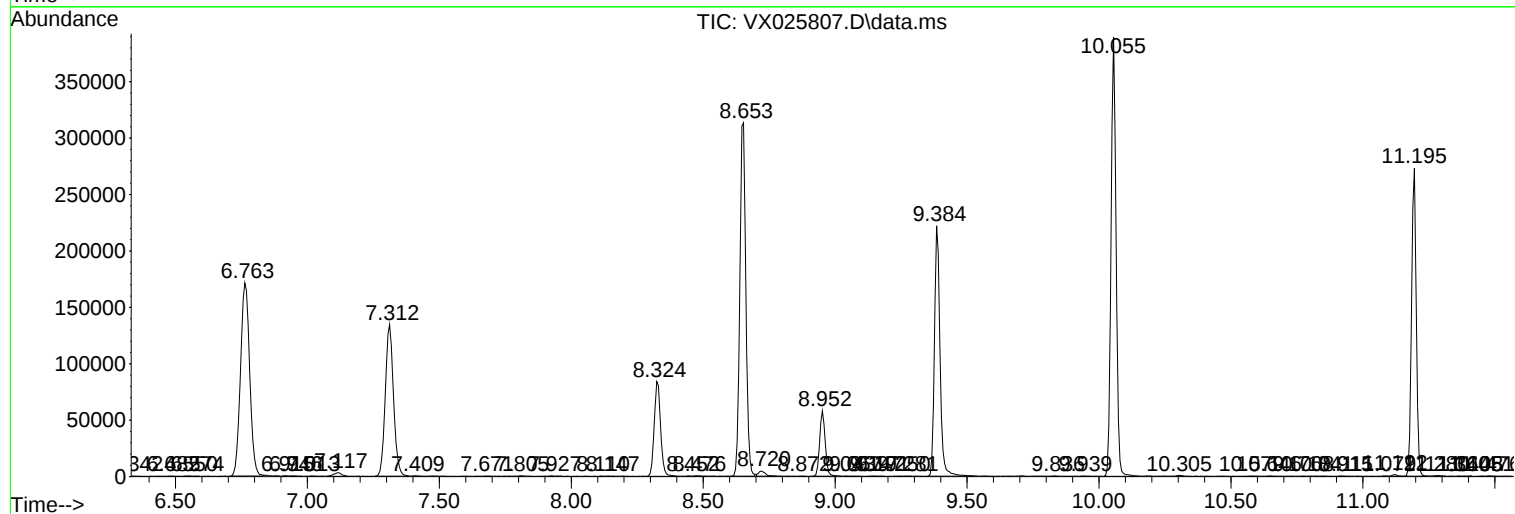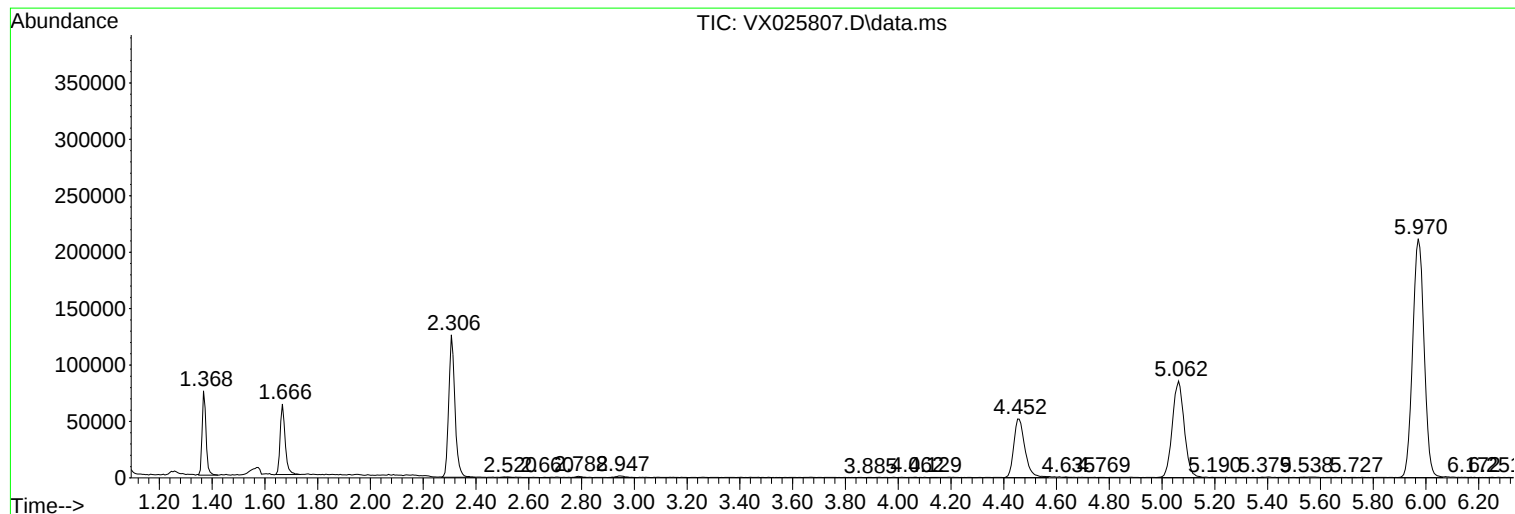

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121521\
Data File : VX025807.D
Acq On : 15 Dec 2021 11:09
Operator : JC/MD
Sample : M5026-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121521\
Data File : VX025807.D
Acq On : 15 Dec 2021 11:09
Operator : JC/MD
Sample : M5026-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML112221WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc