
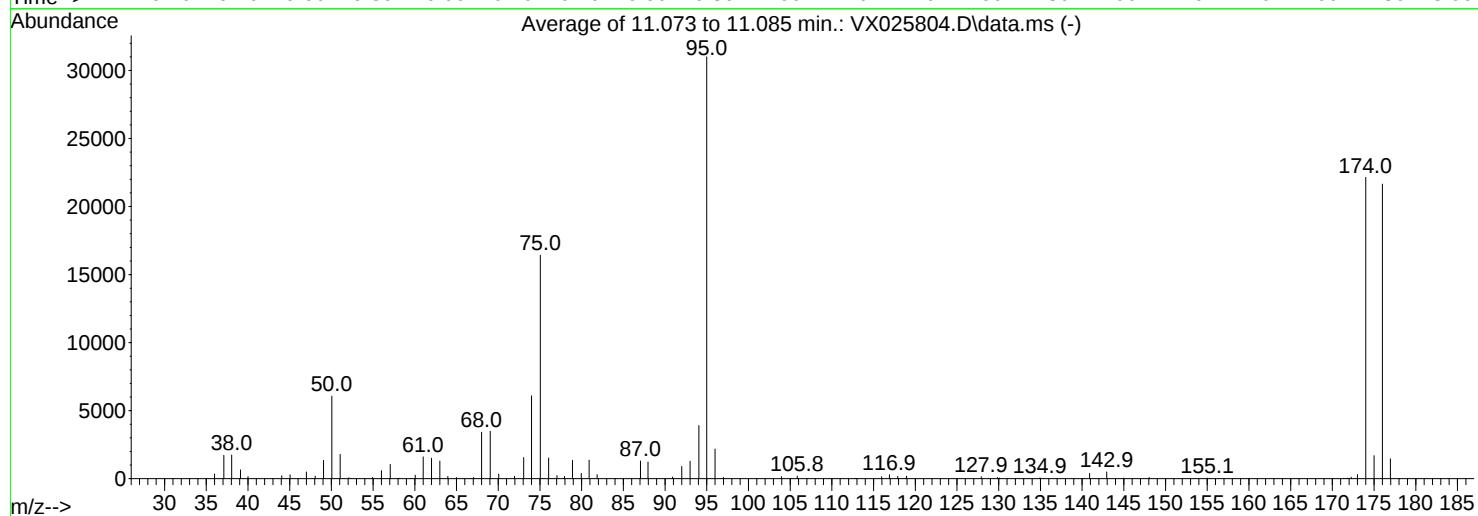


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121521\
 Data File : VX025804.D
 Acq On : 15 Dec 2021 09:30
 Operator : JC/MD
 Sample : BFB624
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB624

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM112221WMA.M
 Title : VOC Analysis
 Last Update : Thu Dec 16 00:37:00 2021

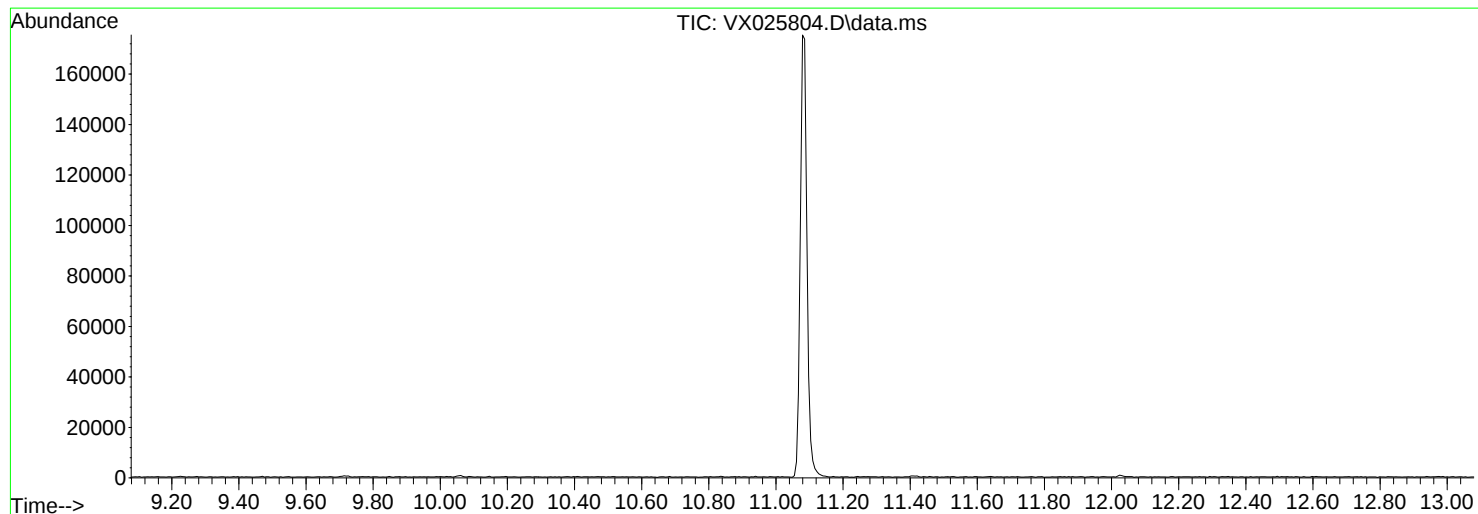

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	6073	PASS
75	95	30	80	53.0	16427	PASS
95	95	100	100	100.0	31003	PASS
96	95	5	9	7.0	2174	PASS
173	174	0.00	2	1.3	297	PASS
174	95	50	120	71.4	22140	PASS
175	174	5	9	7.6	1689	PASS
176	174	95	101	97.8	21655	PASS
177	176	5	9	6.7	1457	PASS

m/z	Abundance
40.00	207.0
44.10	140.0

Instrument :
MSVOA_X
ClientSampleId :
BFB624

m/z	Abundance
36.00	284.0
37.10	1309.0
38.10	1557.0
39.10	538.0
40.00	332.0
44.10	250.0
45.10	187.0
47.10	480.0
48.10	174.0
49.10	1056.0
50.00	4670.0
51.00	1403.0
52.20	53.0
55.00	66.0
56.00	462.0
57.00	891.0
60.00	220.0
61.00	1186.0
62.00	1134.0
63.00	951.0
64.00	118.0
66.70	61.0
67.10	61.0
68.00	2370.0
69.00	2548.0
70.00	195.0
72.00	82.0
73.10	1093.0
74.00	4200.0
75.00	12432.0
76.10	1199.0
77.00	197.0
78.00	115.0
78.90	881.0
79.90	305.0
80.90	983.0
81.90	270.0
87.10	864.0
88.00	896.0
90.90	88.0
92.00	578.0
93.00	983.0
94.00	2631.0
95.00	22056.0
96.00	1686.0
96.90	111.0
103.90	126.0
105.10	60.0
105.90	183.0
115.90	103.0
116.90	203.0
117.90	122.0
118.80	93.0
127.90	57.0
129.90	103.0
134.90	54.0
140.90	185.0
143.00	341.0
148.00	89.0
155.00	66.0
172.20	107.0
173.10	164.0
174.00	12988.0
175.00	1348.0
176.00	12309.0
176.90	781.0

Instrument :
MSVOA_X
ClientSampleId :
BFB624

m/z	Abundance
36.00	284.0
37.10	1895.0
38.00	1843.0
39.10	713.0
40.00	360.0
44.00	469.0
45.10	339.0
46.90	590.0
48.10	218.0
49.00	1568.0
50.10	6896.0
51.10	2087.0
52.10	108.0
55.00	106.0
56.00	720.0
57.10	1081.0
58.10	101.0
60.10	258.0
61.00	1998.0
62.00	1764.0
63.00	1465.0
64.00	214.0
65.00	156.0
67.00	151.0
68.00	4375.0
69.10	4161.0
70.10	395.0
71.90	230.0
73.00	1784.0
74.00	7571.0
75.00	18992.0
76.00	1560.0
77.10	183.0
77.80	101.0
78.10	93.0
78.90	1651.0
79.90	545.0
80.90	1688.0
81.80	266.0
87.10	1330.0
87.90	1423.0
90.90	168.0
92.00	931.0
93.00	1385.0
94.00	4701.0
95.00	36296.0
96.00	2521.0
97.00	87.0
103.90	221.0
105.80	173.0
116.00	207.0
116.90	304.0
117.80	259.0
119.00	295.0
127.90	183.0
130.10	155.0
135.00	73.0
140.90	456.0
142.80	458.0
145.00	87.0
146.10	84.0
148.10	89.0
155.10	54.0
171.40	69.0
172.30	204.0
173.10	341.0
174.00	25024.0
175.00	1753.0
176.00	25288.0
177.00	1882.0

Instrument :
MSVOA_X
ClientSampleId :
BFB624

m/z	Abundance
36.00	440.0
37.10	1960.0
38.10	1834.0
39.10	678.0
40.00	407.0
44.10	328.0
45.00	311.0
47.00	402.0
47.90	172.0
49.00	1408.0
50.10	6653.0
51.10	1874.0
52.00	54.0
54.90	107.0
56.00	578.0
57.00	1162.0
60.00	295.0
61.00	1607.0
62.00	1625.0
63.00	1463.0
63.90	147.0
65.00	77.0
67.00	86.0
68.00	3504.0
69.00	3737.0
70.10	425.0
72.00	212.0
73.00	1795.0
74.00	6492.0
75.10	17856.0
76.00	1792.0
77.00	298.0
77.90	178.0
78.90	1527.0
80.00	329.0
80.90	1425.0
81.90	333.0
87.00	1693.0
87.90	1368.0
90.90	83.0
92.00	1164.0
93.00	1476.0
94.10	4378.0
95.00	34656.0
96.00	2315.0
97.10	83.0
104.00	129.0
105.90	218.0
112.80	85.0
116.00	111.0
116.90	334.0
118.00	149.0
118.90	275.0
127.90	173.0
128.80	57.0
129.80	150.0
135.00	50.0
140.20	55.0
140.90	527.0
143.00	678.0
145.00	56.0
148.10	53.0
171.80	111.0
172.90	387.0
174.00	28408.0
175.00	1965.0
176.00	27368.0
177.00	1707.0

Instrument :
MSVOA_X
ClientSampleId :
BFB624