

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121522\
 Data File : VX033435.D
 Acq On : 15 Dec 2022 12:32
 Operator : JC/MD
 Sample : N6070-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GW-BR-04-226-245-121422

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M

Title : SW846 8260

Signal : TIC: VX033435.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.489	550	558	570	rBV	14007	37512	1.21%	0.677%
2	5.385	693	705	719	rBV	35044	100451	3.24%	1.812%
3	5.550	721	732	749	rBV	86642	247621	7.99%	4.467%
4	5.958	789	799	811	rBV2	36215	96038	3.10%	1.733%
5	6.763	922	931	948	rBV	176816	420305	13.56%	7.582%
6	7.129	983	991	1002	rVB2	16720	36598	1.18%	0.660%
7	8.647	1234	1240	1246	rBV	139145	221487	7.15%	3.996%
8	8.720	1246	1252	1268	rVB	2088753	3099447	100.00%	55.915%
9	10.055	1465	1471	1487	rVB	371374	493225	15.91%	8.898%
10	11.079	1634	1639	1647	rBV	251869	321314	10.37%	5.797%
11	12.024	1788	1794	1803	rBV	377133	469127	15.14%	8.463%




Sum of corrected areas: 5543125

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121522\
Data File : VX033435.D
Acq On : 15 Dec 2022 12:32
Operator : JC/MD
Sample : N6070-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GW-BR-04-226-245-121422

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

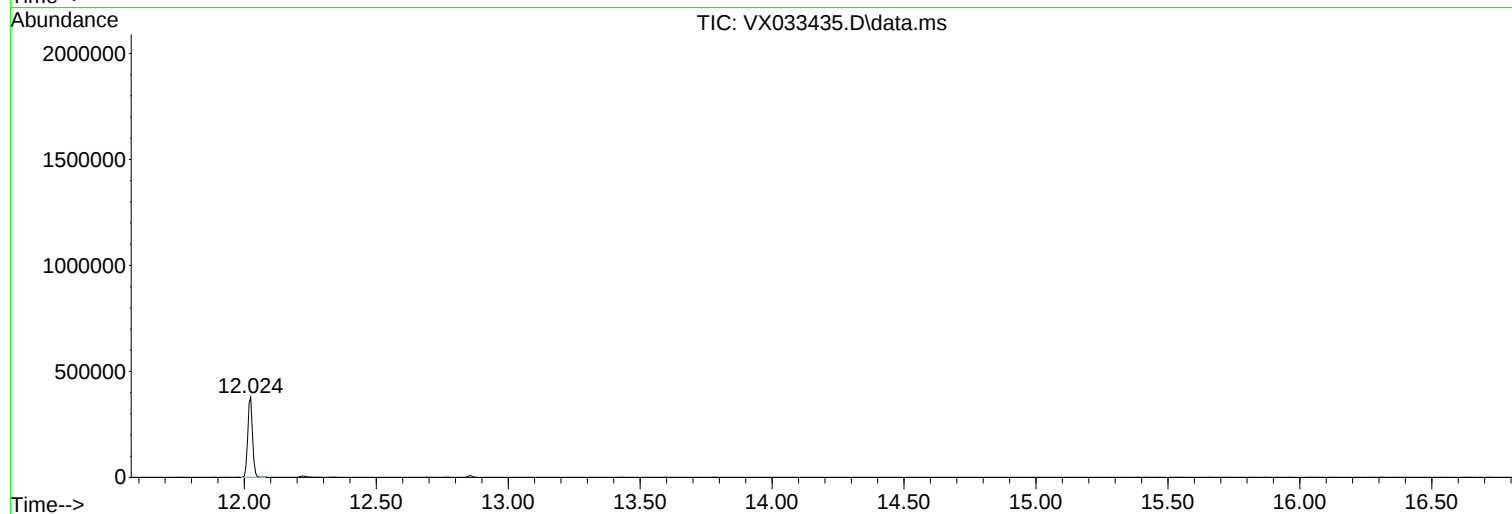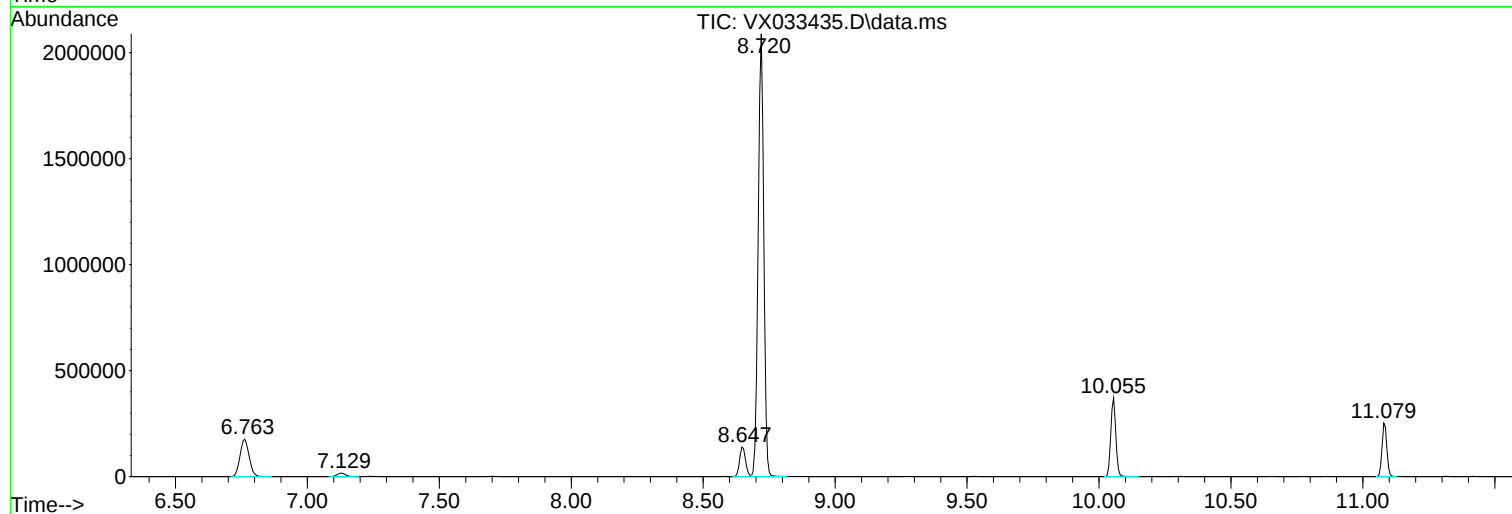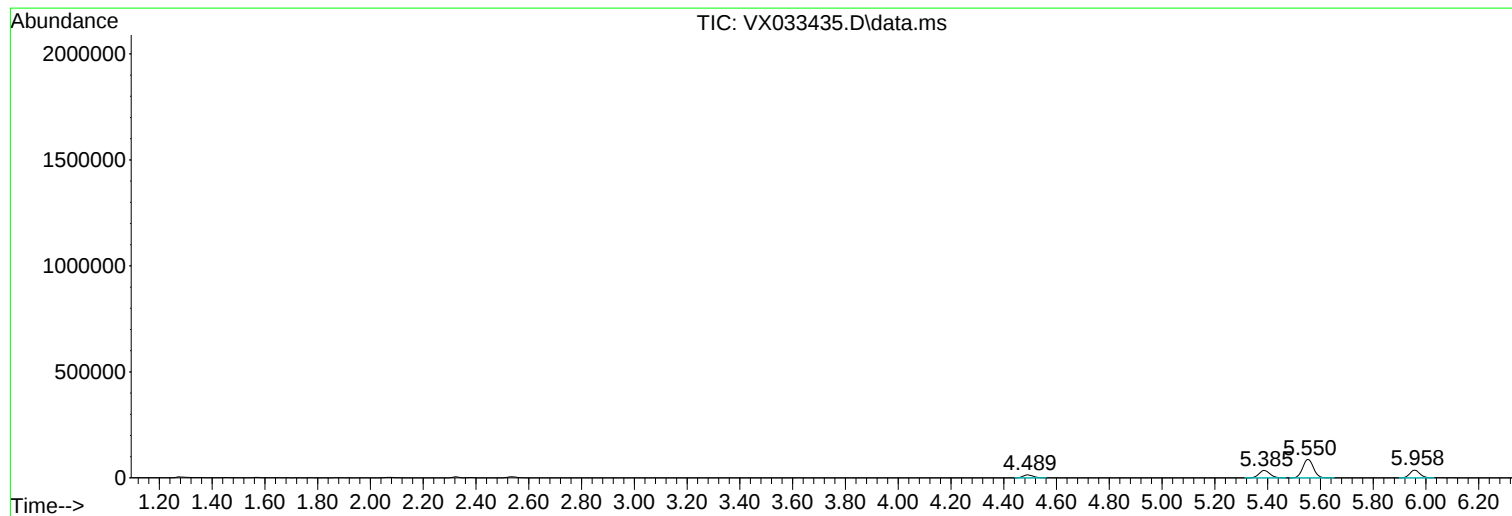

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121522\
Data File : VX033435.D
Acq On : 15 Dec 2022 12:32
Operator : JC/MD
Sample : N6070-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GW-BR-04-226-245-121422

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121522\
Data File : VX033435.D
Acq On : 15 Dec 2022 12:32
Operator : JC/MD
Sample : N6070-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GW-BR-04-226-245-121422

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc