

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121522\
Data File : VX033438.D
Acq On : 15 Dec 2022 13:41
Operator : JC/MD
Sample : N6070-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
OWBR-03-128-148-121422

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Title : SW846 8260

Signal : TIC: VX033438.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.276	28	31	39	rBV	4617	8377	1.72%	0.325%
2	5.093	646	657	670	rBV3	2488	7983	1.64%	0.310%
3	5.385	693	705	721	rBV	46946	134824	27.72%	5.238%
4	5.556	721	733	749	rVB	120184	344080	70.74%	13.369%
5	5.958	789	799	808	rBV	35598	95235	19.58%	3.700%
6	6.037	808	812	822	rVB3	5998	15166	3.12%	0.589%
7	6.763	920	931	947	rBV	180976	424578	87.29%	16.496%
8	8.647	1234	1240	1248	rBV	135306	214527	44.10%	8.335%
9	10.055	1465	1471	1483	rBV	357445	486422	100.00%	18.899%
10	11.079	1634	1639	1654	rBV	235657	309451	63.62%	12.023%
11	12.024	1788	1794	1802	rBV	355144	454975	93.54%	17.677%
12	12.244	1822	1830	1838	rBV	52646	78163	16.07%	3.037%




Sum of corrected areas: 2573781

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121522\
Data File : VX033438.D
Acq On : 15 Dec 2022 13:41
Operator : JC/MD
Sample : N6070-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
OWBR-03-128-148-121422

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

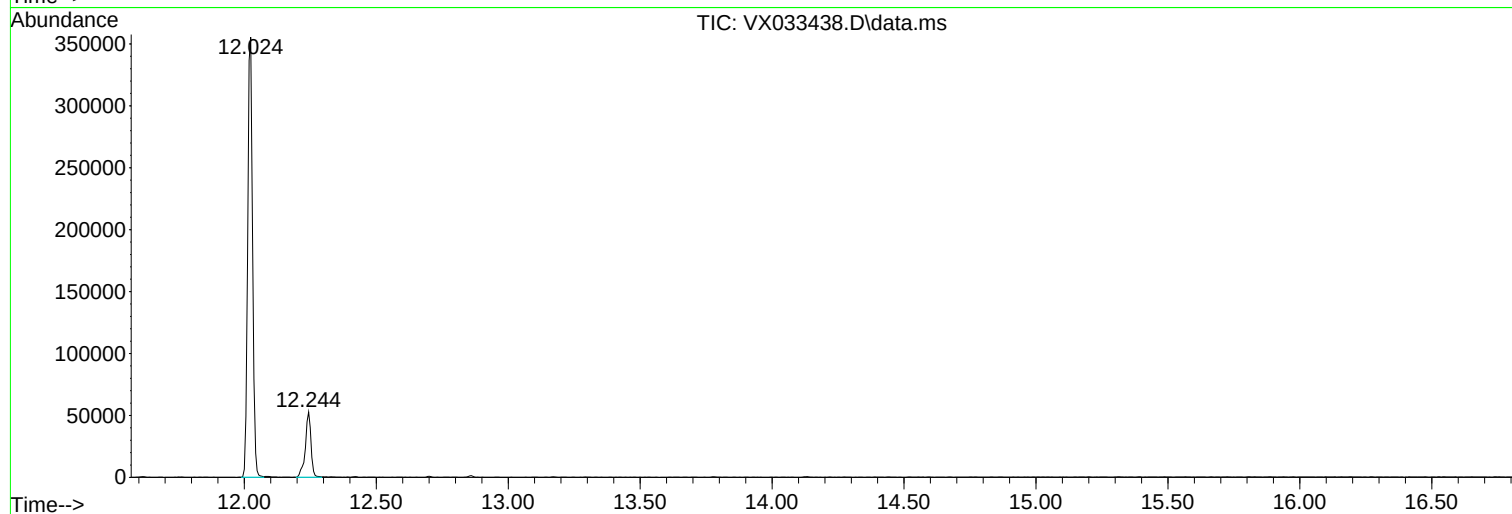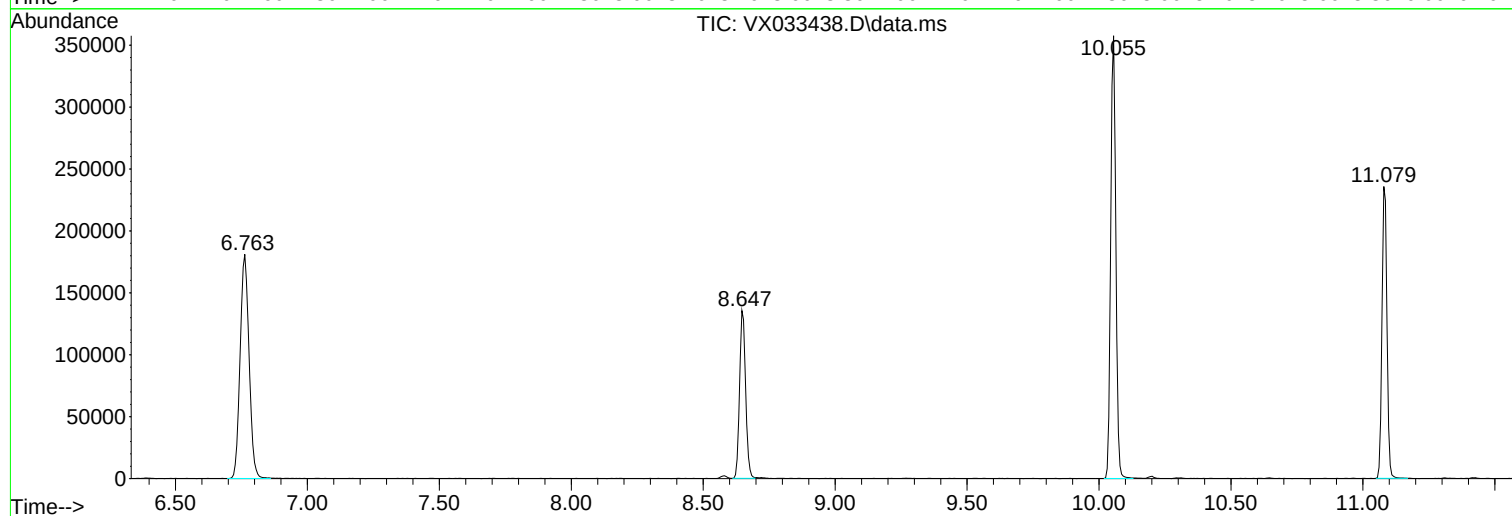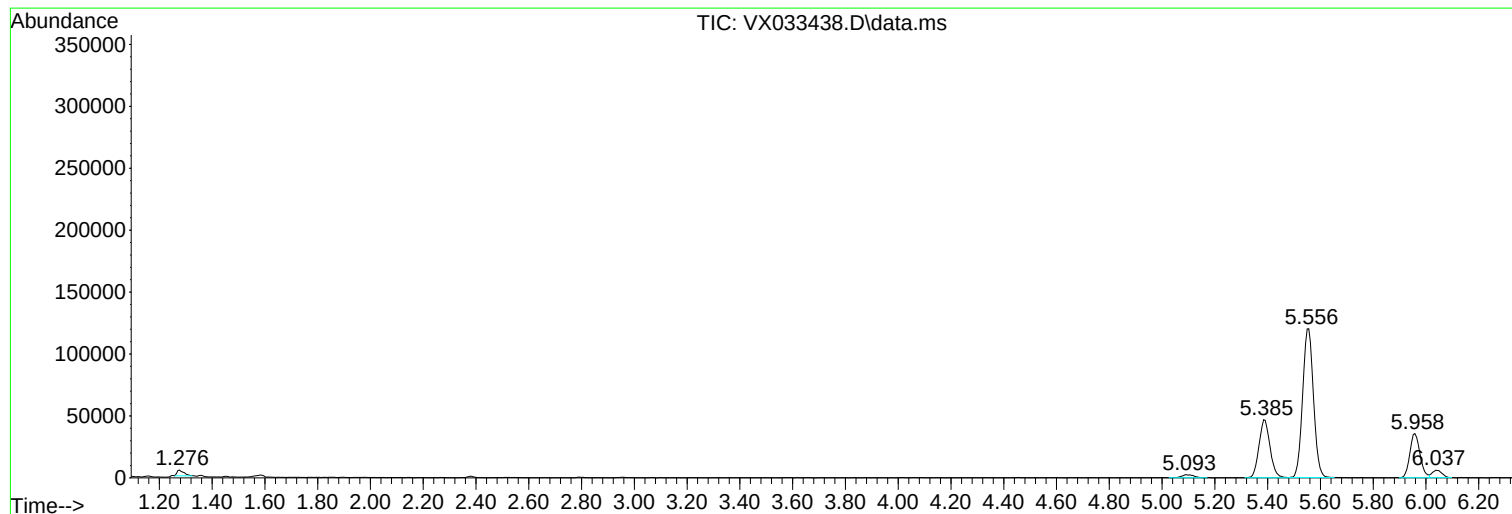

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121522\
Data File : VX033438.D
Acq On : 15 Dec 2022 13:41
Operator : JC/MD
Sample : N6070-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
OWBR-03-128-148-121422










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Indane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.244	8.59 ug/l	78163	1,4-Dichlorobenzene-d4	12.024

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Indane	118	C9H10	000496-11-7	94
2			Benzene, cyclopropyl-	118	C9H10	000873-49-4	81
3			Tetracyclo[3.3.1.0(2,8).0(4,6)]-...	118	C9H10	1000191-13-7	72
4			7-Methylenecycloocta-1,3,5-triene	118	C9H10	002570-13-0	72
5			Deltacyclene	118	C9H10	007785-10-6	64

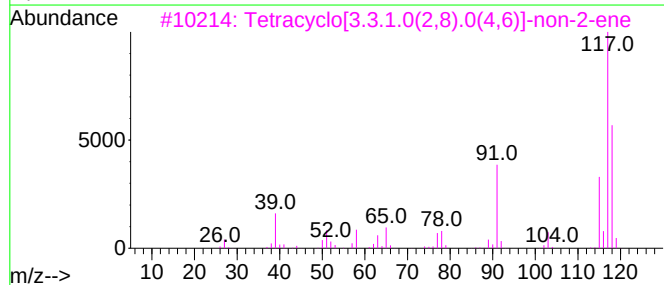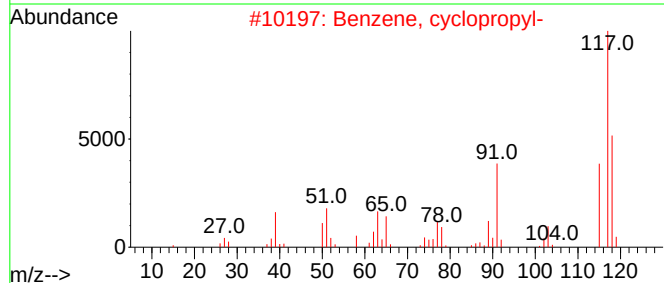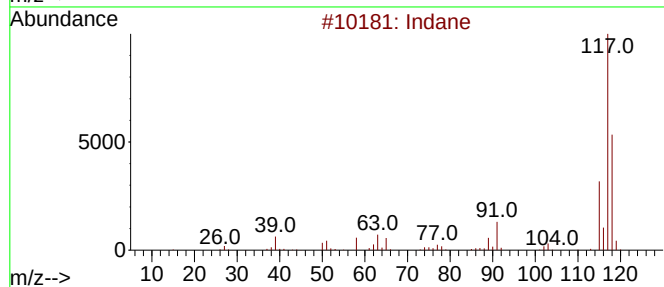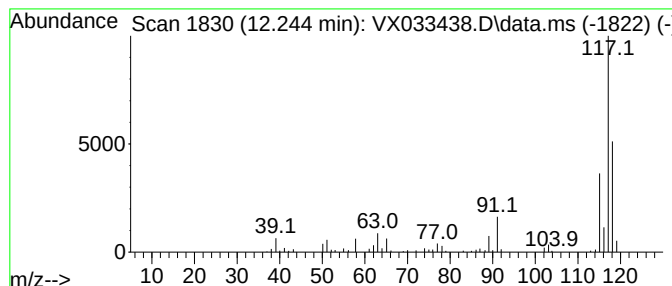

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121522\
Data File : VX033438.D
Acq On : 15 Dec 2022 13:41
Operator : JC/MD
Sample : N6070-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
OWBR-03-128-148-121422

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Indane	12.244	8.6	ug/l	78163	4	12.024	454975	50.0