

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121522\
 Data File : VX033441.D
 Acq On : 15 Dec 2022 14:50
 Operator : JC/MD
 Sample : N6070-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GW-BR-04-226-245-121422

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M

Title : SW846 8260

Signal : TIC: VX033441.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.489	549	558	570	rBV	18443	50271	1.68%	0.910%
2	5.385	693	705	721	rBV	45866	135096	4.52%	2.445%
3	5.550	721	732	751	rVB	117926	334707	11.19%	6.059%
4	5.958	789	799	809	rBV2	34892	93355	3.12%	1.690%
5	6.763	921	931	946	rBV	174848	414600	13.87%	7.505%
6	7.122	984	990	1002	rBV2	15076	34625	1.16%	0.627%
7	8.653	1234	1241	1246	rBV	133216	213381	7.14%	3.862%
8	8.720	1246	1252	1273	rVB	1941985	2989912	100.00%	54.120%
9	10.055	1465	1471	1481	rBV	356999	482963	16.15%	8.742%
10	11.079	1634	1639	1652	rBV	244277	315753	10.56%	5.715%
11	12.024	1788	1794	1806	rBV	380079	459891	15.38%	8.324%




Sum of corrected areas: 5524554

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121522\
Data File : VX033441.D
Acq On : 15 Dec 2022 14:50
Operator : JC/MD
Sample : N6070-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GW-BR-04-226-245-121422

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

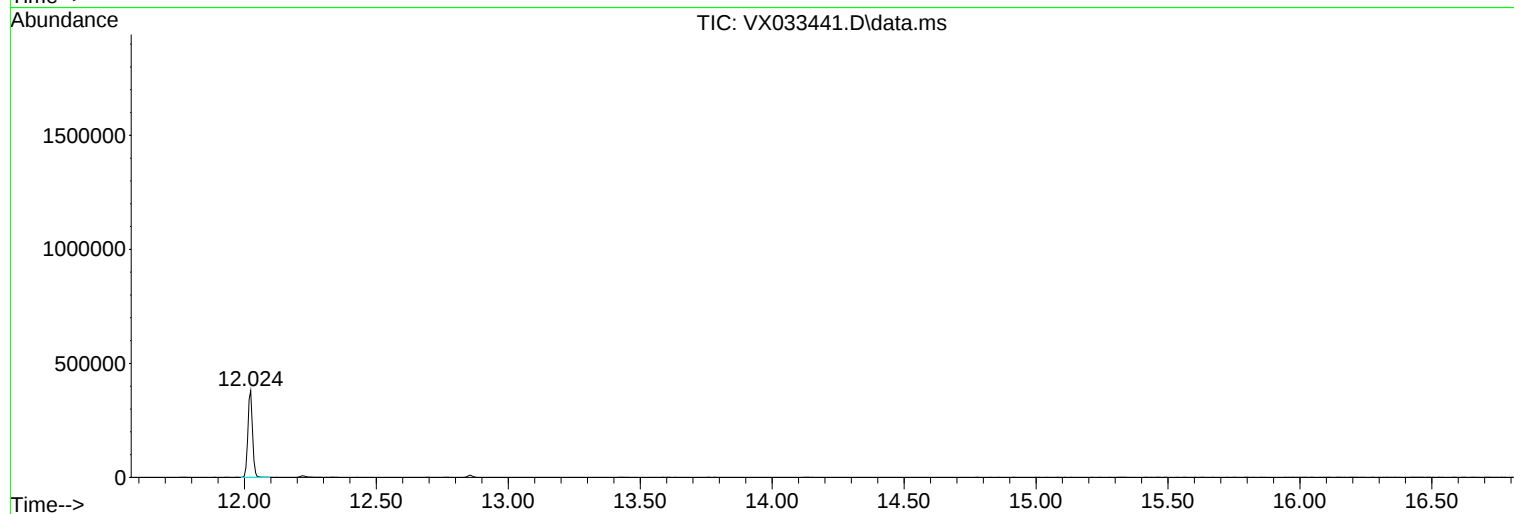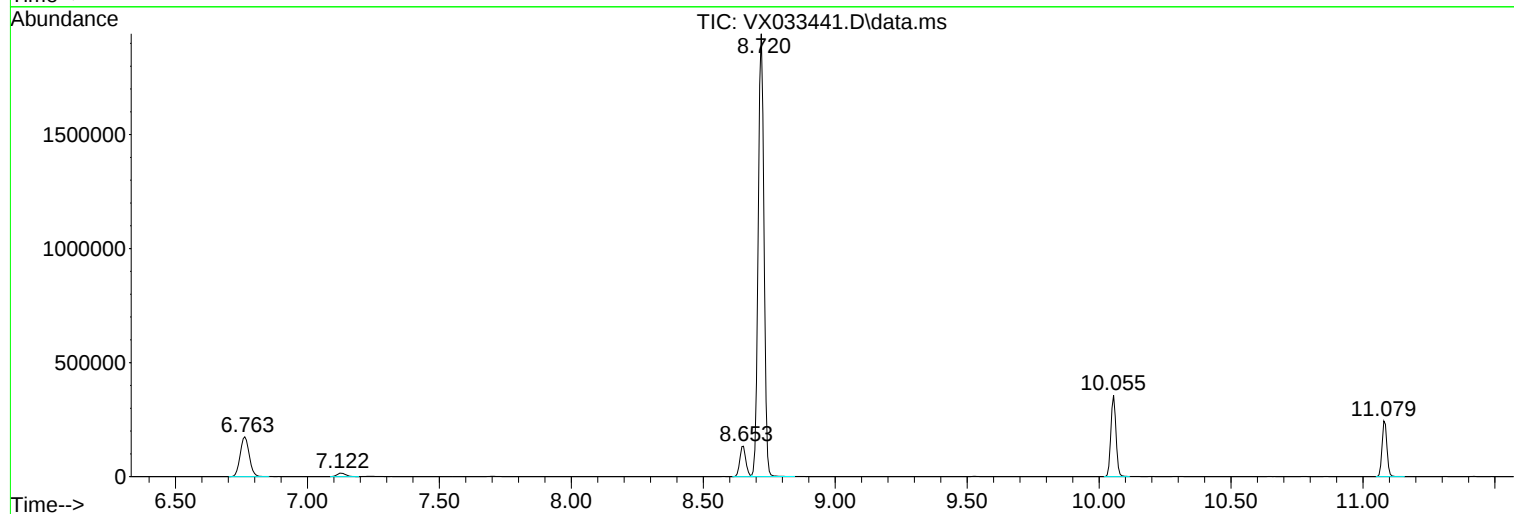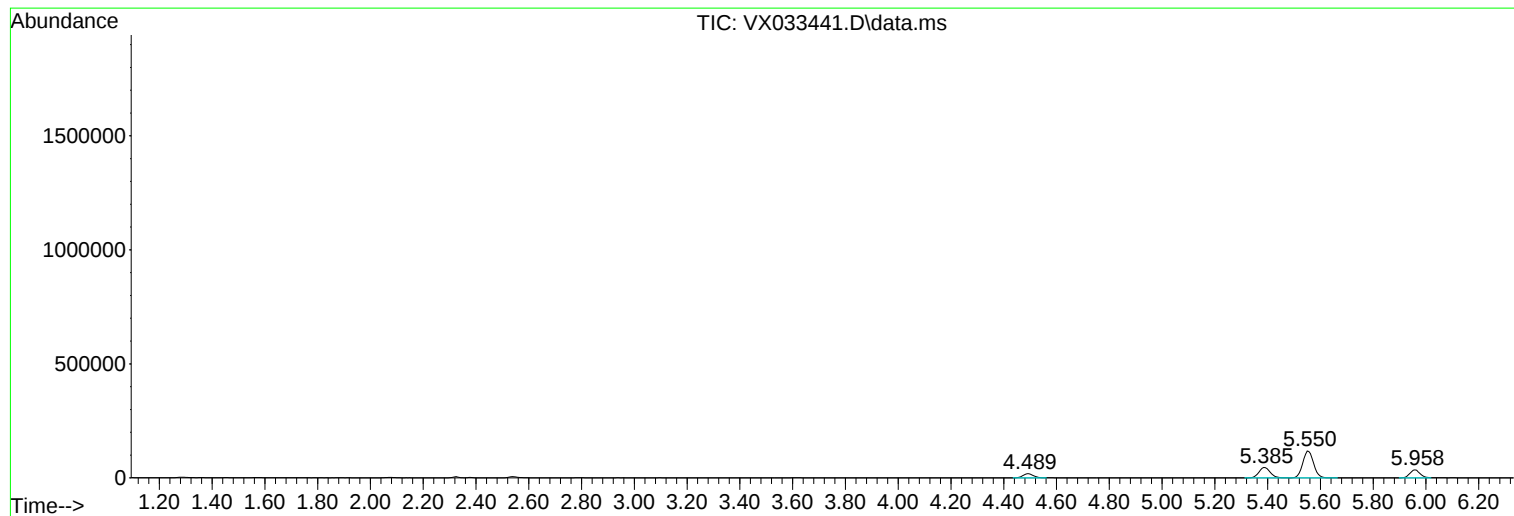

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121522\
Data File : VX033441.D
Acq On : 15 Dec 2022 14:50
Operator : JC/MD
Sample : N6070-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GW-BR-04-226-245-121422

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121522\
Data File : VX033441.D
Acq On : 15 Dec 2022 14:50
Operator : JC/MD
Sample : N6070-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GW-BR-04-226-245-121422

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc