
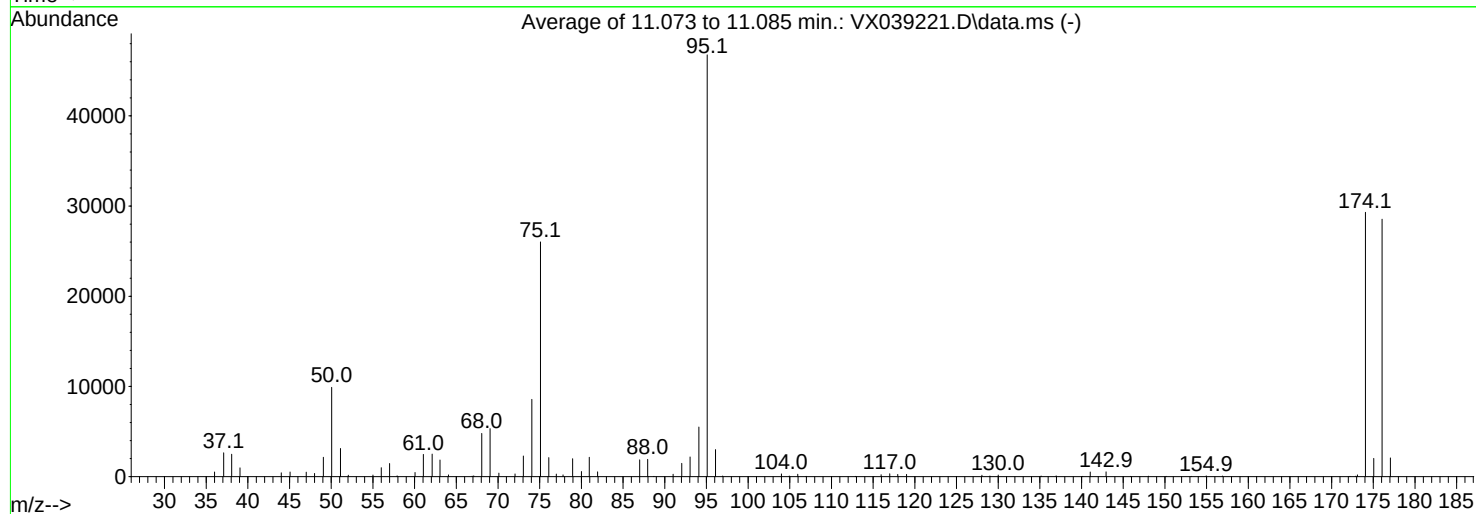


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121523\
Data File : VX039221.D
Acq On : 15 Dec 2023 08:51
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X112423W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Mon Nov 27 03:22:25 2023

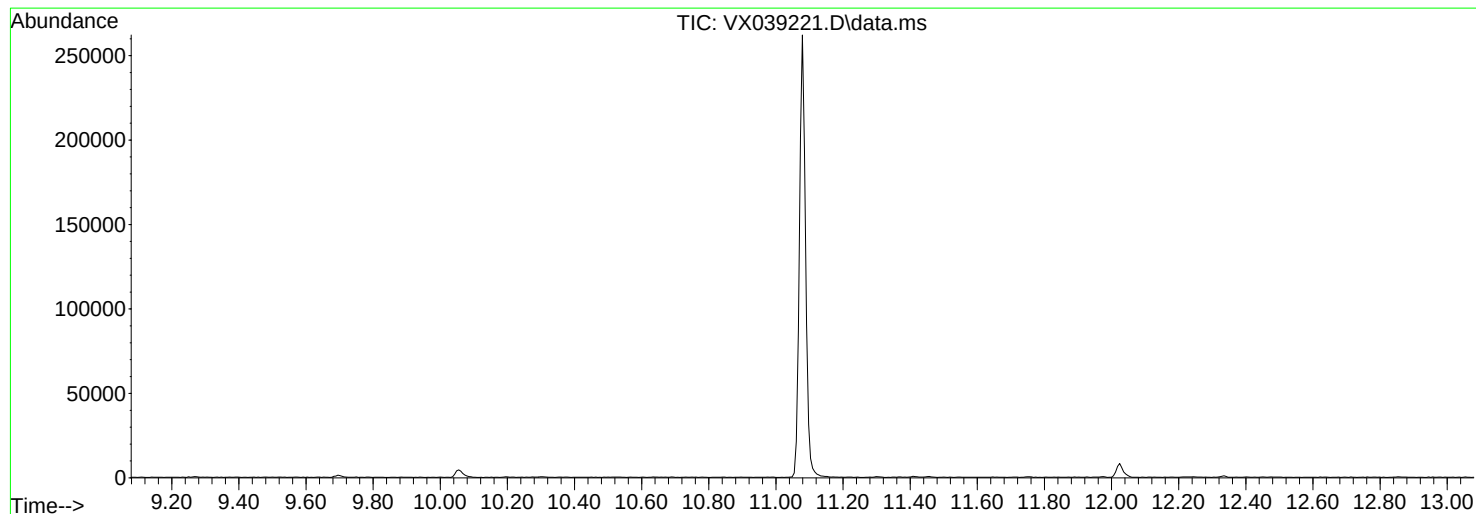

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.2	9905	PASS
75	95	30	60	55.6	26019	PASS
95	95	100	100	100.0	46768	PASS
96	95	5	9	6.4	3003	PASS
173	174	0.00	2	0.7	202	PASS
174	95	50	100	62.7	29301	PASS
175	174	5	9	6.9	2020	PASS
176	174	95	101	97.4	28547	PASS
177	176	5	9	7.3	2085	PASS