

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX121619\  
 Data File : VX014036.D  
 Acq On : 16 Dec 2019 15:37  
 Operator : JC/SP  
 Sample : K6252-13  
 Misc : 5.0mL/MSVOA X/WATER  
 ALS Vial : 15 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 RE135D3-20191210

Quant Time: Dec 17 03:29:33 2019  
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X121319W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue Dec 17 03:01:07 2019  
 Response via : Initial Calibration

| Internal Standards         | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|----------------------------|-------|------|----------|-------|-------|----------|
| 1) Pentafluorobenzene      | 5.65  | 168  | 577650   | 50.00 | ug/l  | 0.00     |
| 34) 1,4-Difluorobenzene    | 6.85  | 114  | 886771   | 50.00 | ug/l  | 0.00     |
| 63) Chlorobenzene-d5       | 10.11 | 117  | 788331   | 50.00 | ug/l  | 0.00     |
| 72) 1,4-Dichlorobenzene-d4 | 12.07 | 152  | 341237   | 50.00 | ug/l  | 0.00     |

| System Monitoring Compounds | R.T.  | QIon | Response | Conc  | Units   | Dev(Min) |
|-----------------------------|-------|------|----------|-------|---------|----------|
| 33) 1,2-Dichloroethane-d4   | 6.05  | 65   | 321057   | 49.04 | ug/l    | 0.00     |
| Spiked Amount               |       |      | Recovery | =     | 98.08%  |          |
| 35) Dibromofluoromethane    | 5.49  | 113  | 270133   | 50.11 | ug/l    | 0.00     |
| Spiked Amount               |       |      | Recovery | =     | 100.22% |          |
| 50) Toluene-d8              | 8.71  | 98   | 1053133  | 50.18 | ug/l    | 0.00     |
| Spiked Amount               |       |      | Recovery | =     | 100.36% |          |
| 62) 4-Bromofluorobenzene    | 11.14 | 95   | 348325   | 45.40 | ug/l    | 0.00     |
| Spiked Amount               |       |      | Recovery | =     | 90.80%  |          |


| Target Compounds               | R.T.  | QIon | Response | Conc   | Units  | Qvalue |
|--------------------------------|-------|------|----------|--------|--------|--------|
| 3) Chloromethane               | 1.32  | 50   | 1709     | 0.246  | ug/l # | 42     |
| 6) Chloroethane                | 1.60  | 64   | 2778     | 0.615  | ug/l   | 94     |
| 9) 1,1,2-Trichlorotrifluoroet  | 2.38  | 101  | 21776    | 3.988  | ug/l   | 97     |
| 10) Methyl Iodide              | 2.49  | 142  | 71       | 2.630  | ug/l # | 1      |
| 11) Tert butyl alcohol         | 3.02  | 59   | 2320     | 1.640  | ug/l   | 100    |
| 12) 1,1-Dichloroethene         | 2.37  | 96   | 3294     | 0.593  | ug/l   | 82     |
| 13) Acrolein                   | 2.29  | 56   | 612      | 0.756  | ug/l   | 96     |
| 16) Acetone                    | 2.43  | 43   | 8772     | 2.064  | ug/l   | 89     |
| 17) Carbon Disulfide           | 2.55  | 76   | 1462     | 0.844  | ug/l # | 45     |
| 20) Methylene Chloride         | 2.84  | 84   | 2191     | 0.327  | ug/l # | 60     |
| 24) 1,1-Dichloroethane         | 3.70  | 63   | 3897     | 0.354  | ug/l # | 77     |
| 27) cis-1,2-Dichloroethene     | 4.58  | 96   | 22305    | 3.222  | ug/l   | 84     |
| 28) Bromochloromethane         | 5.02  | 49   | 668      | 0.610  | ug/l # | 57     |
| 32) 1,1,1-Trichloroethane      | 5.49  | 97   | 1840     | 0.207  | ug/l # | 23     |
| 36) 1,1-Dichloropropene        | 5.65  | 75   | 39581    | 4.865  | ug/l # | 51     |
| 38) Carbon Tetrachloride       | 5.65  | 117  | 51747    | 6.981  | ug/l # | 17     |
| 44) Trichloroethene            | 7.20  | 130  | 81990    | 11.857 | ug/l   | 99     |
| 45) 1,2-Dichloropropane        | 7.51  | 63   | 19761    | 3.080  | ug/l   | 93     |
| 49) 1,4-Dioxane                | 7.74  | 88   | 128      | 0.864  | ug/l # | 1      |
| 60) Dibromochloromethane       | 9.33  | 129  | 61586    | 9.769  | ug/l # | 12     |
| 64) Tetrachloroethene          | 9.33  | 164  | 69375    | 9.945  | ug/l   | 96     |
| 76) 1,2,3-Trichloropropane     | 11.13 | 75   | 171384   | 23.134 | ug/l # | 39     |
| 81) trans-1,4-Dichloro-2-buten | 11.13 | 75   | 171384   | 65.297 | ug/l # | 12     |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX121619\  
Data File : VX014036.D  
Acq On : 16 Dec 2019 15:37  
Operator : JC/SP  
Sample : K6252-13  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
RE135D3-20191210

Quant Time: Dec 17 03:29:33 2019  
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X121319W.M  
Quant Title : SW846 8260  
QLast Update : Tue Dec 17 03:01:07 2019  
Response via : Initial Calibration

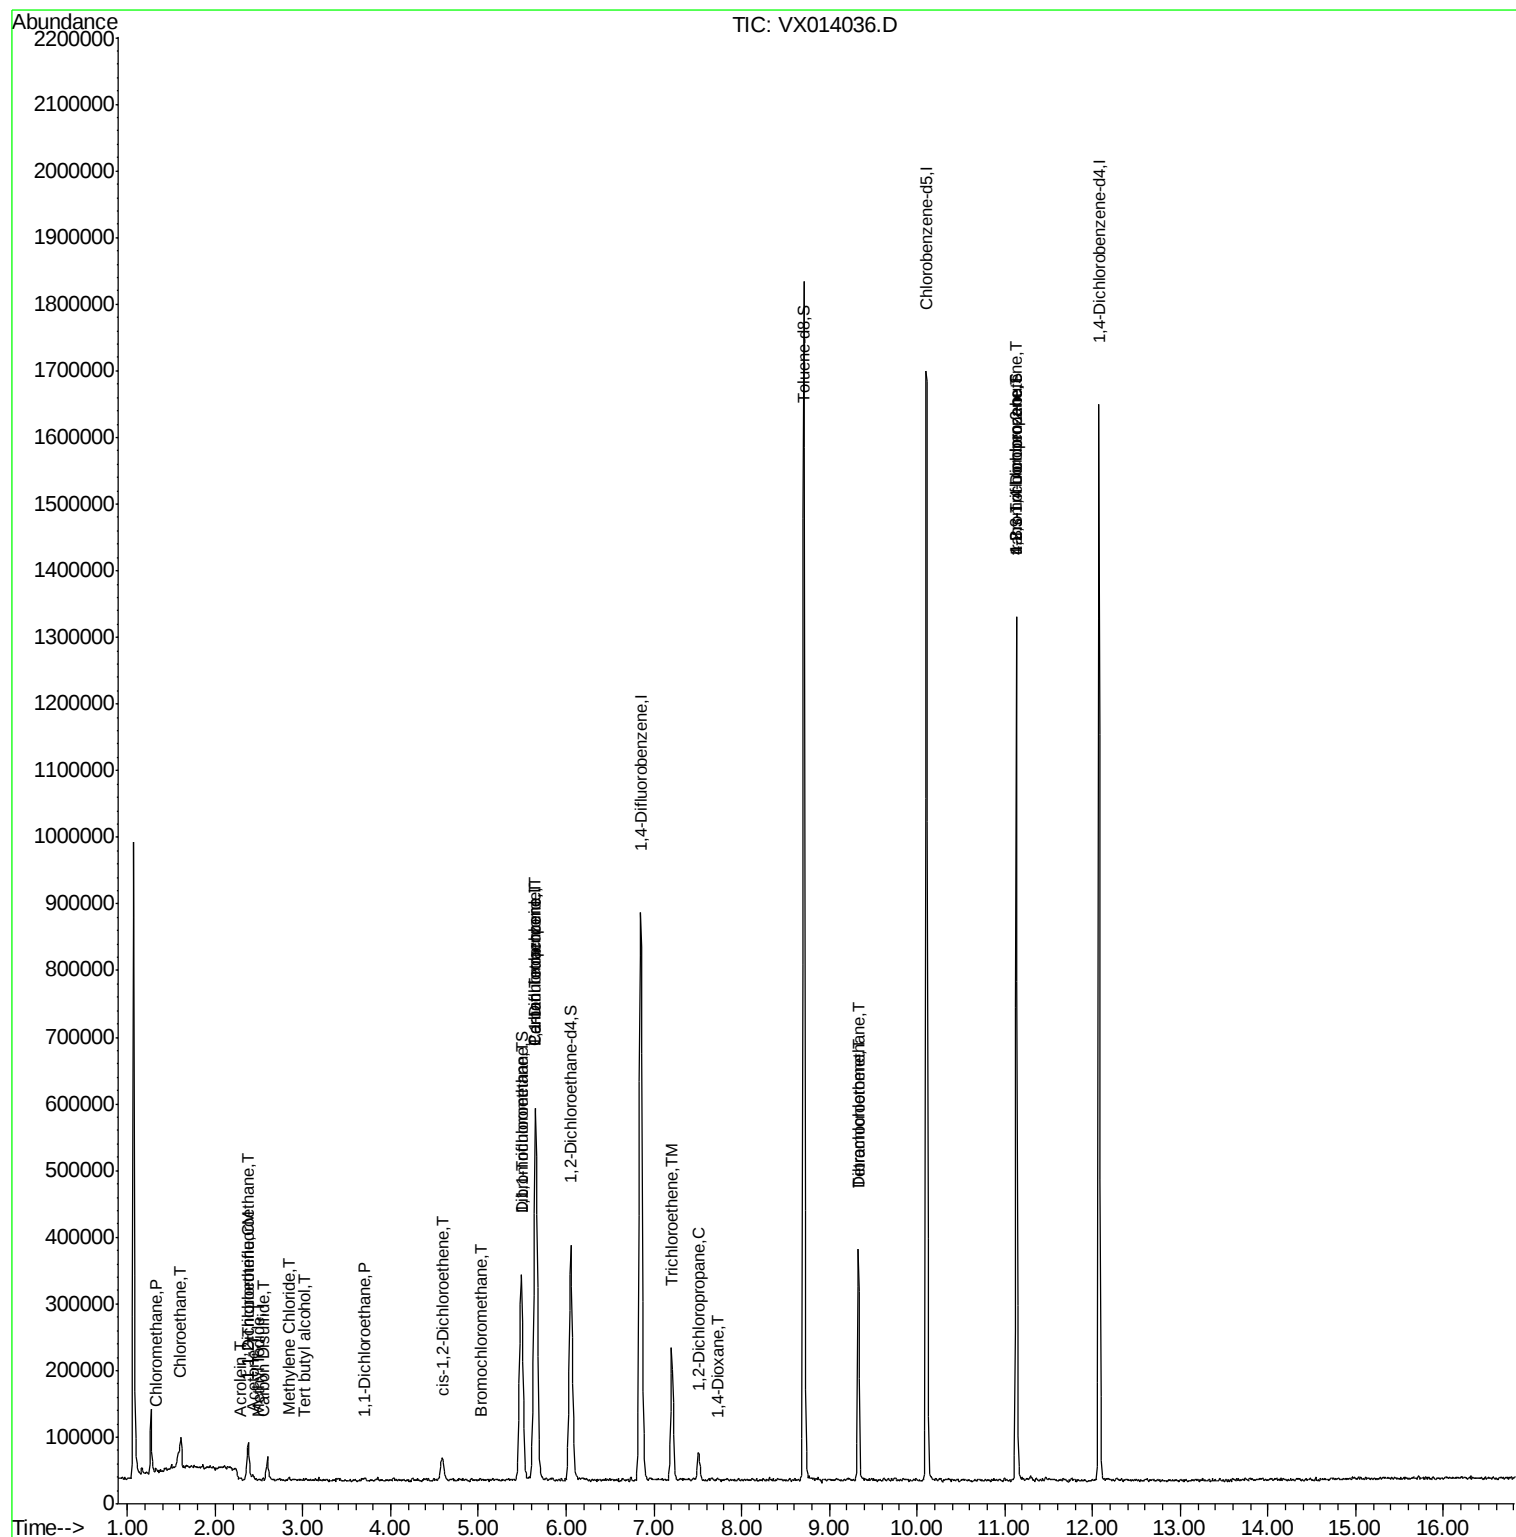







#1

Pentafluorobenzene  
 Concen: 50.000 ug/l  
 RT: 5.65 min Scan# 782  
 Delta R.T. 0.01 min  
 Lab File: VX014036.D  
 Acq: 16 Dec 2019 15:37

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 RE135D3-20191210




Tot Ion:168 Resp: 577650  
 Ion Ratio Lower Upper  
 168 100  
 99 49.5 40.3 60.5

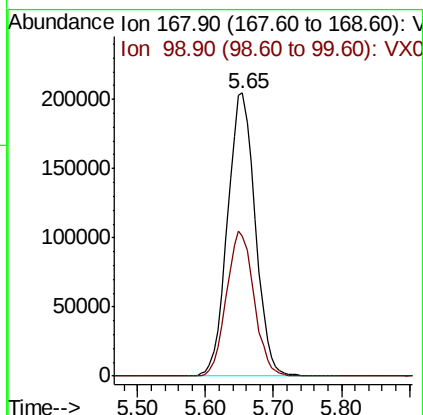

#3

Chloromethane  
 Concen: 0.246 ug/l  
 RT: 1.32 min Scan# 71  
 Delta R.T. 0.00 min  
 Lab File: VX014036.D  
 Acq: 16 Dec 2019 15:37

Tgt Ion: 50 Resp: 1709  
 Ion Ratio Lower Upper  
 50 100  
 52 0.0 26.2 39.4#

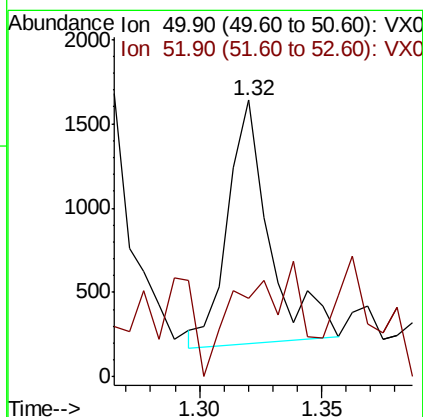



#6

Chloroethane

Concen: 0.615 ug/l

RT: 1.60 min Scan# 117

Delta R.T. -0.10 min

Lab File: VX014036.D

Acq: 16 Dec 2019 15:37

Instrument :

MSVOA\_X

ClientSampleId :





RE135D3-20191210

Tot Ion: 64 Resp: 2778

Ion Ratio Lower Upper

64 100

66 32.8 23.4 35.2

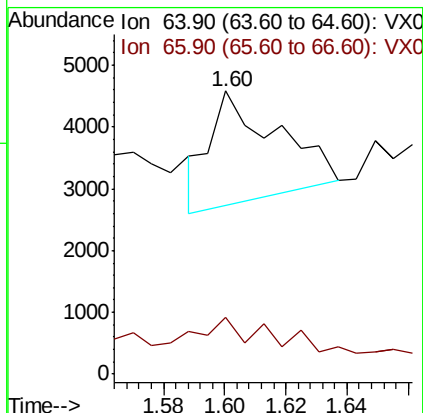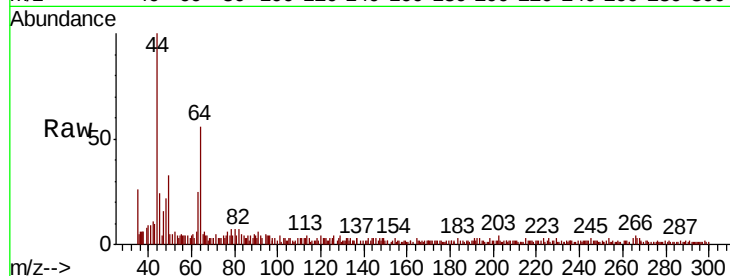

#9

1,1,2-Trichlorotrifluoroethane

Concen: 3.988 ug/l

RT: 2.38 min Scan# 245

Delta R.T. 0.01 min

Lab File: VX014036.D

Acq: 16 Dec 2019 15:37




Tgt Ion: 101 Resp: 21776


Ion Ratio Lower Upper

101 100

85 40.9 33.7 50.5

151 83.9 64.5 96.7

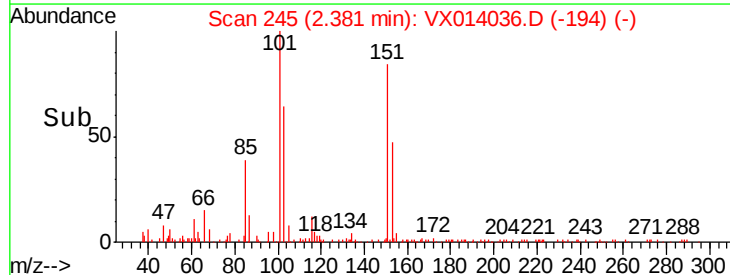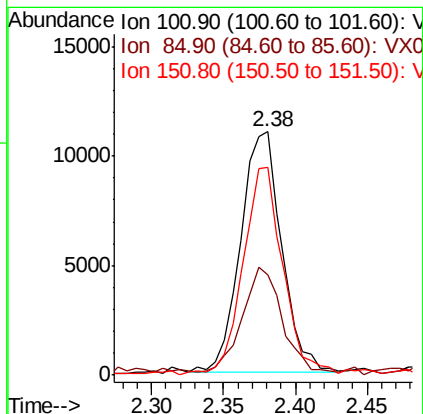



#10

Methyl Iodide

Concen: 2.630 ug/l

RT: 2.49 min Scan# 263

Delta R.T. -0.01 min

Lab File: VX014036.D

Acq: 16 Dec 2019 15:37

Instrument :

MSVOA\_X

ClientSampleId :

RE135D3-20191210


Tot Ion:142 Resp: 71

Ion Ratio Lower Upper

142 100

127 409.9 31.6 47.4#




141 150.7 11.6 17.4#

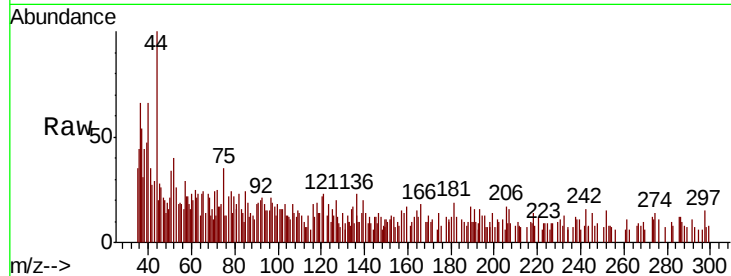

Abundance Ion 141.80 (141.50 to 142.50): V

Ion 126.80 (126.50 to 127.50): V

Ion 140.80 (140.50 to 141.50): V

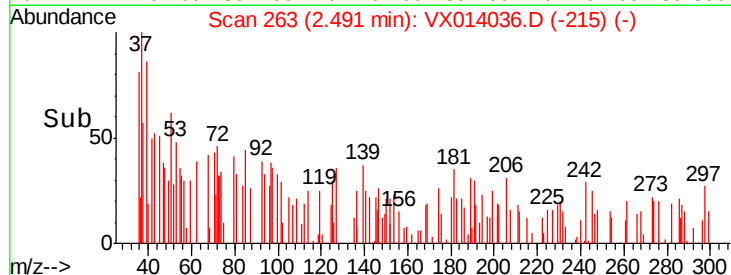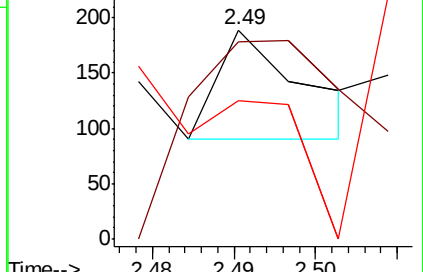

#11

Tert butyl alcohol

Concen: 1.640 ug/l

RT: 3.02 min Scan# 350

Delta R.T. -0.02 min

Lab File: VX014036.D


Acq: 16 Dec 2019 15:37

Tgt Ion: 59 Resp: 2320

Ion Ratio Lower Upper



59 100


57 10.4 8.4 12.6

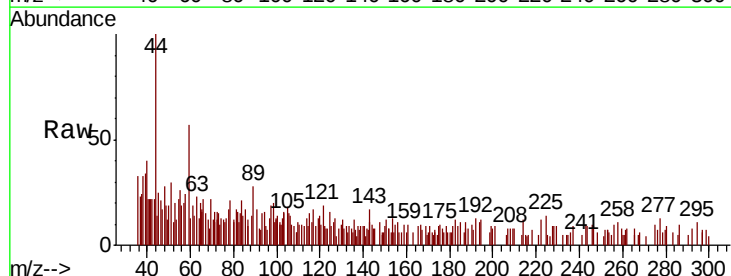

Abundance Ion 59.00 (58.70 to 59.70): VX0

Ion 57.00 (56.70 to 57.70): VX0




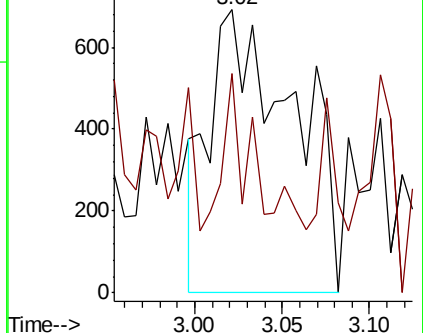


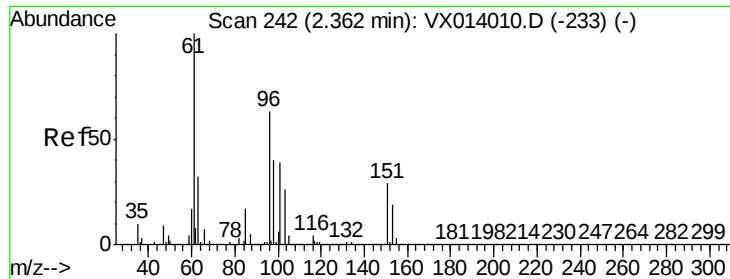

#12  
 1,1-Dichloroethene  
 Concen: 0.593 ug/l  
 RT: 2.37 min Scan# 243  
 Delta R.T. 0.01 min  
 Lab File: VX014036.D  
 Acq: 16 Dec 2019 15:37




Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 RE135D3-20191210


| Tot Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 96      | 100   |       |       |
| 61      | 187.0 | 127.9 | 191.9 |
| 98      | 53.2  | 50.5  | 75.7  |

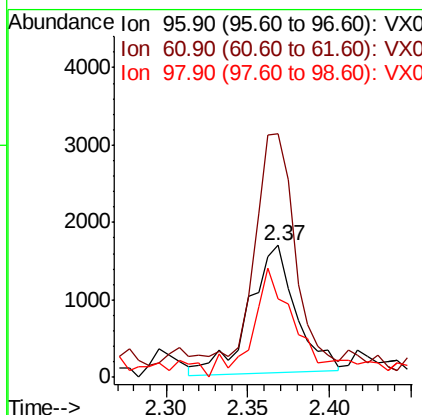

#13  
 Acrolein  
 Concen: 0.756 ug/l  
 RT: 2.29 min Scan# 230  
 Delta R.T. 0.01 min  
 Lab File: VX014036.D  
 Acq: 16 Dec 2019 15:37

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 56      | 100   |       |       |
| 55      | 67.8  | 56.9  | 85.3  |

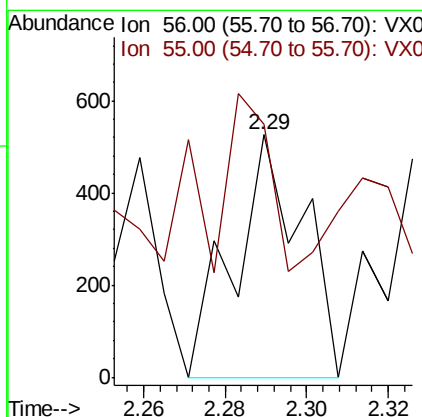

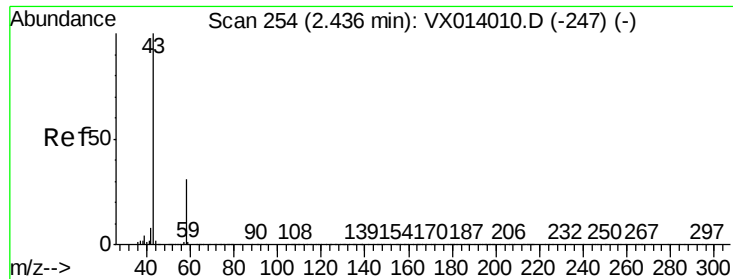

#16

Acetone

Concen: 2.064 ug/l

RT: 2.43 min Scan# 253

Delta R.T. -0.01 min

Lab File: VX014036.D

Acq: 16 Dec 2019 15:37

Instrument :

MSVOA\_X

ClientSampleId :





RE135D3-20191210

Tot Ion: 43 Resp: 8772

Ion Ratio Lower Upper

43 100

58 25.3 24.9 37.3

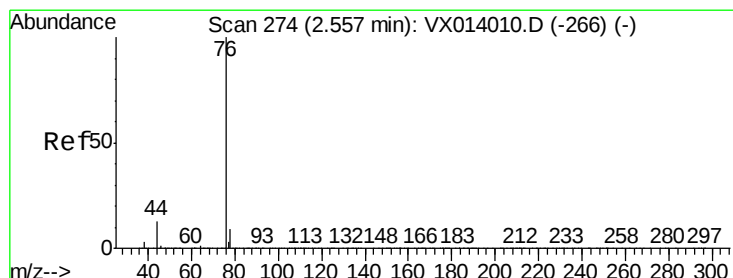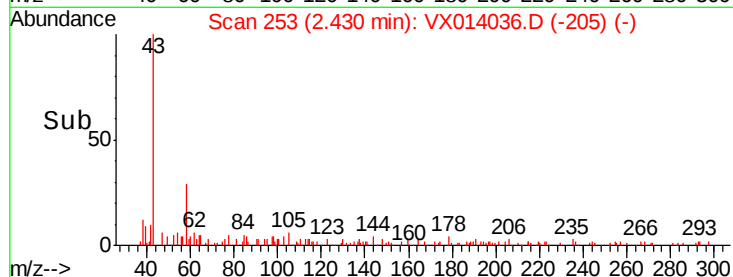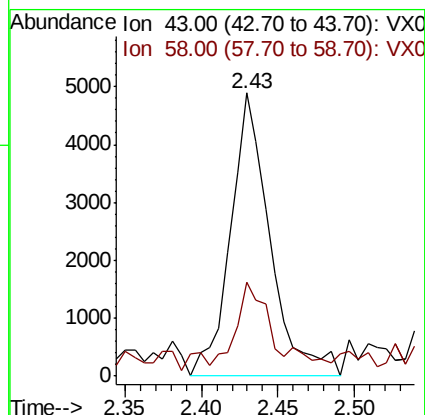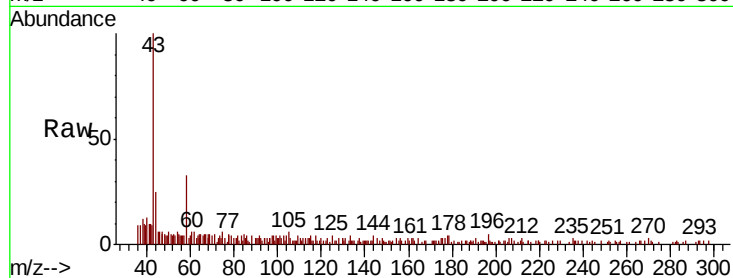

#17

Carbon Disulfide

Concen: 0.844 ug/l

RT: 2.55 min Scan# 273

Delta R.T. -0.01 min

Lab File: VX014036.D




Acq: 16 Dec 2019 15:37


Tgt Ion: 76 Resp: 1462

Ion Ratio Lower Upper

76 100

78 29.0 7.2 10.8#


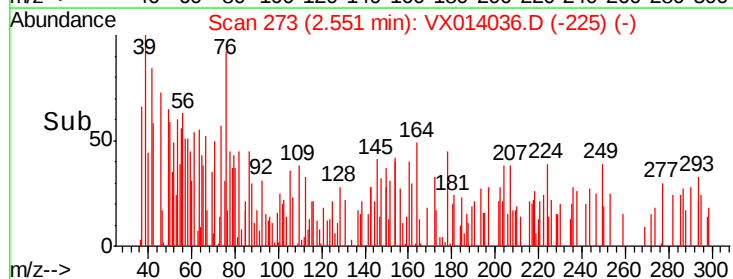
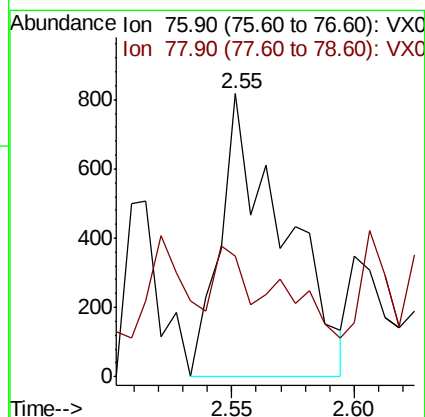
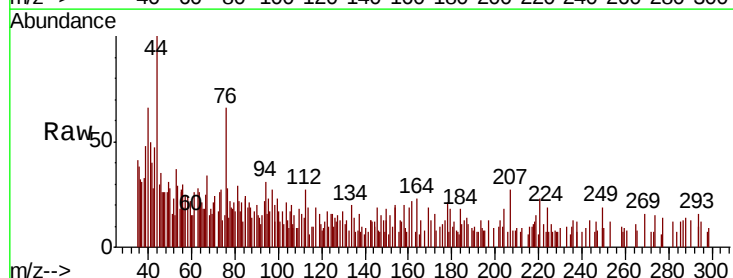


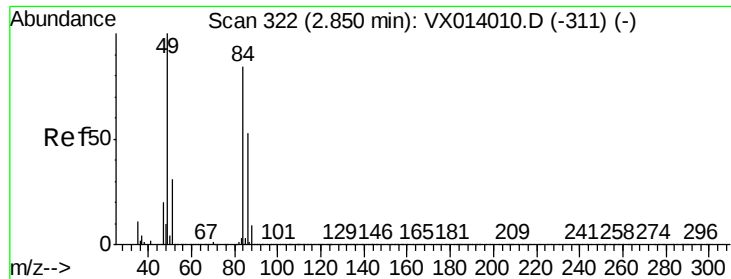

#20  
Methvlene Chloride  
Concen: 0.327 ug/l  
RT: 2.84 min Scan# 321  
Delta R.T. -0.01 min  
Lab File: VX014036.D  
Acq: 16 Dec 2019 15:37




Instrument :  
MSVOA\_X  
ClientSampleId :  
RE135D3-20191210


| Tot Ion: | 84    | Resp: | 2191   |
|----------|-------|-------|--------|
| Ion      | Ratio | Lower | Upper  |
| 84       | 100   |       |        |
| 49       | 71.5  | 95.8  | 143.6# |
| 51       | 50.5  | 29.8  | 44.8#  |
| 86       | 28.0  | 50.8  | 76.2#  |

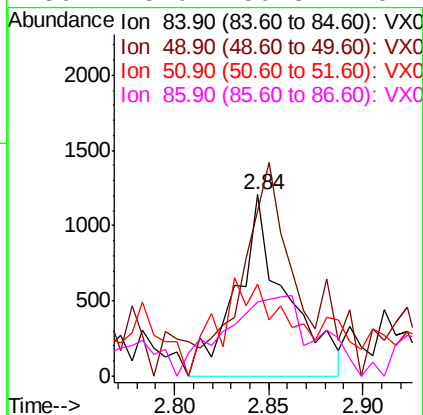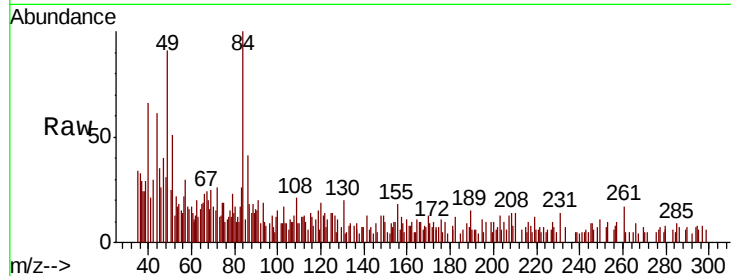

#24  
1,1-Dichloroethane  
Concen: 0.354 ug/l  
RT: 3.70 min Scan# 461  
Delta R.T. 0.01 min  
Lab File: VX014036.D  
Acq: 16 Dec 2019 15:37

| Tgt Ion: | 63    | Resp: | 3897  |
|----------|-------|-------|-------|
| Ion      | Ratio | Lower | Upper |
| 63       | 100   |       |       |
| 98       | 17.4  | 3.6   | 10.8# |
| 100      | 0.1   | 2.3   | 6.8#  |

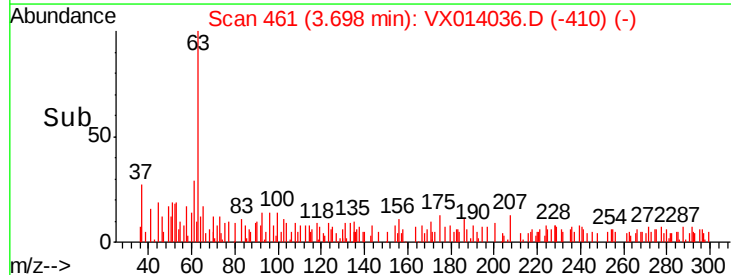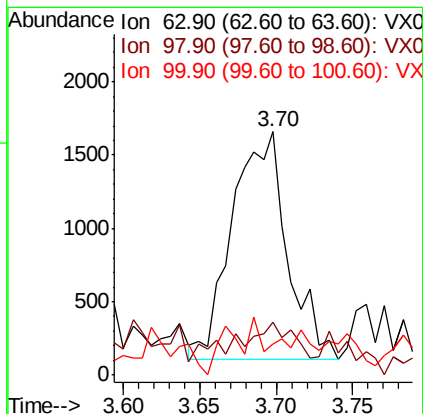




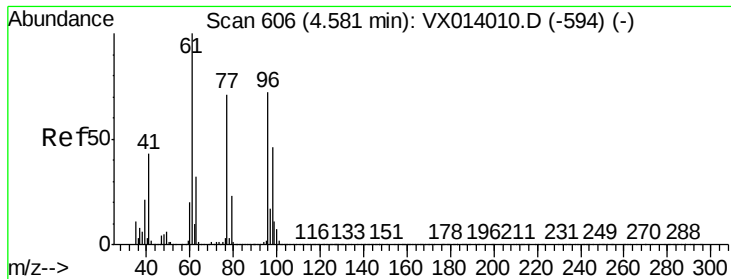


#27

cis-1,2-Dichloroethene  
Concen: 3.222 ug/l  
RT: 4.58 min Scan# 606  
Delta R.T. 0.00 min  
Lab File: VX014036.D  
Acq: 16 Dec 2019 15:37

Instrument :  
MSVOA\_X  
ClientSampleId :  
RE135D3-20191210




| Tot Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 96      | 100   |       |       |
| 61      | 116.8 | 0.0   | 288.4 |
| 98      | 62.1  | 0.0   | 129.6 |

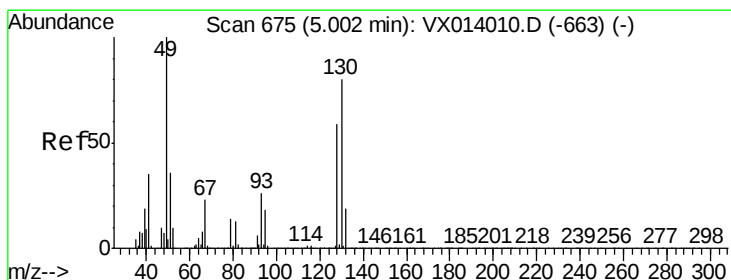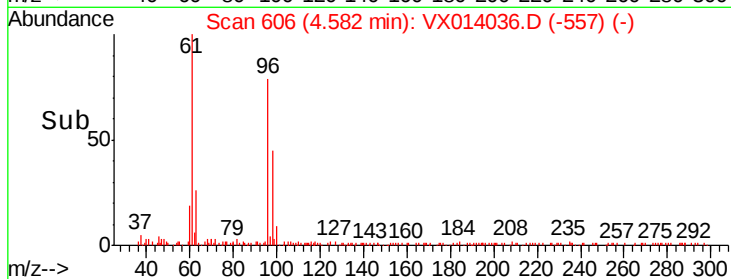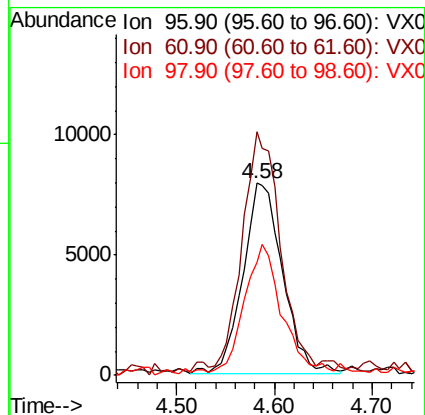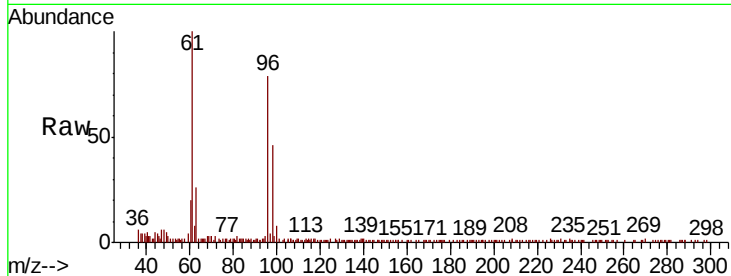


#28

Bromochloromethane  
Concen: 0.610 ug/l  
RT: 5.02 min Scan# 678  
Delta R.T. 0.02 min  
Lab File: VX014036.D  
Acq: 16 Dec 2019 15:37

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 49      | 100   |       |       |
| 129     | 82.8  | 0.0   | 5.0#  |
| 130     | 48.1  | 64.6  | 97.0# |

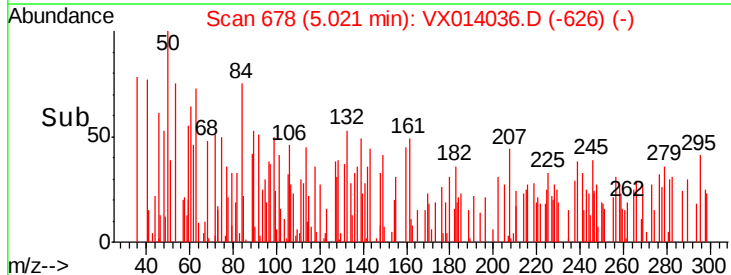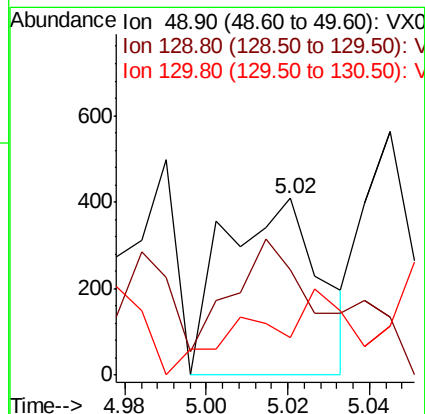



#32

1,1,1-Trichloroethane

Concen: 0.207 ug/l

RT: 5.49 min Scan# 755

Delta R.T. 0.01 min

Lab File: VX014036.D

Acq: 16 Dec 2019 15:37

Instrument :

MSVOA\_X

ClientSampleId :

RE135D3-20191210





Tot Ion: 97 Resp: 1840

Ion Ratio Lower Upper

97 100

99 0.0 52.0 78.0#

61 0.0 36.7 55.1#

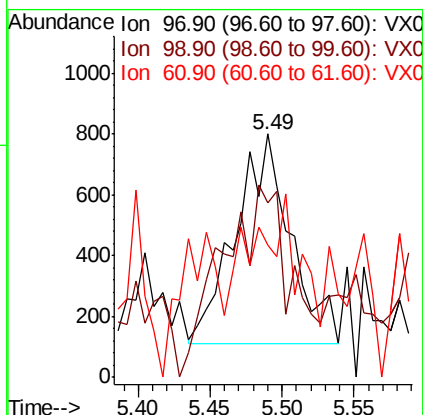

#33

1,2-Dichloroethane-d4

Concen: 49.040 ug/l

RT: 6.05 min Scan# 847

Delta R.T. 0.00 min

Lab File: VX014036.D




Acq: 16 Dec 2019 15:37


Tgt Ion: 65 Resp: 321057

Ion Ratio Lower Upper

65 100

67 53.9 0.0 106.4

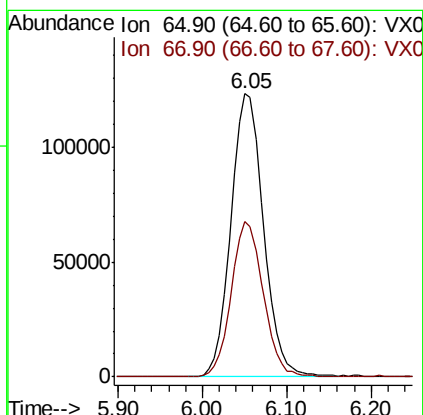



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.85 min Scan# 978

Delta R.T. 0.00 min

Lab File: VX014036.D

Acq: 16 Dec 2019 15:37

Instrument :

MSVOA\_X

ClientSampleId :

RE135D3-20191210


Tot Ion:114 Resp: 886771

Ion Ratio Lower Upper

114 100

63 20.5 0.0 40.8




88 15.8 0.0 30.4

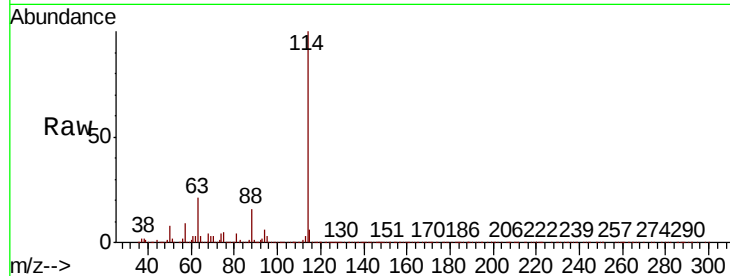

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

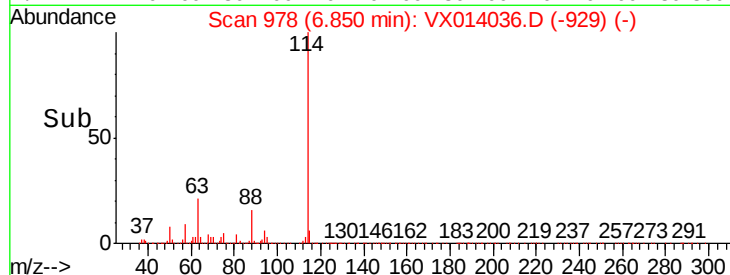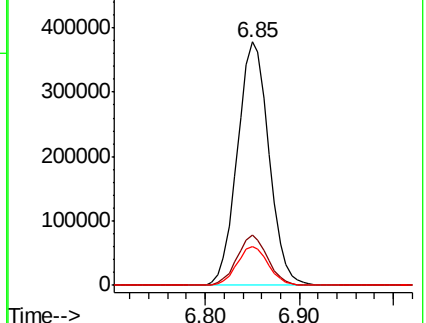

#35

Dibromofluoromethane

Concen: 50.112 ug/l

RT: 5.49 min Scan# 755

Delta R.T. 0.00 min

Lab File: VX014036.D

Acq: 16 Dec 2019 15:37


Tgt Ion:113 Resp: 270133

Ion Ratio Lower Upper

113 100

111 101.2 82.0 123.0



192 22.4 19.3 28.9

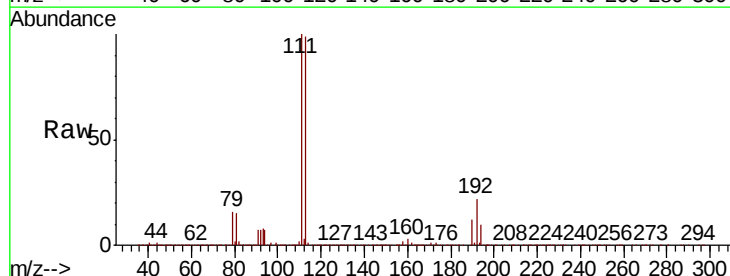


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

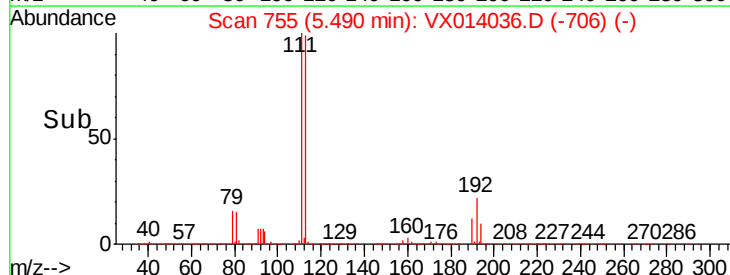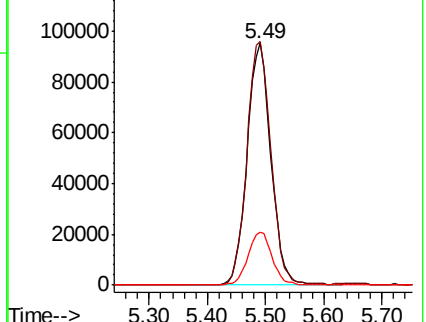



#36

1,1-Dichloropropene

Concen: 4.865 ug/l

RT: 5.65 min Scan# 781

Delta R.T. -0.14 min

Lab File: VX014036.D

Acq: 16 Dec 2019 15:37

Instrument :

MSVOA\_X

ClientSampleId :

RE135D3-20191210





Tot Ion: 75 Resp: 39581

Ion Ratio Lower Upper

75 100

110 10.7 18.3 54.9#

77 0.0 24.8 37.2#

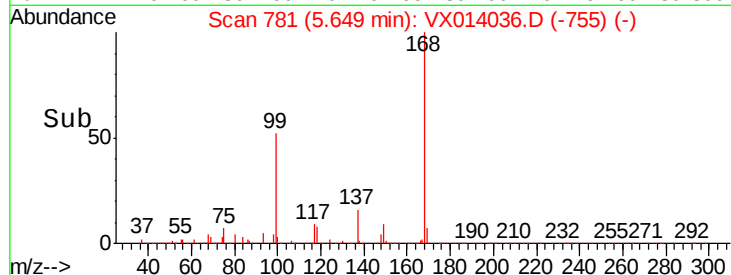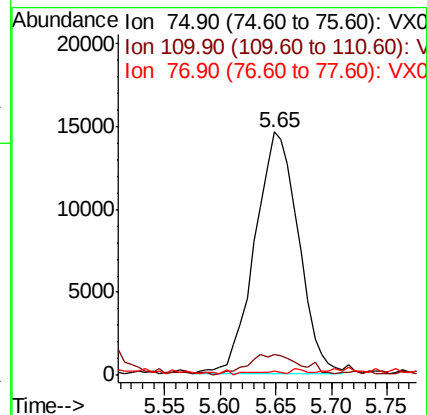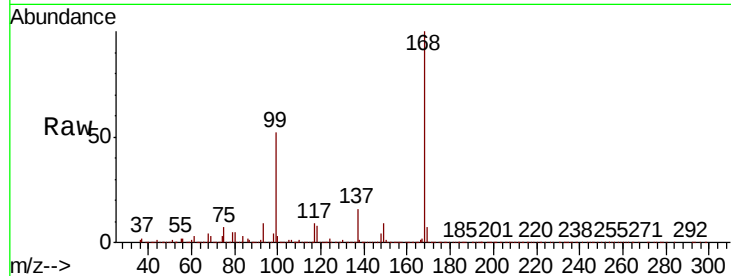

#38

Carbon Tetrachloride

Concen: 6.981 ug/l

RT: 5.65 min Scan# 782

Delta R.T. -0.12 min

Lab File: VX014036.D

Acq: 16 Dec 2019 15:37




Tgt Ion: 117 Resp: 51747


Ion Ratio Lower Upper

117 100

119 5.8 76.2 114.4#

121 0.0 23.6 35.4#

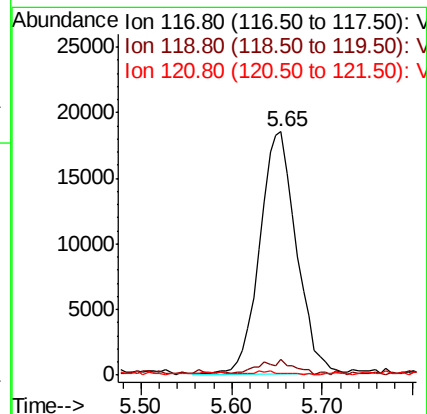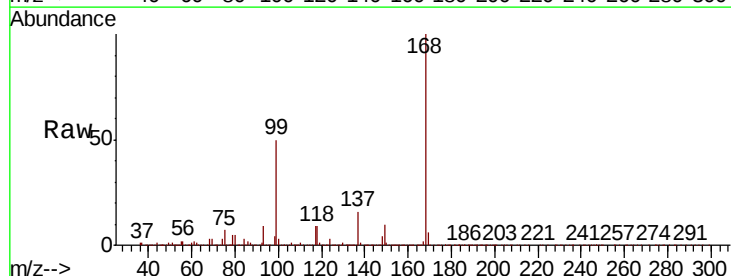



#44

Trichloroethene

Concen: 11.857 ug/l

RT: 7.20 min Scan# 1036

Delta R.T. -0.01 min

Lab File: VX014036.D

Acq: 16 Dec 2019 15:37

Instrument :

MSVOA\_X

ClientSampleId :


RE135D3-20191210

Tot Ion:130 Resp: 81990

Ion Ratio Lower Upper

130 100

95 94.1 0.0 185.6



Abundance Ion 129.80 (129.50 to 130.50): V

Ion 94.90 (94.60 to 95.60): VX0

7.20

40000

30000



20000

10000

0

7.10 7.20 7.30

Time-->



#45

1,2-Dichloropropane

Concen: 3.080 ug/l

RT: 7.51 min Scan# 1086

Delta R.T. 0.00 min

Lab File: VX014036.D


Acq: 16 Dec 2019 15:37

Tgt Ion: 63 Resp: 19761

Ion Ratio Lower Upper

63 100

65 28.6 25.8 38.8



Abundance Ion 62.90 (62.60 to 63.60): VX0

Ion 64.90 (64.60 to 65.60): VX0

10000

8000

6000


4000


2000

0

7.40 7.45 7.50 7.55 7.60

Time-->





#49

1,4-Dioxane

Concen: 0.864 ug/l

RT: 7.74 min Scan# 1124

Delta R.T. 0.01 min

Lab File: VX014036.D

Acq: 16 Dec 2019 15:37

Instrument :

MSVOA\_X

ClientSampleId :

RE135D3-20191210





Tot Ion: 88 Resp: 128

Ion Ratio Lower Upper

88 100

43 864.1 26.5 39.7#

58 178.9 56.8 85.2#

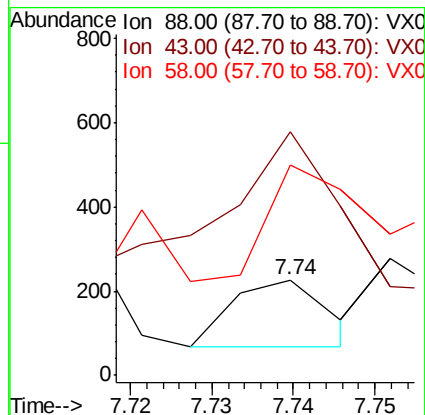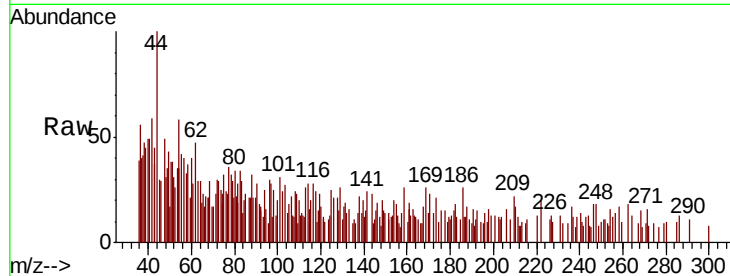

#50

Toluene-d8

Concen: 50.181 ug/l

RT: 8.71 min Scan# 1283

Delta R.T. 0.00 min

Lab File: VX014036.D




Acq: 16 Dec 2019 15:37


Tgt Ion: 98 Resp: 1053133

Ion Ratio Lower Upper

98 100

100 66.1 52.9 79.3



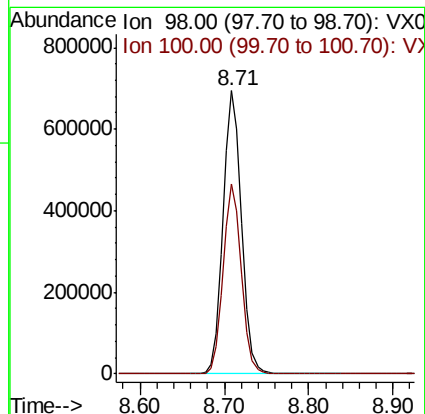
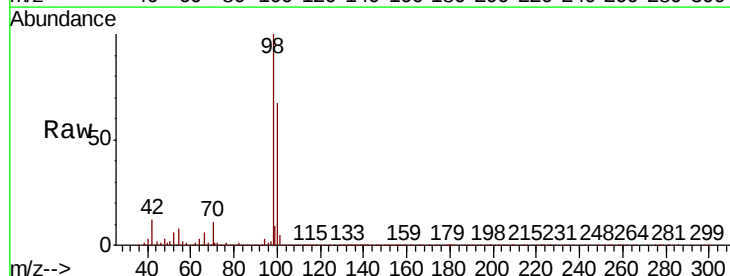




#60  
 Dibromochloromethane  
 Concen: 9.769 ug/l  
 RT: 9.33 min Scan# 1385  
 Delta R.T. -0.25 min  
 Lab File: VX014036.D  
 Acq: 16 Dec 2019 15:37




Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 RE135D3-20191210


Tot Ion:129 Resp: 61586  
 Ion Ratio Lower Upper  
 129 100  
 127 0.6 38.4 115.2#

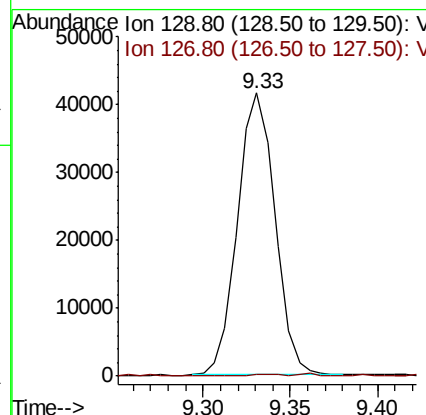

#62  
 4-Bromofluorobenzene  
 Concen: 45.404 ug/l  
 RT: 11.14 min Scan# 1681  
 Delta R.T. 0.00 min  
 Lab File: VX014036.D  
 Acq: 16 Dec 2019 15:37

Tgt Ion: 95 Resp: 348325  
 Ion Ratio Lower Upper  
 95 100  
 174 88.2 0.0 175.8  
 176 85.7 0.0 173.0



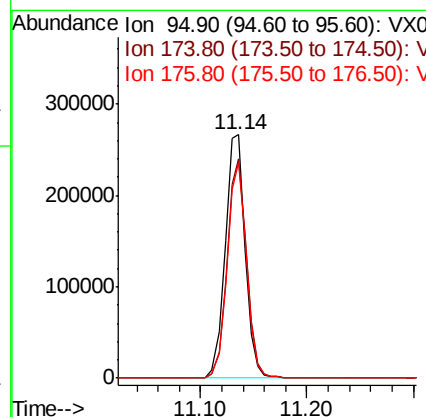





#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 10.11 min Scan# 1513  
Delta R.T. 0.00 min  
Lab File: VX014036.D  
Acq: 16 Dec 2019 15:37




Instrument :  
MSVOA\_X  
ClientSampleId :  
RE135D3-20191210


Tot Ion:117 Resp: 788331  
Ion Ratio Lower Upper  
117 100  
82 53.8 42.2 63.4  
119 32.9 25.1 37.7

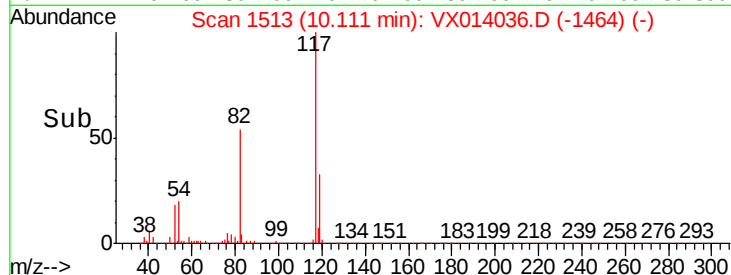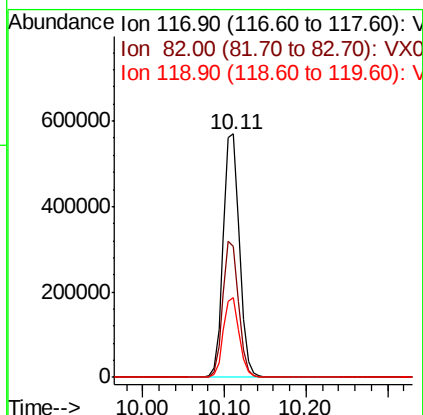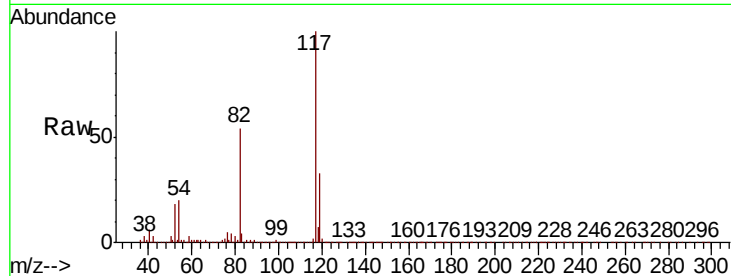

#64  
Tetrachloroethene  
Concen: 9.945 ug/l  
RT: 9.33 min Scan# 1385  
Delta R.T. 0.00 min  
Lab File: VX014036.D  
Acq: 16 Dec 2019 15:37

Tgt Ion:164 Resp: 69375  
Ion Ratio Lower Upper  
164 100  
166 133.8 104.0 156.0  
129 86.5 72.2 108.4  
131 90.6 69.6 104.4

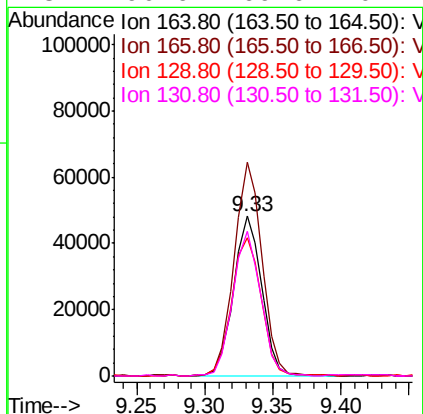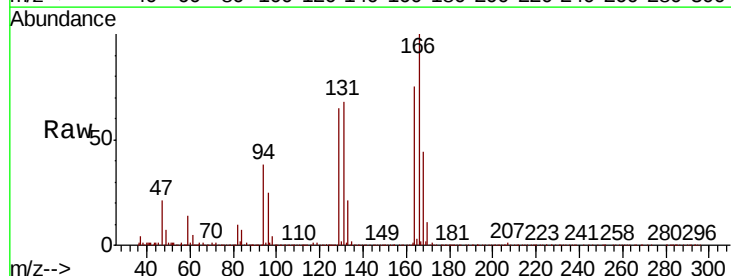



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.07 min Scan# 1835

Delta R.T. 0.00 min

Lab File: VX014036.D

Acq: 16 Dec 2019 15:37

Instrument :

MSVOA\_X

ClientSampleId :

RE135D3-20191210


Tot Ion:152 Resp: 341237

Ion Ratio Lower Upper

152 100

115 54.4 38.3 114.9




150 154.9 0.0 345.4



Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

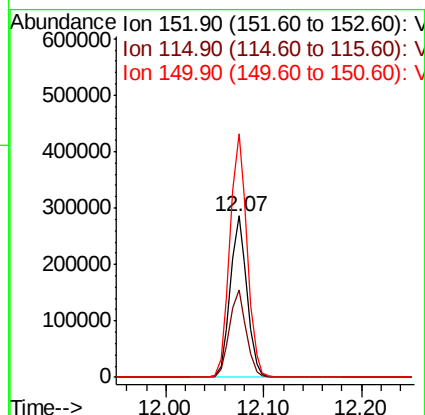

#76

1,2,3-Trichloropropane

Concen: 23.134 ug/l

RT: 11.13 min Scan# 1680

Delta R.T. -0.16 min

Lab File: VX014036.D


Acq: 16 Dec 2019 15:37

Tgt Ion: 75 Resp: 171384

Ion Ratio Lower Upper



75 100


77 1.4 19.3 57.8#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

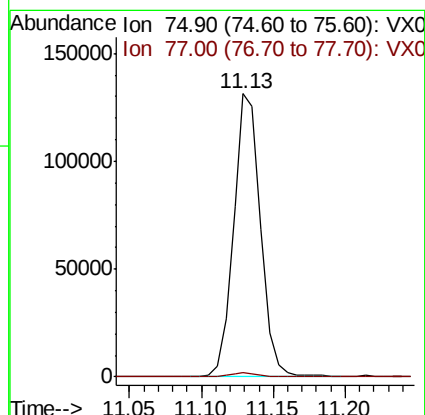



#81

trans-1,4-Dichloro-2-butene

Concen: 65.297 ug/l

RT: 11.13 min Scan# 1680

Delta R.T. 0.06 min

Lab File: VX014036.D

Acq: 16 Dec 2019 15:37

Instrument :

MSVOA\_X

ClientSampleId :

RE135D3-20191210


Tot Ion: 75 Resp: 171384

Ion Ratio Lower Upper

75 100

53 0.2 76.7 115.1#

89 0.1 34.6 51.8#

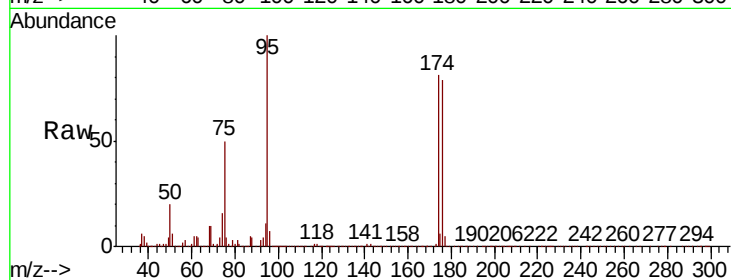

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 53.00 (52.70 to 53.70): VX0

Ion 88.90 (88.60 to 89.60): VX0

