
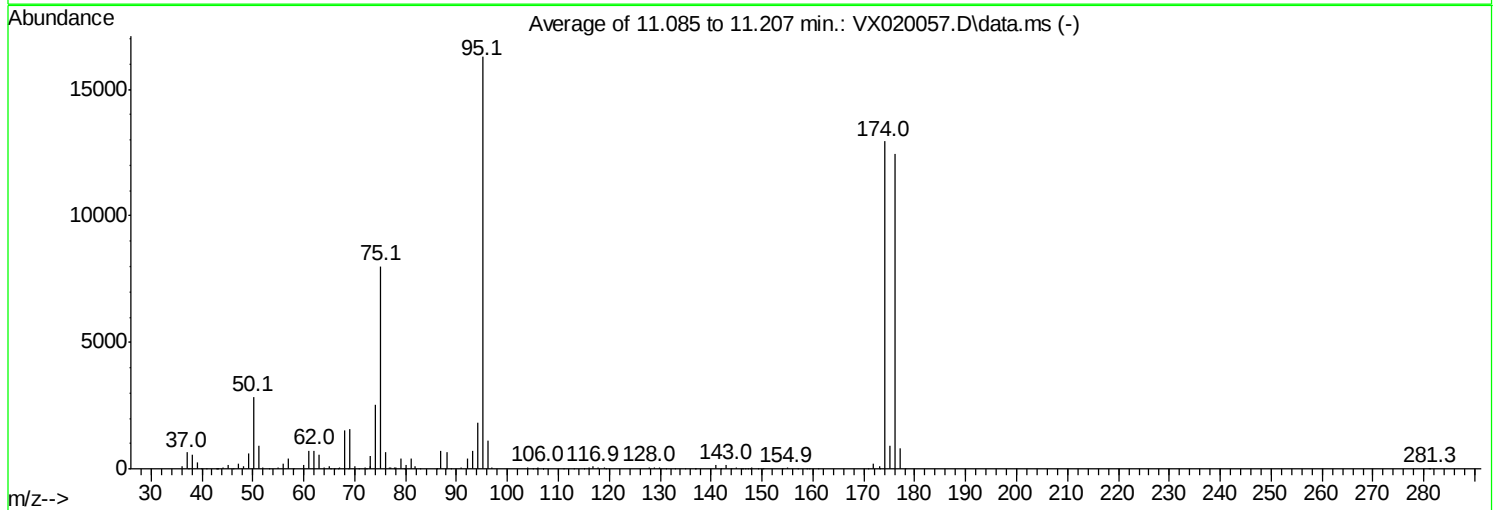


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121620\
 Data File : VX020057.D
 Acq On : 16 Dec 2020 10:41
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\624X120820W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : wed Dec 09 06:09:21 2020

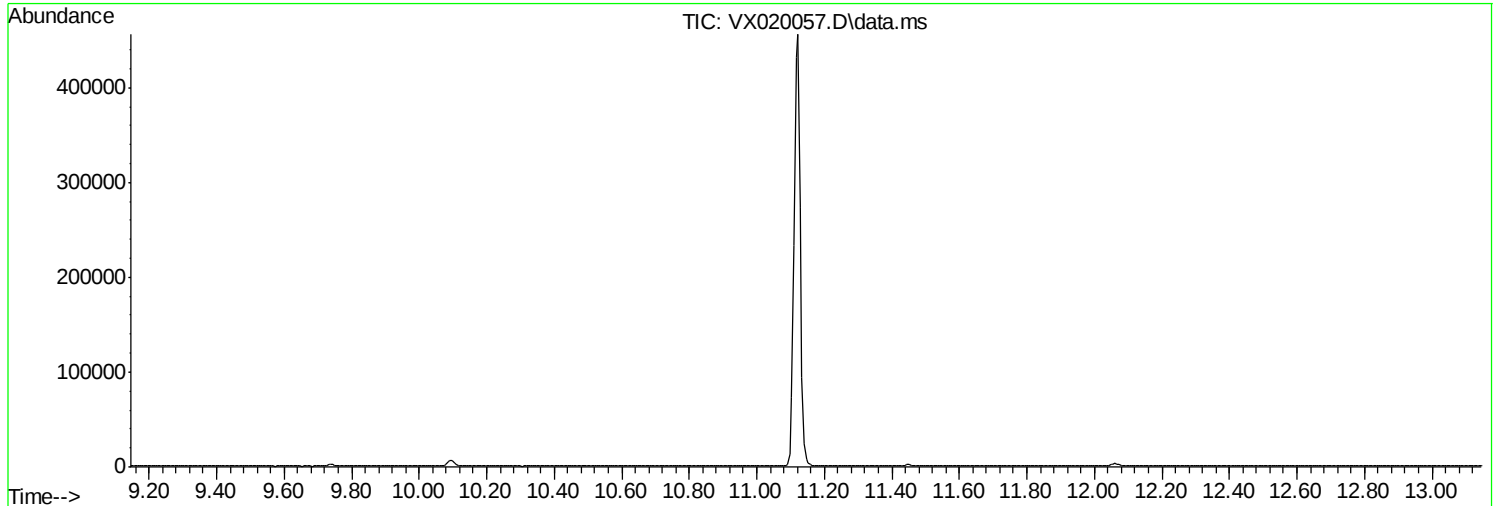

AutoFind: Averaged scan 1640 to 1660; Bkg corrected with scan 1639

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	2847	PASS
75	95	30	60	49.2	8012	PASS
95	95	100	100	100.0	16296	PASS
96	95	5	9	6.9	1129	PASS
173	174	0.00	2	0.8	103	PASS
174	95	50	100	79.5	12951	PASS
175	174	5	9	7.0	912	PASS
176	174	95	101	96.1	12440	PASS
177	176	5	9	6.6	824	PASS