

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121622\
 Data File : VX033461.D
 Acq On : 16 Dec 2022 15:20
 Operator : JC/MD
 Sample : VX1216WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1216WBL02

Quant Time: Dec 17 08:09:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
 Quant Title : SW846 8260
 QLast Update : Wed Dec 07 12:43:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	130199	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	198269	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	174806	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	82027	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	35919	43.003	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	86.000%
35) Dibromofluoromethane	5.385	113	41077	46.062	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	92.120%
50) Toluene-d8	8.647	98	84875	45.496	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	91.000%#
62) 4-Bromofluorobenzene	11.079	95	65386	45.839	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	91.680%


Target Compounds Qvalue

 (#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121622\
Data File : VX033461.D
Acq On : 16 Dec 2022 15:20
Operator : JC/MD
Sample : VX1216WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1216WBL02

Quant Time: Dec 17 08:09:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260
QLast Update : Wed Dec 07 12:43:54 2022
Response via : Initial Calibration




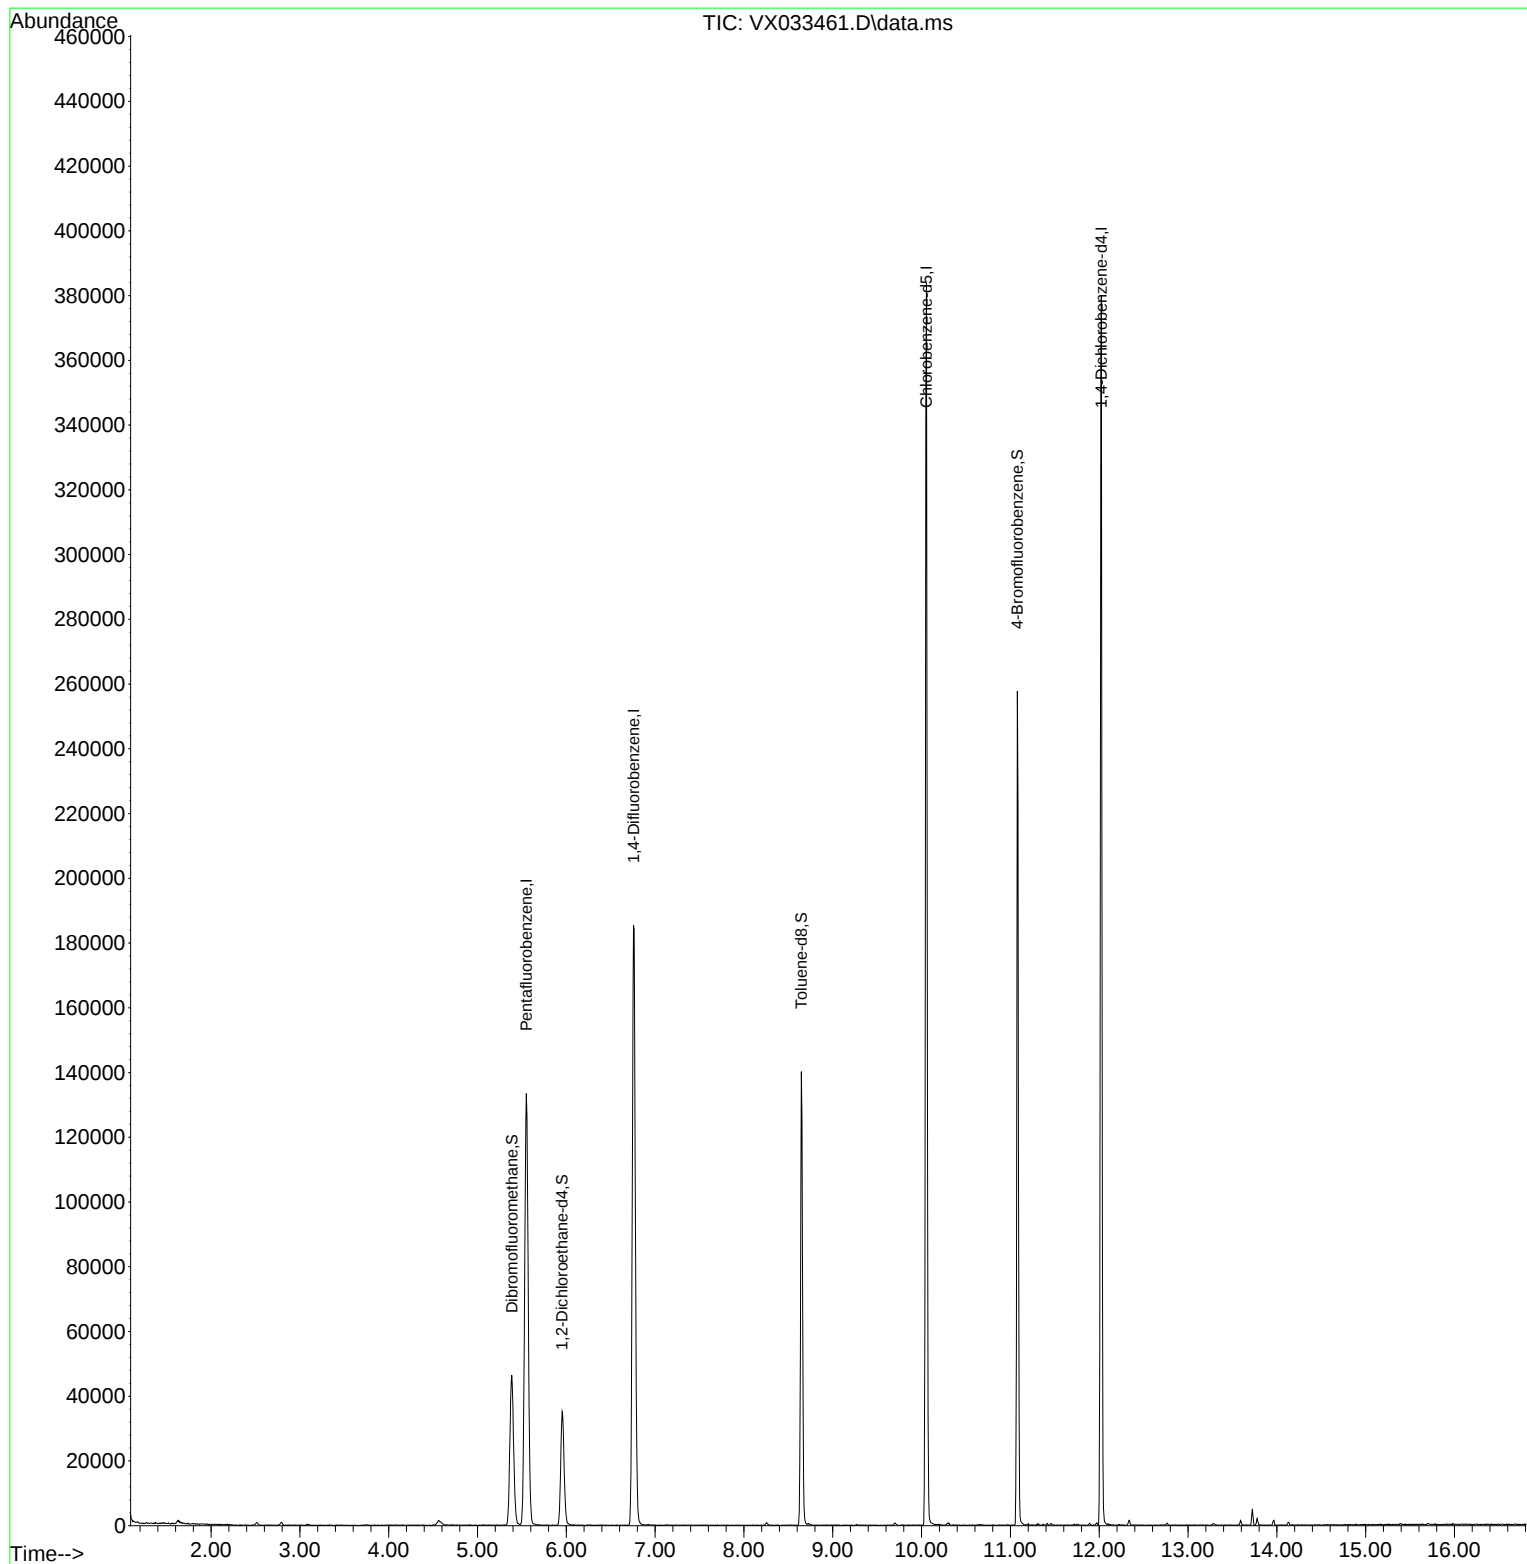




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX033461.D
Acq: 16 Dec 2022 15:20




Instrument :
MSVOA_X
ClientSampleId :
VX1216WBL02


Tgt Ion:168 Resp: 130199
Ion Ratio Lower Upper
168 100
99 56.0 46.1 69.1

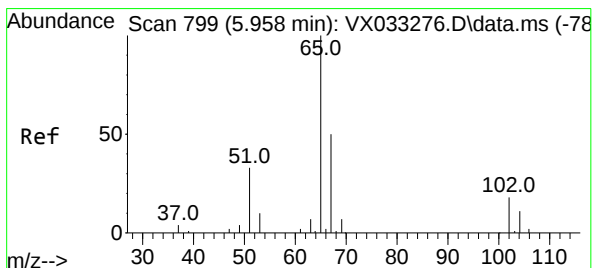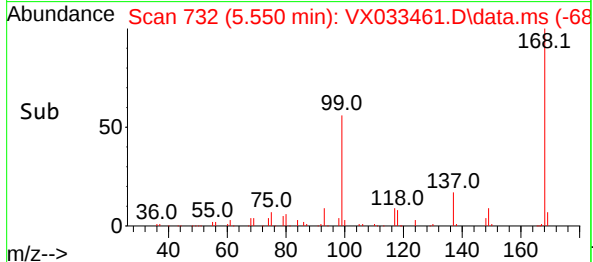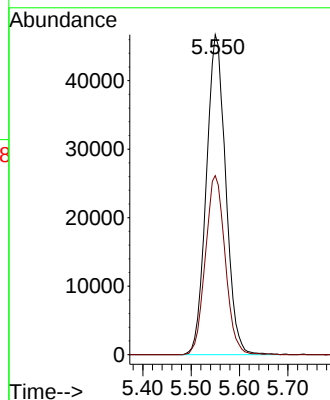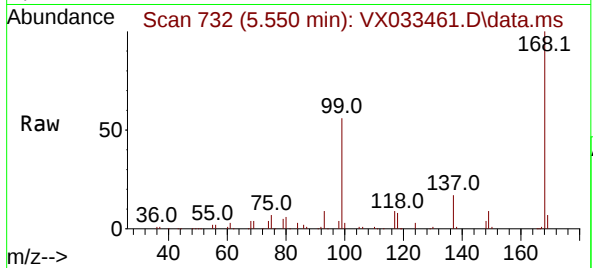

#33
1,2-Dichloroethane-d4
Concen: 43.003 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.006 min
Lab File: VX033461.D
Acq: 16 Dec 2022 15:20

Tgt Ion: 65 Resp: 35919
Ion Ratio Lower Upper
65 100
67 50.7 0.0 101.8


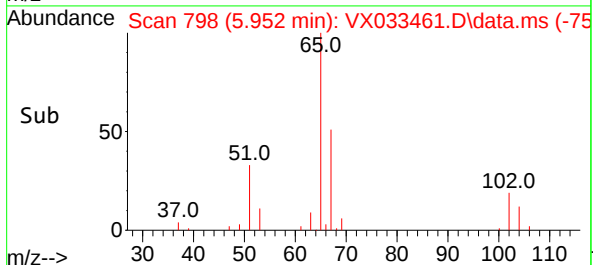
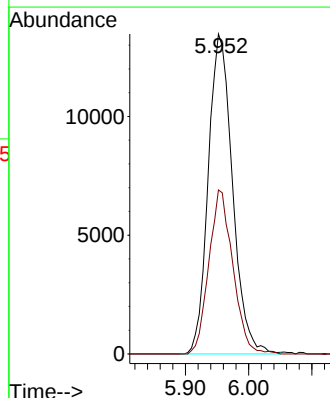
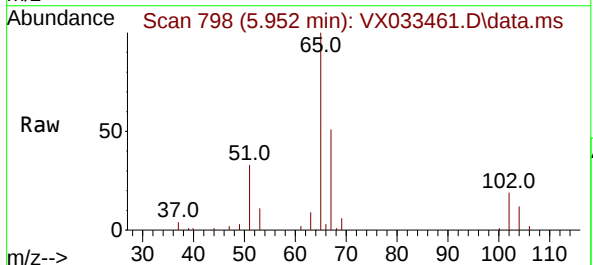


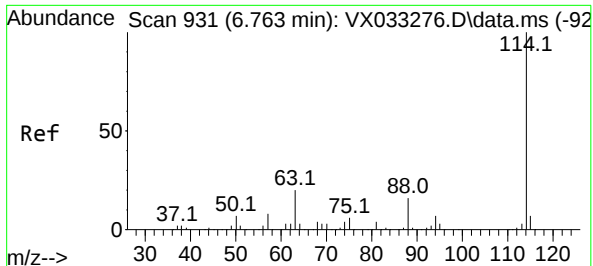

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. -0.006 min
Lab File: VX033461.D
Acq: 16 Dec 2022 15:20




Instrument :
MSVOA_X
ClientSampleId :
VX1216WBL02


Tgt Ion:114 Resp: 198269
Ion Ratio Lower Upper
114 100
63 19.2 0.0 41.6
88 15.4 0.0 33.4

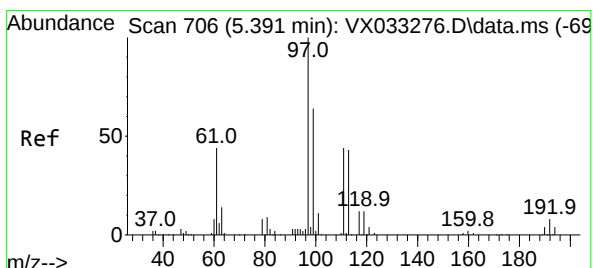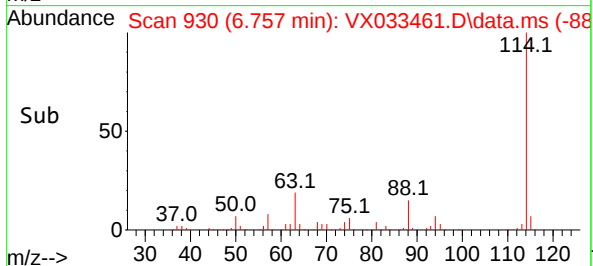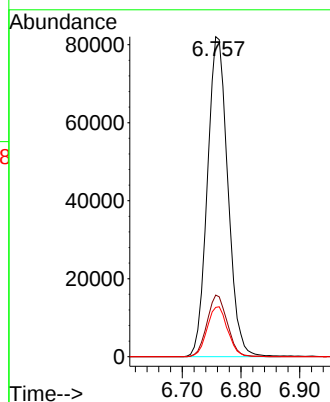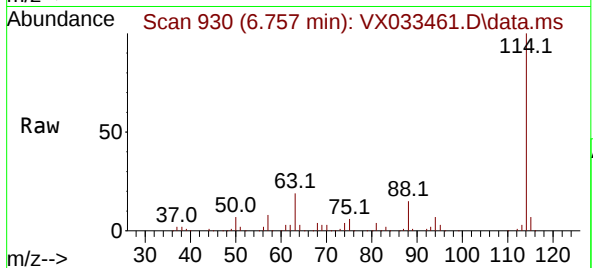

#35
Dibromofluoromethane
Concen: 46.062 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.006 min
Lab File: VX033461.D
Acq: 16 Dec 2022 15:20

Tgt Ion:113 Resp: 41077
Ion Ratio Lower Upper
113 100
111 103.2 82.4 123.6
192 19.6 15.4 23.2


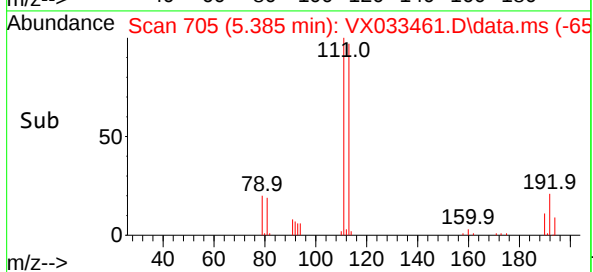
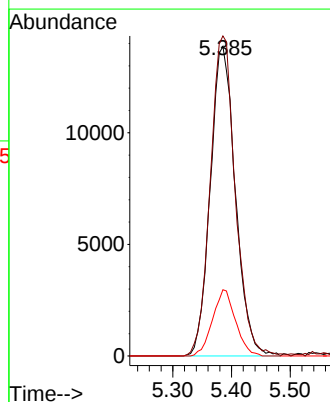
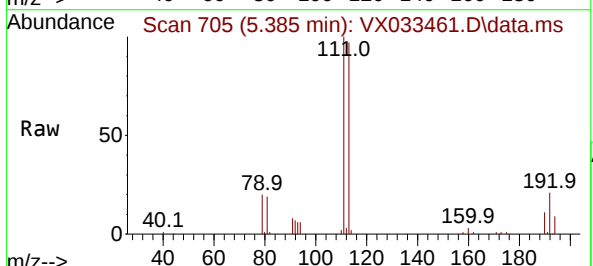


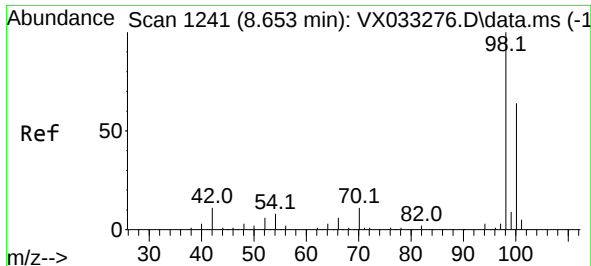

#50
Toluene-d8
Concen: 45.496 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX033461.D
Acq: 16 Dec 2022 15:20




Instrument :
MSVOA_X
ClientSampleId :
VX1216WBL02


Tgt Ion: 98 Resp: 84875
Ion Ratio Lower Upper
98 100
100 63.3 50.9 76.3

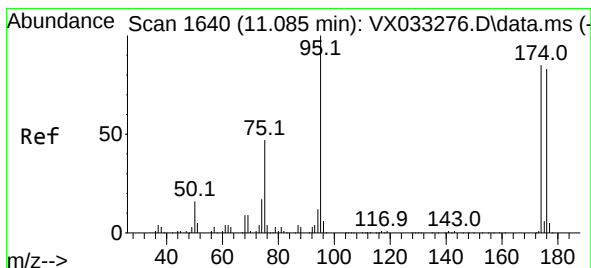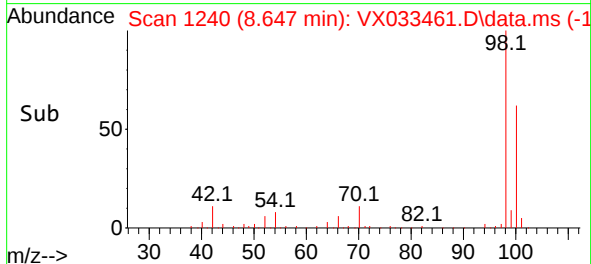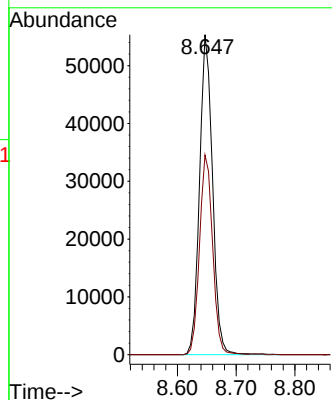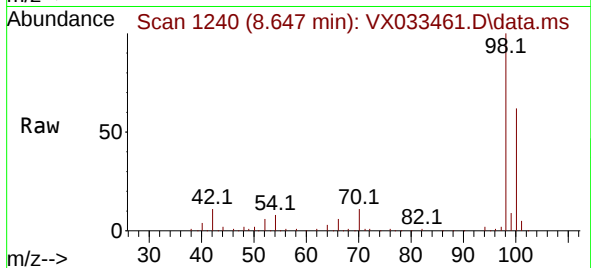

#62
4-Bromofluorobenzene
Concen: 45.839 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.006 min
Lab File: VX033461.D
Acq: 16 Dec 2022 15:20

Tgt Ion: 95 Resp: 65386
Ion Ratio Lower Upper
95 100
174 83.0 0.0 164.0
176 79.4 0.0 154.4


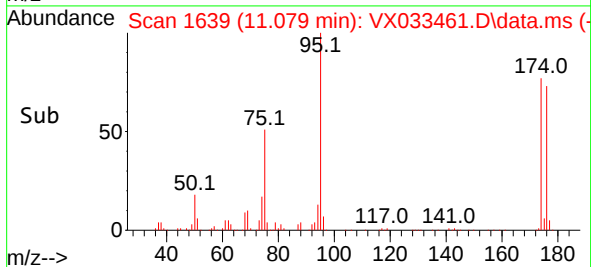
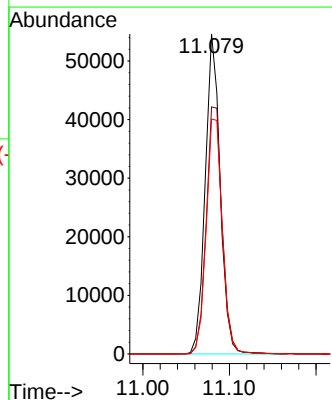
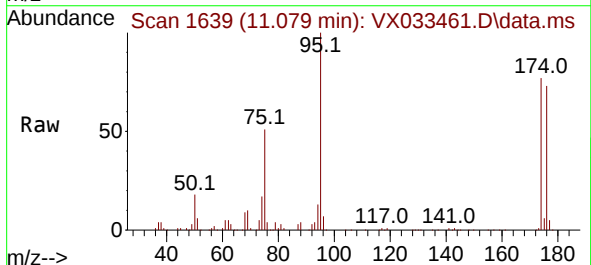


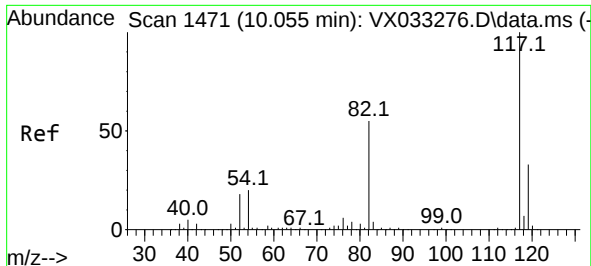

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX033461.D
Acq: 16 Dec 2022 15:20

Instrument :
MSVOA_X
ClientSampleId :
VX1216WBL02

Tgt Ion:117 Resp: 174806
Ion Ratio Lower Upper
117 100
82 54.0 44.3 66.5
119 32.1 25.7 38.5

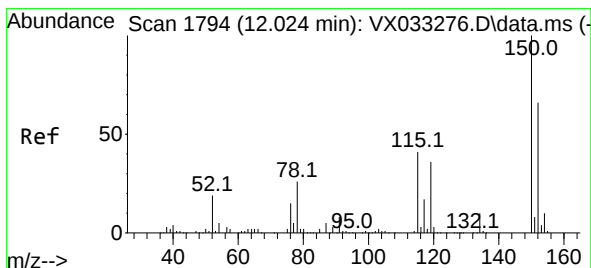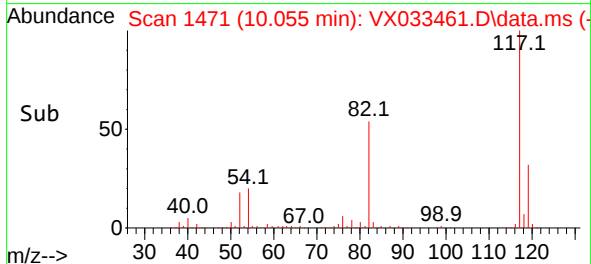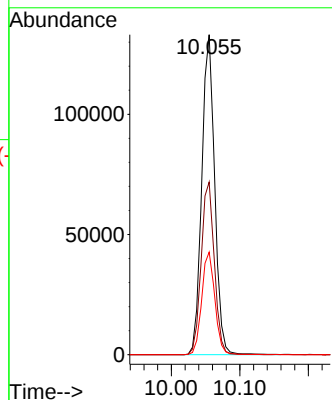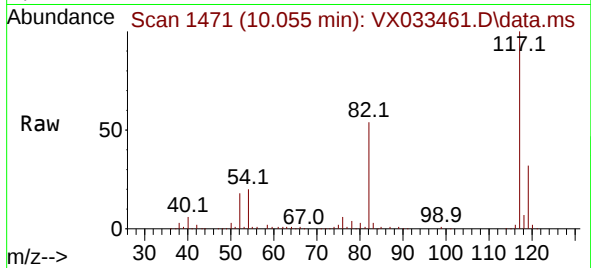

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX033461.D
Acq: 16 Dec 2022 15:20

Tgt Ion:152 Resp: 82027
Ion Ratio Lower Upper
152 100
115 58.9 44.0 132.0
150 154.8 0.0 351.8

