




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121623\
Data File : VX039257.D
Acq On : 16 Dec 2023 02:23
Operator : JC/MD
Sample : 05845-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YCHD8

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/16/2023
Supervised By :Mahesh Dadoda 12/18/2023

Quant Time: Dec 16 04:21:09 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Dec 12 03:50:51 2023
Response via : Initial Calibration

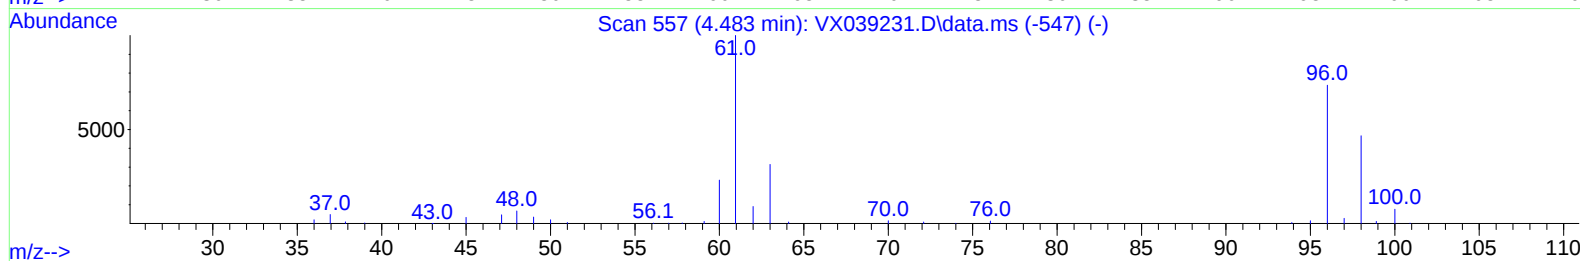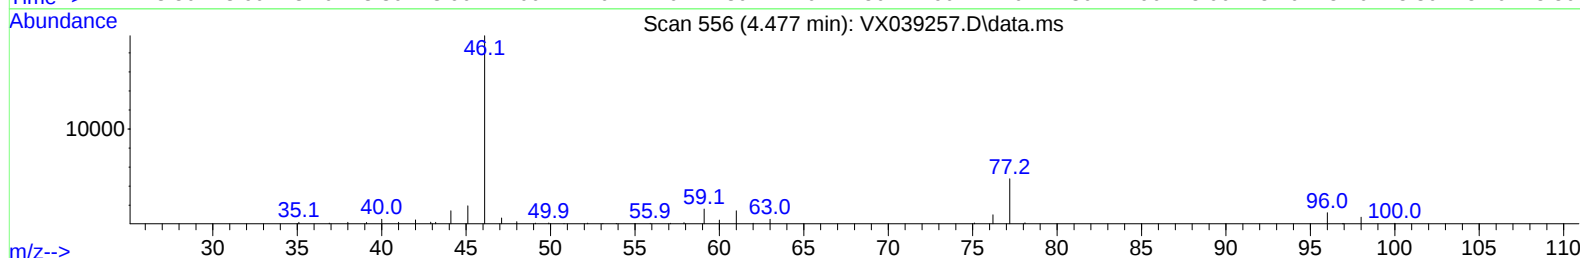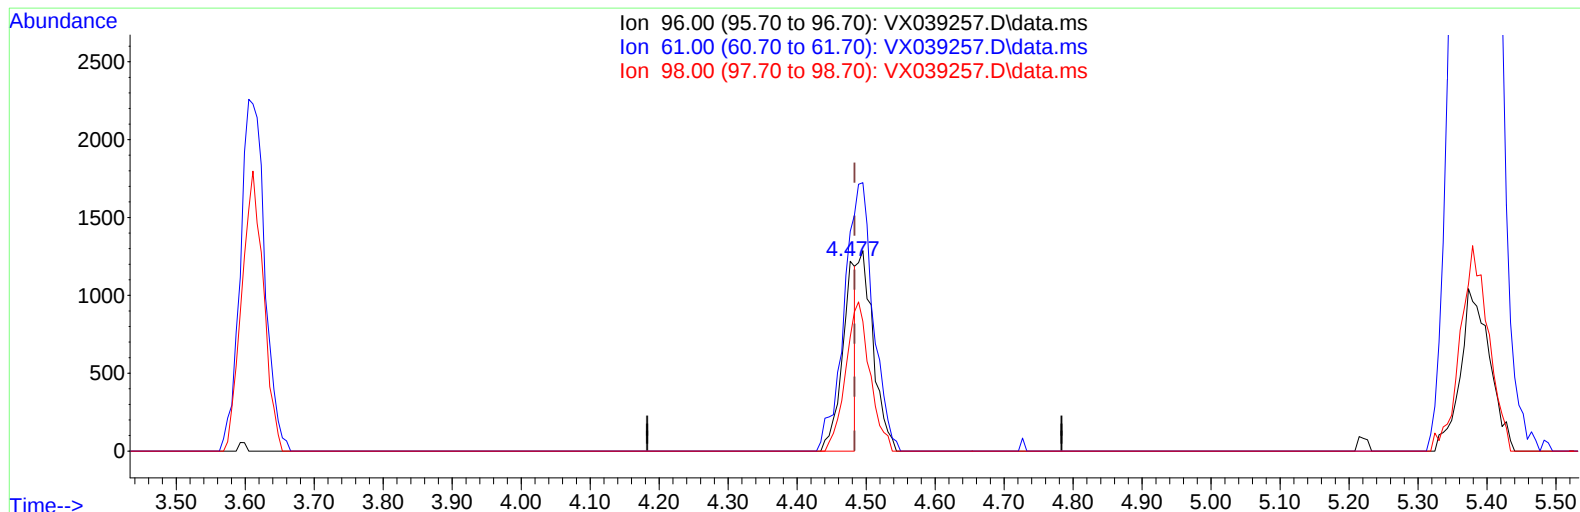

TIC: VX039257.D\data.ms

(20) cis-1,2-Dichloroethene (T)

4.477min (-0.006) 0.91 ug/L

response 1659

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	131.00	115.67
98.00	63.20	60.13
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121623\
Data File : VX039257.D
Acq On : 16 Dec 2023 02:23
Operator : JC/MD
Sample : 05845-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YCHD8

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/16/2023
Supervised By :Mahesh Dadoda 12/18/2023

Quant Time: Dec 16 04:21:09 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Dec 12 03:50:51 2023
Response via : Initial Calibration

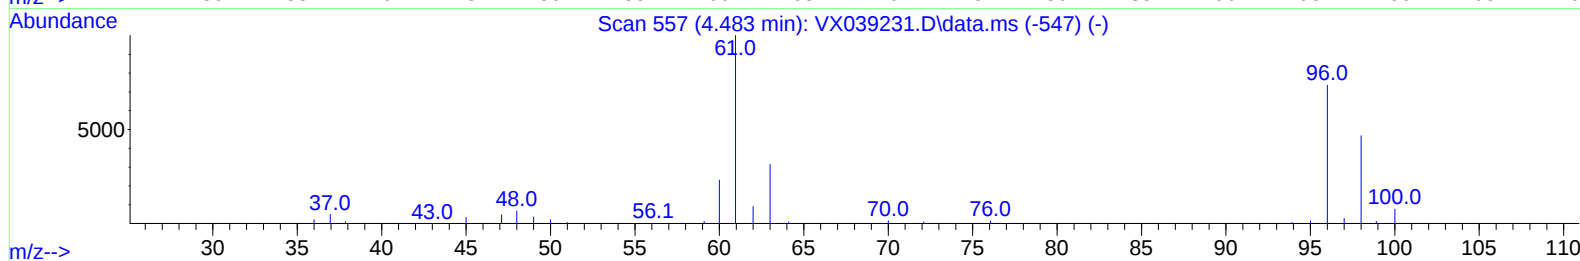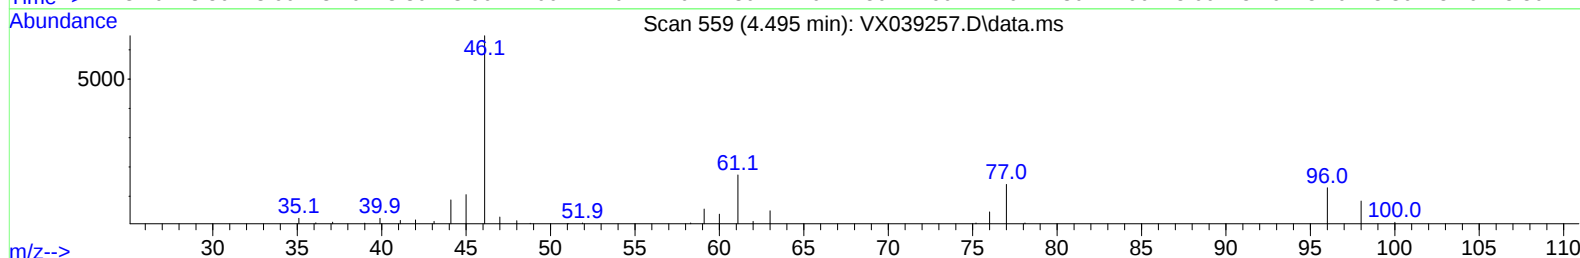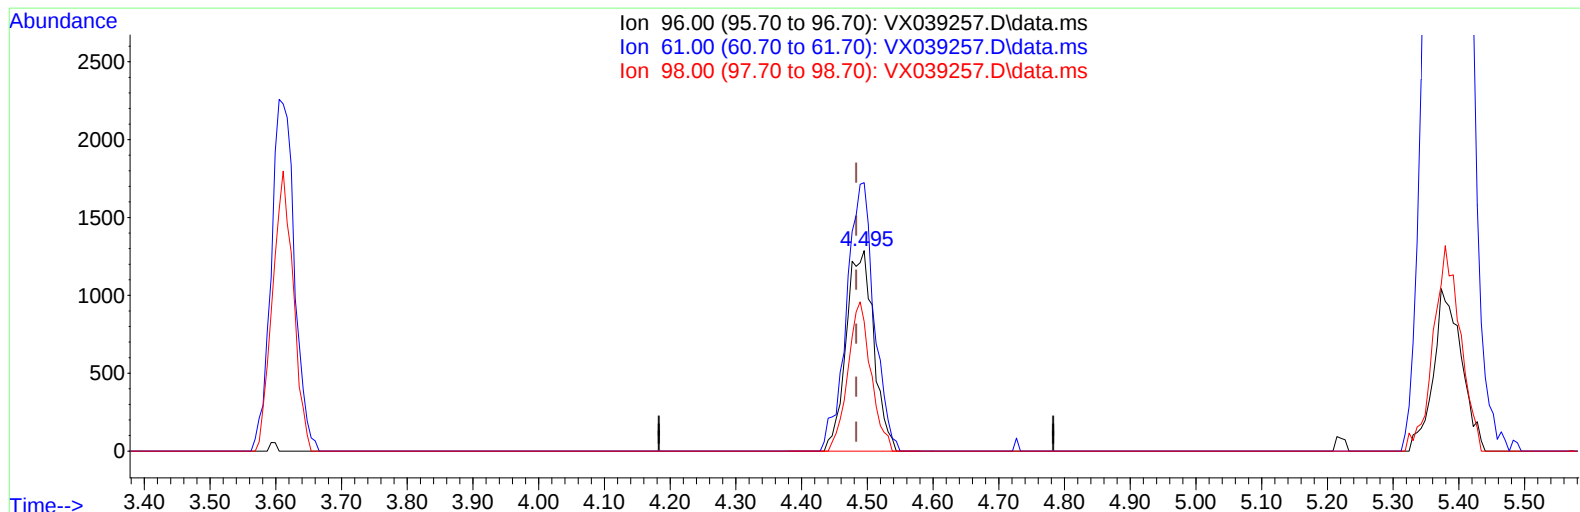

TIC: VX039257.D\data.ms

(20) cis-1,2-Dichloroethene (T)

4.495min (+ 0.012) 2.05 ug/L m

response 3730

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	131.00	133.95
98.00	63.20	64.65
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121623\
 Data File : VX039257.D
 Acq On : 16 Dec 2023 02:23
 Operator : JC/MD
 Sample : 05845-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YCHD8

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/16/2023
 Supervised By :Mahesh Dadoda 12/18/2023

Quant Time: Dec 16 04:21:09 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Dec 12 03:50:51 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	231474	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	219093	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	100023	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	61367	33.801	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	67.600%		
7) Chloroethane-d5	1.672	69	48999	36.513	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	73.020%		
11) 1,1-Dichloroethene-d2	2.306	65	33523	42.064	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	84.120%		
21) 2-Butanone-d5	4.446	46	150526	91.592	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	91.590%		
24) Chloroform-d	5.056	84	140714	43.782	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.560%		
26) 1,2-Dichloroethane-d4	5.952	65	101288	48.662	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.320%		
32) Benzene-d6	5.970	84	280935	41.548	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	83.100%		
36) 1,2-Dichloropropane-d6	7.306	67	92398	42.462	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	84.920%		
41) Toluene-d8	8.647	98	249999	40.799	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	81.600%		
43) trans-1,3-Dichloroprop...	8.952	79	42291	38.191	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	76.380%		
47) 2-Hexanone-d5	9.384	63	106808	82.181	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	82.180%		
56) 1,1,2,2-Tetrachloroeth...	11.189	84	136099	44.089	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	88.180%		
66) 1,2-Dichlorobenzene-d4	12.317	152	88623	46.875	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	93.760%		
Target Compounds						
5) Vinyl chloride	1.374	62	2666	1.402	ug/L #	54
10) 1,1,2-Trichloro-1,2,2-...	2.325	101	7666	4.836	ug/L #	82
12) 1,1-Dichloroethene	2.319	96	378423	253.774	ug/L #	72
13) Acetone	2.374	43	222907	141.187	ug/L	96
18) Methyl tert-butyl Ether	3.111	73	11898	2.176	ug/L	97
19) 1,1-Dichloroethane	3.611	63	64068	20.623	ug/L	98
20) cis-1,2-Dichloroethene	4.495	96	3730m	2.047	ug/L	
22) 2-Butanone	4.568	43	16944	8.745	ug/L	98
27) 1,2-Dichloroethane	6.086	62	28544	11.671	ug/L #	92
30) 1,1,1-Trichloroethane	5.379	97	93961	35.346	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121623\
Data File : VX039257.D
Acq On : 16 Dec 2023 02:23
Operator : JC/MD
Sample : 05845-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YCHD8

Manual IntegrationsAPPROVED

Quant Time: Dec 16 04:21:09 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Dec 12 03:50:51 2023
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/16/2023
Supervised By :Mahesh Dadoda 12/18/2023

