

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121623\
 Data File : VX039290.D
 Acq On : 16 Dec 2023 15:07
 Operator : JC/MD
 Sample : 05845-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YCHE3

Quant Time: Dec 16 21:12:46 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Dec 12 03:50:51 2023
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By :Mahesh Dadoda 12/18/2023
 Supervised By :Semsettin Yesilyurt 12/18/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	212697	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	198302	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	92634	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	68450	41.030	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	82.060%		
7) Chloroethane-d5	1.666	69	51811	42.017	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	84.040%		
11) 1,1-Dichloroethene-d2	2.306	65	35506	48.485	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	96.960%		
21) 2-Butanone-d5	4.452	46	152135	100.743	ug/L	0.01
Spiked Amount 100.000	Range 40 - 130		Recovery =	100.740%		
24) Chloroform-d	5.056	84	142336	48.196	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.400%		
26) 1,2-Dichloroethane-d4	5.952	65	98371	51.433	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	102.860%		
32) Benzene-d6	5.976	84	289347	47.279	ug/L	0.01
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.560%		
36) 1,2-Dichloropropane-d6	7.312	67	93001	47.220	ug/L	0.01
Spiked Amount 50.000	Range 70 - 120		Recovery =	94.440%		
41) Toluene-d8	8.647	98	262183	47.273	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	94.540%		
43) trans-1,3-Dichloroprop...	8.952	79	42117	42.022	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	84.040%		
47) 2-Hexanone-d5	9.384	63	108326	92.087	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	92.090%		
56) 1,1,2,2-Tetrachloroeth...	11.189	84	132025	47.254	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	94.500%		
66) 1,2-Dichlorobenzene-d4	12.317	152	86432	49.363	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	98.720%		
Target Compounds						
5) Vinyl chloride	1.374	62	2032	1.163	ug/L #	12
12) 1,1-Dichloroethene	2.319	96	25828	18.850	ug/L #	42
13) Acetone	2.373	43	49859	34.368	ug/L	95
19) 1,1-Dichloroethane	3.611	63	6579	2.305	ug/L	97
20) cis-1,2-Dichloroethene	4.489	96	43413	25.925	ug/L	95
22) 2-Butanone	4.556	43	42549	23.898	ug/L	100
30) 1,1,1-Trichloroethane	5.379	97	3701m	1.538	ug/L	
34) Trichloroethene	7.123	95	82280	49.405	ug/L	98
37) 1,2-Dichloropropane	7.440	63	1724	0.986	ug/L	99
46) Tetrachloroethene	9.275	164	1462	1.331	ug/L #	83

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121623\
Data File : VX039290.D
Acq On : 16 Dec 2023 15:07
Operator : JC/MD
Sample : 05845-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 61 Sample Multiplier: 1


Instrument :
MSVOA_X
ClientSampleId :
YCHE3

Quant Time: Dec 16 21:12:46 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Dec 12 03:50:51 2023
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 12/18/2023
Supervised By :Semsettin Yesilyurt 12/18/2023

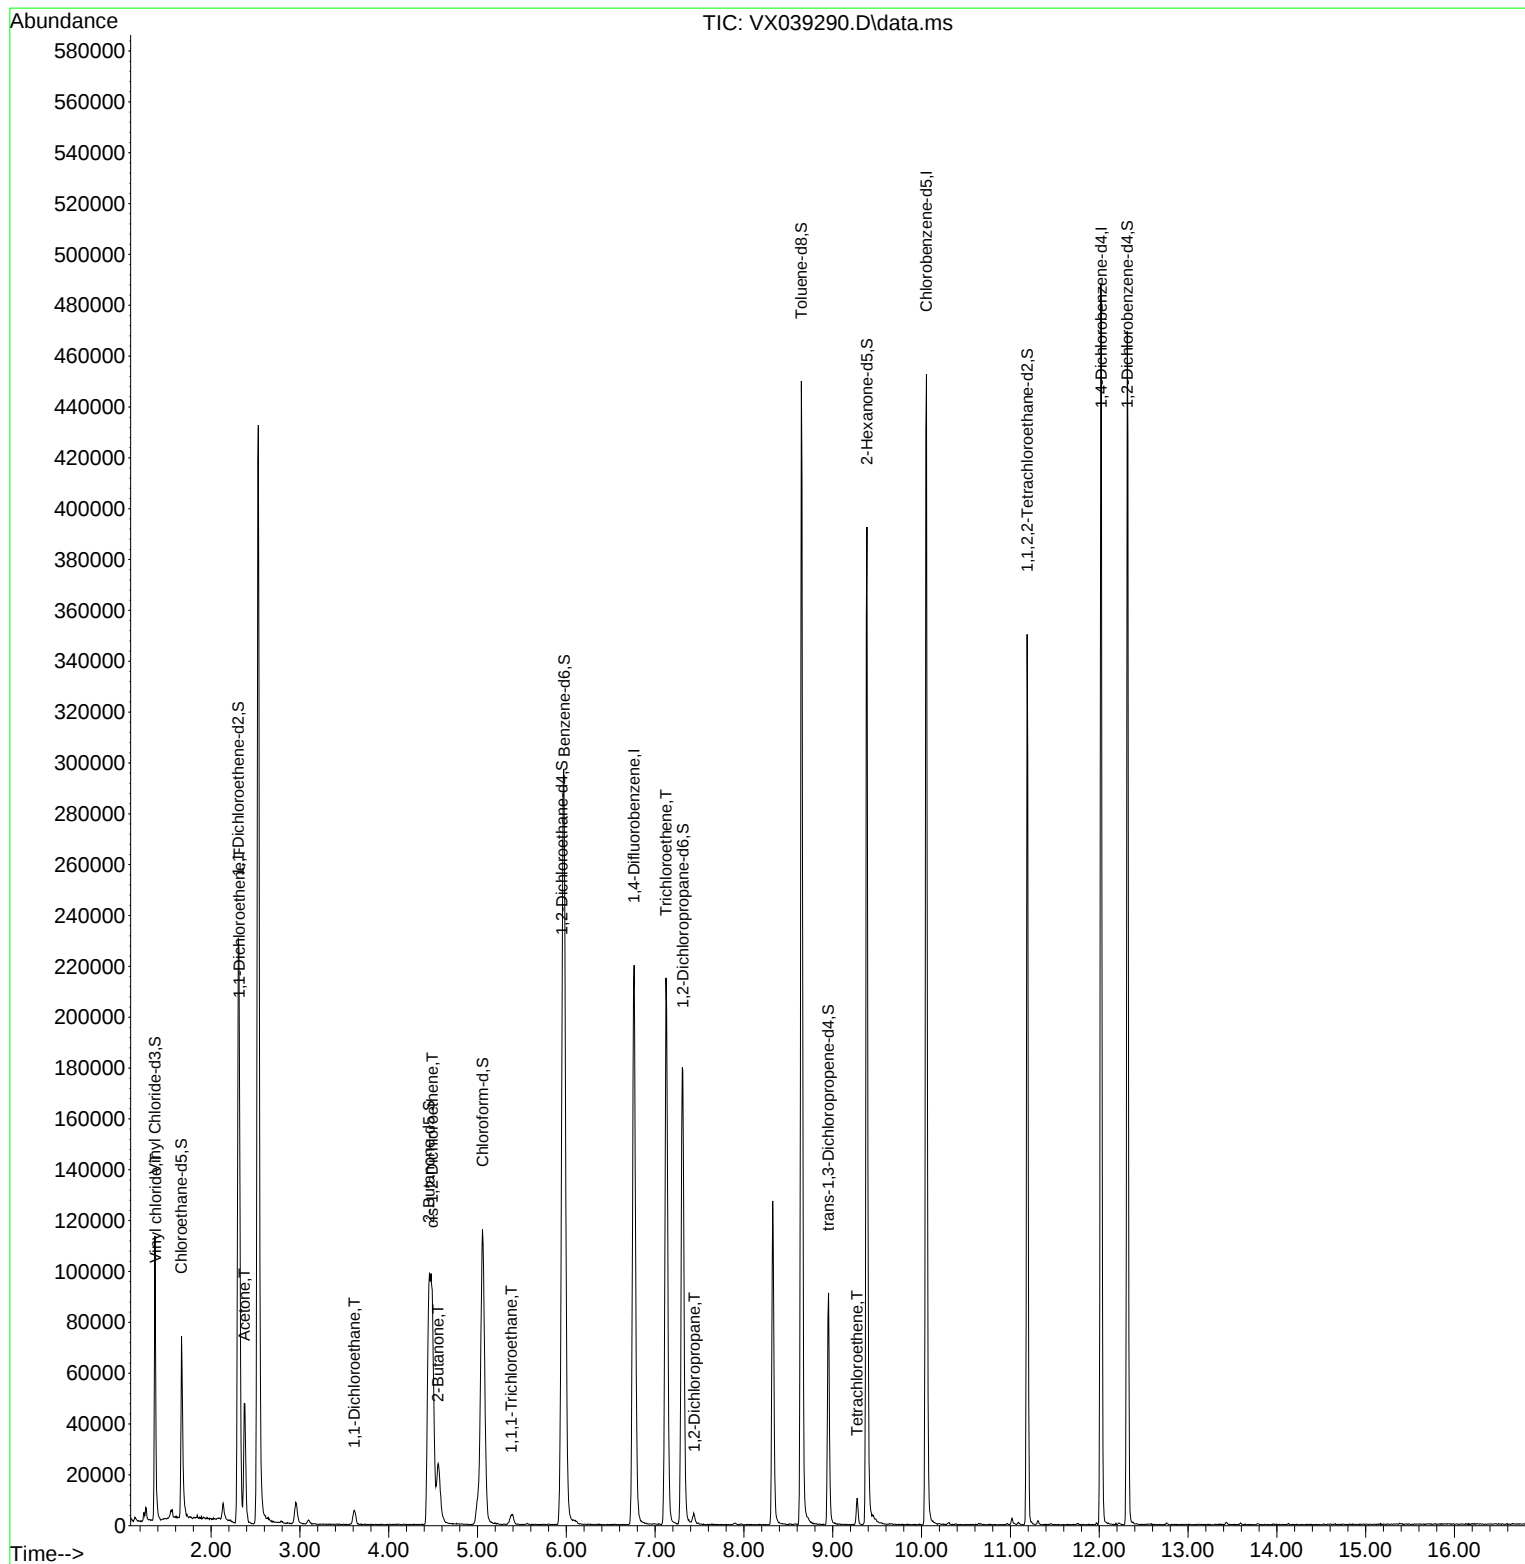

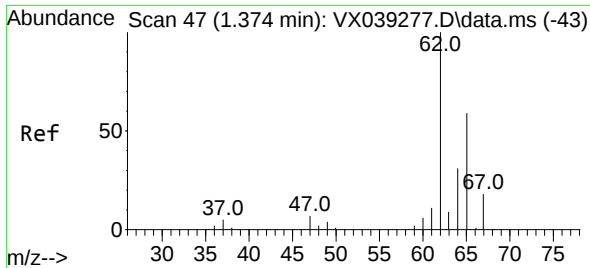





#5
 Vinyl chloride
 Concen: 1.163 ug/L
 RT: 1.374 min Scan# 41
 Delta R.T. -0.000 min
 Lab File: VX039290.D
 Acq: 16 Dec 2023 15:07

Instrument :
 MSVOA_X
 ClientSampleId :
 YCHE3

Tgt Ion: 62 Resp: 203
 Ion Ratio Lower Upper
 62 100
 64 80.8 22.3 41.3




Manual Integrations
 APPROVED


Reviewed By :Mahesh Dadoda 12/18/2023
 Supervised By :Semsettin Yesilyurt 12/18/2023

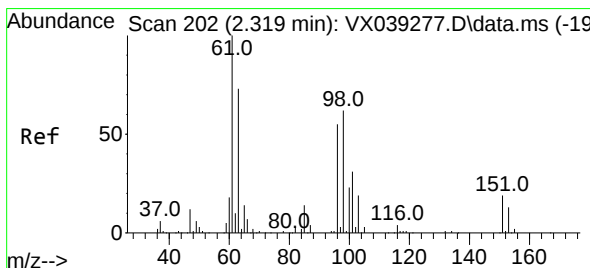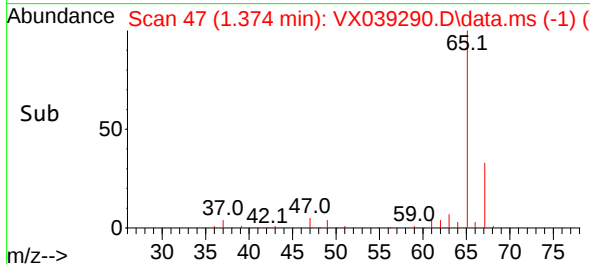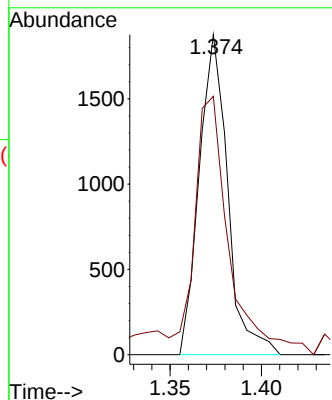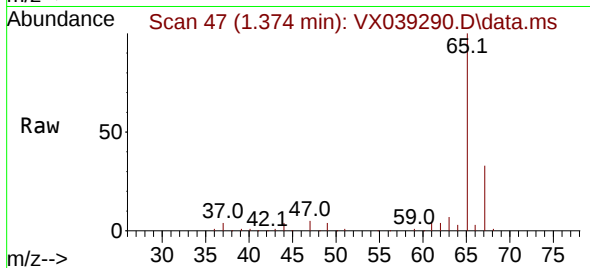

#12
 1,1-Dichloroethene
 Concen: 18.850 ug/L
 RT: 2.319 min Scan# 202
 Delta R.T. -0.000 min
 Lab File: VX039290.D
 Acq: 16 Dec 2023 15:07

Tgt Ion: 96 Resp: 25828
 Ion Ratio Lower Upper
 96 100
 61 206.2 128.0 237.6
 63 283.7 101.5 188.5

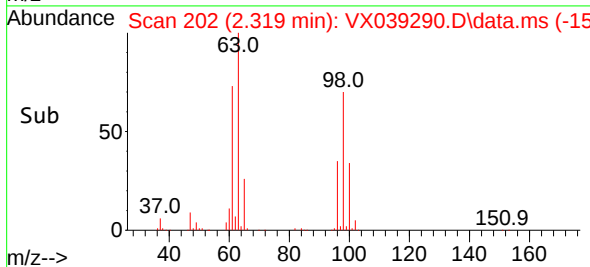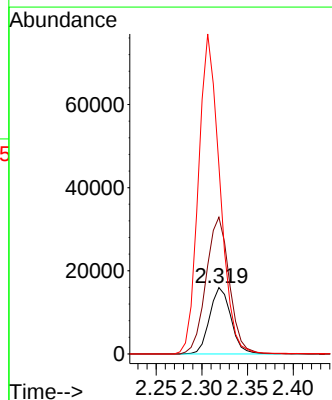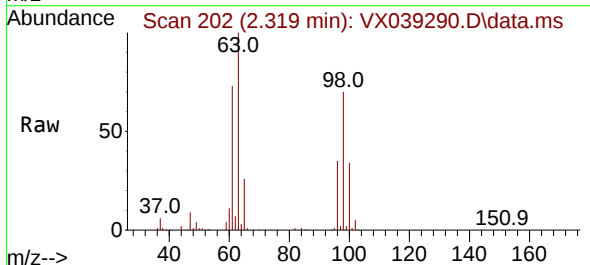

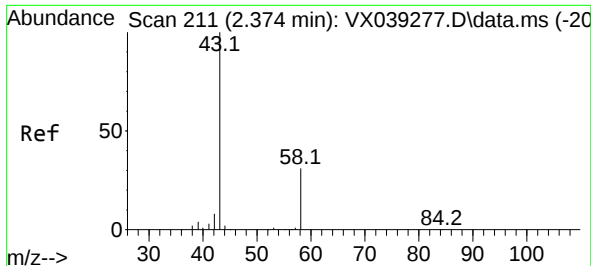





#13
Acetone
Concen: 34.368 ug/L
RT: 2.373 min Scan# 211
Delta R.T. -0.000 min
Lab File: VX039290.D
Acq: 16 Dec 2023 15:07

Instrument :
MSVOA_X
ClientSampleId :
YCHE3

Tgt Ion: 43 Resp: 4985
Ion Ratio Lower Upper
43 100
58 30.0 0.0 65.8




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 12/18/2023
Supervised By :Semsettin Yesilyurt 12/18/2023

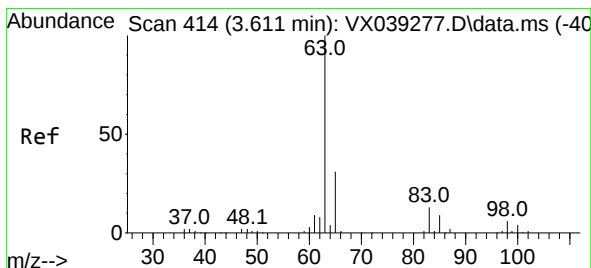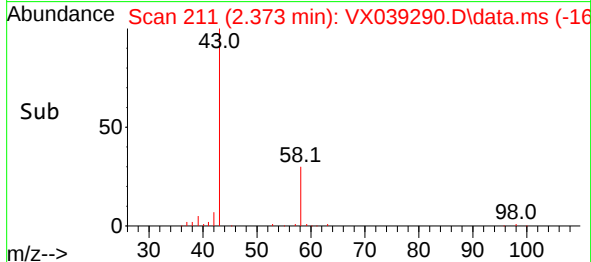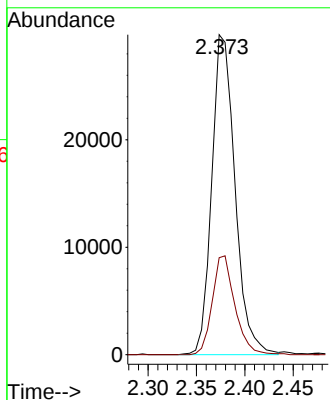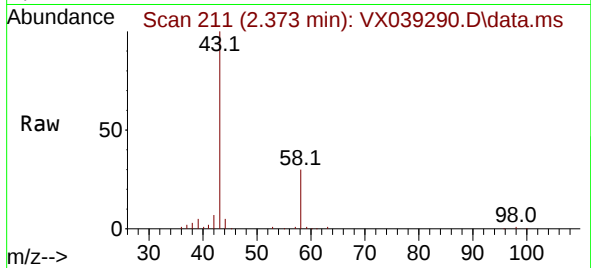

#19
1,1-Dichloroethane
Concen: 2.305 ug/L
RT: 3.611 min Scan# 414
Delta R.T. 0.006 min
Lab File: VX039290.D
Acq: 16 Dec 2023 15:07

Tgt Ion: 63 Resp: 6579
Ion Ratio Lower Upper
63 100
65 28.2 21.1 39.3
83 14.2 9.7 17.9

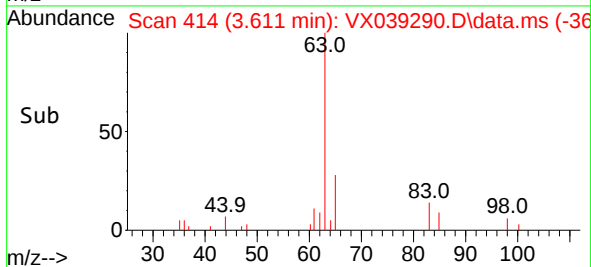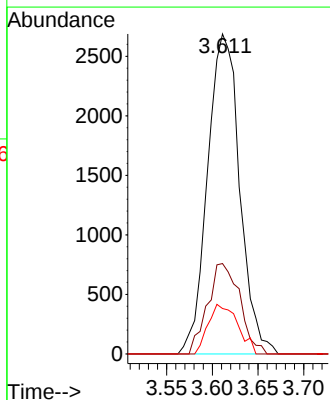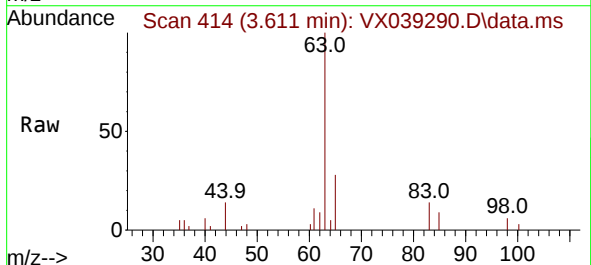

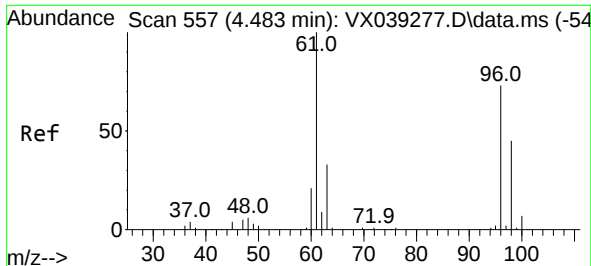





#20
cis-1,2-Dichloroethene
Concen: 25.925 ug/L
RT: 4.489 min Scan# 511
Delta R.T. 0.006 min
Lab File: VX039290.D
Acq: 16 Dec 2023 15:07

Instrument :
MSVOA_X
ClientSampleId :
YCHE3

Tgt Ion: 96 Resp: 4341
Ion Ratio Lower Upper
96 100
61 137.8 91.7 170.3
98 64.6 44.2 82.2




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 12/18/2023
Supervised By :Semsettin Yesilyurt 12/18/2023

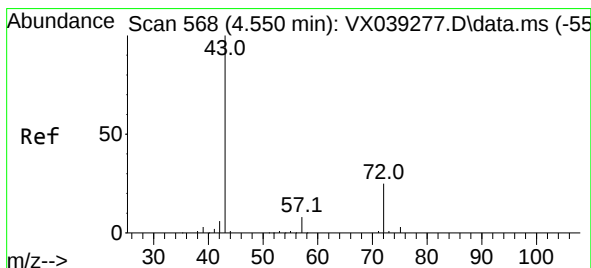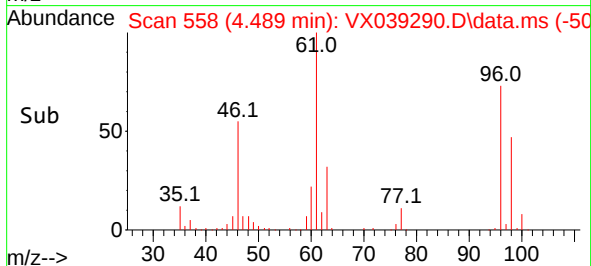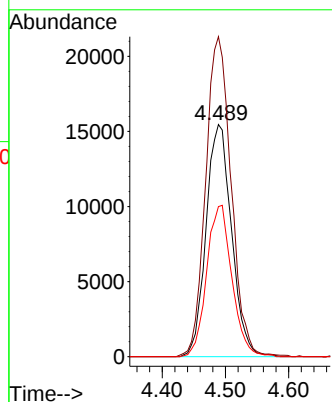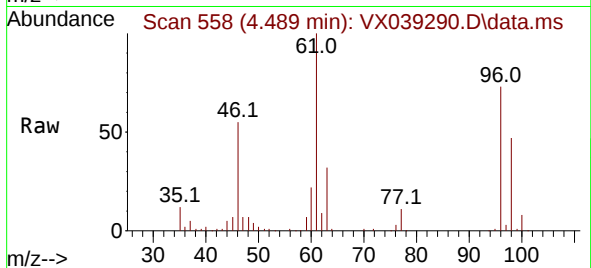

#22
2-Butanone
Concen: 23.898 ug/L
RT: 4.556 min Scan# 569
Delta R.T. 0.012 min
Lab File: VX039290.D
Acq: 16 Dec 2023 15:07

Tgt Ion: 43 Resp: 42549
Ion Ratio Lower Upper
43 100
72 25.3 12.6 37.6

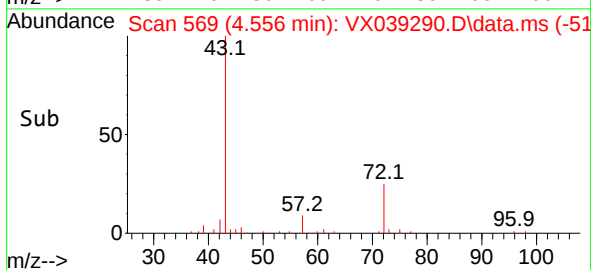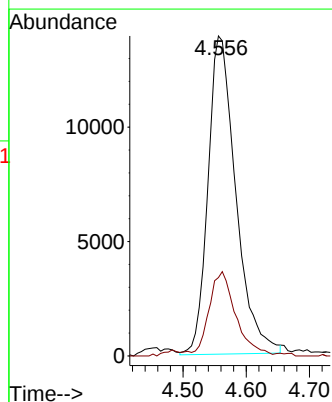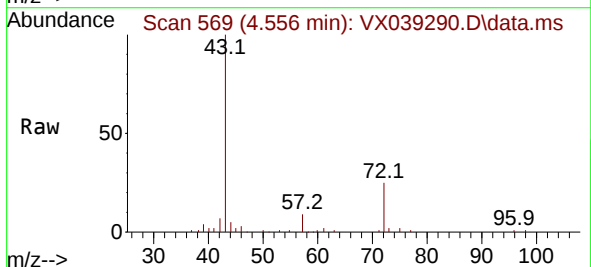

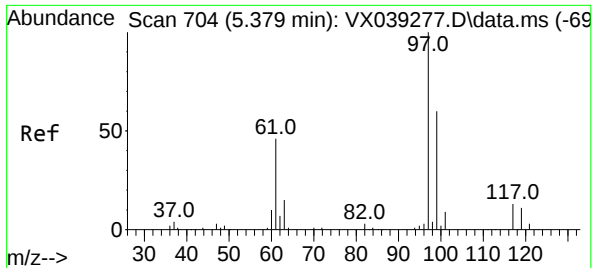

#30

1,1,1-Trichloroethane

Concen: 1.538 ug/L m

RT: 5.379 min Scan# 704

Delta R.T. 0.006 min

Lab File: VX039290.D

Acq: 16 Dec 2023 15:07

Instrument :

MSVOA_X

ClientSampleId :

YCCE3





Tgt Ion: 97 Resp: 370

Ion	Ratio	Lower	Upper
97	100		
99	0.0	51.0	76.4
61	0.0	36.7	55.1

Manual Integrations

APPROVED

Reviewed By :Mahesh Dadoda 12/18/2023
Supervised By :Semsettin Yesilyurt 12/18/2023

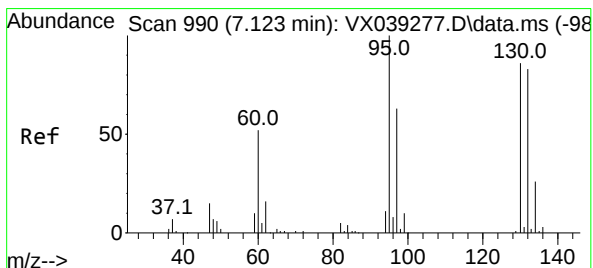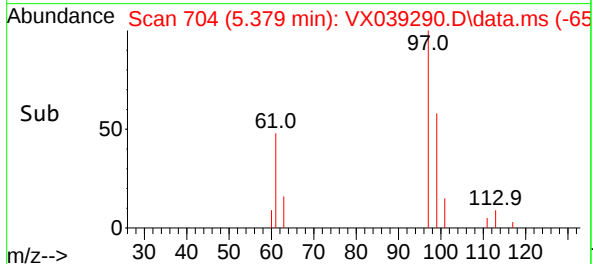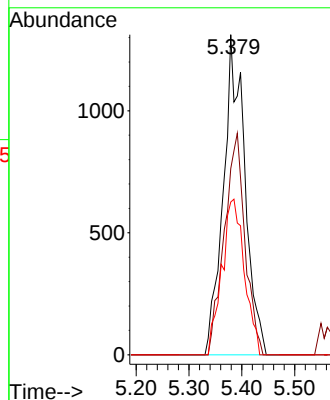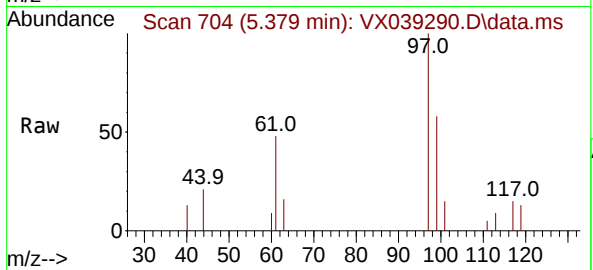

#34

Trichloroethene

Concen: 49.405 ug/L

RT: 7.123 min Scan# 990




Delta R.T. 0.006 min


Lab File: VX039290.D

Acq: 16 Dec 2023 15:07

Tgt Ion: 95 Resp: 82280

Ion	Ratio	Lower	Upper
95	100		
97	62.7	45.5	84.5
132	89.1	62.2	115.4
130	92.4	67.0	124.4

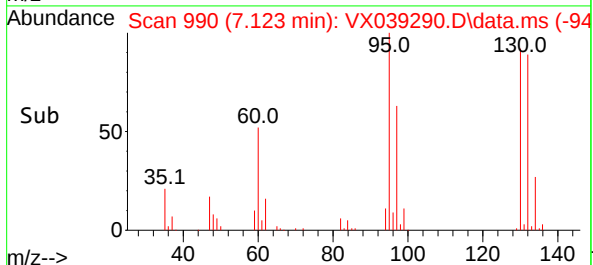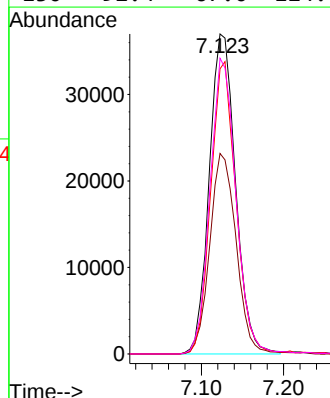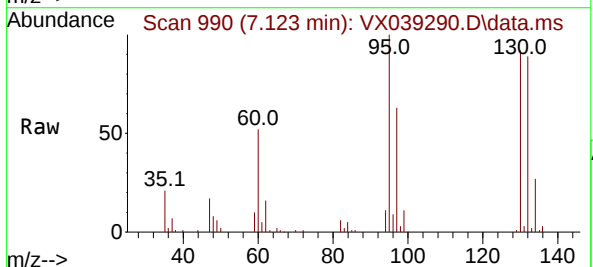

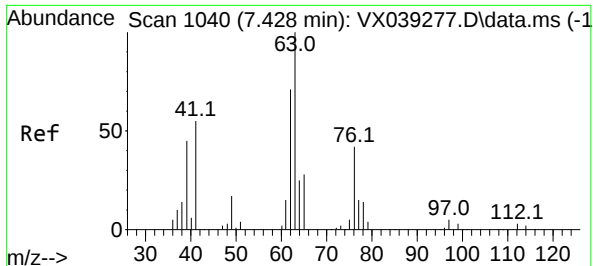

#37

1,2-Dichloropropane

Concen: 0.986 ug/L

RT: 7.440 min Scan# 1042

Delta R.T. 0.012 min

Lab File: VX039290.D

Acq: 16 Dec 2023 15:07

Instrument :

MSVOA_X

ClientSampleId :





YCCE3

Tgt Ion: 63 Resp: 1724
 Ion Ratio Lower Upper
 63 100
 112 3.1 2.8 4.2

Manual Integrations

APPROVED

Reviewed By :Mahesh Dadoda 12/18/2023
 Supervised By :Semsettin Yesilyurt 12/18/2023

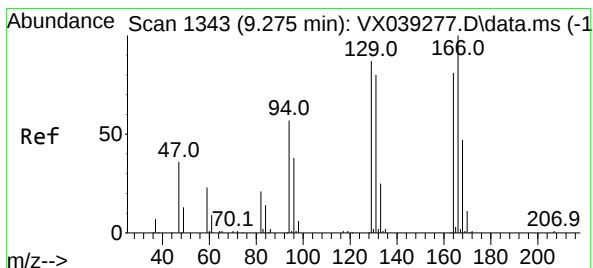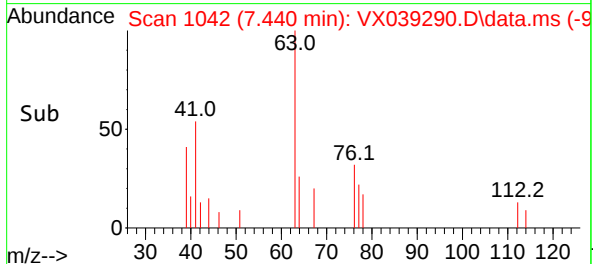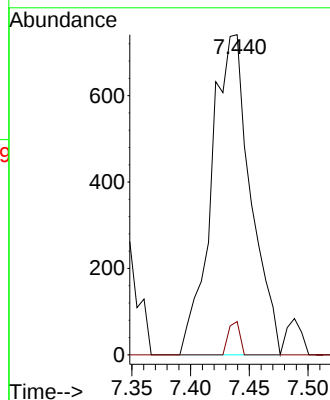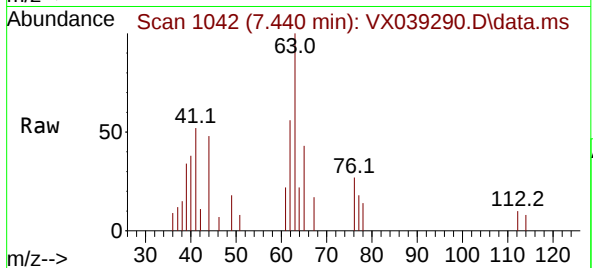

#46

Tetrachloroethene

Concen: 1.331 ug/L

RT: 9.275 min Scan# 1343

Delta R.T. 0.006 min

Lab File: VX039290.D

Acq: 16 Dec 2023 15:07

Tgt Ion:164 Resp: 1462
 Ion Ratio Lower Upper
 164 100
 129 110.3 71.9 133.5
 131 136.1 69.5 129.1#
 166 140.9 90.3 167.7

