

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121623\
 Data File : VX039250.D
 Acq On : 15 Dec 2023 23:43
 Operator : JC/MD
 Sample : 05844-21
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YCHK8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039250.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.233	22	24	27	rBV3	979	1219	0.13%	0.017%
2	1.367	42	46	55	rBV	99130	105118	11.60%	1.494%
3	1.666	91	95	112	rVB	63042	97885	10.81%	1.392%
4	2.306	194	200	208	rBV	186240	292478	32.29%	4.158%
5	2.526	231	236	241	rBV2	514	999	0.11%	0.014%
6	2.666	256	259	262	rBV2	341	391	0.04%	0.006%
7	2.788	276	279	285	rVB4	482	819	0.09%	0.012%
8	2.946	301	305	312	rVB2	1355	2708	0.30%	0.038%
9	3.050	318	322	324	rBV2	233	339	0.04%	0.005%
10	3.105	328	331	334	rBV2	254	397	0.04%	0.006%
11	3.257	354	356	359	rBV2	240	266	0.03%	0.004%
12	3.623	415	416	419	rBV2	229	241	0.03%	0.003%
13	4.099	492	494	495	rVB	455	197	0.02%	0.003%
14	4.282	522	524	527	rBV2	220	251	0.03%	0.004%
15	4.306	527	528	531	rVB	313	239	0.03%	0.003%
16	4.452	543	552	565	rBV	86174	246206	27.18%	3.500%
17	4.970	635	637	640	rBV	283	271	0.03%	0.004%
18	5.056	640	651	672	rVV	113447	362452	40.01%	5.153%
19	5.397	703	707	711	rVB4	421	706	0.08%	0.010%
20	5.495	718	723	724	rBV2	299	440	0.05%	0.006%
21	5.629	743	745	749	rVB2	259	319	0.04%	0.005%
22	5.763	764	767	770	rBV	211	270	0.03%	0.004%
23	5.970	788	801	826	rBV2	300012	905852	100.00%	12.878%
24	6.214	839	841	844	rBV	253	280	0.03%	0.004%
25	6.245	844	846	851	rVB2	390	374	0.04%	0.005%
26	6.458	878	881	885	rBV3	376	588	0.06%	0.008%
27	6.543	892	895	898	rVB3	251	333	0.04%	0.005%
28	6.592	902	903	908	rBV	256	228	0.03%	0.003%
29	6.757	921	930	948	rBV	223205	539258	59.53%	7.666%
30	6.970	963	965	969	rVB2	224	206	0.02%	0.003%
31	7.098	984	986	987	rBV2	347	285	0.03%	0.004%
32	7.305	1012	1020	1039	rBV	186704	416855	46.02%	5.926%
33	7.659	1075	1078	1080	rBV2	381	470	0.05%	0.007%
34	7.708	1085	1086	1089	rVB2	276	198	0.02%	0.003%
35	8.104	1146	1151	1153	rBV2	213	349	0.04%	0.005%
36	8.208	1165	1168	1170	rBV	256	211	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121623\
 Data File : VX039250.D
 Acq On : 15 Dec 2023 23:43
 Operator : JC/MD
 Sample : 05844-21
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YCHK8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

37	8.324	1180	1187	1197	rBV	131534	215743	23.82%	3.067%
38	8.445	1204	1207	1210	rBV2	362	425	0.05%	0.006%
39	8.476	1210	1212	1213	rVB	392	222	0.02%	0.003%
40	8.506	1213	1217	1218	rBV2	254	329	0.04%	0.005%
41	8.647	1233	1240	1255	rBV	460908	712585	78.66%	10.130%
42	8.951	1284	1290	1306	rBV	94548	144190	15.92%	2.050%
43	9.269	1340	1342	1348	rVB2	568	724	0.08%	0.010%
44	9.329	1348	1352	1355	rVB3	379	401	0.04%	0.006%
45	9.384	1355	1361	1378	rBV	383547	568231	62.73%	8.078%
46	9.787	1425	1427	1429	rBV2	258	299	0.03%	0.004%
47	9.951	1450	1454	1456	rVB2	192	216	0.02%	0.003%
48	10.055	1465	1471	1487	rBV	471275	658348	72.68%	9.359%
49	10.213	1494	1497	1500	rVB2	258	344	0.04%	0.005%
50	10.262	1502	1505	1506	rBV	206	245	0.03%	0.003%
51	10.299	1508	1511	1515	rVB2	234	336	0.04%	0.005%
52	10.622	1562	1564	1567	rBV2	233	252	0.03%	0.004%
53	10.658	1567	1570	1574	rVB2	200	275	0.03%	0.004%
54	10.689	1574	1575	1577	rBV2	269	246	0.03%	0.003%
55	11.085	1637	1640	1646	rBV4	1045	1573	0.17%	0.022%
56	11.140	1646	1649	1651	rVV2	218	289	0.03%	0.004%
57	11.189	1651	1657	1668	rVV	368253	466467	51.49%	6.631%
58	11.311	1672	1677	1683	rVV4	1172	1945	0.21%	0.028%
59	11.408	1691	1693	1695	rBV	265	258	0.03%	0.004%
60	11.451	1698	1700	1705	rBV	243	334	0.04%	0.005%
61	11.494	1705	1707	1709	rVB2	244	211	0.02%	0.003%
62	11.555	1715	1717	1720	rBV2	182	211	0.02%	0.003%
63	11.707	1740	1742	1744	rVB2	317	212	0.02%	0.003%
64	11.750	1747	1749	1752	rBV2	319	325	0.04%	0.005%
65	11.969	1782	1785	1788	rBV2	263	436	0.05%	0.006%
66	12.018	1788	1793	1807	rBV	485290	632879	69.87%	8.997%
67	12.317	1837	1842	1856	rVV	501883	636438	70.26%	9.048%
68	12.530	1874	1877	1883	rVB2	193	367	0.04%	0.005%
69	12.585	1883	1886	1887	rBV	261	286	0.03%	0.004%
70	12.737	1908	1911	1912	rBV	211	218	0.02%	0.003%
71	12.762	1912	1915	1918	rVV	543	567	0.06%	0.008%
72	12.786	1918	1919	1924	rVB2	269	359	0.04%	0.005%
73	13.085	1967	1968	1972	rBV2	188	217	0.02%	0.003%
74	13.329	2005	2008	2010	rBV2	210	231	0.03%	0.003%
75	13.378	2012	2016	2017	rBV	317	345	0.04%	0.005%
76	13.597	2049	2052	2054	rBV2	330	349	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121623\
 Data File : VX039250.D
 Acq On : 15 Dec 2023 23:43
 Operator : JC/MD
 Sample : 05844-21
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YCHK8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

77	13.780	2080	2082	2084	rBV2	309	263	0.03%	0.004%
78	13.871	2094	2097	2099	rBV	256	258	0.03%	0.004%
79	13.914	2103	2104	2108	rVV	219	247	0.03%	0.004%
80	13.975	2112	2114	2116	rVV	251	213	0.02%	0.003%
81	14.018	2119	2121	2122	rVV	399	228	0.03%	0.003%
82	14.085	2128	2132	2135	rBV2	253	415	0.05%	0.006%
83	14.133	2138	2140	2142	rVV	338	287	0.03%	0.004%
84	14.231	2154	2156	2157	rBV	269	207	0.02%	0.003%
85	14.646	2220	2224	2225	rBV	297	258	0.03%	0.004%
86	14.780	2245	2246	2248	rBV	346	275	0.03%	0.004%
87	14.865	2258	2260	2262	rVB	217	201	0.02%	0.003%
88	14.908	2265	2267	2268	rBV	396	303	0.03%	0.004%
89	15.005	2281	2283	2288	rBV2	198	253	0.03%	0.004%
90	15.206	2313	2316	2317	rBV2	267	249	0.03%	0.004%
91	15.456	2355	2357	2358	rBV2	293	218	0.02%	0.003%
92	15.749	2403	2405	2407	rBV	273	286	0.03%	0.004%
93	15.853	2421	2422	2424	rBV	330	214	0.02%	0.003%
94	15.981	2439	2443	2444	rBV2	318	384	0.04%	0.005%
95	16.115	2464	2465	2467	rBV2	349	207	0.02%	0.003%
96	16.231	2483	2484	2486	rBV	298	196	0.02%	0.003%
97	16.340	2499	2502	2506	rBV3	323	547	0.06%	0.008%
98	16.511	2529	2530	2535	rBV2	343	407	0.04%	0.006%
99	16.584	2540	2542	2544	rBV3	241	263	0.03%	0.004%
100	16.718	2563	2564	2565	rBV	461	200	0.02%	0.003%

Sum of corrected areas: 7034205




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121623\
Data File : VX039250.D
Acq On : 15 Dec 2023 23:43
Operator : JC/MD
Sample : 05844-21
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YCHK8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

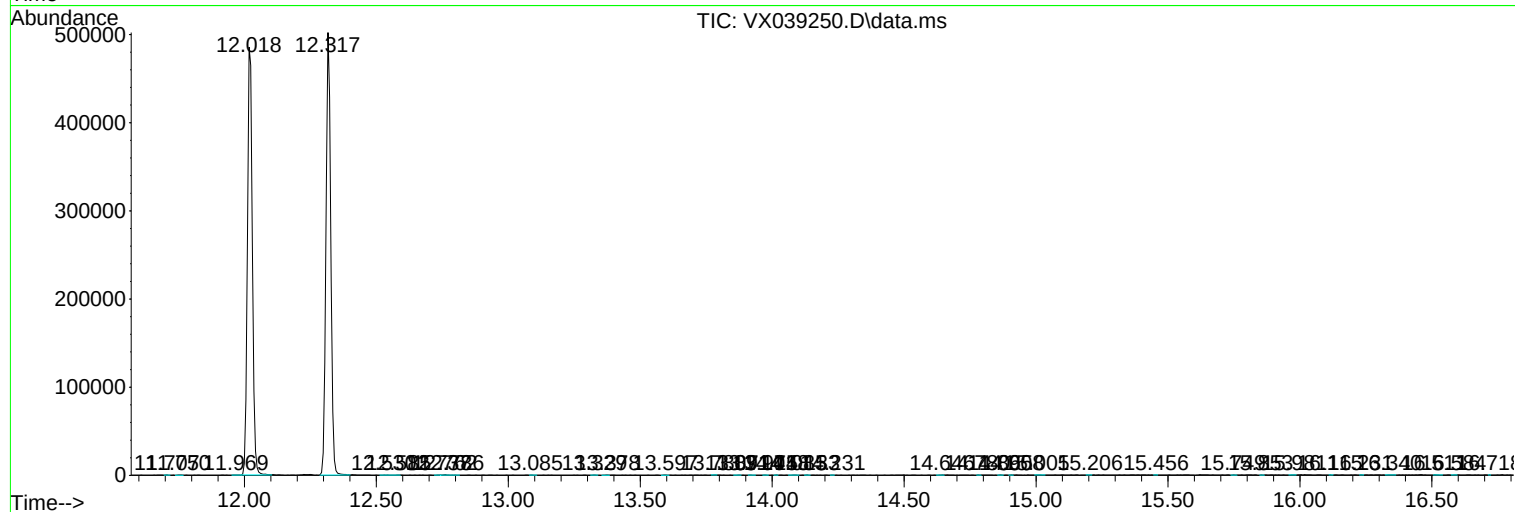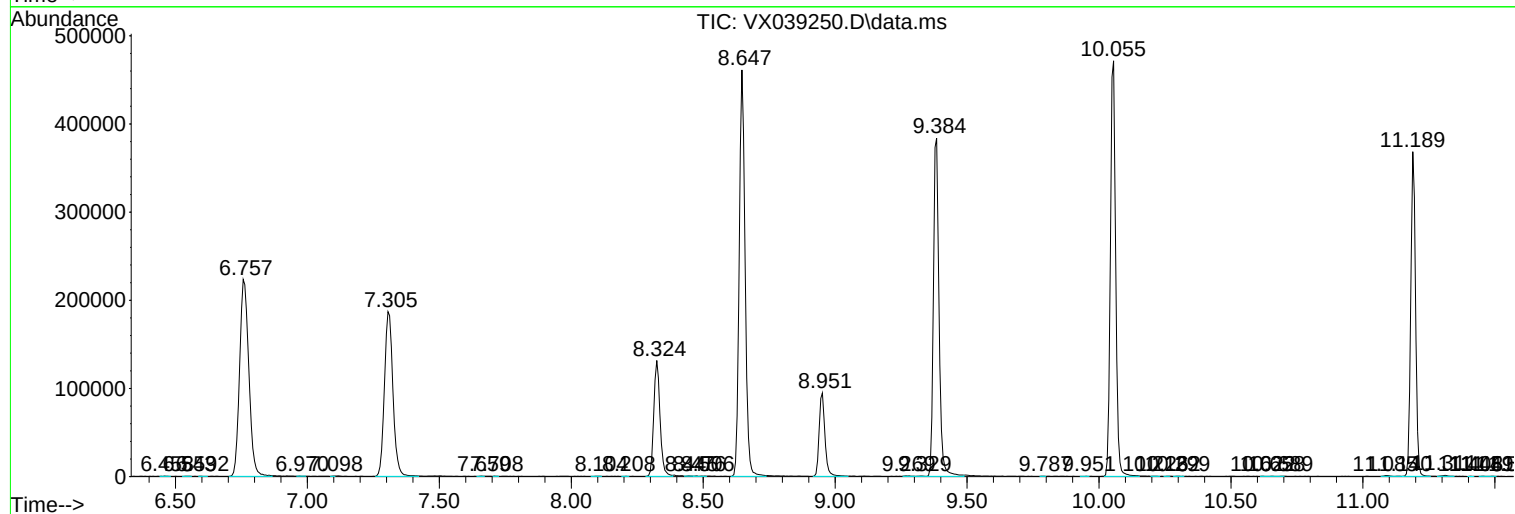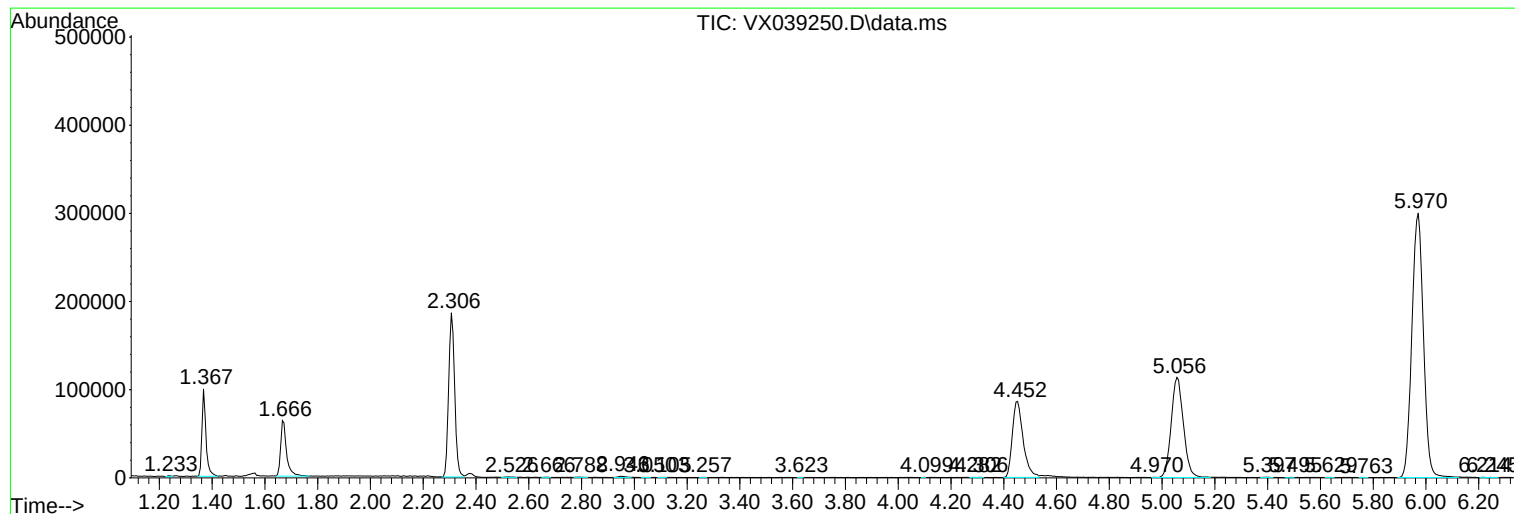

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121623\
Data File : VX039250.D
Acq On : 15 Dec 2023 23:43
Operator : JC/MD
Sample : 05844-21
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YCHK8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121623\
Data File : VX039250.D
Acq On : 15 Dec 2023 23:43
Operator : JC/MD
Sample : 05844-21
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YCHK8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc