

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121623\
 Data File : VX039255.D
 Acq On : 16 Dec 2023 01:37
 Operator : JC/MD
 Sample : VX1216WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK646

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039255.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	57	rBV	114346	124909	13.45%	1.750%
2	1.666	91	95	109	rBV	71016	105908	11.41%	1.484%
3	2.306	194	200	210	rBV	205032	322491	34.73%	4.519%
4	2.459	223	225	227	rVB2	366	271	0.03%	0.004%
5	2.508	229	233	239	rBV2	2653	4667	0.50%	0.065%
6	2.642	253	255	257	rBV2	250	212	0.02%	0.003%
7	2.782	275	278	286	rVB4	1238	2069	0.22%	0.029%
8	2.947	301	305	309	rVB3	466	819	0.09%	0.011%
9	3.020	313	317	319	rBV2	262	319	0.03%	0.004%
10	3.093	325	329	334	rBV2	1191	2055	0.22%	0.029%
11	3.294	359	362	365	rBV2	191	229	0.02%	0.003%
12	3.507	393	397	398	rBV2	182	208	0.02%	0.003%
13	3.562	404	406	409	rVB2	156	153	0.02%	0.002%
14	3.605	409	413	415	rBV	355	569	0.06%	0.008%
15	3.702	425	429	431	rBV	183	203	0.02%	0.003%
16	3.837	448	451	452	rBV2	153	168	0.02%	0.002%
17	3.989	473	476	478	rBV	145	163	0.02%	0.002%
18	4.099	492	494	496	rBV2	201	219	0.02%	0.003%
19	4.446	543	551	568	rBV	81509	236170	25.43%	3.310%
20	4.678	587	589	591	rVB2	299	204	0.02%	0.003%
21	4.702	591	593	595	rBB2	352	202	0.02%	0.003%
22	5.056	638	651	668	rBV2	112510	366986	39.52%	5.143%
23	5.324	693	695	698	rBV2	140	154	0.02%	0.002%
24	5.403	702	708	711	rVV2	343	564	0.06%	0.008%
25	5.550	731	732	734	rBV	361	342	0.04%	0.005%
26	5.726	759	761	764	rVB2	197	193	0.02%	0.003%
27	5.824	774	777	778	rBV	274	237	0.03%	0.003%
28	5.970	789	801	816	rBV2	306870	928606	100.00%	13.013%
29	6.330	859	860	862	rBV	230	155	0.02%	0.002%
30	6.379	866	868	871	rVV2	206	160	0.02%	0.002%
31	6.519	889	891	893	rBV2	357	309	0.03%	0.004%
32	6.757	921	930	948	rBV	211655	513559	55.30%	7.197%
33	6.995	968	969	972	rBV3	297	354	0.04%	0.005%
34	7.037	974	976	979	rBV2	131	154	0.02%	0.002%
35	7.116	984	989	999	rVB7	1715	4135	0.45%	0.058%
36	7.305	1012	1020	1042	rVV	188228	420846	45.32%	5.898%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121623\
 Data File : VX039255.D
 Acq On : 16 Dec 2023 01:37
 Operator : JC/MD
 Sample : VX1216WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK646

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	7.470	1045	1047	1049	rBV	261	230	0.02%	0.003%
38	7.549	1058	1060	1062	rBV	250	219	0.02%	0.003%
39	7.897	1116	1117	1120	rBV	241	260	0.03%	0.004%
40	8.049	1138	1142	1145	rBV2	211	275	0.03%	0.004%
41	8.226	1169	1171	1174	rBV	206	286	0.03%	0.004%
42	8.324	1180	1187	1203	rBV	132374	223661	24.09%	3.134%
43	8.519	1216	1219	1220	rBV	269	221	0.02%	0.003%
44	8.580	1225	1229	1232	rBV3	407	728	0.08%	0.010%
45	8.647	1234	1240	1251	rBV	473290	742604	79.97%	10.406%
46	8.952	1284	1290	1304	rVV	92373	146985	15.83%	2.060%
47	9.153	1322	1323	1326	rVV	240	154	0.02%	0.002%
48	9.275	1339	1343	1346	rBV4	1581	2171	0.23%	0.030%
49	9.384	1355	1361	1375	rBV	389282	561149	60.43%	7.864%
50	9.616	1394	1399	1403	rVB3	544	914	0.10%	0.013%
51	9.720	1414	1416	1418	rBV	259	236	0.03%	0.003%
52	9.842	1435	1436	1439	rVB2	282	278	0.03%	0.004%
53	9.890	1439	1444	1447	rVB2	239	455	0.05%	0.006%
54	9.927	1447	1450	1451	rVB2	265	235	0.03%	0.003%
55	9.939	1451	1452	1454	rBV2	246	189	0.02%	0.003%
56	9.964	1454	1456	1459	rVB	423	308	0.03%	0.004%
57	10.055	1465	1471	1488	rBV	446839	637700	68.67%	8.936%
58	10.195	1491	1494	1500	rVB2	1813	2465	0.27%	0.035%
59	10.305	1508	1512	1518	rBV3	1556	2440	0.26%	0.034%
60	10.470	1537	1539	1543	rBV2	212	298	0.03%	0.004%
61	10.652	1564	1569	1575	rVV3	1837	4051	0.44%	0.057%
62	10.963	1616	1620	1626	rBV2	2199	2947	0.32%	0.041%
63	11.091	1637	1641	1644	rBV3	743	918	0.10%	0.013%
64	11.189	1652	1657	1665	rBV	344689	446921	48.13%	6.263%
65	11.311	1675	1677	1682	rVB4	510	572	0.06%	0.008%
66	11.457	1695	1701	1706	rBV3	1773	2630	0.28%	0.037%
67	11.671	1734	1736	1738	rBV	342	260	0.03%	0.004%
68	11.713	1742	1743	1745	rVV2	252	172	0.02%	0.002%
69	11.756	1746	1750	1756	rVB	2396	3096	0.33%	0.043%
70	11.969	1781	1785	1788	rBV	2526	3270	0.35%	0.046%
71	12.018	1788	1793	1803	rVV	502239	637108	68.61%	8.928%
72	12.128	1809	1811	1814	rVB2	432	474	0.05%	0.007%
73	12.183	1818	1820	1822	rBV	250	168	0.02%	0.002%
74	12.317	1837	1842	1852	rBV	499854	638550	68.76%	8.948%
75	12.506	1871	1873	1875	rVB	392	228	0.02%	0.003%
76	12.542	1876	1879	1881	rVB2	176	154	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121623\
 Data File : VX039255.D
 Acq On : 16 Dec 2023 01:37
 Operator : JC/MD
 Sample : VX1216WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK646

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	12.689	1901	1903	1906	rVB2	261	260	0.03%	0.004%
78	12.725	1906	1909	1911	rBV2	165	211	0.02%	0.003%
79	12.756	1911	1914	1919	rBV2	430	665	0.07%	0.009%
80	12.890	1934	1936	1937	rBV	292	177	0.02%	0.002%
81	13.030	1957	1959	1962	rVB2	244	204	0.02%	0.003%
82	13.115	1968	1973	1981	rBV2	3491	4195	0.45%	0.059%
83	13.585	2047	2050	2055	rVB2	4680	5947	0.64%	0.083%
84	13.780	2077	2082	2087	rVV	5876	8173	0.88%	0.115%
85	13.865	2094	2096	2101	rBV2	194	262	0.03%	0.004%
86	13.963	2108	2112	2118	rVB4	4978	6173	0.66%	0.087%
87	14.134	2135	2140	2142	rBV3	620	969	0.10%	0.014%
88	14.383	2179	2181	2184	rBV2	155	251	0.03%	0.004%
89	14.481	2195	2197	2200	rBV2	350	350	0.04%	0.005%
90	14.640	2221	2223	2224	rBV2	307	191	0.02%	0.003%
91	14.743	2237	2240	2243	rBV2	298	503	0.05%	0.007%
92	15.078	2293	2295	2298	rBV2	242	236	0.03%	0.003%
93	15.767	2406	2408	2410	rBV	292	275	0.03%	0.004%
94	15.908	2428	2431	2434	rBV2	598	531	0.06%	0.007%
95	16.042	2451	2453	2454	rBV2	268	174	0.02%	0.002%
96	16.158	2471	2472	2475	rVB2	264	172	0.02%	0.002%
97	16.286	2491	2493	2494	rBV	284	224	0.02%	0.003%
98	16.334	2499	2501	2504	rVB2	500	344	0.04%	0.005%
99	16.432	2516	2517	2519	rVB	364	199	0.02%	0.003%
100	16.560	2536	2538	2540	rBV2	370	369	0.04%	0.005%

Sum of corrected areas: 7135997


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121623\
Data File : VX039255.D
Acq On : 16 Dec 2023 01:37
Operator : JC/MD
Sample : VX1216WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK646

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

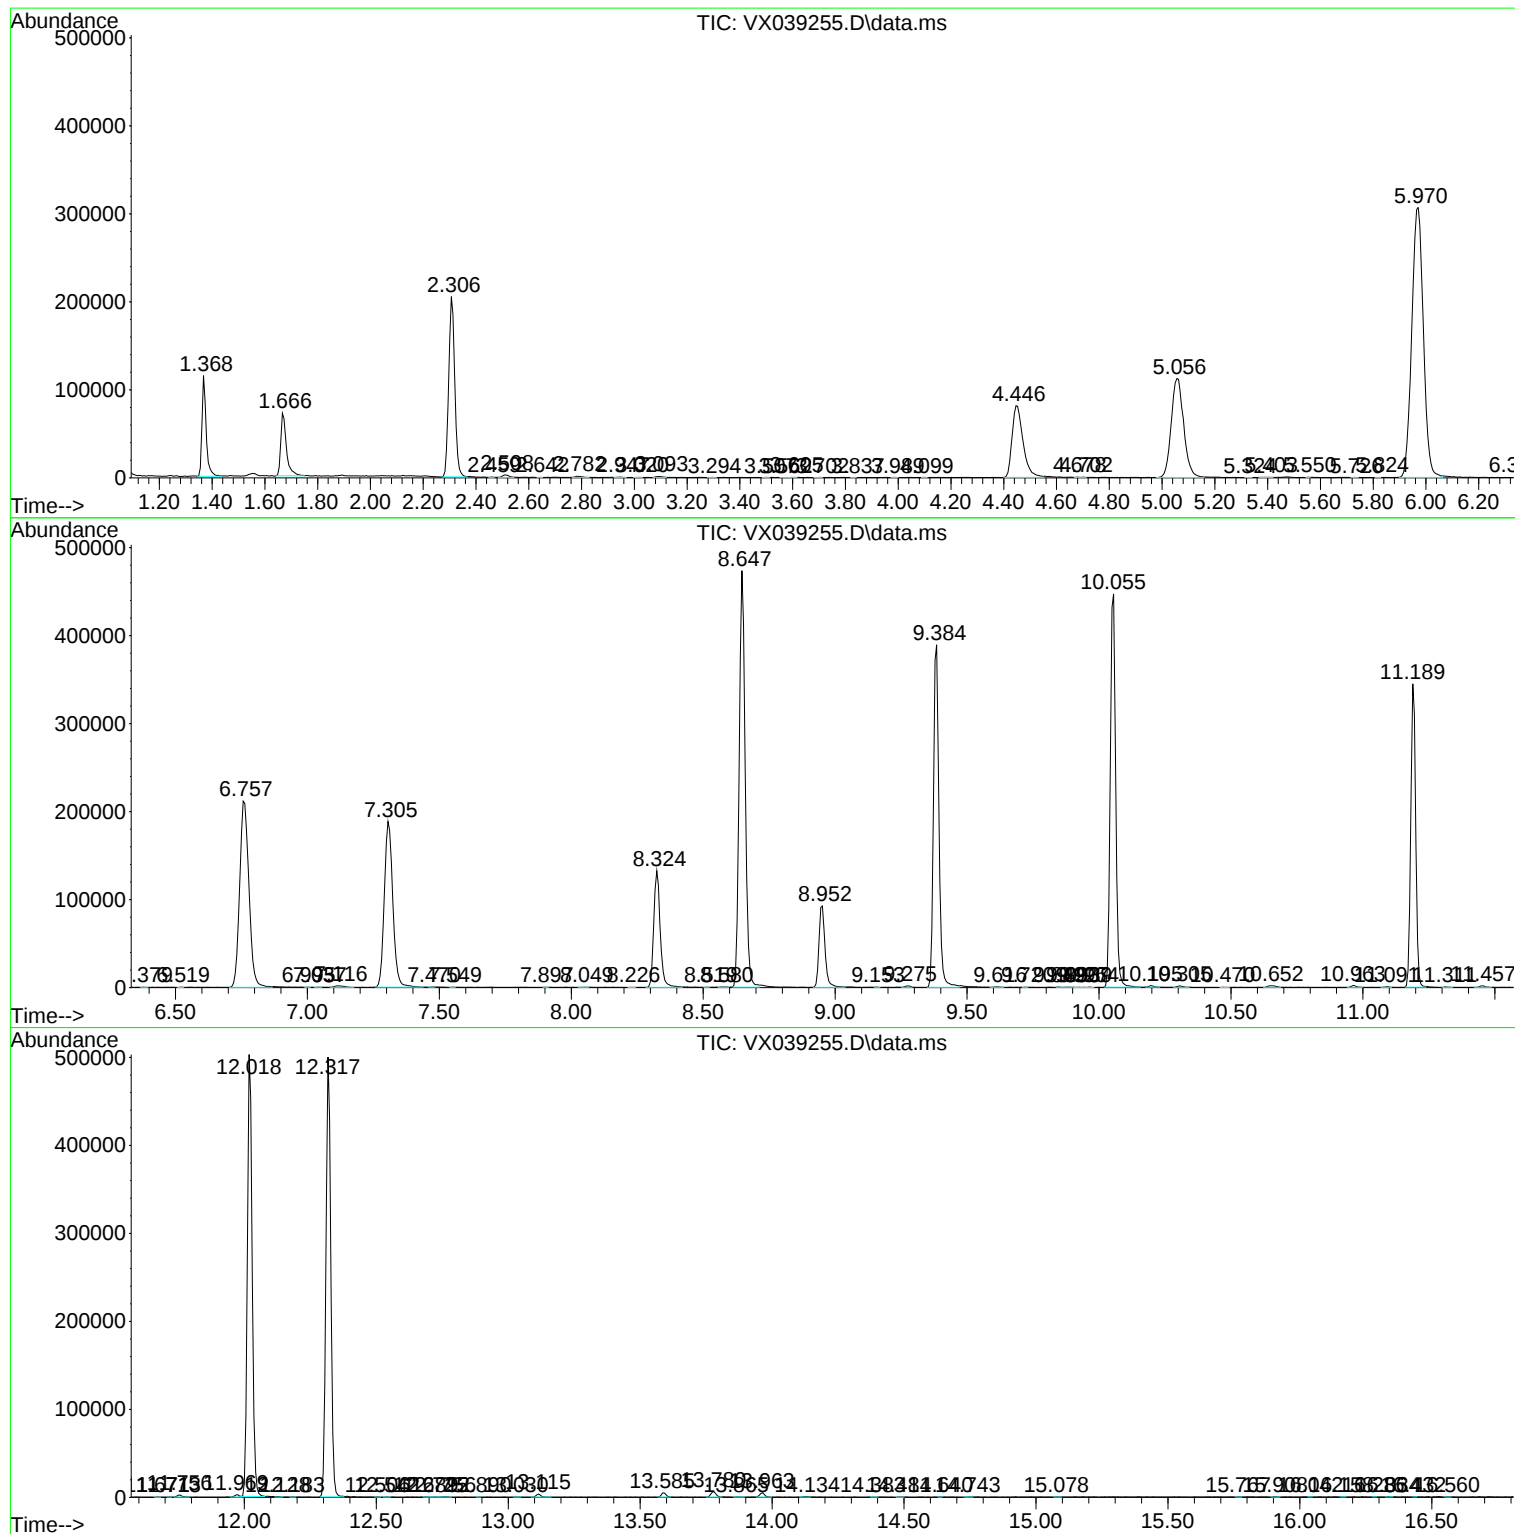

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121623\
Data File : VX039255.D
Acq On : 16 Dec 2023 01:37
Operator : JC/MD
Sample : VX1216WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK646

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121623\
Data File : VX039255.D
Acq On : 16 Dec 2023 01:37
Operator : JC/MD
Sample : VX1216WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK646

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
