

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121623\
 Data File : VX039273.D
 Acq On : 16 Dec 2023 08:28
 Operator : JC/MD
 Sample : 05845-21
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YCHL0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039273.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	33	rVB2	3018	4769	0.54%	0.070%
2	1.368	42	46	57	rBV	109749	121379	13.63%	1.772%
3	1.673	91	96	109	rVB	67983	102141	11.47%	1.491%
4	2.307	193	200	208	rBV	194948	306603	34.43%	4.477%
5	2.569	242	243	245	rVB	397	148	0.02%	0.002%
6	2.794	279	280	286	rVB2	798	639	0.07%	0.009%
7	3.160	338	340	341	rBV	197	200	0.02%	0.003%
8	3.203	345	347	350	rVB2	230	236	0.03%	0.003%
9	3.331	364	368	369	rBV2	336	429	0.05%	0.006%
10	3.386	374	377	382	rVB	191	289	0.03%	0.004%
11	3.434	382	385	388	rBV2	213	305	0.03%	0.004%
12	3.575	406	408	409	rBV	219	201	0.02%	0.003%
13	3.630	415	417	418	rBV	260	143	0.02%	0.002%
14	3.727	431	433	434	rVB	240	140	0.02%	0.002%
15	4.032	479	483	485	rBV2	225	292	0.03%	0.004%
16	4.446	543	551	568	rBV	78247	225363	25.31%	3.291%
17	4.806	608	610	611	rBV	199	212	0.02%	0.003%
18	4.873	619	621	625	rBV2	224	277	0.03%	0.004%
19	5.056	638	651	666	rBV	109577	354300	39.79%	5.173%
20	5.276	685	687	690	rBV2	301	311	0.03%	0.005%
21	5.556	731	733	735	rBV3	281	233	0.03%	0.003%
22	5.745	762	764	766	rVB	243	178	0.02%	0.003%
23	5.782	768	770	773	rBV	195	191	0.02%	0.003%
24	5.971	789	801	820	rBV2	292681	890510	100.00%	13.003%
25	6.452	877	880	882	rBV2	200	257	0.03%	0.004%
26	6.550	895	896	899	rVB2	258	211	0.02%	0.003%
27	6.757	922	930	948	rBV	211054	514649	57.79%	7.515%
28	7.123	987	990	992	rBV3	481	506	0.06%	0.007%
29	7.306	1012	1020	1038	rBV	182139	406053	45.60%	5.929%
30	7.592	1064	1067	1068	rBV2	252	284	0.03%	0.004%
31	7.659	1076	1078	1081	rVV3	343	362	0.04%	0.005%
32	8.086	1146	1148	1152	rVB2	143	141	0.02%	0.002%
33	8.202	1165	1167	1171	rBV2	194	195	0.02%	0.003%
34	8.324	1181	1187	1202	rBV	119696	200695	22.54%	2.930%
35	8.580	1225	1229	1230	rBV2	396	357	0.04%	0.005%
36	8.647	1234	1240	1257	rBV	456912	712929	80.06%	10.410%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121623\
 Data File : VX039273.D
 Acq On : 16 Dec 2023 08:28
 Operator : JC/MD
 Sample : 05845-21
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YCHL0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

37	8.812	1265	1267	1270	rVB2	405	354	0.04%	0.005%
38	8.952	1284	1290	1302	rBV	86978	134918	15.15%	1.970%
39	9.135	1318	1320	1324	rVB2	294	266	0.03%	0.004%
40	9.238	1334	1337	1338	rBV2	195	227	0.03%	0.003%
41	9.269	1338	1342	1346	rVB3	660	1091	0.12%	0.016%
42	9.311	1346	1349	1352	rBV3	270	417	0.05%	0.006%
43	9.385	1355	1361	1377	rBV	357841	526680	59.14%	7.690%
44	9.665	1405	1407	1408	rBV2	201	139	0.02%	0.002%
45	9.836	1433	1435	1438	rBV2	169	192	0.02%	0.003%
46	9.878	1440	1442	1444	rBV	153	147	0.02%	0.002%
47	10.055	1465	1471	1483	rBV	439353	637745	71.62%	9.312%
48	10.244	1501	1502	1504	rBV	224	167	0.02%	0.002%
49	10.305	1509	1512	1515	rBV3	678	774	0.09%	0.011%
50	10.330	1515	1516	1518	rVB	331	134	0.02%	0.002%
51	10.555	1551	1553	1555	rBV2	122	149	0.02%	0.002%
52	10.872	1603	1605	1608	rVV2	157	143	0.02%	0.002%
53	11.092	1639	1641	1644	rVB2	551	666	0.07%	0.010%
54	11.189	1652	1657	1668	rBV	342666	429334	48.21%	6.269%
55	11.311	1674	1677	1682	rVB3	1065	1370	0.15%	0.020%
56	11.390	1686	1690	1693	rBV2	270	410	0.05%	0.006%
57	11.451	1696	1700	1702	rBV3	429	662	0.07%	0.010%
58	11.604	1722	1725	1729	rBV2	283	479	0.05%	0.007%
59	11.640	1729	1731	1733	rVB2	264	219	0.02%	0.003%
60	11.707	1739	1742	1744	rBV	187	179	0.02%	0.003%
61	11.756	1746	1750	1754	rBV2	428	751	0.08%	0.011%
62	11.829	1759	1762	1765	rBV2	250	390	0.04%	0.006%
63	11.909	1774	1775	1777	rBV2	180	140	0.02%	0.002%
64	11.957	1780	1783	1784	rBV	355	282	0.03%	0.004%
65	12.018	1788	1793	1802	rBV	508124	640793	71.96%	9.357%
66	12.195	1820	1822	1823	rVB	261	133	0.01%	0.002%
67	12.226	1823	1827	1828	rBV3	515	593	0.07%	0.009%
68	12.317	1837	1842	1853	rBV	491097	613613	68.91%	8.960%
69	12.506	1871	1873	1876	rBV3	270	287	0.03%	0.004%
70	12.549	1876	1880	1883	rVV2	289	454	0.05%	0.007%
71	12.610	1888	1890	1894	rBV2	108	165	0.02%	0.002%
72	12.664	1897	1899	1901	rBV2	149	160	0.02%	0.002%
73	12.756	1912	1914	1918	rVB	409	498	0.06%	0.007%
74	12.835	1924	1927	1928	rBV	224	200	0.02%	0.003%
75	13.061	1962	1964	1969	rVB2	207	257	0.03%	0.004%
76	13.213	1988	1989	1991	rBV	238	153	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121623\
 Data File : VX039273.D
 Acq On : 16 Dec 2023 08:28
 Operator : JC/MD
 Sample : 05845-21
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 YCHL0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	13.274	1998	1999	2002	rVB	192	137	0.02%	0.002%
78	13.353	2009	2012	2014	rBV2	149	147	0.02%	0.002%
79	13.408	2019	2021	2025	rBV2	274	400	0.04%	0.006%
80	13.597	2048	2052	2055	rBV2	460	657	0.07%	0.010%
81	13.652	2060	2061	2064	rBV	219	146	0.02%	0.002%
82	13.695	2066	2068	2071	rBV	289	271	0.03%	0.004%
83	13.780	2078	2082	2087	rVB2	546	871	0.10%	0.013%
84	13.835	2089	2091	2094	rVB2	179	176	0.02%	0.003%
85	13.865	2094	2096	2100	rBV2	185	240	0.03%	0.004%
86	13.902	2100	2102	2105	rBV2	220	266	0.03%	0.004%
87	14.103	2132	2135	2137	rBV	198	178	0.02%	0.003%
88	14.164	2141	2145	2149	rVV2	175	269	0.03%	0.004%
89	14.250	2157	2159	2162	rBV2	185	180	0.02%	0.003%
90	14.402	2182	2184	2186	rBV	229	171	0.02%	0.002%
91	14.469	2194	2195	2198	rVB2	313	291	0.03%	0.004%
92	14.518	2201	2203	2206	rVB2	228	213	0.02%	0.003%
93	14.597	2214	2216	2219	rVB	228	214	0.02%	0.003%
94	14.621	2219	2220	2225	rBV	433	363	0.04%	0.005%
95	14.743	2239	2240	2242	rBV	255	155	0.02%	0.002%
96	15.073	2292	2294	2296	rBV2	231	249	0.03%	0.004%
97	15.213	2316	2317	2318	rBV	262	145	0.02%	0.002%
98	16.072	2456	2458	2460	rVB	442	305	0.03%	0.004%
99	16.255	2487	2488	2491	rBV	358	223	0.03%	0.003%
100	16.755	2565	2570	2571	rBV2	302	370	0.04%	0.005%


Sum of corrected areas: 6848496

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121623\
Data File : VX039273.D
Acq On : 16 Dec 2023 08:28
Operator : JC/MD
Sample : 05845-21
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YCHL0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

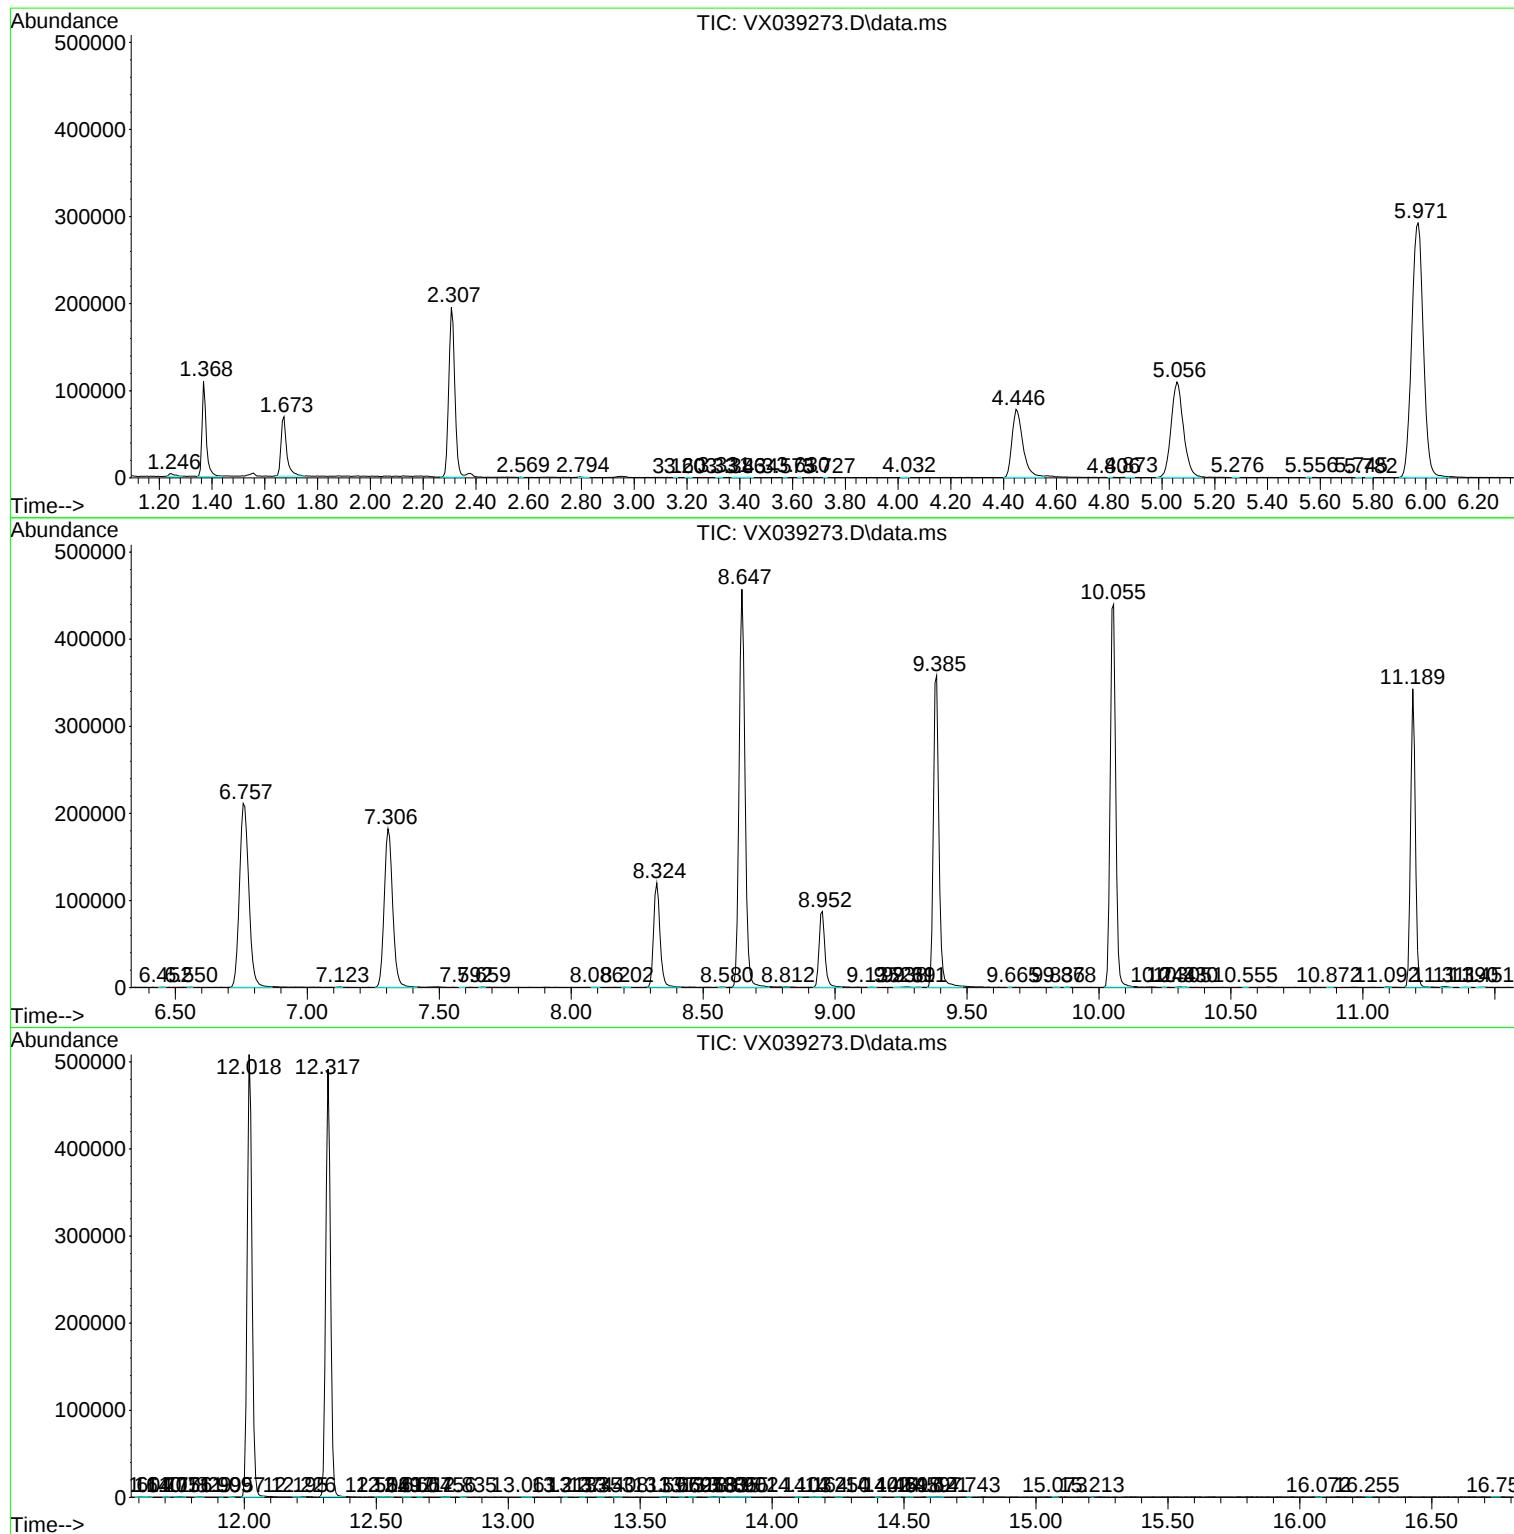

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121623\
Data File : VX039273.D
Acq On : 16 Dec 2023 08:28
Operator : JC/MD
Sample : 05845-21
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YCHL0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121623\
Data File : VX039273.D
Acq On : 16 Dec 2023 08:28
Operator : JC/MD
Sample : 05845-21
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
YCHL0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc