

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121623\
 Data File : VX039278.D
 Acq On : 16 Dec 2023 10:24
 Operator : JC/MD
 Sample : VX1216WBL03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK647

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M

Title : VOC Analysis

Signal : TIC: VX039278.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	33	rBV3	2332	4138	0.44%	0.057%
2	1.368	42	46	55	rBV	115189	123083	13.10%	1.688%
3	1.666	91	95	107	rBV	73352	110181	11.73%	1.511%
4	2.307	194	200	209	rBV	207722	323430	34.43%	4.435%
5	2.514	230	234	239	rVB	2142	3305	0.35%	0.045%
6	2.581	243	245	246	rVB	316	169	0.02%	0.002%
7	2.794	273	280	287	rVB3	2644	5692	0.61%	0.078%
8	2.965	304	308	311	rVV	268	323	0.03%	0.004%
9	3.093	325	329	337	rBV3	922	1825	0.19%	0.025%
10	3.483	391	393	396	rBV2	268	354	0.04%	0.005%
11	3.623	414	416	417	rVV2	394	272	0.03%	0.004%
12	3.721	431	432	434	rBV	283	210	0.02%	0.003%
13	3.971	472	473	476	rVB2	257	218	0.02%	0.003%
14	4.367	536	538	541	rVB2	223	226	0.02%	0.003%
15	4.452	543	552	570	rBV	80175	233976	24.90%	3.208%
16	4.873	620	621	623	rBV2	234	177	0.02%	0.002%
17	4.904	623	626	627	rBV	229	248	0.03%	0.003%
18	5.056	639	651	671	rBV	116064	370352	39.42%	5.078%
19	5.452	713	716	718	rBV2	319	499	0.05%	0.007%
20	5.562	729	734	739	rVB4	371	824	0.09%	0.011%
21	5.599	739	740	744	rBV	257	181	0.02%	0.002%
22	5.690	752	755	757	rBV2	279	281	0.03%	0.004%
23	5.781	768	770	773	rVB	262	207	0.02%	0.003%
24	5.970	789	801	822	rBV2	308209	939478	100.00%	12.882%
25	6.147	828	830	832	rVB	334	170	0.02%	0.002%
26	6.214	839	841	843	rVB2	439	368	0.04%	0.005%
27	6.239	843	845	849	rBV2	287	394	0.04%	0.005%
28	6.294	852	854	857	rVB2	294	290	0.03%	0.004%
29	6.324	857	859	860	rBV	198	174	0.02%	0.002%
30	6.385	867	869	872	rBV2	153	176	0.02%	0.002%
31	6.464	878	882	883	rBV	158	221	0.02%	0.003%
32	6.568	897	899	901	rBV	327	313	0.03%	0.004%
33	6.696	917	920	921	rVB	199	191	0.02%	0.003%
34	6.757	921	930	951	rBV	220071	545307	58.04%	7.477%
35	7.129	985	991	996	rVB5	1182	2701	0.29%	0.037%
36	7.245	1008	1010	1011	rBV2	210	174	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121623\
 Data File : VX039278.D
 Acq On : 16 Dec 2023 10:24
 Operator : JC/MD
 Sample : VX1216WBL03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK647

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	7.306	1012	1020	1039	rVV	194511	426375	45.38%	5.846%
38	7.525	1055	1056	1058	rBV2	345	220	0.02%	0.003%
39	7.617	1069	1071	1073	rBV2	216	231	0.02%	0.003%
40	7.769	1094	1096	1098	rVB2	231	204	0.02%	0.003%
41	7.873	1111	1113	1114	rBV2	281	219	0.02%	0.003%
42	7.946	1122	1125	1127	rBV2	150	238	0.03%	0.003%
43	8.324	1181	1187	1205	rVV	143304	231952	24.69%	3.180%
44	8.464	1208	1210	1211	rVV	383	261	0.03%	0.004%
45	8.580	1225	1229	1234	rBV3	957	1333	0.14%	0.018%
46	8.647	1234	1240	1252	rBV	478185	753892	80.25%	10.337%
47	8.836	1269	1271	1273	rVB2	304	260	0.03%	0.004%
48	8.866	1273	1276	1278	rVB	336	360	0.04%	0.005%
49	8.897	1278	1281	1284	rVB2	234	197	0.02%	0.003%
50	8.952	1284	1290	1304	rBV	98837	152969	16.28%	2.097%
51	9.092	1312	1313	1316	rVB2	219	201	0.02%	0.003%
52	9.153	1322	1323	1327	rBV2	172	174	0.02%	0.002%
53	9.275	1340	1343	1348	rBV3	1035	1265	0.13%	0.017%
54	9.378	1355	1360	1378	rBV	376111	550179	58.56%	7.544%
55	9.689	1407	1411	1415	rBV2	201	344	0.04%	0.005%
56	9.939	1449	1452	1455	rVB2	248	289	0.03%	0.004%
57	10.055	1465	1471	1484	rBV	471712	669022	71.21%	9.173%
58	10.311	1507	1513	1520	rVB3	1139	1929	0.21%	0.026%
59	10.464	1537	1538	1540	rBV	228	197	0.02%	0.003%
60	10.659	1565	1570	1576	rVB6	1263	2574	0.27%	0.035%
61	10.963	1614	1620	1623	rBV3	1276	1833	0.20%	0.025%
62	11.079	1637	1639	1640	rBV2	221	192	0.02%	0.003%
63	11.092	1640	1641	1644	rVV2	409	272	0.03%	0.004%
64	11.189	1651	1657	1671	rBV	350688	448761	47.77%	6.153%
65	11.348	1681	1683	1688	rVB2	240	302	0.03%	0.004%
66	11.402	1689	1692	1694	rVV2	156	171	0.02%	0.002%
67	11.451	1697	1700	1709	rVB3	1370	1971	0.21%	0.027%
68	11.695	1738	1740	1742	rBV2	201	208	0.02%	0.003%
69	11.756	1745	1750	1754	rVB	1484	1738	0.18%	0.024%
70	11.866	1765	1768	1770	rVV	268	193	0.02%	0.003%
71	11.969	1781	1785	1788	rVV3	2013	2476	0.26%	0.034%
72	12.018	1788	1793	1817	rVV	532739	689226	73.36%	9.450%
73	12.201	1821	1823	1825	rVB2	198	178	0.02%	0.002%
74	12.317	1837	1842	1854	rBV	504740	656925	69.92%	9.007%
75	12.622	1889	1892	1896	rBV2	228	259	0.03%	0.004%
76	12.792	1919	1920	1924	rVB2	225	224	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121623\
 Data File : VX039278.D
 Acq On : 16 Dec 2023 10:24
 Operator : JC/MD
 Sample : VX1216WBL03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK647

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	12.945	1943	1945	1948	rVB3	318	288	0.03%	0.004%
78	13.079	1965	1967	1969	rVV	206	176	0.02%	0.002%
79	13.116	1969	1973	1977	rVV3	2329	2662	0.28%	0.036%
80	13.183	1980	1984	1986	rBV2	178	268	0.03%	0.004%
81	13.408	2019	2021	2025	rBV	264	378	0.04%	0.005%
82	13.475	2030	2032	2035	rVV	216	216	0.02%	0.003%
83	13.536	2038	2042	2044	rBV	315	328	0.03%	0.004%
84	13.591	2047	2051	2055	rVV3	3206	4102	0.44%	0.056%
85	13.780	2077	2082	2088	rBV	4259	6373	0.68%	0.087%
86	13.963	2108	2112	2117	rVV2	2903	3839	0.41%	0.053%
87	14.128	2134	2139	2145	rVB4	742	1186	0.13%	0.016%
88	14.378	2178	2180	2182	rBV	221	218	0.02%	0.003%
89	14.420	2184	2187	2189	rBV2	205	245	0.03%	0.003%
90	14.579	2211	2213	2215	rVB	322	206	0.02%	0.003%
91	14.627	2219	2221	2222	rBV2	216	179	0.02%	0.002%
92	14.792	2245	2248	2250	rBV3	280	298	0.03%	0.004%
93	14.908	2265	2267	2270	rVB2	238	176	0.02%	0.002%
94	15.243	2320	2322	2325	rVB3	335	284	0.03%	0.004%
95	15.658	2388	2390	2391	rBV2	281	192	0.02%	0.003%
96	15.767	2407	2408	2412	rBV2	413	463	0.05%	0.006%
97	15.871	2423	2425	2428	rVB2	226	215	0.02%	0.003%
98	15.902	2428	2430	2433	rBV	329	388	0.04%	0.005%
99	16.139	2467	2469	2471	rBV2	353	327	0.03%	0.004%
100	16.560	2536	2538	2541	rBV	325	283	0.03%	0.004%




Sum of corrected areas: 7293232

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121623\
Data File : VX039278.D
Acq On : 16 Dec 2023 10:24
Operator : JC/MD
Sample : VX1216WBL03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK647

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

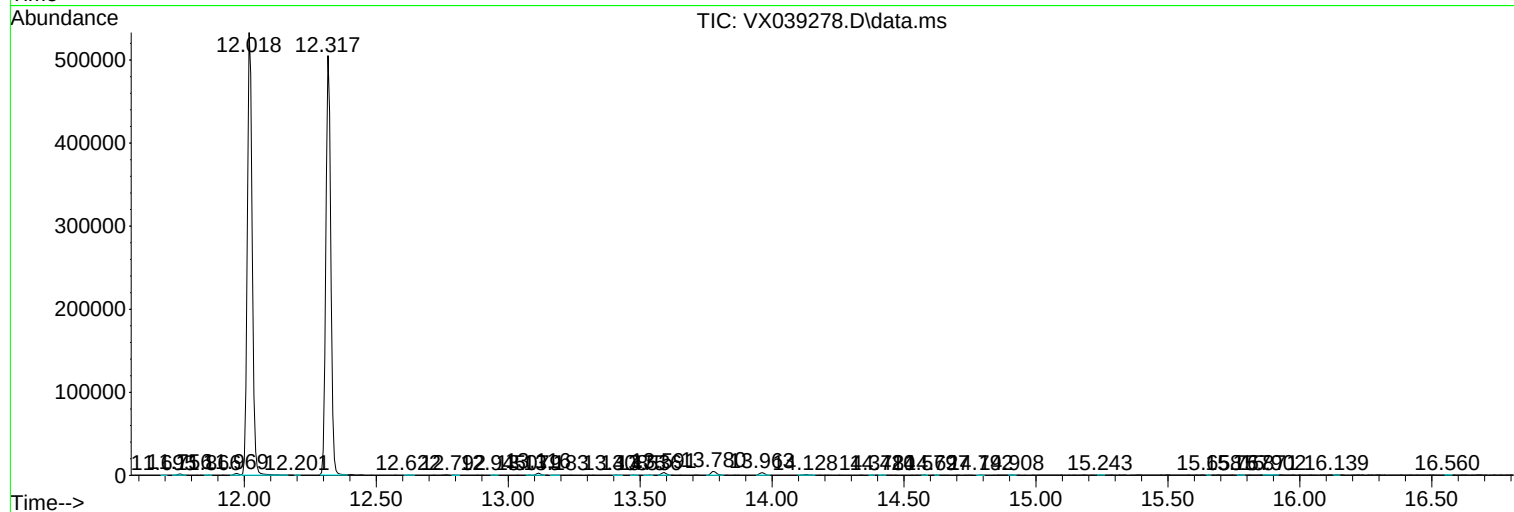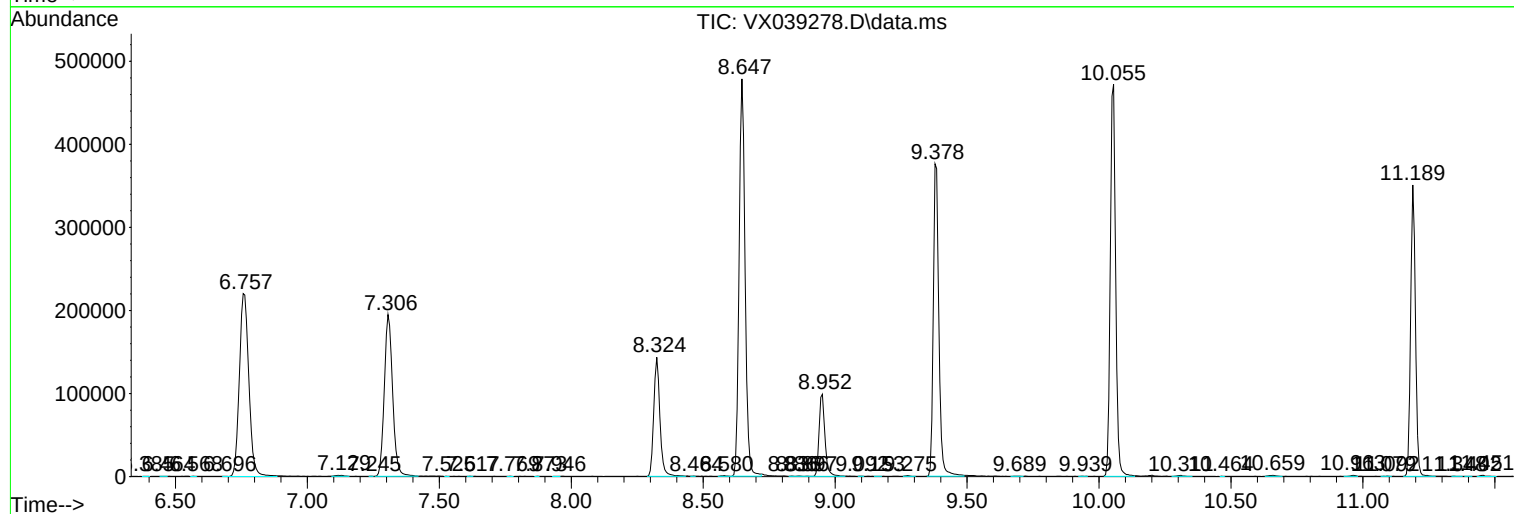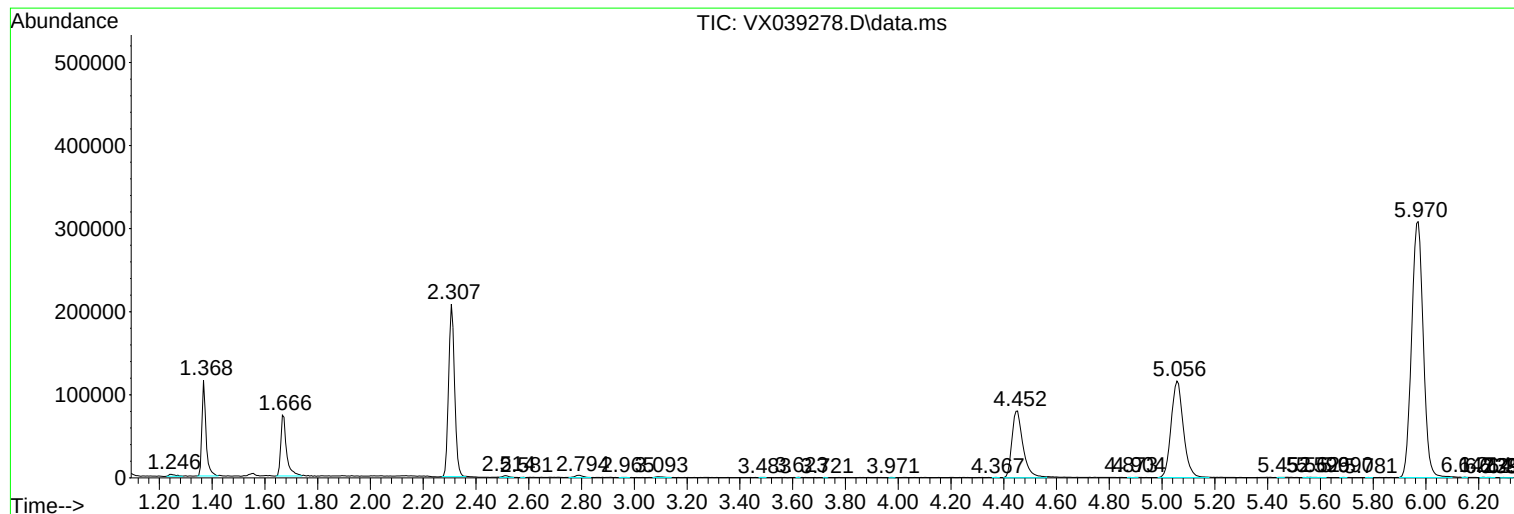

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121623\
Data File : VX039278.D
Acq On : 16 Dec 2023 10:24
Operator : JC/MD
Sample : VX1216WBL03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK647

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121623\
Data File : VX039278.D
Acq On : 16 Dec 2023 10:24
Operator : JC/MD
Sample : VX1216WBL03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK647

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------