

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121623\
 Data File : VX039283.D
 Acq On : 16 Dec 2023 12:26
 Operator : JC/MD
 Sample : 05844-22
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M

Title : VOC Analysis

Signal : TIC: VX039283.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	28	rBV	2219	2656	0.30%	0.039%
2	1.368	42	46	56	rBV	97657	104246	11.89%	1.542%
3	1.666	91	95	108	rBV	68708	98720	11.26%	1.461%
4	2.307	194	200	211	rBV	178649	276244	31.51%	4.087%
5	2.788	276	279	283	rVB3	1072	1571	0.18%	0.023%
6	2.892	294	296	299	rBV	211	234	0.03%	0.003%
7	2.947	301	305	307	rVV	183	229	0.03%	0.003%
8	3.093	326	329	333	rVB3	418	501	0.06%	0.007%
9	3.123	333	334	337	rVB2	358	267	0.03%	0.004%
10	3.166	337	341	344	rBV2	198	268	0.03%	0.004%
11	3.416	381	382	385	rBV2	261	315	0.04%	0.005%
12	3.630	415	417	420	rVV2	213	282	0.03%	0.004%
13	4.020	477	481	483	rBV2	167	248	0.03%	0.004%
14	4.099	492	494	497	rVB	248	179	0.02%	0.003%
15	4.264	520	521	524	rVB	362	227	0.03%	0.003%
16	4.300	524	527	531	rBV2	310	474	0.05%	0.007%
17	4.331	531	532	536	rVB	322	280	0.03%	0.004%
18	4.453	543	552	571	rBV	83610	243958	27.83%	3.610%
19	5.056	640	651	668	rBV	110272	347377	39.62%	5.140%
20	5.276	685	687	691	rVB2	239	231	0.03%	0.003%
21	5.367	699	702	703	rBV2	288	302	0.03%	0.004%
22	5.458	712	717	718	rBV2	303	371	0.04%	0.005%
23	5.550	729	732	733	rBV3	284	333	0.04%	0.005%
24	5.971	788	801	819	rBV2	288920	876673	100.00%	12.972%
25	6.300	854	855	857	rBV	221	179	0.02%	0.003%
26	6.318	857	858	860	rVV	212	179	0.02%	0.003%
27	6.373	862	867	868	rVV2	191	218	0.02%	0.003%
28	6.550	892	896	897	rBV	236	226	0.03%	0.003%
29	6.763	921	931	943	rBV	206556	487799	55.64%	7.218%
30	7.123	983	990	994	rBV5	1150	2474	0.28%	0.037%
31	7.196	999	1002	1004	rBV	272	274	0.03%	0.004%
32	7.306	1012	1020	1039	rBV	180588	405427	46.25%	5.999%
33	7.489	1047	1050	1051	rVB3	397	318	0.04%	0.005%
34	7.586	1064	1066	1071	rVB2	220	235	0.03%	0.003%
35	7.647	1074	1076	1077	rBV	267	180	0.02%	0.003%
36	7.818	1102	1104	1108	rVB2	283	368	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121623\
 Data File : VX039283.D
 Acq On : 16 Dec 2023 12:26
 Operator : JC/MD
 Sample : 05844-22
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

37	7.873	1108	1113	1115	rBV2	314	464	0.05%	0.007%
38	7.946	1122	1125	1126	rBV	195	185	0.02%	0.003%
39	8.324	1181	1187	1200	rBV	128640	213891	24.40%	3.165%
40	8.464	1208	1210	1212	rBV	358	214	0.02%	0.003%
41	8.580	1225	1229	1234	rBV3	538	832	0.09%	0.012%
42	8.647	1234	1240	1264	rVV	428394	687598	78.43%	10.174%
43	8.860	1274	1275	1278	rVB2	259	257	0.03%	0.004%
44	8.952	1284	1290	1302	rBV	92873	144487	16.48%	2.138%
45	9.135	1318	1320	1323	rBV2	218	233	0.03%	0.003%
46	9.269	1341	1342	1347	rVB	359	374	0.04%	0.006%
47	9.385	1355	1361	1377	rBV	387468	560436	63.93%	8.292%
48	9.787	1425	1427	1431	rVB2	184	204	0.02%	0.003%
49	10.055	1465	1471	1489	rBV	439318	615179	70.17%	9.102%
50	10.287	1507	1509	1510	rBV	207	198	0.02%	0.003%
51	10.403	1525	1528	1529	rBV	230	185	0.02%	0.003%
52	10.506	1541	1545	1547	rVB	208	201	0.02%	0.003%
53	10.531	1547	1549	1552	rBV	179	192	0.02%	0.003%
54	10.628	1561	1565	1566	rBV	308	412	0.05%	0.006%
55	10.647	1566	1568	1571	rVV2	349	484	0.06%	0.007%
56	10.726	1578	1581	1583	rBV2	211	244	0.03%	0.004%
57	10.793	1588	1592	1593	rBV2	216	224	0.03%	0.003%
58	10.964	1617	1620	1624	rBV3	748	847	0.10%	0.013%
59	11.092	1635	1641	1643	rBV4	783	1009	0.12%	0.015%
60	11.189	1652	1657	1664	rBV	358558	445968	50.87%	6.599%
61	11.457	1698	1701	1704	rBV3	668	794	0.09%	0.012%
62	11.592	1719	1723	1726	rVB	205	258	0.03%	0.004%
63	11.713	1739	1743	1745	rBV2	360	469	0.05%	0.007%
64	11.835	1762	1763	1766	rVB	237	194	0.02%	0.003%
65	11.976	1783	1786	1788	rBV2	519	657	0.07%	0.010%
66	12.018	1788	1793	1803	rBV	473371	615419	70.20%	9.106%
67	12.189	1817	1821	1822	rBV2	286	325	0.04%	0.005%
68	12.207	1822	1824	1827	rVV2	301	235	0.03%	0.003%
69	12.317	1837	1842	1851	rBV	486438	600508	68.50%	8.885%
70	12.756	1912	1914	1919	rVB	611	733	0.08%	0.011%
71	12.799	1919	1921	1923	rBV2	223	199	0.02%	0.003%
72	12.835	1925	1927	1929	rBV	236	208	0.02%	0.003%
73	12.890	1935	1936	1938	rBV	241	197	0.02%	0.003%
74	13.110	1971	1972	1976	rVB2	292	386	0.04%	0.006%
75	13.335	2008	2009	2012	rBV2	262	247	0.03%	0.004%
76	13.396	2017	2019	2021	rBV	205	192	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121623\
 Data File : VX039283.D
 Acq On : 16 Dec 2023 12:26
 Operator : JC/MD
 Sample : 05844-22
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	13.414	2021	2022	2025	rVV2	305	292	0.03%	0.004%
78	13.536	2039	2042	2044	rBV2	232	214	0.02%	0.003%
79	13.555	2044	2045	2047	rVV2	317	231	0.03%	0.003%
80	13.597	2049	2052	2055	rVV2	654	765	0.09%	0.011%
81	13.695	2066	2068	2069	rBV2	229	186	0.02%	0.003%
82	13.786	2079	2083	2089	rBV3	537	1123	0.13%	0.017%
83	13.969	2110	2113	2114	rVV	362	329	0.04%	0.005%
84	14.128	2136	2139	2142	rVB2	671	880	0.10%	0.013%
85	14.219	2151	2154	2156	rBV	220	203	0.02%	0.003%
86	14.274	2162	2163	2165	rVB	395	228	0.03%	0.003%
87	14.506	2197	2201	2203	rBV3	297	433	0.05%	0.006%
88	14.640	2221	2223	2227	rVB	241	262	0.03%	0.004%
89	14.689	2229	2231	2233	rVB2	347	268	0.03%	0.004%
90	14.841	2254	2256	2258	rVB2	299	209	0.02%	0.003%
91	14.951	2270	2274	2276	rBV2	369	510	0.06%	0.008%
92	15.262	2323	2325	2326	rBV2	282	214	0.02%	0.003%
93	15.457	2355	2357	2359	rVB	429	254	0.03%	0.004%
94	15.707	2397	2398	2400	rBV2	225	232	0.03%	0.003%
95	15.780	2404	2410	2411	rBV3	250	413	0.05%	0.006%
96	15.835	2417	2419	2421	rVB	403	289	0.03%	0.004%
97	15.883	2424	2427	2429	rBV2	393	417	0.05%	0.006%
98	16.219	2480	2482	2487	rVB2	331	346	0.04%	0.005%
99	16.304	2492	2496	2498	rBV3	371	498	0.06%	0.007%
100	16.597	2542	2544	2546	rVB	359	187	0.02%	0.003%


Sum of corrected areas: 6758385

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121623\
Data File : VX039283.D
Acq On : 16 Dec 2023 12:26
Operator : JC/MD
Sample : 05844-22
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

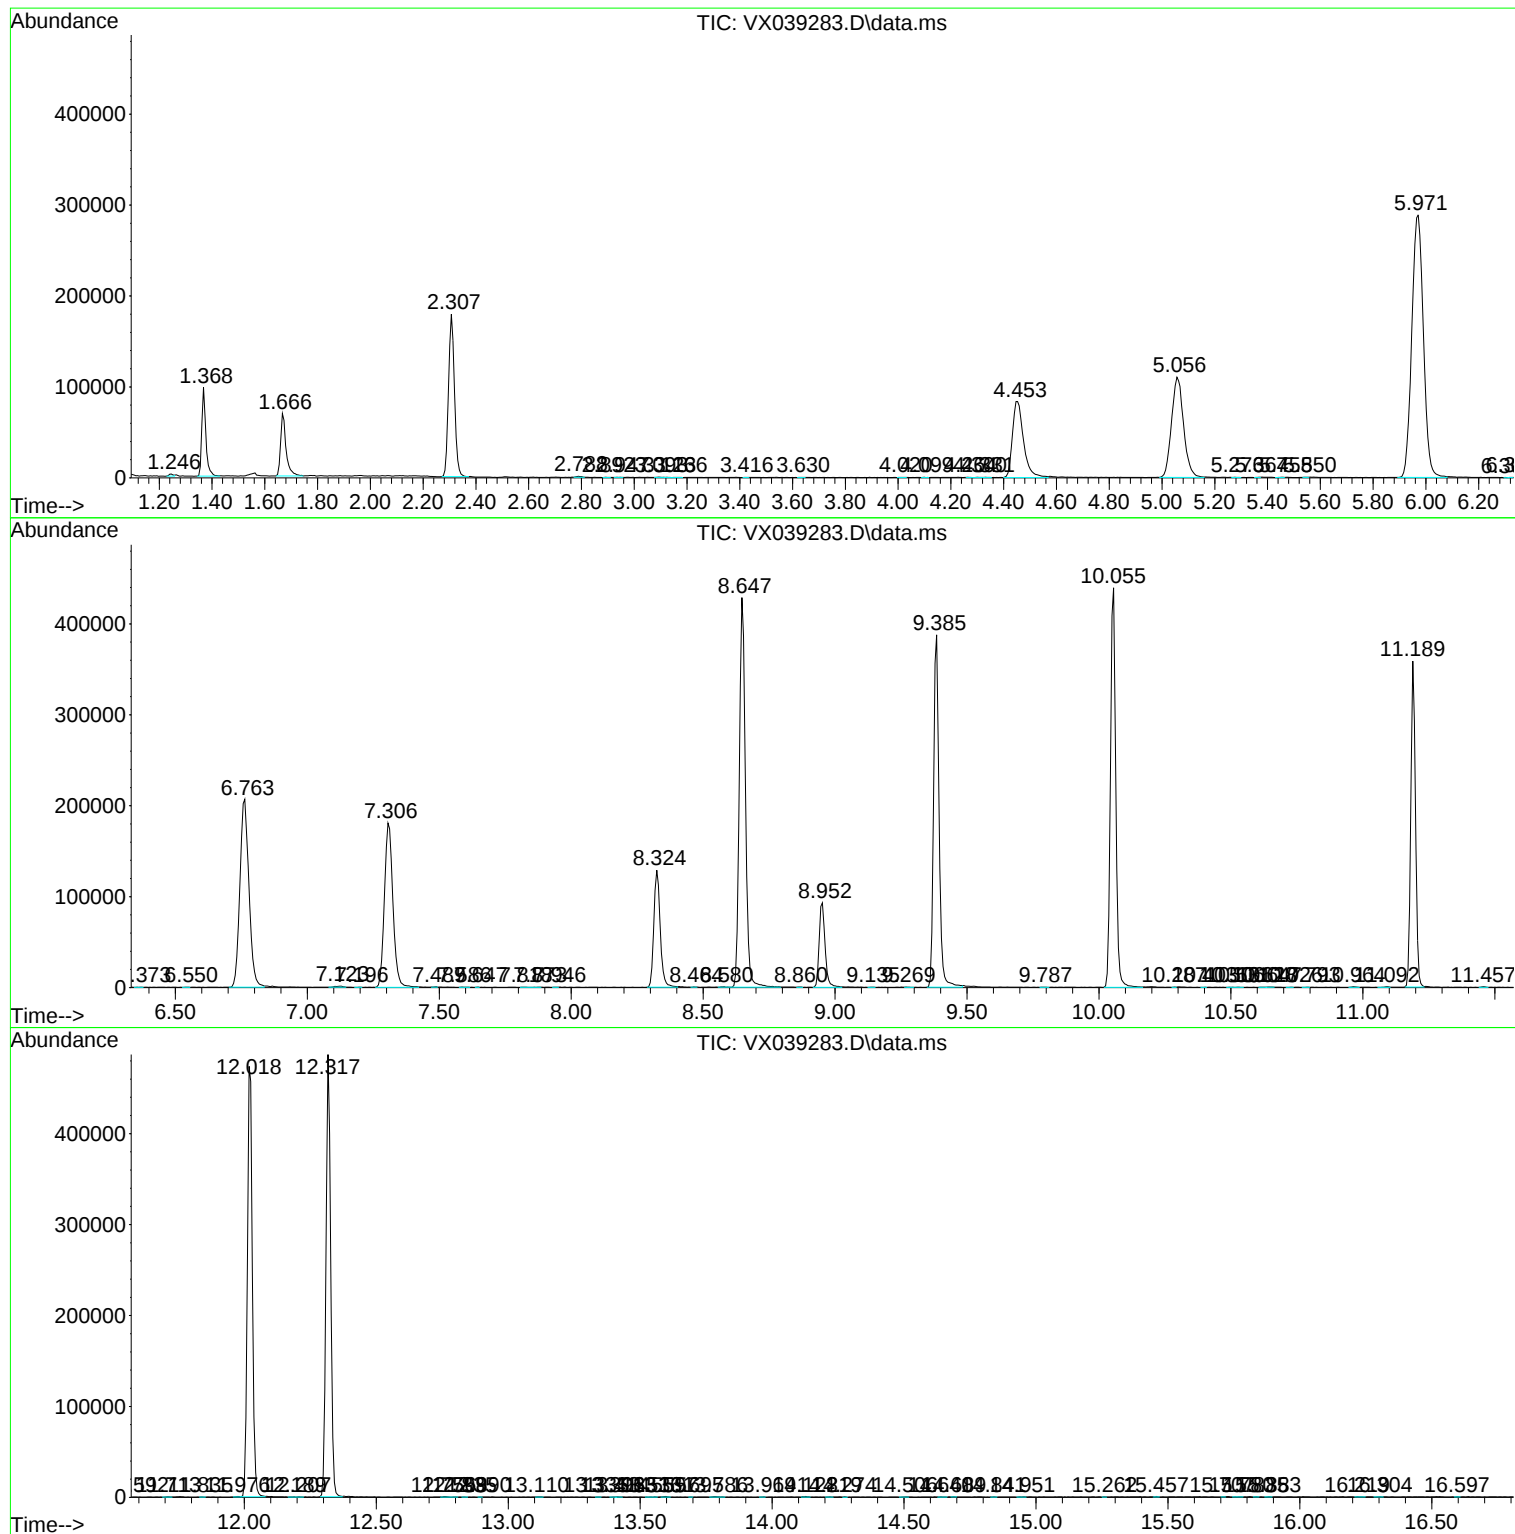

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121623\
Data File : VX039283.D
Acq On : 16 Dec 2023 12:26
Operator : JC/MD
Sample : 05844-22
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121623\
Data File : VX039283.D
Acq On : 16 Dec 2023 12:26
Operator : JC/MD
Sample : 05844-22
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc