
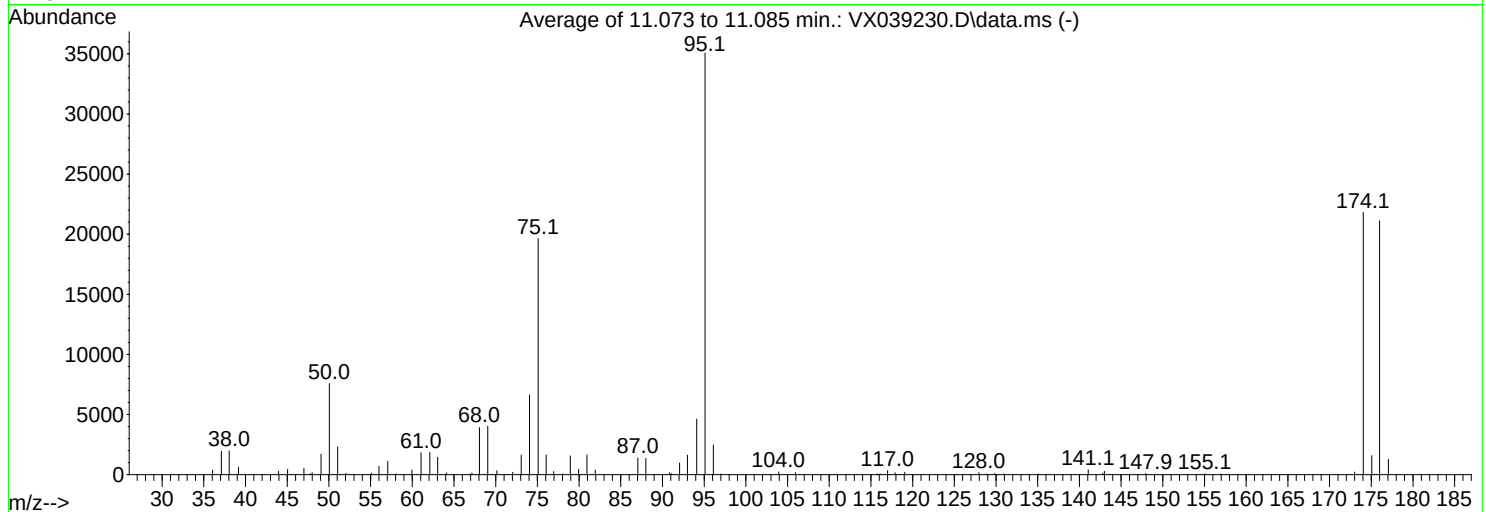


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121623\
Data File : VX039230.D
Acq On : 15 Dec 2023 15:17
Operator : JC/MD
Sample : BFB655
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB655

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Title : VOC Analysis
Last Update : Tue Dec 12 03:50:51 2023

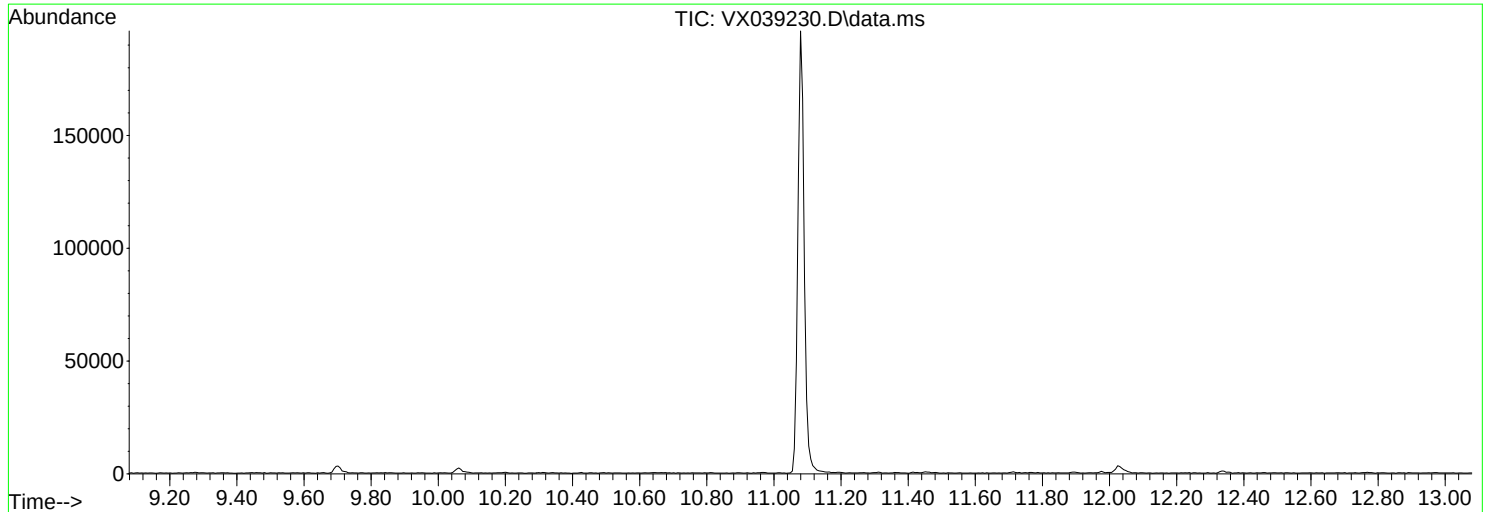

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	7580	PASS
75	95	30	80	56.0	19651	PASS
95	95	100	100	100.0	35088	PASS
96	95	5	9	7.0	2468	PASS
173	174	0.00	2	1.0	208	PASS
174	95	50	120	62.2	21811	PASS
175	174	5	9	7.3	1587	PASS
176	174	95	101	96.8	21110	PASS
177	176	5	9	6.0	1273	PASS

m/z	Abundance
39.90	191.0
43.90	181.0

Instrument :
MSVOA_X
ClientSampleId :
BFB655

m/z	Abundance
36.10	382.0
37.10	1791.0
38.10	1850.0
39.10	499.0
40.00	271.0
44.00	447.0
45.00	443.0
47.10	489.0
47.80	249.0
49.10	1418.0
50.00	7011.0
51.10	2179.0
52.00	111.0
55.10	61.0
56.10	598.0
57.10	963.0
58.10	68.0
60.00	323.0
61.00	1647.0
62.10	1676.0
63.10	1096.0
64.10	147.0
66.80	116.0
67.20	114.0
68.10	3310.0
69.10	3588.0
70.10	320.0
72.20	158.0
73.00	1540.0
74.10	5817.0
75.10	16992.0
76.10	1481.0
77.00	230.0
79.00	1276.0
80.00	395.0
80.90	1214.0
81.90	302.0
87.00	1144.0
88.00	1103.0
90.90	186.0
92.20	817.0
93.00	1254.0
94.10	3899.0
95.10	28864.0
96.10	2400.0
97.00	62.0
103.90	175.0
106.00	161.0
113.00	81.0
116.10	89.0
117.00	251.0
118.00	197.0
119.00	128.0
127.90	125.0
128.80	82.0
141.10	283.0
142.80	382.0
148.10	64.0
154.70	55.0
156.90	93.0
173.00	105.0
174.10	14888.0
175.00	1136.0
176.00	14250.0
177.10	856.0

Instrument :
MSVOA_X
ClientSampleId :
BFB655

m/z	Abundance
36.00	478.0
37.10	2112.0
38.00	2256.0
39.10	749.0
40.00	190.0
44.00	542.0
45.10	613.0
47.10	470.0
48.00	302.0
49.00	2084.0
50.10	9038.0
51.00	2753.0
52.10	139.0
55.10	188.0
56.00	981.0
57.00	1261.0
58.00	76.0
59.90	404.0
61.10	2232.0
62.10	2295.0
63.00	1846.0
64.00	147.0
67.10	169.0
68.00	4664.0
69.10	4621.0
70.10	331.0
72.00	241.0
73.10	1932.0
74.10	7541.0
75.10	22712.0
76.10	1971.0
77.00	303.0
78.10	124.0
79.00	1956.0
80.00	513.0
80.90	2093.0
82.00	444.0
87.00	1619.0
88.00	1616.0
90.80	282.0
92.00	1227.0
93.00	2051.0
94.10	5614.0
95.10	42320.0
96.10	2818.0
97.00	59.0
104.00	218.0
105.90	183.0
115.80	192.0
116.90	434.0
117.80	133.0
119.00	238.0
127.90	189.0
129.90	183.0
131.00	65.0
135.10	57.0
140.90	414.0
143.00	396.0
146.00	54.0
147.90	120.0
155.10	104.0
156.90	61.0
173.00	335.0
174.00	26032.0
175.00	1889.0
176.00	24928.0
177.00	1656.0

Instrument :
MSVOA_X
ClientSampleId :
BFB655

m/z	Abundance
36.00	262.0
37.10	1927.0
38.10	1835.0
39.20	597.0
40.00	214.0
44.00	400.0
45.00	252.0
46.90	591.0
48.00	187.0
49.00	1605.0
50.10	6690.0
51.10	1998.0
52.10	99.0
55.10	148.0
55.90	517.0
57.00	1097.0
58.00	50.0
60.00	439.0
61.00	1614.0
62.10	1614.0
63.00	1379.0
64.20	119.0
67.20	78.0
68.00	3809.0
69.00	3951.0
70.20	345.0
71.90	204.0
73.10	1397.0
74.00	6516.0
75.10	19248.0
76.00	1476.0
76.90	244.0
78.00	134.0
78.90	1463.0
79.90	398.0
81.00	1590.0
82.00	404.0
87.10	1373.0
88.00	1371.0
91.10	277.0
92.00	858.0
93.00	1583.0
94.10	4355.0
95.10	34080.0
96.10	2186.0
97.00	76.0
103.90	284.0
104.90	73.0
106.00	181.0
116.10	129.0
117.10	324.0
117.90	152.0
119.10	254.0
128.00	203.0
128.90	79.0
129.80	88.0
130.90	84.0
135.10	91.0
137.00	82.0
141.10	496.0
143.00	446.0
146.00	59.0
147.90	95.0
155.00	129.0
173.00	183.0
174.10	24512.0
175.10	1737.0
176.00	24152.0
177.10	1306.0

Instrument :
MSVOA_X
ClientSampleId :
BFB655