

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121625\
 Data File : VX048894.D
 Acq On : 16 Dec 2025 18:08
 Operator : JC/MD
 Sample : VX1216WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1216WBL01

Quant Time: Dec 17 03:26:36 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121625W.M
 Quant Title : SW846 8260
 QLast Update : Wed Dec 17 03:22:16 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.538	168	95567	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.745	114	159021	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.037	117	136648	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.006	152	60256	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.940	65	66298	41.503	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	83.000%		
35) Dibromofluoromethane	5.373	113	52786	44.659	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	89.320%		
50) Toluene-d8	8.635	98	194934	46.195	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	92.400%		
62) 4-Bromofluorobenzene	11.061	95	58612	38.688	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	77.380%#		
Target Compounds						
					Qvalue	
3) Chloromethane	1.307	50	382	0.278	ug/l #	79
5) Bromomethane	1.636	94	465	0.554	ug/l #	68
10) Methyl Iodide	2.459	142	1297	0.901	ug/l #	81
15) Acrylonitrile	3.075	53	260	0.515	ug/l	87
16) Acetone	2.386	43	251	0.746	ug/l #	43
17) Carbon Disulfide	2.520	76	2208	0.733	ug/l	96
20) Methylene Chloride	2.788	84	429	0.309	ug/l #	79
31) Cyclohexane	5.531	56	2448	1.364	ug/l #	47
36) 1,1-Dichloropropene	5.538	75	8150	5.494	ug/l #	48
38) Carbon Tetrachloride	5.538	117	9803	5.544	ug/l #	16
44) Trichloroethene	7.123	130	342	0.279	ug/l	49
51) 4-Methyl-2-Pentanone	8.561	43	308	0.234	ug/l #	35
58) 2-Chloroethyl Vinyl ether	8.244	63	213	0.229	ug/l #	45
59) 2-Hexanone	9.427	43	276	0.309	ug/l #	24
64) Tetrachloroethene	9.256	164	222	0.253	ug/l #	76
68) m/p-Xylenes	10.287	106	493	0.258	ug/l	88
76) 1,2,3-Trichloropropane	11.061	75	31943	32.970	ug/l #	30
77) Bromobenzene	11.183	156	277	0.263	ug/l	55
78) n-propylbenzene	11.287	91	1384	0.278	ug/l	95
79) 2-Chlorotoluene	11.354	91	702	0.228	ug/l	94
81) trans-1,4-Dichloro-2-b...	11.061	75	31943	83.737	ug/l #	3
82) 4-Chlorotoluene	11.445	91	1021	0.290	ug/l	79
84) 1,2,4-Trimethylbenzene	11.738	105	717	0.210	ug/l	90
85) sec-Butylbenzene	11.872	105	1048	0.244	ug/l	87
86) p-Isopropyltoluene	11.988	119	957	0.271	ug/l #	70
87) 1,3-Dichlorobenzene	11.957	146	885	0.449	ug/l	96
88) 1,4-Dichlorobenzene	11.957	146	885	0.428	ug/l	98
89) n-Butylbenzene	12.317	91	2039	0.605	ug/l	99
91) 1,2-Dichlorobenzene	12.323	146	590	0.303	ug/l	99
93) 1,2,4-Trichlorobenzene	13.573	180	1066	0.951	ug/l	95
94) Hexachlorobutadiene	13.701	225	637	1.316	ug/l	83
95) Naphthalene	13.762	128	2031	0.717	ug/l	98
96) 1,2,3-Trichlorobenzene	13.951	180	929	0.922	ug/l	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Instrument :
MSVOA_X
ClientSampleId :
VX1216WBL01

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121625\
Data File : VX048894.D
Acq On : 16 Dec 2025 18:08
Operator : JC/MD
Sample : VX1216MBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1216WBL01

Quant Time: Dec 17 03:26:36 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121625W.M
Quant Title : SW846 8260
QLast Update : Wed Dec 17 03:22:16 2025
Response via : Initial Calibration




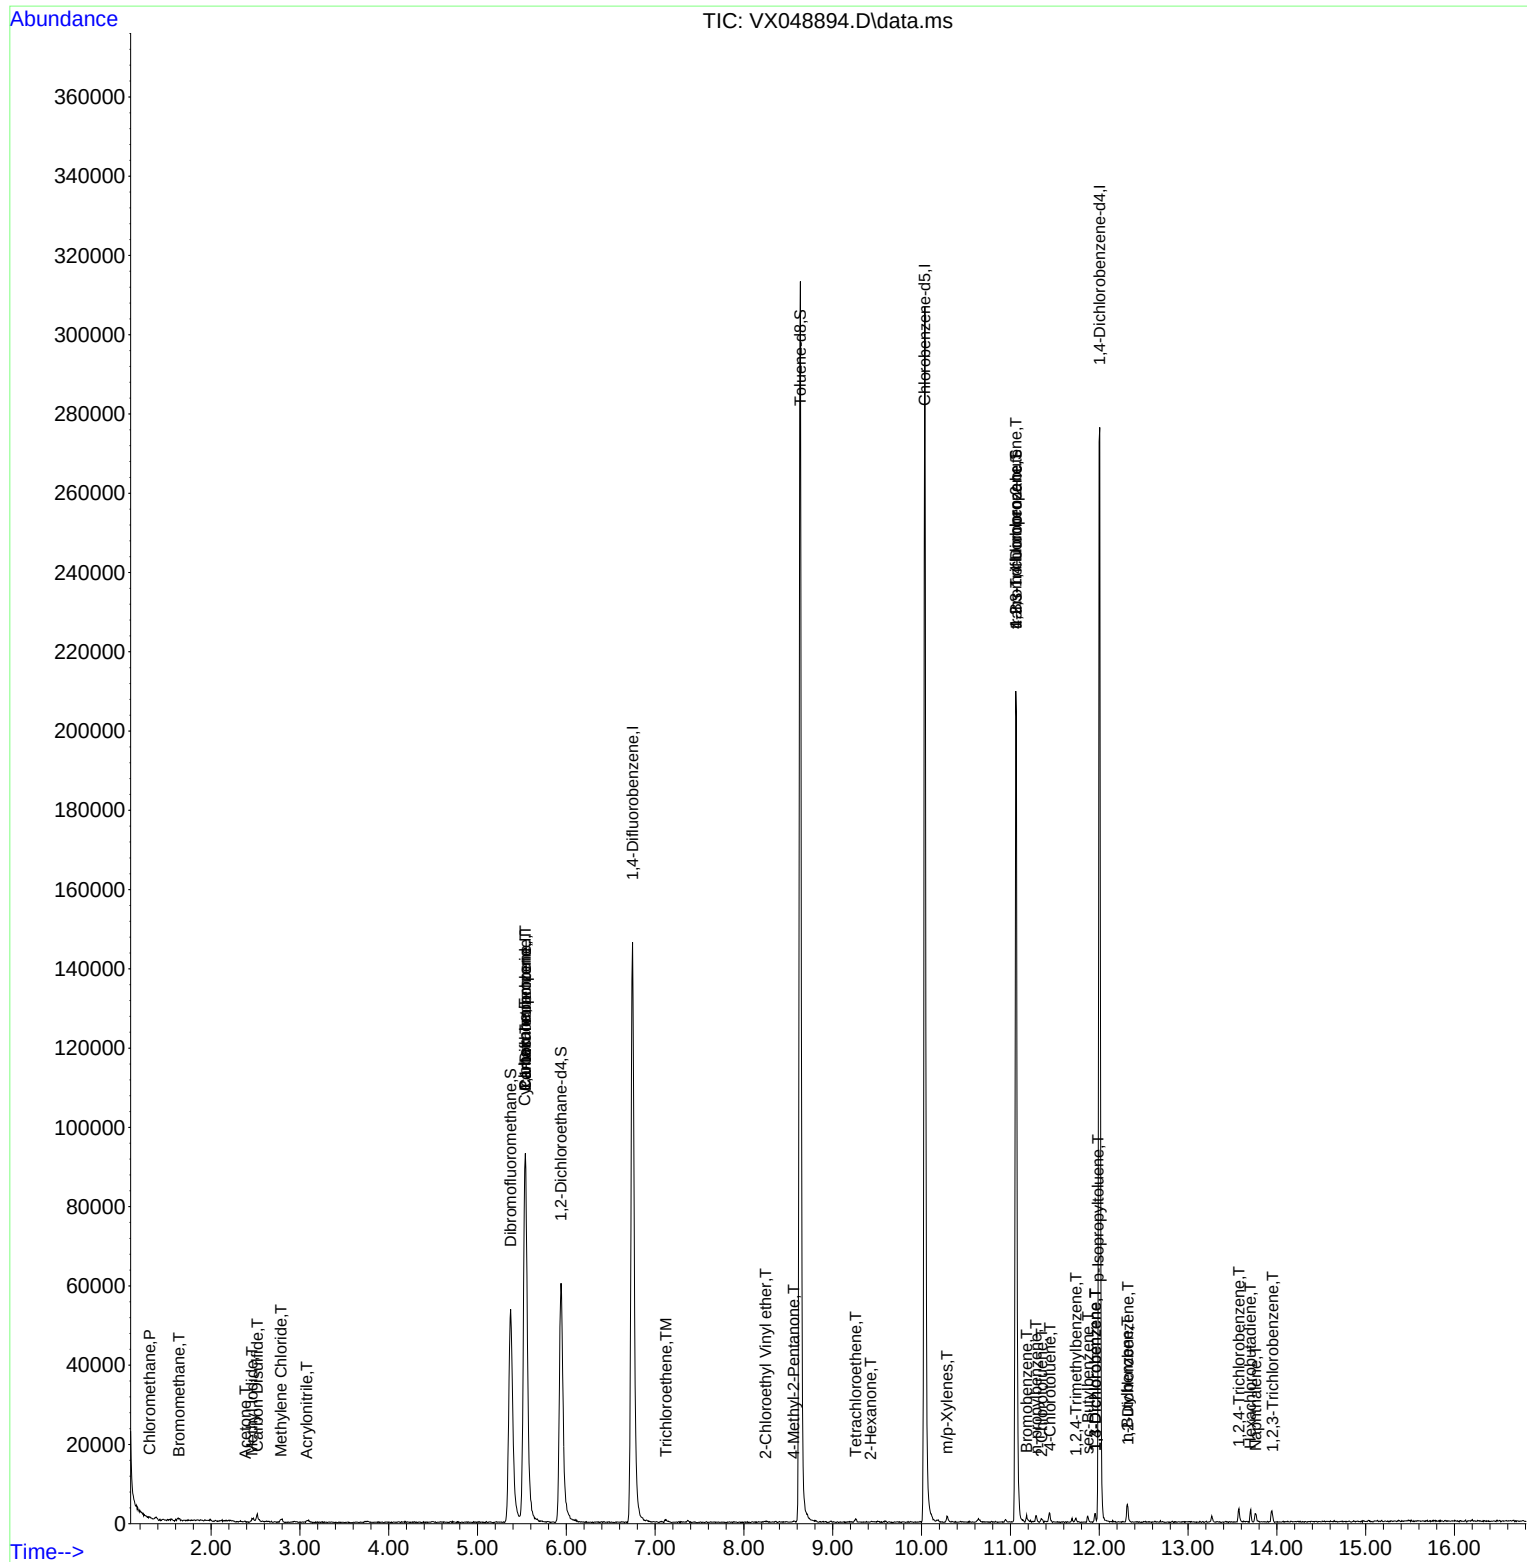




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.538 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX048894.D
Acq: 16 Dec 2025 18:08




Instrument :
MSVOA_X
ClientSampleId :
VX1216WBL01

Tgt Ion:168 Resp: 95567
Ion Ratio Lower Upper
168 100
99 58.7 44.2 66.4

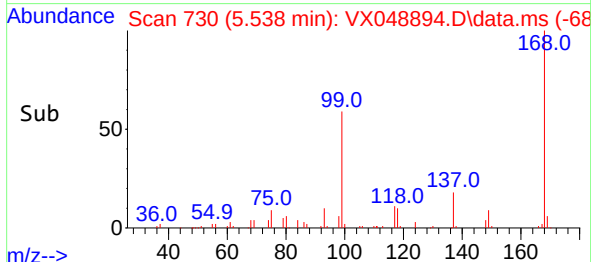

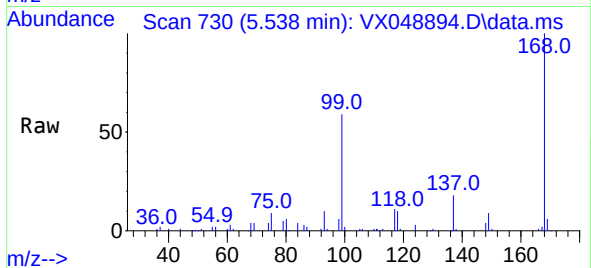


#3
Chloromethane
Concen: 0.278 ug/l
RT: 1.307 min Scan# 36
Delta R.T. 0.006 min
Lab File: VX048894.D
Acq: 16 Dec 2025 18:08

Tgt Ion: 50 Resp: 382
Ion Ratio Lower Upper
50 100
52 21.1 26.4 39.6#

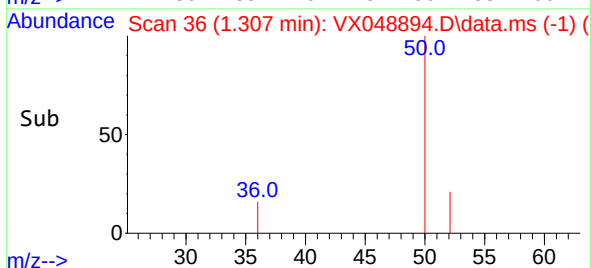





Abundance Scan 87 (1.618 min): VX048717.D\data.ms (-81)

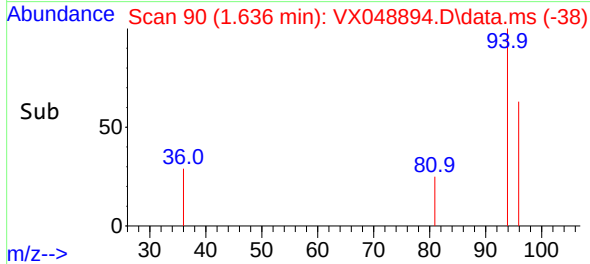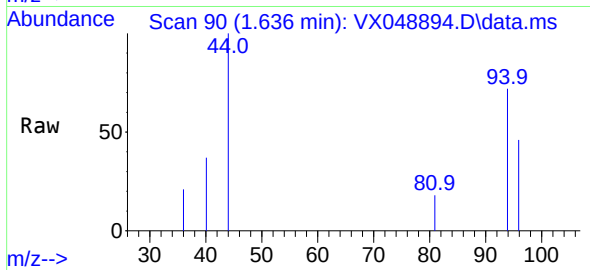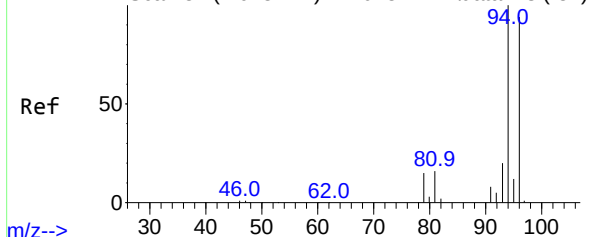

#5
Bromomethane
Concen: 0.554 ug/l
RT: 1.636 min Scan# 90
Delta R.T. 0.018 min
Lab File: VX048894.D
Acq: 16 Dec 2025 18:08


Instrument :
MSVOA_X
ClientSampleId :
VX1216WBL01


Tgt Ion: 94 Resp: 465
Ion Ratio Lower Upper
94 100
96 63.4 75.2 112.8#

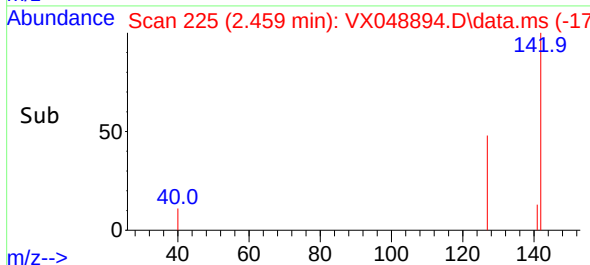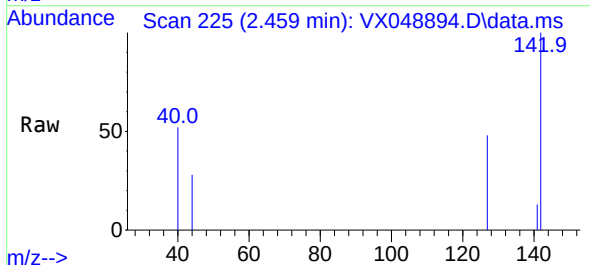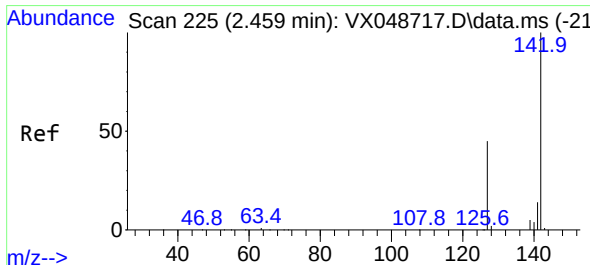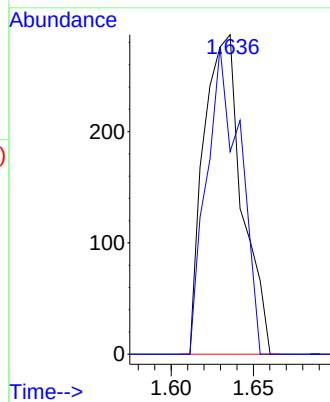

#10
Methyl Iodide
Concen: 0.901 ug/l
RT: 2.459 min Scan# 225
Delta R.T. -0.000 min
Lab File: VX048894.D
Acq: 16 Dec 2025 18:08

Tgt Ion: 142 Resp: 1297
Ion Ratio Lower Upper
142 100
127 59.3 35.8 53.6#
141 10.6 11.1 16.7#

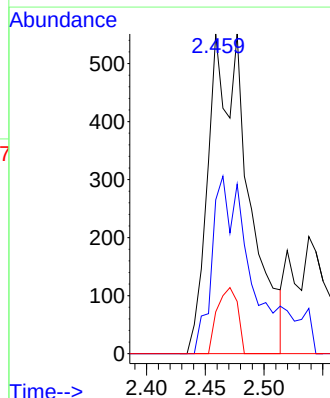



#15

Acrylonitrile

Concen: 0.515 ug/l

RT: 3.075 min Scan# 31

Delta R.T. 0.018 min

Lab File: VX048894.D

Acq: 16 Dec 2025 18:08

Instrument :





MSVOA_X

ClientSampleId :

VX1216WBL01

Tgt Ion: 53 Resp: 260

Ion	Ratio	Lower	Upper
53	100		
52	71.2	66.3	99.5
51	29.2	28.7	43.1

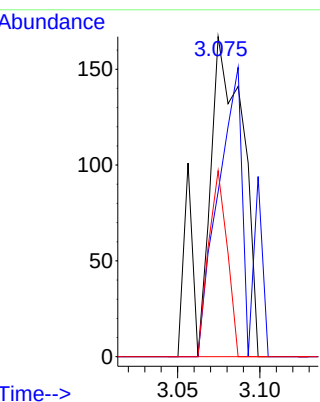

#16

Acetone

Concen: 0.746 ug/l

RT: 2.386 min Scan# 213




Delta R.T. 0.012 min


Lab File: VX048894.D

Acq: 16 Dec 2025 18:08

Tgt Ion: 43 Resp: 251

Ion	Ratio	Lower	Upper
43	100		
58	0.0	25.0	37.4#


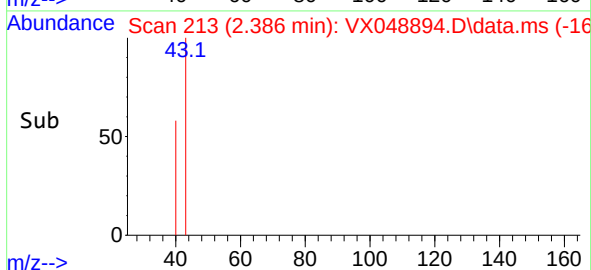

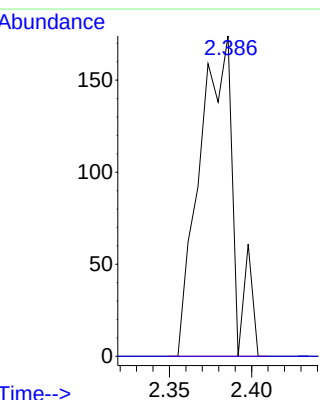




#17
Carbon Disulfide
Concen: 0.733 ug/l
RT: 2.520 min Scan# 211
Delta R.T. -0.000 min
Lab File: VX048894.D
Acq: 16 Dec 2025 18:08




Instrument :
MSVOA_X
ClientSampleId :
VX1216WBL01


Tgt Ion: 76 Resp: 2208
Ion Ratio Lower Upper
76 100
78 10.8 7.4 11.2

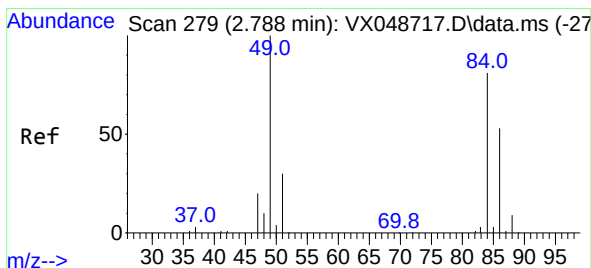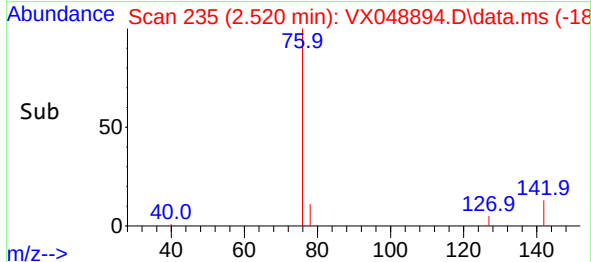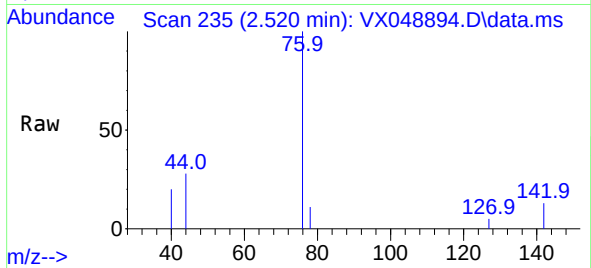

#20
Methylene Chloride
Concen: 0.309 ug/l
RT: 2.788 min Scan# 279
Delta R.T. -0.000 min
Lab File: VX048894.D
Acq: 16 Dec 2025 18:08


Tgt Ion: 84 Resp: 429
Ion Ratio Lower Upper
84 100
49 98.1 98.7 148.1#
51 25.1 29.4 44.2#
86 51.0 52.5 78.7#

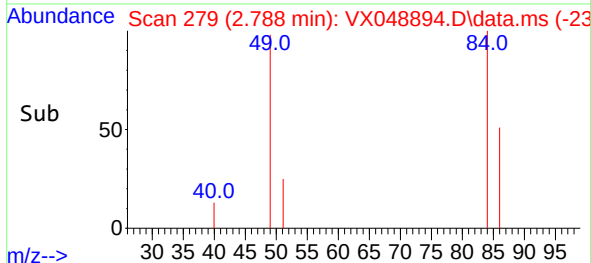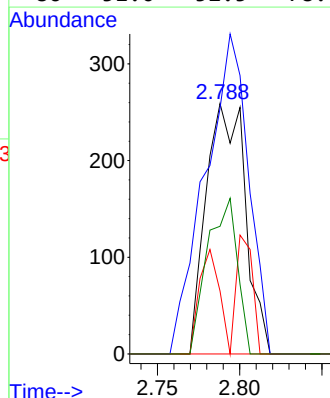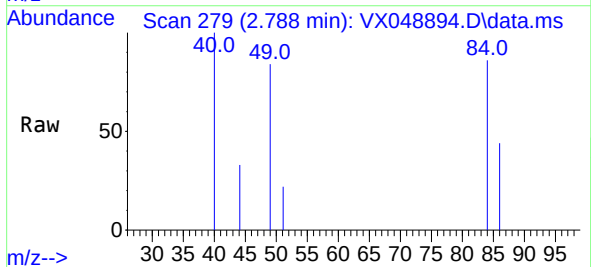



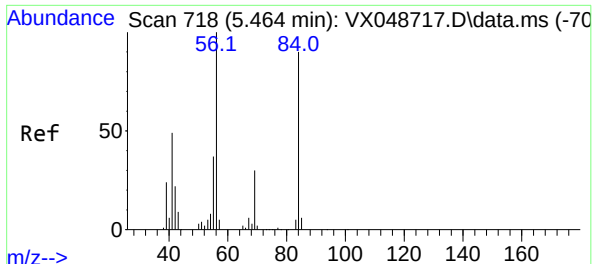


#31
Cyclohexane
Concen: 1.364 ug/l
RT: 5.531 min Scan# 718
Delta R.T. 0.073 min
Lab File: VX048894.D
Acq: 16 Dec 2025 18:08

Instrument :
MSVOA_X
ClientSampleId :
VX1216WBL01



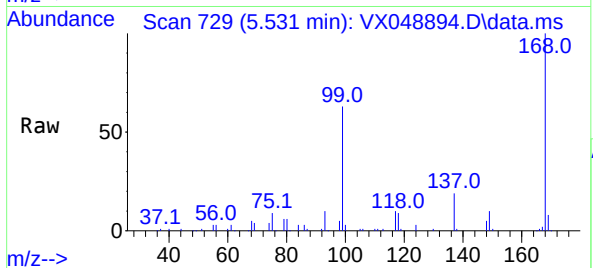



Tgt Ion: 56 Resp: 2448
Ion Ratio Lower Upper
56 100
69 121.1 24.2 36.2#
84 104.3 72.1 108.1

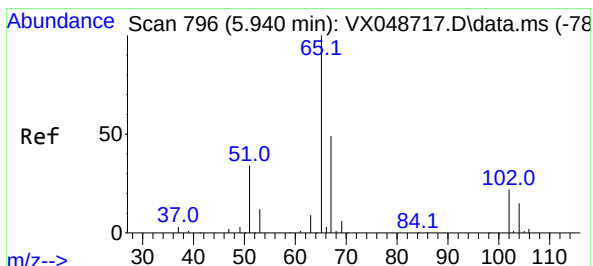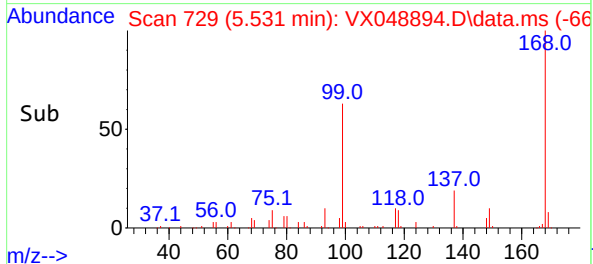

#33
1,2-Dichloroethane-d4
Concen: 41.503 ug/l
RT: 5.940 min Scan# 796
Delta R.T. -0.000 min
Lab File: VX048894.D
Acq: 16 Dec 2025 18:08

Tgt Ion: 65 Resp: 66298
Ion Ratio Lower Upper
65 100
67 50.3 0.0 107.4


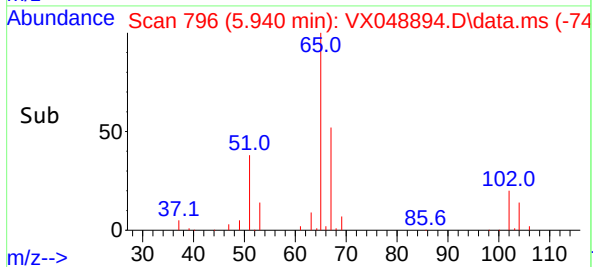

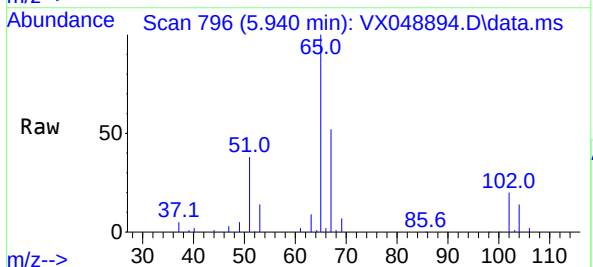




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.745 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX048894.D
Acq: 16 Dec 2025 18:08




Instrument :
MSVOA_X
ClientSampleId :
VX1216WBL01


Tgt Ion:114 Resp: 159021
Ion Ratio Lower Upper
114 100
63 21.9 0.0 39.0
88 15.3 0.0 31.8

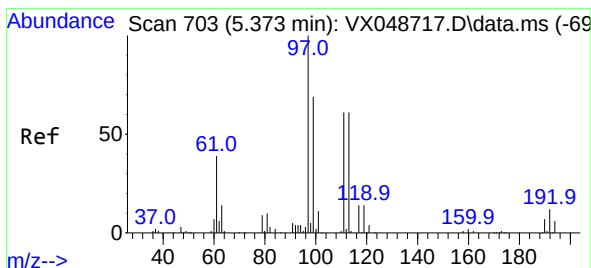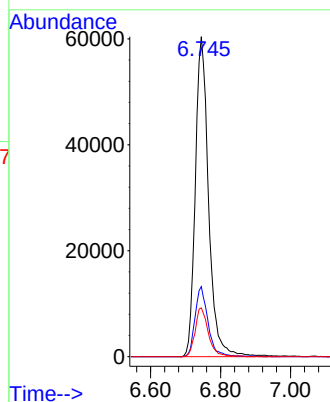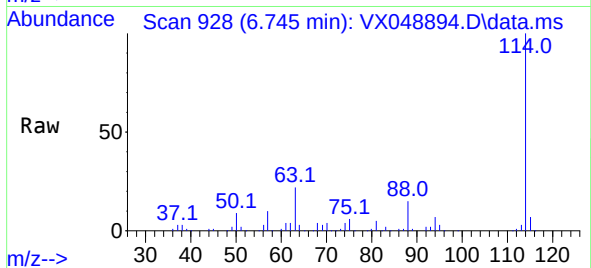

#35
Dibromofluoromethane
Concen: 44.659 ug/l
RT: 5.373 min Scan# 703
Delta R.T. 0.006 min
Lab File: VX048894.D
Acq: 16 Dec 2025 18:08

Tgt Ion:113 Resp: 52786
Ion Ratio Lower Upper
113 100
111 99.9 79.5 119.3
192 18.8 16.1 24.1


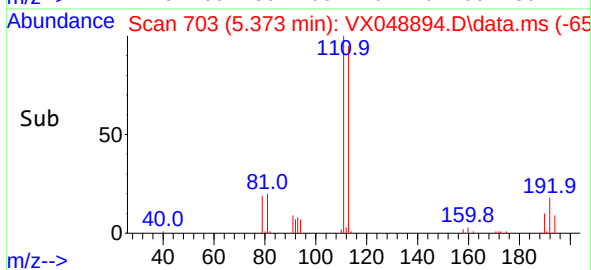
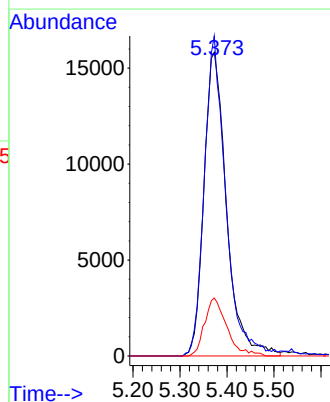
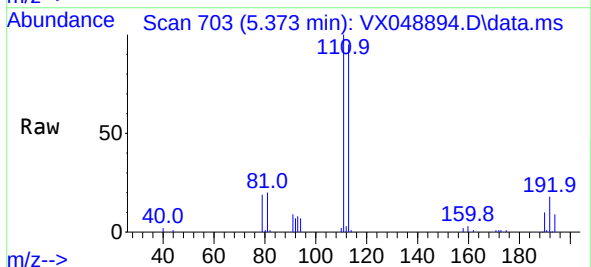


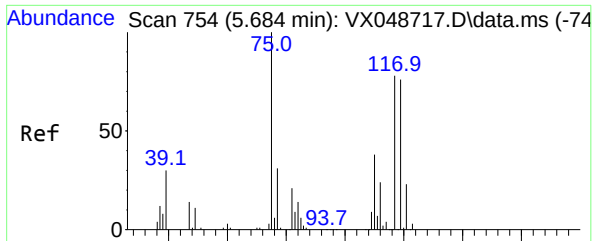

#36
1,1-Dichloropropene
Concen: 5.494 ug/l
RT: 5.538 min Scan# 71
Delta R.T. -0.146 min
Lab File: VX048894.D
Acq: 16 Dec 2025 18:08




Instrument :
MSVOA_X
ClientSampleId :
VX1216WBL01


Tgt Ion: 75 Resp: 8150
Ion Ratio Lower Upper
75 100
110 8.4 18.6 55.8#
77 0.0 25.3 37.9#

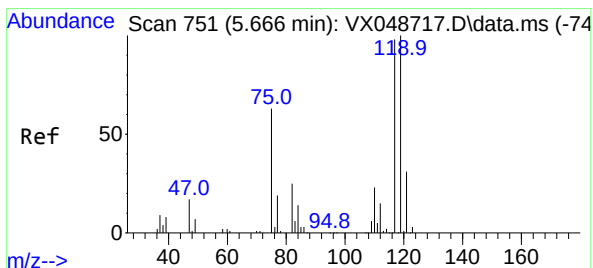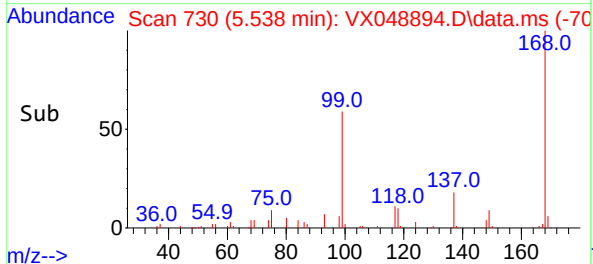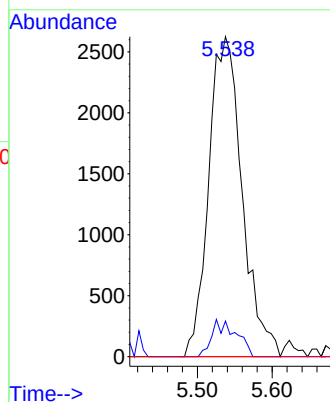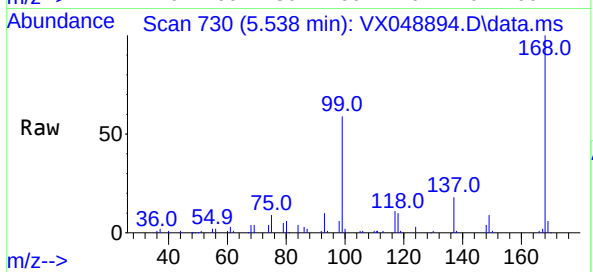

#38
Carbon Tetrachloride
Concen: 5.544 ug/l
RT: 5.538 min Scan# 730
Delta R.T. -0.128 min
Lab File: VX048894.D
Acq: 16 Dec 2025 18:08

Tgt Ion: 117 Resp: 9803
Ion Ratio Lower Upper
117 100
119 7.6 80.5 120.7#
121 0.0 25.4 38.0#


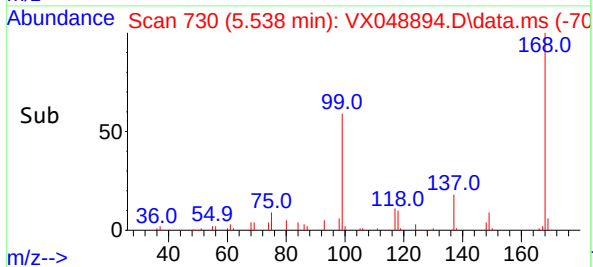

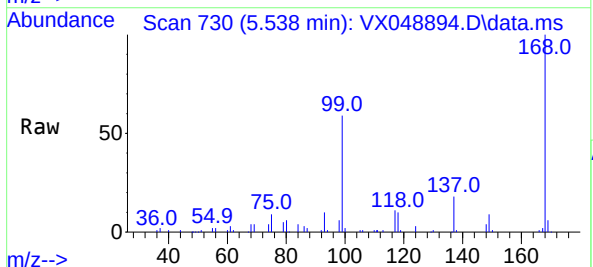




#44
Trichloroethene
Concen: 0.279 ug/l
RT: 7.123 min Scan# 990
Delta R.T. 0.012 min
Lab File: VX048894.D
Acq: 16 Dec 2025 18:08




Instrument :
MSVOA_X
ClientSampleId :
VX1216WBL01


Tgt Ion:130 Resp: 342
Ion Ratio Lower Upper
130 100
95 45.6 0.0 189.6



#50
Toluene-d8
Concen: 46.195 ug/l
RT: 8.635 min Scan# 1238
Delta R.T. -0.000 min
Lab File: VX048894.D
Acq: 16 Dec 2025 18:08

Tgt Ion: 98 Resp: 194934
Ion Ratio Lower Upper
98 100
100 63.8 53.4 80.0


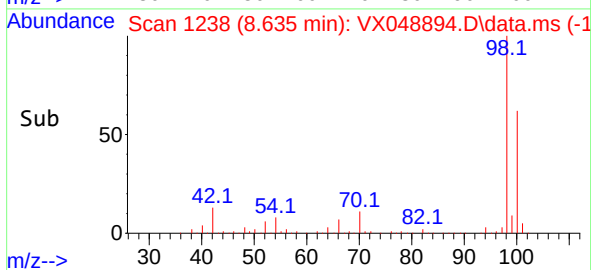




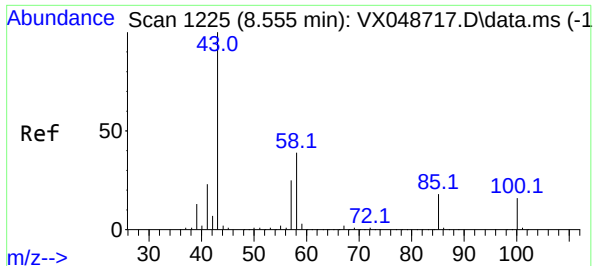

#51
4-Methyl-2-Pentanone
Concen: 0.234 ug/l
RT: 8.561 min Scan# 1174
Delta R.T. 0.006 min
Lab File: VX048894.D
Acq: 16 Dec 2025 18:08




Instrument :
MSVOA_X
ClientSampleId :
VX1216WBL01


Tgt Ion: 43 Resp: 308
Ion Ratio Lower Upper
43 100
58 0.0 32.2 48.4#

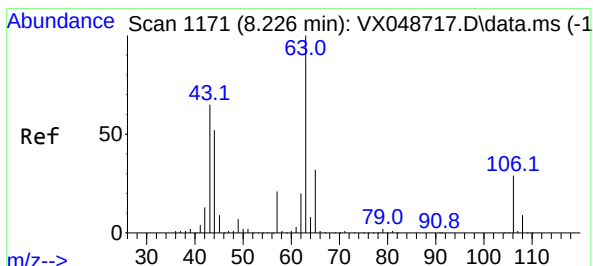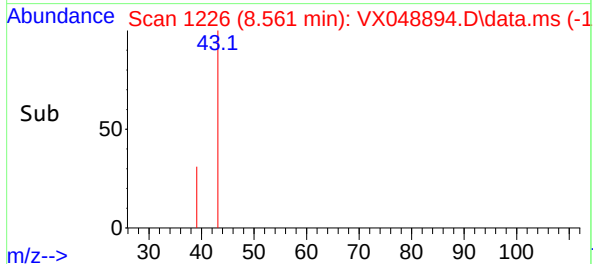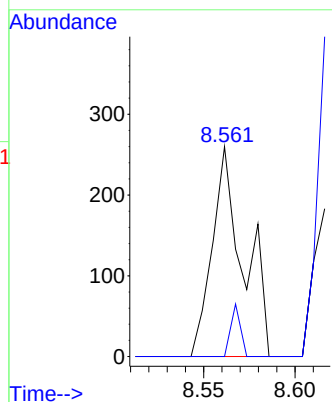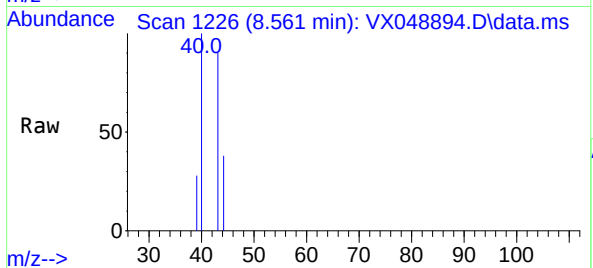

#58
2-Chloroethyl Vinyl ether
Concen: 0.229 ug/l
RT: 8.244 min Scan# 1174
Delta R.T. 0.018 min
Lab File: VX048894.D
Acq: 16 Dec 2025 18:08

Tgt Ion: 63 Resp: 213
Ion Ratio Lower Upper
63 100
106 0.0 23.4 35.2#


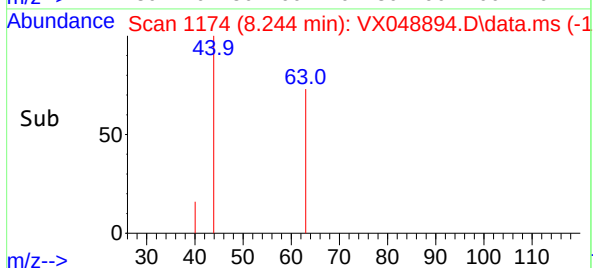

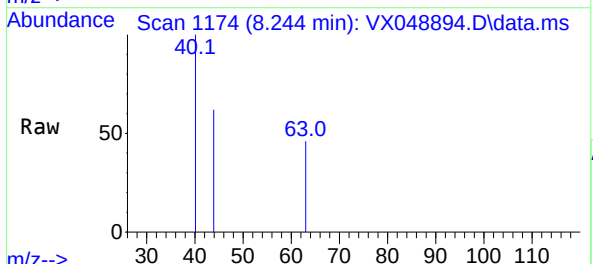


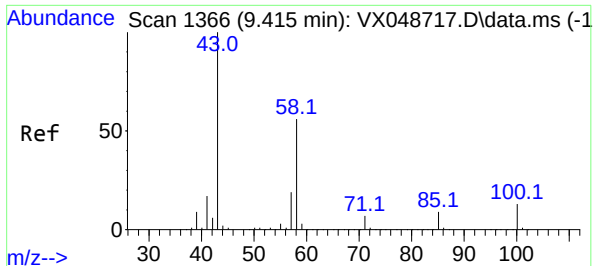

#59
2-Hexanone
Concen: 0.309 ug/l
RT: 9.427 min Scan# 11
Delta R.T. 0.012 min
Lab File: VX048894.D
Acq: 16 Dec 2025 18:08




Instrument :
MSVOA_X
ClientSampleId :
VX1216WBL01


Tgt Ion: 43 Resp: 276
Ion Ratio Lower Upper
43 100
58 0.0 27.8 83.4#

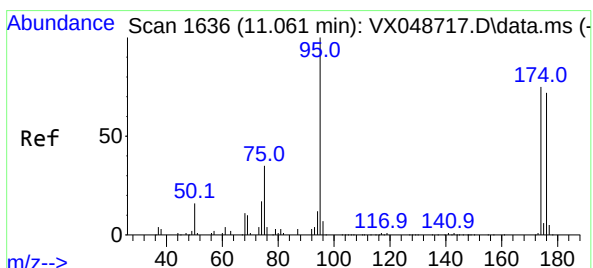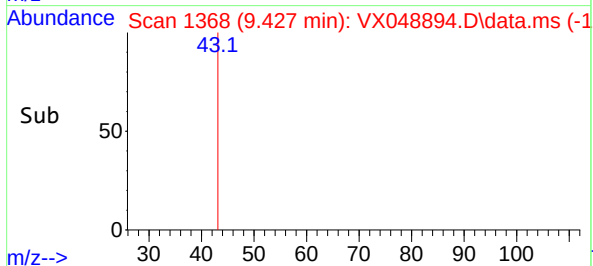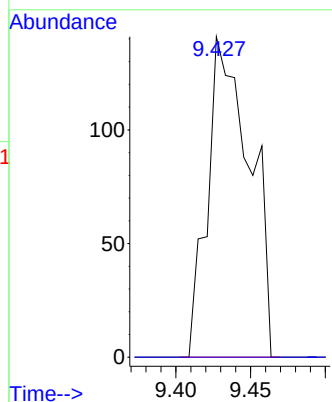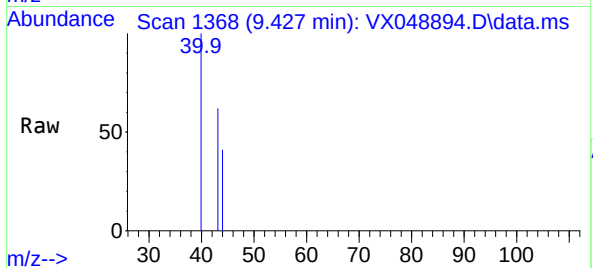

#62
4-Bromofluorobenzene
Concen: 38.688 ug/l
RT: 11.061 min Scan# 1636
Delta R.T. -0.000 min
Lab File: VX048894.D
Acq: 16 Dec 2025 18:08

Tgt Ion: 95 Resp: 58612
Ion Ratio Lower Upper
95 100
174 80.2 0.0 157.8
176 77.5 0.0 154.0


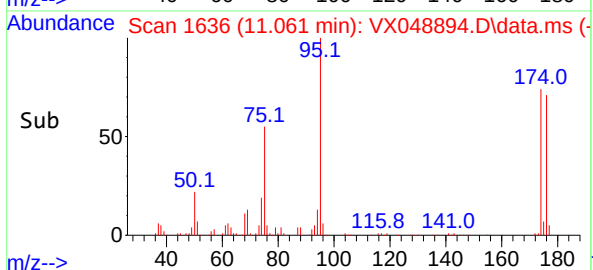

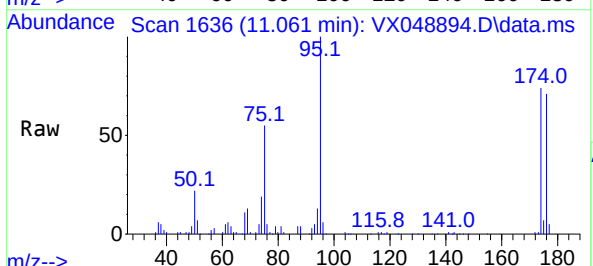




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.037 min Scan# 1468
Delta R.T. -0.000 min
Lab File: VX048894.D
Acq: 16 Dec 2025 18:08




Instrument :
MSVOA_X
ClientSampleId :
VX1216WBL01


Tgt Ion:117 Resp: 136648
Ion Ratio Lower Upper
117 100
82 57.7 44.1 66.1
119 32.3 25.2 37.8

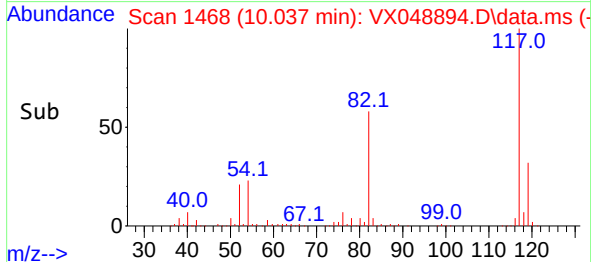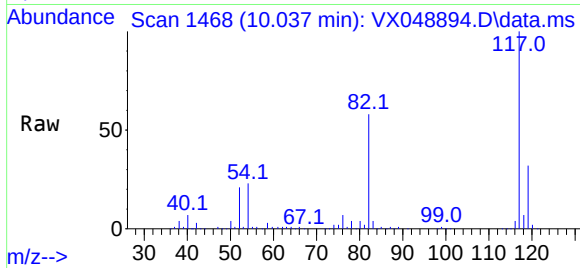

#64
Tetrachloroethene
Concen: 0.253 ug/l
RT: 9.256 min Scan# 1340
Delta R.T. -0.000 min
Lab File: VX048894.D
Acq: 16 Dec 2025 18:08

Tgt Ion:164 Resp: 222
Ion Ratio Lower Upper
164 100
166 119.3 103.1 154.7
129 51.3 76.9 115.3#
131 71.3 75.1 112.7#


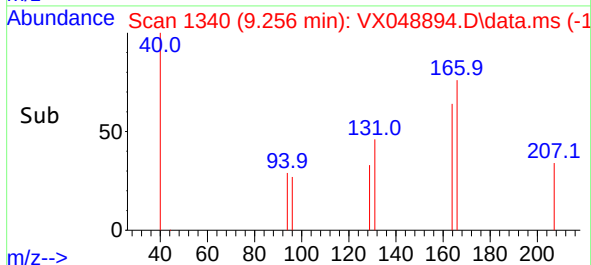
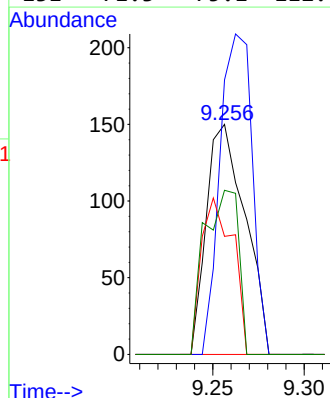
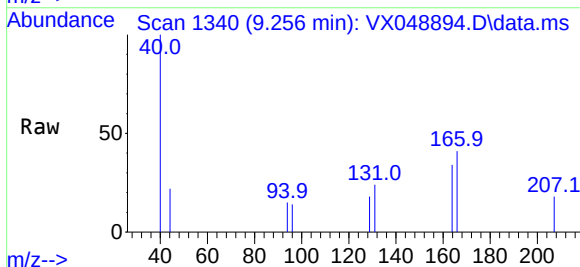




#68
m/p-Xylenes
Concen: 0.258 ug/l
RT: 10.287 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX048894.D
Acq: 16 Dec 2025 18:08




Instrument :
MSVOA_X
ClientSampleId :
VX1216WBL01


Tgt Ion:106 Resp: 493
Ion Ratio Lower Upper
106 100
91 223.7 164.2 246.4

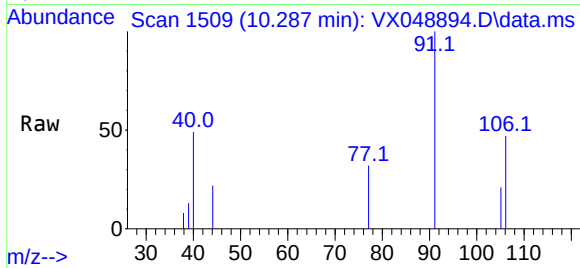

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.006 min Scan# 1791
Delta R.T. 0.006 min
Lab File: VX048894.D
Acq: 16 Dec 2025 18:08

Tgt Ion:152 Resp: 60256
Ion Ratio Lower Upper
152 100
115 58.1 42.1 126.4
150 155.0 0.0 347.8


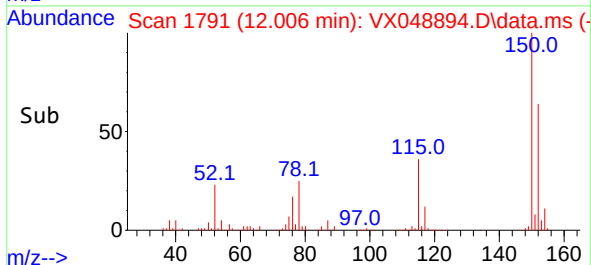
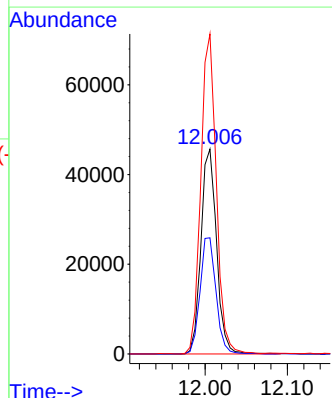
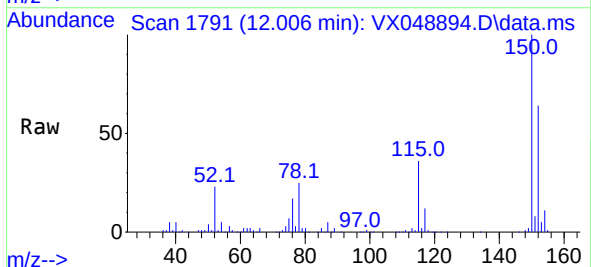




#76
1,2,3-Trichloropropane
Concen: 32.970 ug/l
RT: 11.061 min Scan# 1636
Delta R.T. -0.159 min
Lab File: VX048894.D
Acq: 16 Dec 2025 18:08




Instrument :
MSVOA_X
ClientSampleId :
VX1216WBL01


Tgt Ion: 75 Resp: 31943
Ion Ratio Lower Upper
75 100
77 1.4 24.3 73.0#

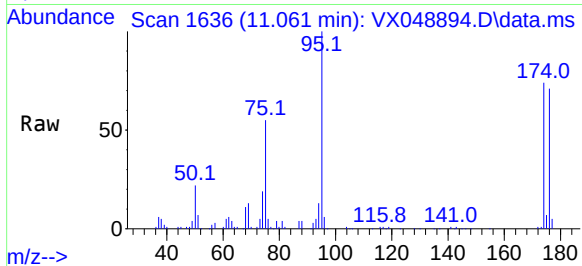

#77
Bromobenzene
Concen: 0.263 ug/l
RT: 11.183 min Scan# 1656
Delta R.T. 0.006 min
Lab File: VX048894.D
Acq: 16 Dec 2025 18:08

Tgt Ion:156 Resp: 277
Ion Ratio Lower Upper
156 100
77 234.3 80.3 240.9
158 124.2 48.9 146.6


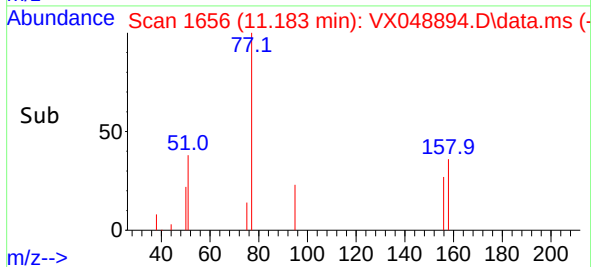

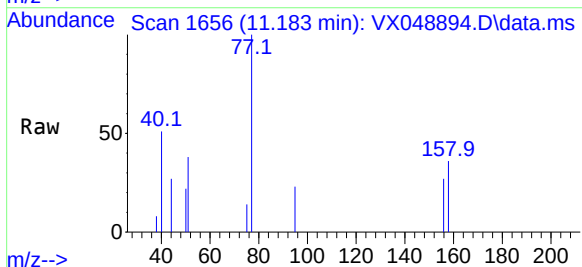




#78
n-propylbenzene
Concen: 0.278 ug/l
RT: 11.287 min Scan# 1673
Delta R.T. -0.000 min
Lab File: VX048894.D
Acq: 16 Dec 2025 18:08




Instrument :
MSVOA_X
ClientSampleId :
VX1216WBL01


Tgt Ion: 91 Resp: 1384
Ion Ratio Lower Upper
91 100
120 20.2 11.4 34.2



#79
2-Chlorotoluene
Concen: 0.228 ug/l
RT: 11.354 min Scan# 1684
Delta R.T. 0.006 min
Lab File: VX048894.D
Acq: 16 Dec 2025 18:08

Tgt Ion: 91 Resp: 702
Ion Ratio Lower Upper
91 100
126 30.2 16.8 50.3


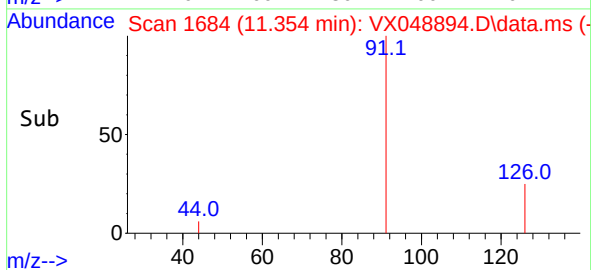






#81
trans-1,4-Dichloro-2-butene
Concen: 83.737 ug/l
RT: 11.061 min Scan# 1636
Delta R.T. 0.061 min
Lab File: VX048894.D
Acq: 16 Dec 2025 18:08




Instrument :
MSVOA_X
ClientSampleId :
VX1216WBL01


Tgt Ion: 75 Resp: 31943
Ion Ratio Lower Upper
75 100
53 0.0 79.9 119.9#
89 0.0 67.1 100.7#

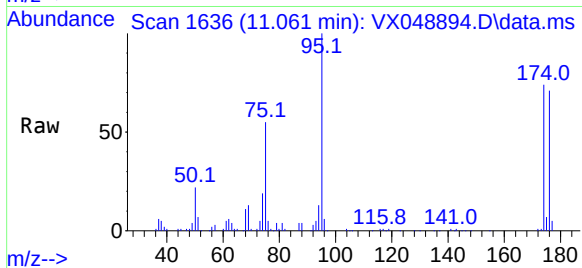

#82
4-Chlorotoluene
Concen: 0.290 ug/l
RT: 11.445 min Scan# 1699
Delta R.T. 0.012 min
Lab File: VX048894.D
Acq: 16 Dec 2025 18:08

Tgt Ion: 91 Resp: 1021
Ion Ratio Lower Upper
91 100
126 40.5 14.7 44.1


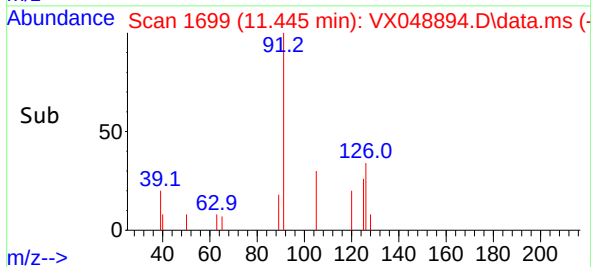

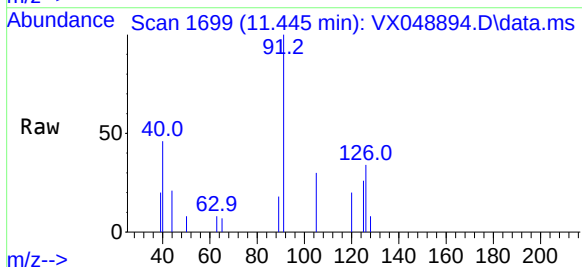




#84
1,2,4-Trimethylbenzene
Concen: 0.210 ug/l
RT: 11.738 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX048894.D
Acq: 16 Dec 2025 18:08




Instrument :
MSVOA_X
ClientSampleId :
VX1216WBL01


Tgt Ion:105 Resp: 717
Ion Ratio Lower Upper
105 100
120 37.8 22.3 66.8

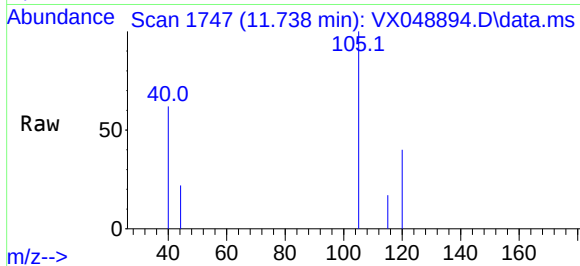

#85
sec-Butylbenzene
Concen: 0.244 ug/l
RT: 11.872 min Scan# 1769
Delta R.T. -0.000 min
Lab File: VX048894.D
Acq: 16 Dec 2025 18:08

Tgt Ion:105 Resp: 1048
Ion Ratio Lower Upper
105 100
134 13.8 9.8 29.5


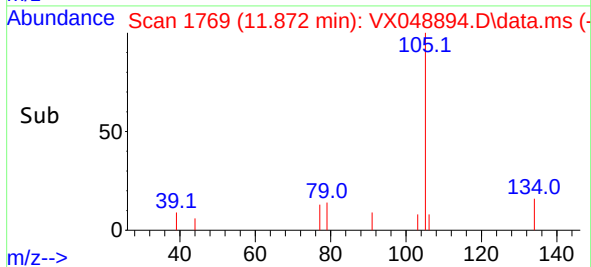

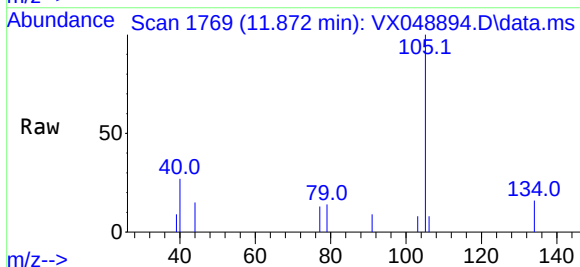




#86
p-Isopropyltoluene
Concen: 0.271 ug/l
RT: 11.988 min Scan# 1788
Delta R.T. -0.000 min
Lab File: VX048894.D
Acq: 16 Dec 2025 18:08




Instrument :
MSVOA_X
ClientSampleId :
VX1216WBL01


Tgt Ion:	119	Resp:	957
Ion	Ratio	Lower	Upper
119	100		
134	37.5	13.1	39.3
91	42.1	11.8	35.4

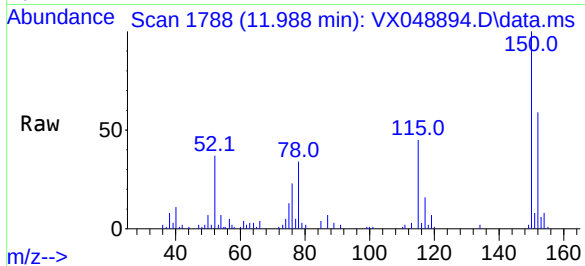

#87
1,3-Dichlorobenzene
Concen: 0.449 ug/l
RT: 11.957 min Scan# 1783
Delta R.T. 0.006 min
Lab File: VX048894.D
Acq: 16 Dec 2025 18:08


Tgt Ion:	146	Resp:	885
Ion	Ratio	Lower	Upper
146	100		
111	35.5	20.3	60.8
148	63.2	32.1	96.5

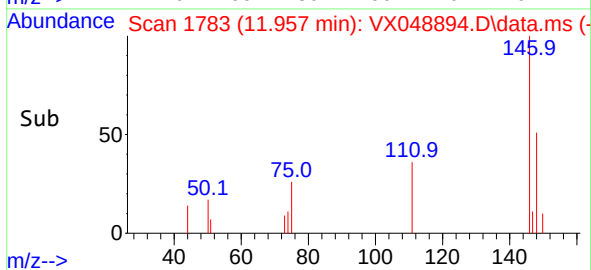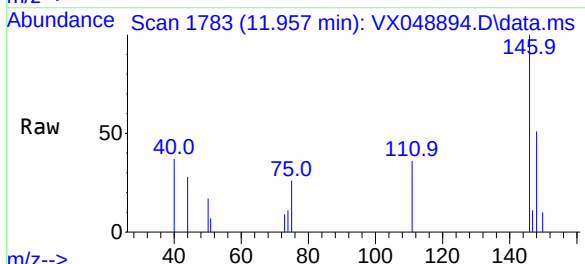



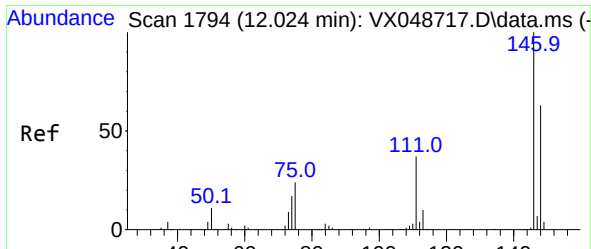


#88
1,4-Dichlorobenzene
Concen: 0.428 ug/l
RT: 11.957 min Scan# 11
Delta R.T. -0.061 min
Lab File: VX048894.D
Acq: 16 Dec 2025 18:08

Instrument :
MSVOA_X
ClientSampleId :
VX1216WBL01



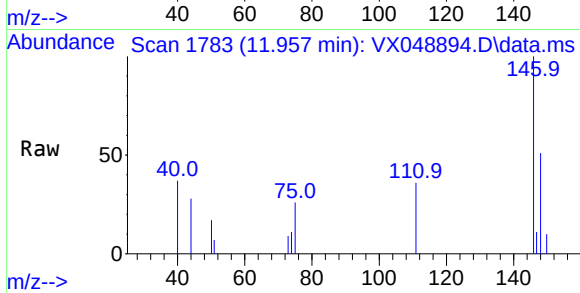



Tgt Ion:146 Resp: 885
Ion Ratio Lower Upper
146 100
111 35.5 19.6 58.7
148 63.2 31.6 94.7

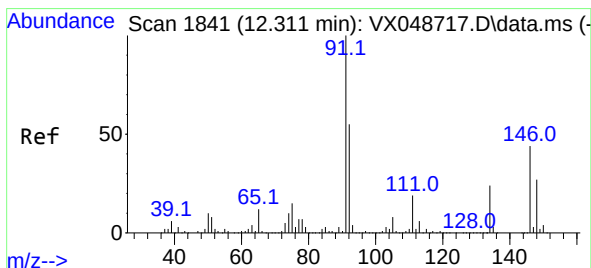

#89
n-Butylbenzene
Concen: 0.605 ug/l
RT: 12.317 min Scan# 1842
Delta R.T. 0.006 min
Lab File: VX048894.D
Acq: 16 Dec 2025 18:08

Tgt Ion: 91 Resp: 2039
Ion Ratio Lower Upper
91 100
92 53.5 27.1 81.3
134 26.0 12.9 38.6


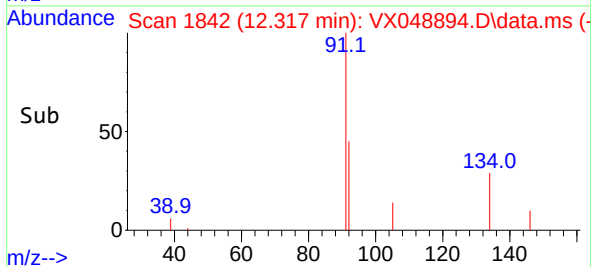

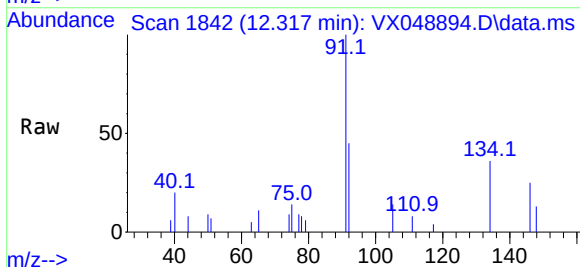




#91
1,2-Dichlorobenzene
Concen: 0.303 ug/l
RT: 12.323 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX048894.D
Acq: 16 Dec 2025 18:08




Instrument :
MSVOA_X
ClientSampleId :
VX1216WBL01


Tgt Ion:	146	Resp:	590
Ion	Ratio	Lower	Upper
146	100		
111	40.2	20.8	62.5
148	63.6	32.0	96.0

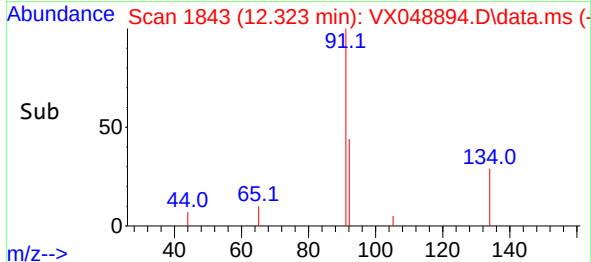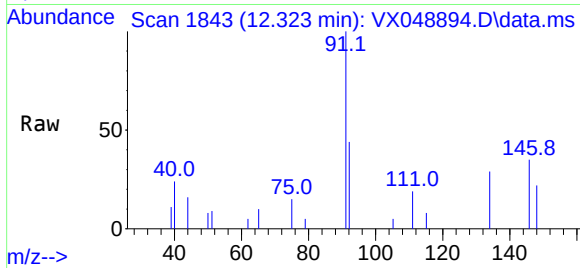

#93
1,2,4-Trichlorobenzene
Concen: 0.951 ug/l
RT: 13.573 min Scan# 2048
Delta R.T. 0.006 min
Lab File: VX048894.D
Acq: 16 Dec 2025 18:08

Tgt Ion:	180	Resp:	1066
Ion	Ratio	Lower	Upper
180	100		
182	99.2	46.9	140.8
145	31.8	15.1	45.3


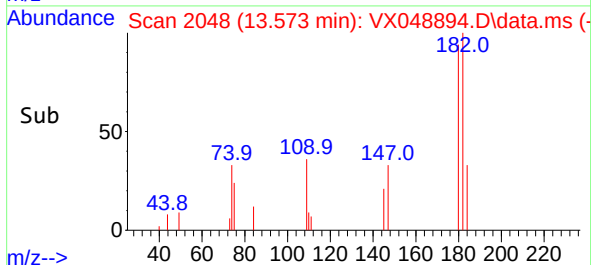
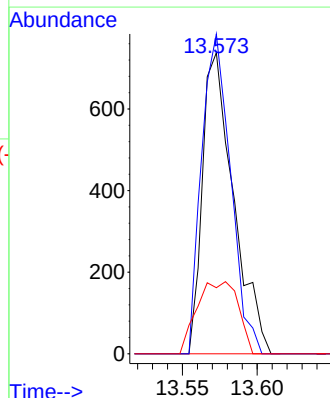
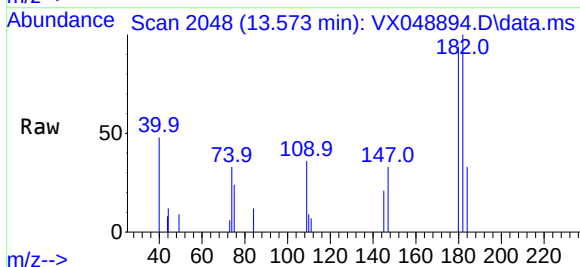




#94
Hexachlorobutadiene
Concen: 1.316 ug/l
RT: 13.701 min Scan# 2070
Delta R.T. -0.006 min
Lab File: VX048894.D
Acq: 16 Dec 2025 18:08




Instrument :
MSVOA_X
ClientSampleId :
VX1216WBL01


Tgt Ion:	225	Resp:	637
Ion	Ratio	Lower	Upper
225	100		
223	53.2	33.0	98.9
227	51.2	32.9	98.7

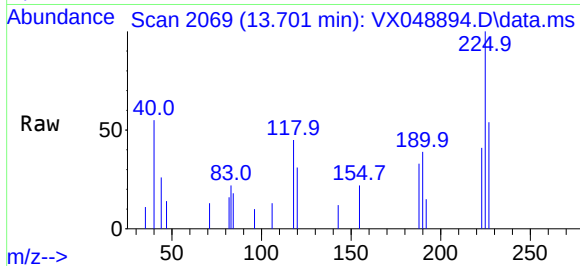

#95
Naphthalene
Concen: 0.717 ug/l
RT: 13.762 min Scan# 2079
Delta R.T. 0.006 min
Lab File: VX048894.D
Acq: 16 Dec 2025 18:08


Tgt Ion:	128	Resp:	2031
Ion	Ratio	Lower	Upper
128	100		
127	11.7	10.2	15.2
129	11.3	8.6	13.0

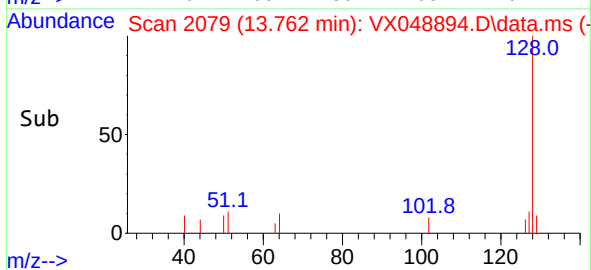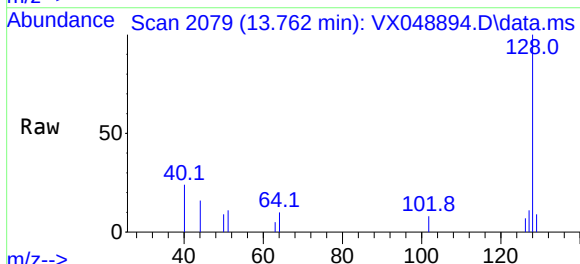



#96
 1,2,3-Trichlorobenzene
 Concen: 0.922 ug/l
 RT: 13.951 min Scan# 21
 Delta R.T. 0.012 min
 Lab File: VX048894.D
 Acq: 16 Dec 2025 18:08

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1216WBL01

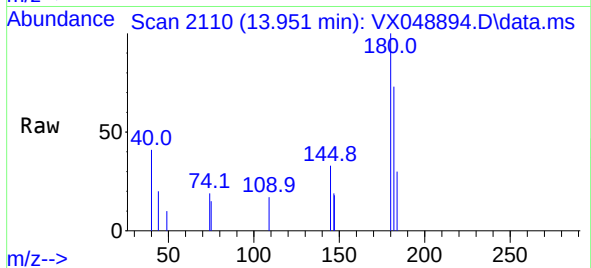

Tgt Ion:	180	Resp:	929
Ion	Ratio	Lower	Upper
180	100		
182	104.4	48.0	144.2
145	34.0	16.6	49.8

