

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX121718\  
 Data File : VX006576.D  
 Acq On : 17 Dec 2018 16:46  
 Operator : JC/MD  
 Sample : J6405-13  
 Misc : 5.0mL/MSVOA X/WATER  
 ALS Vial : 17 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 EB01-20181211

Quant Time: Dec 18 00:40:46 2018  
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X112918W.M  
 Quant Title : SW846 8260  
 QLast Update : Fri Nov 30 03:55:33 2018  
 Response via : Initial Calibration

| Internal Standards         | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|----------------------------|-------|------|----------|-------|-------|----------|
| 1) Pentafluorobenzene      | 5.67  | 168  | 666910   | 50.00 | ug/l  | 0.00     |
| 34) 1,4-Difluorobenzene    | 6.86  | 114  | 1065259  | 50.00 | ug/l  | 0.00     |
| 63) Chlorobenzene-d5       | 10.12 | 117  | 973369   | 50.00 | ug/l  | 0.00     |
| 72) 1,4-Dichlorobenzene-d4 | 12.08 | 152  | 456340   | 50.00 | ug/l  | 0.00     |

| System Monitoring Compounds | R.T.  | QIon | Response | Conc  | Units   | Dev(Min) |
|-----------------------------|-------|------|----------|-------|---------|----------|
| 33) 1,2-Dichloroethane-d4   | 6.07  | 65   | 369132   | 54.22 | ug/l    | 0.00     |
| Spiked Amount               |       |      | Recovery | =     | 108.44% |          |
| 35) Dibromofluoromethane    | 5.50  | 113  | 320936   | 46.53 | ug/l    | 0.00     |
| Spiked Amount               |       |      | Recovery | =     | 93.06%  |          |
| 50) Toluene-d8              | 8.71  | 98   | 1263443  | 50.36 | ug/l    | 0.00     |
| Spiked Amount               |       |      | Recovery | =     | 100.72% |          |
| 62) 4-Bromofluorobenzene    | 11.13 | 95   | 461605   | 48.83 | ug/l    | 0.00     |
| Spiked Amount               |       |      | Recovery | =     | 97.66%  |          |


| Target Compounds               | R.T.  | QIon | Response | Conc   | Units  | Qvalue |
|--------------------------------|-------|------|----------|--------|--------|--------|
| 11) Tert butyl alcohol         | 3.02  | 59   | 11222    | 6.027  | ug/l # | 73     |
| 13) Acrolein                   | 2.31  | 56   | 357      | 0.351  | ug/l # | 42     |
| 16) Acetone                    | 2.45  | 43   | 12275    | 3.842  | ug/l   | 95     |
| 20) Methylene Chloride         | 2.85  | 84   | 1839     | 0.270  | ug/l # | 48     |
| 25) 2-Butanone                 | 4.69  | 43   | 1126     | 0.247  | ug/l # | 47     |
| 36) 1,1-Dichloropropene        | 5.66  | 75   | 44806    | 4.995  | ug/l # | 47     |
| 38) Carbon Tetrachloride       | 5.67  | 117  | 62769    | 5.948  | ug/l # | 16     |
| 43) Isopropyl Acetate          | 6.46  | 43   | 7701     | 0.460  | ug/l # | 85     |
| 44) Trichloroethene            | 7.21  | 130  | 67899    | 8.342  | ug/l   | 91     |
| 49) 1,4-Dioxane                | 7.73  | 88   | 281      | 1.399  | ug/l # | 47     |
| 76) 1,2,3-Trichloropropane     | 11.13 | 75   | 215706   | 24.490 | ug/l # | 37     |
| 81) trans-1,4-Dichloro-2-buten | 11.13 | 75   | 215706   | 57.470 | ug/l # | 15     |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX121718\  
Data File : VX006576.D  
Acq On : 17 Dec 2018 16:46  
Operator : JC/MD  
Sample : J6405-13  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 17 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleID :  
EB01-20181211

Quant Time: Dec 18 00:40:46 2018  
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X112918W.M  
Quant Title : SW846 8260  
QLast Update : Fri Nov 30 03:55:33 2018  
Response via : Initial Calibration

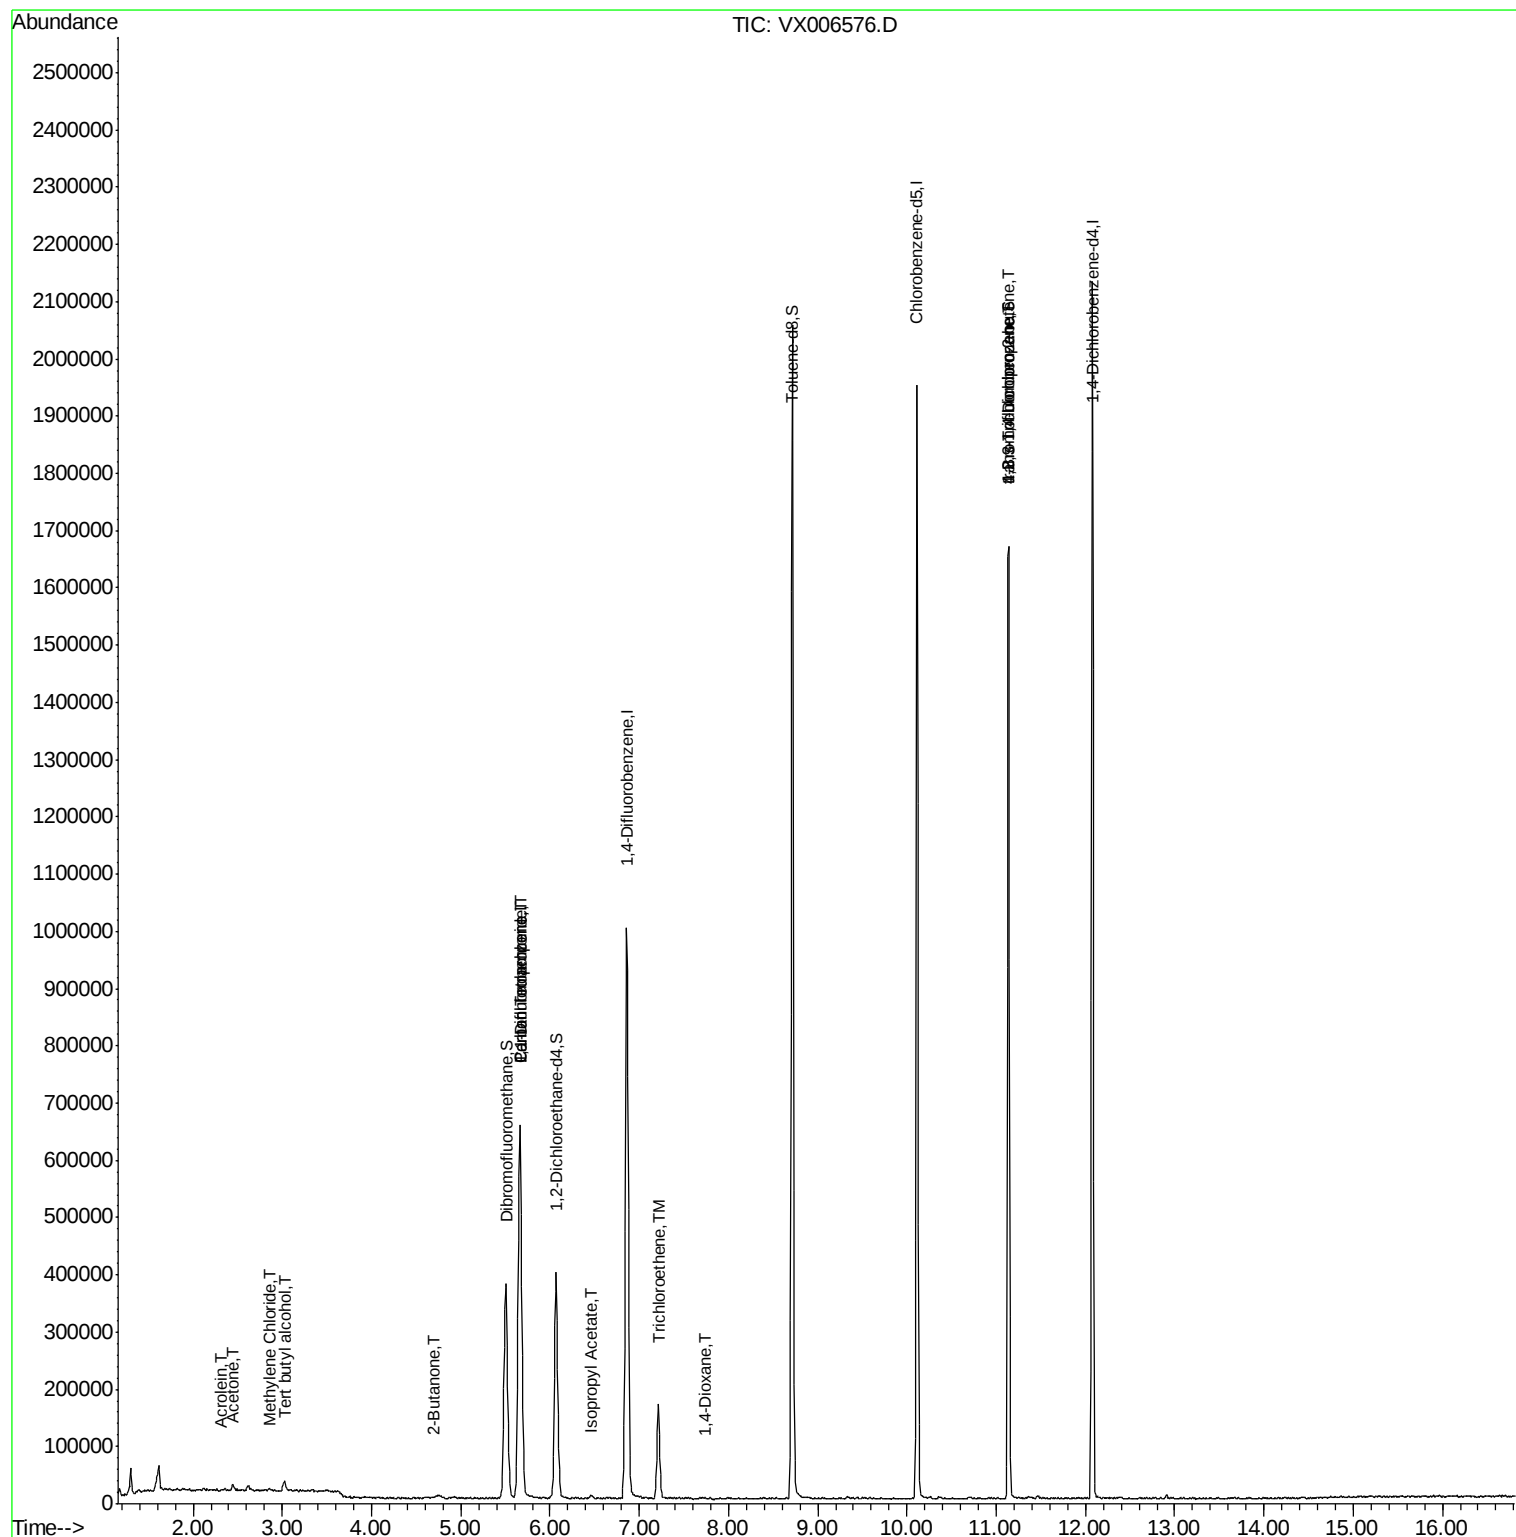

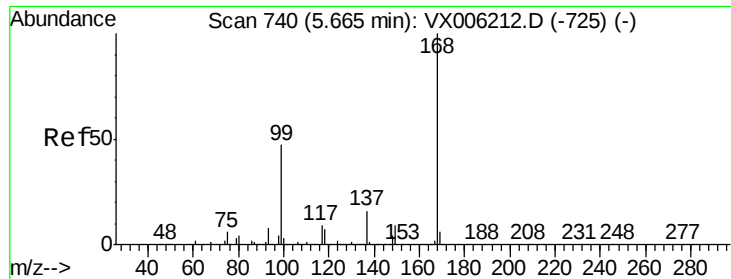

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. 0.00 min

Lab File: VX006576.D

Acq: 17 Dec 2018 16:46

Instrument :

MSVOA\_X

ClientSampleId :


EB01-20181211

Tot Ion:168 Resp: 666910

Ion Ratio Lower Upper

168 100

99 55.9 37.8 56.8

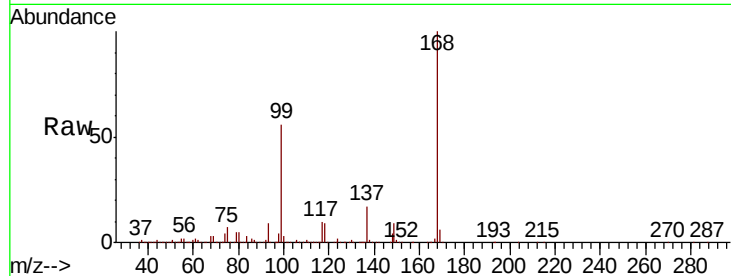

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

250000

200000

150000



100000

50000

0

Time-->

5.50 5.60 5.70 5.80

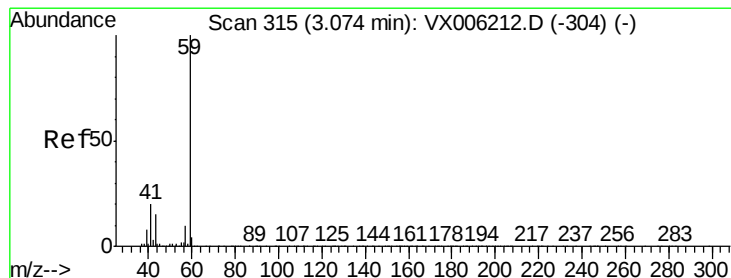

#11

Tert butyl alcohol

Concen: 6.027 ug/l

RT: 3.02 min Scan# 306

Delta R.T. -0.05 min

Lab File: VX006576.D


Acq: 17 Dec 2018 16:46

Tgt Ion: 59 Resp: 11222

Ion Ratio Lower Upper

59 100

57 0.0 8.2 12.2#

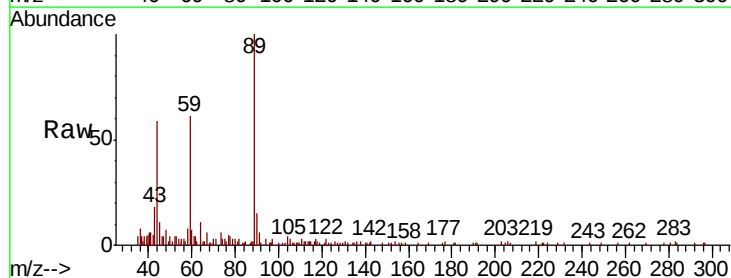

Abundance Ion 59.00 (58.70 to 59.70): VX0

Ion 57.00 (56.70 to 57.70): VX0

3.02

4000

3000


2000


1000

0

Time-->

2.90 2.95 3.00 3.05 3.10



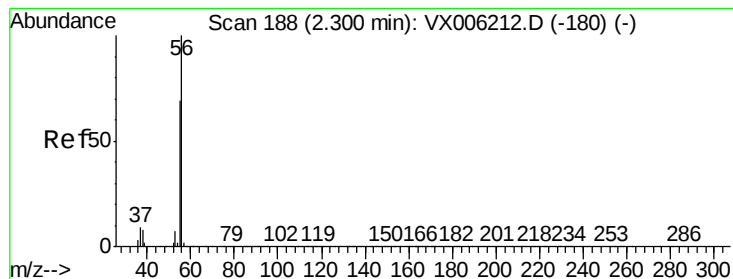

#13

Acrolein

Concen: 0.351 ug/l

RT: 2.31 min Scan# 189

Delta R.T. 0.01 min

Lab File: VX006576.D

Acq: 17 Dec 2018 16:46

Instrument :

MSVOA\_X

ClientSampled :





EB01-20181211

Tot Ion: 56 Resp: 357

Ion Ratio Lower Upper

56 100

55 121.0 57.8 86.6#

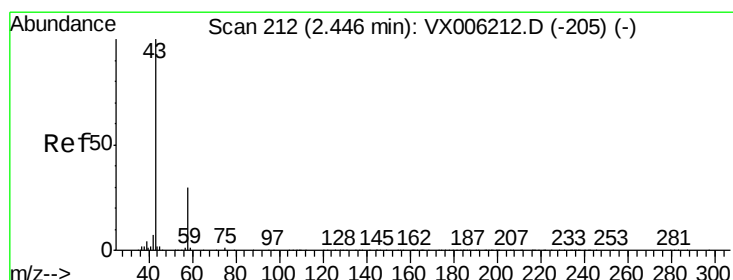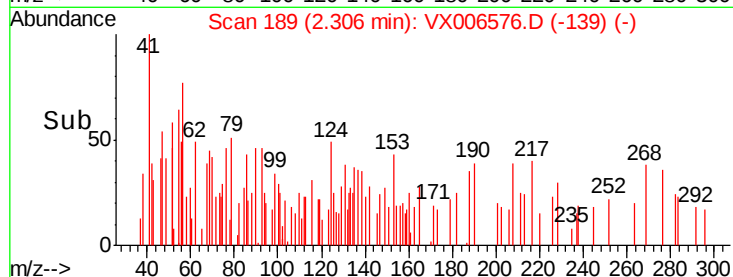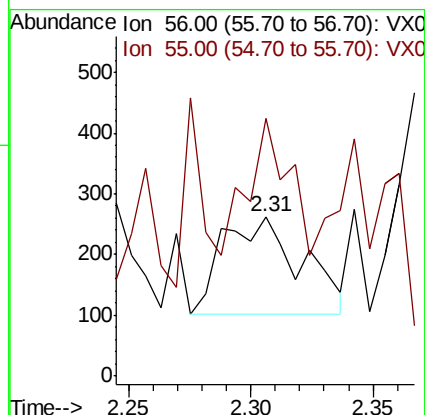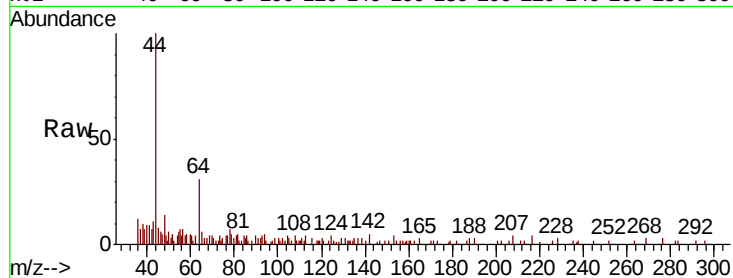

#16

Acetone

Concen: 3.842 ug/l

RT: 2.45 min Scan# 212

Delta R.T. 0.00 min

Lab File: VX006576.D




Acq: 17 Dec 2018 16:46


Tgt Ion: 43 Resp: 12275

Ion Ratio Lower Upper

43 100

58 32.8 24.0 36.0


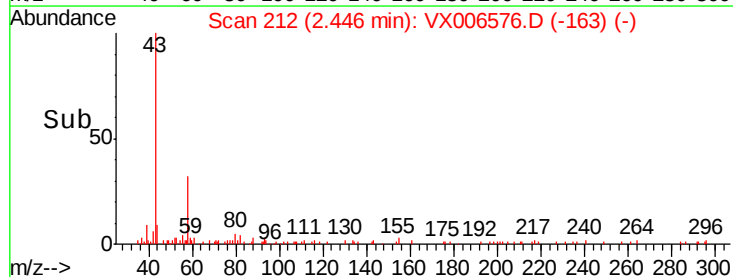
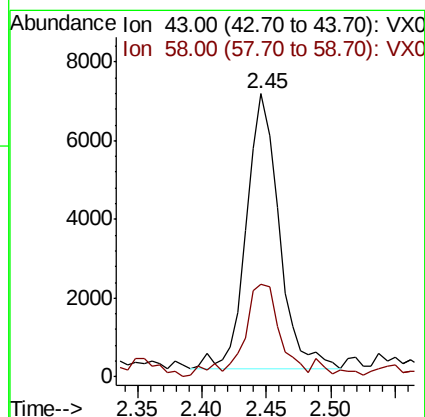
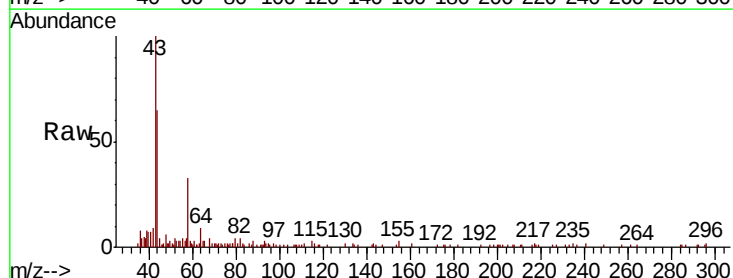




#20  
Methvlene Chloride  
Concen: 0.270 ug/l  
RT: 2.85 min Scan# 279  
Delta R.T. -0.01 min  
Lab File: VX006576.D  
Acq: 17 Dec 2018 16:46




Instrument :  
MSVOA\_X  
ClientSampled :  
EB01-20181211


Tot Ion: 84 Resp: 1839  
Ion Ratio Lower Upper  
84 100  
49 59.8 102.2 153.4#  
51 9.3 31.1 46.7#  
86 33.2 53.7 80.5#

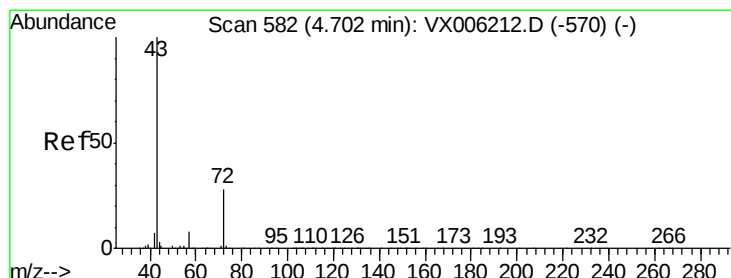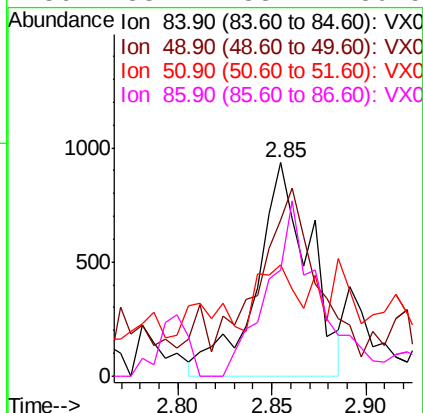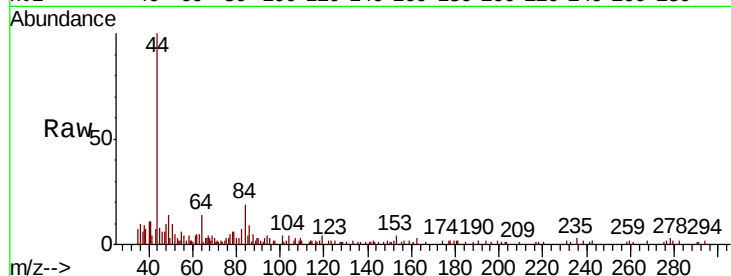

#25  
2-Butanone  
Concen: 0.247 ug/l  
RT: 4.69 min Scan# 580  
Delta R.T. -0.01 min  
Lab File: VX006576.D  
Acq: 17 Dec 2018 16:46

Tgt Ion: 43 Resp: 1126  
Ion Ratio Lower Upper  
43 100  
72 0.0 22.6 33.8#

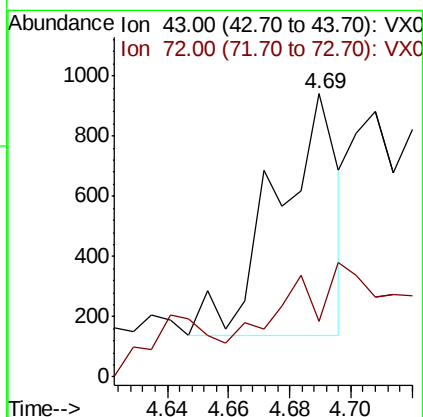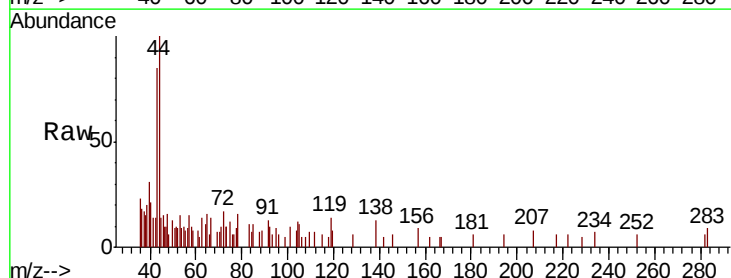

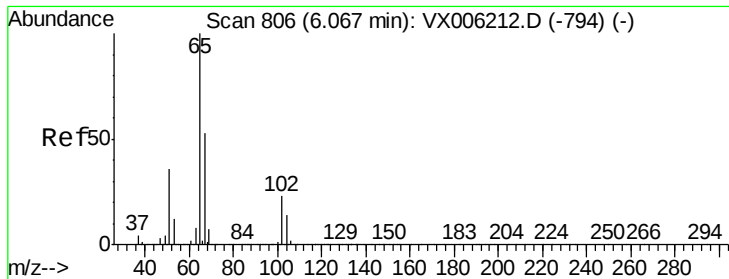

#33

1,2-Dichloroethane-d4

Concen: 54.220 ug/l

RT: 6.07 min Scan# 806

Delta R.T. 0.00 min

Lab File: VX006576.D

Acq: 17 Dec 2018 16:46

Instrument :

MSVOA\_X

ClientSampleId :


EB01-20181211

Tot Ion: 65 Resp: 369132

Ion Ratio Lower Upper




65 100

67 52.5 0.0 107.2

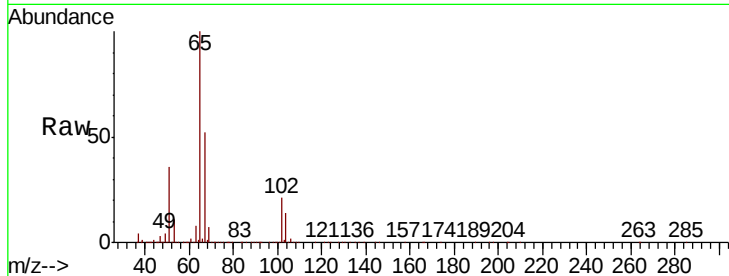

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

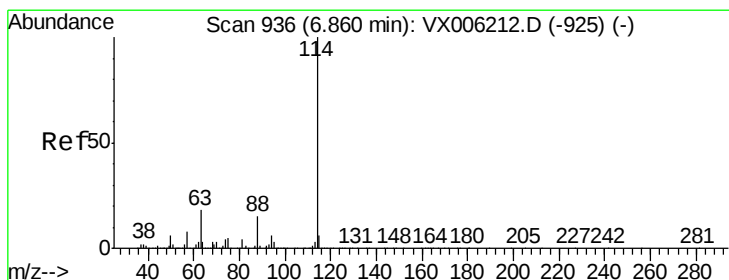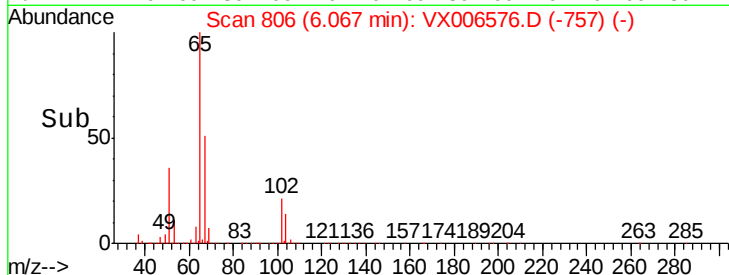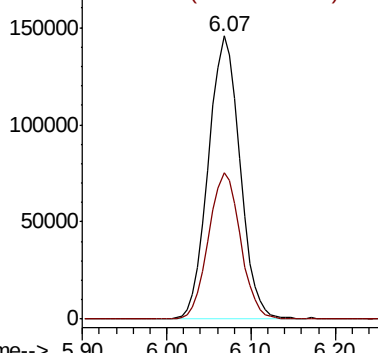

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.86 min Scan# 936

Delta R.T. 0.00 min

Lab File: VX006576.D

Acq: 17 Dec 2018 16:46


Tgt Ion: 114 Resp: 1065259

Ion Ratio Lower Upper

114 100

63 18.4 0.0 36.6



88 15.5 0.0 29.0

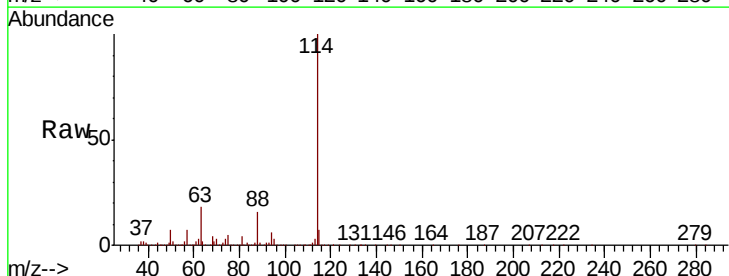


Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

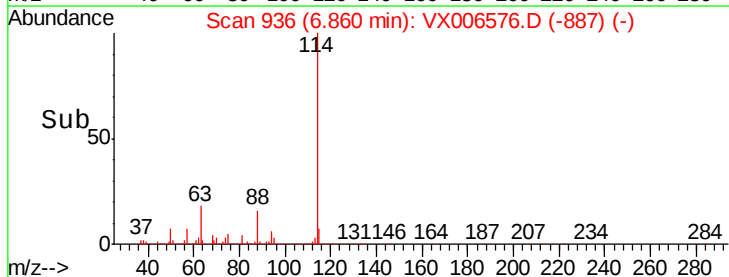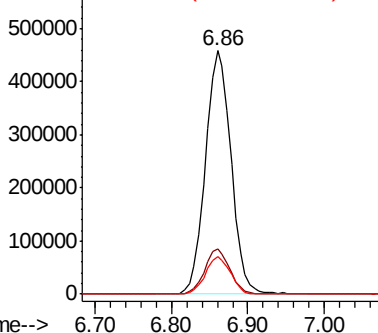

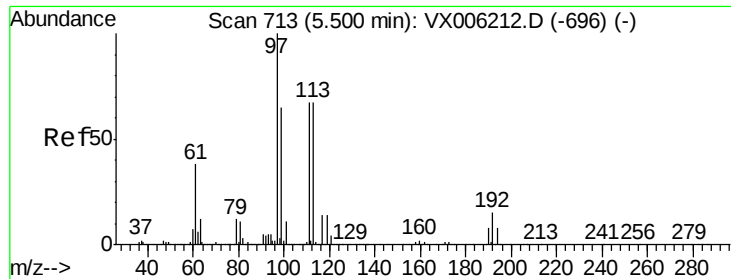

#35

Dibromofluoromethane

Concen: 46.532 ug/l

RT: 5.50 min Scan# 713

Delta R.T. 0.00 min

Lab File: VX006576.D

Acq: 17 Dec 2018 16:46

Instrument :

MSVOA\_X

ClientSampleId :

EB01-20181211


Tot Ion:113 Resp: 320936

Ion Ratio Lower Upper




113 100

111 102.7 81.1 121.7

192 20.3 18.2 27.2

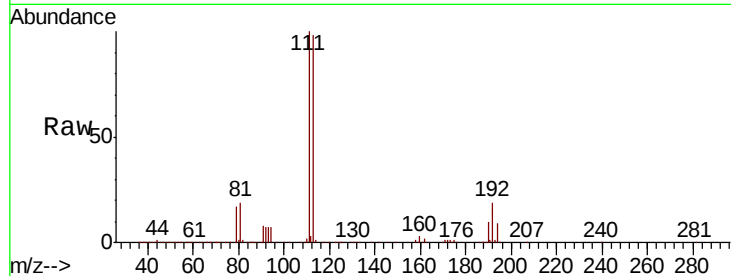

Abundance Ion 112.80 (112.50 to 113.50): V  
Ion 110.80 (110.50 to 111.50): V  
Ion 191.70 (191.40 to 192.40): V

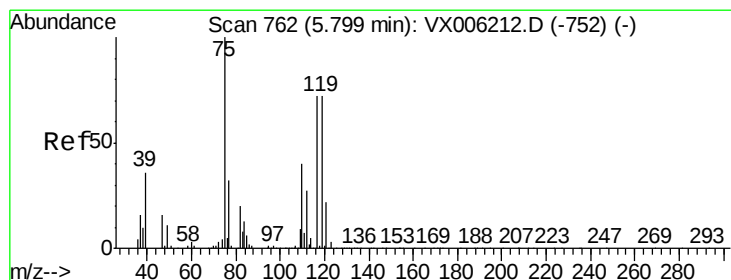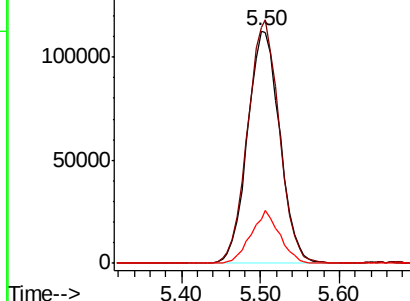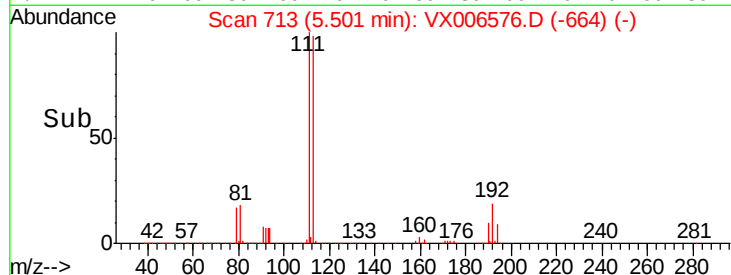

#36

1,1-Dichloropropene

Concen: 4.995 ug/l

RT: 5.66 min Scan# 739

Delta R.T. -0.14 min

Lab File: VX006576.D

Acq: 17 Dec 2018 16:46


Tgt Ion: 75 Resp: 44806

Ion Ratio Lower Upper



75 100


110 9.6 20.4 61.3#

77 0.0 24.9 37.3#

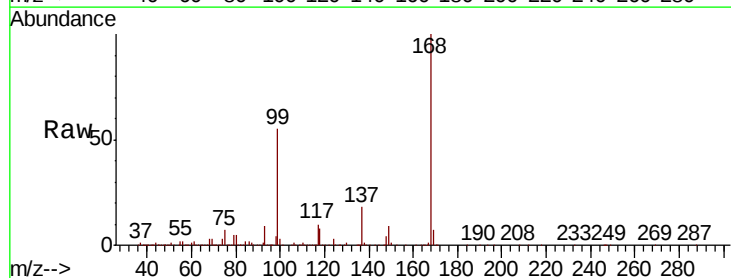

Abundance Ion 74.90 (74.60 to 75.60): VX0  
Ion 109.90 (109.60 to 110.60): V  
Ion 76.90 (76.60 to 77.60): VX0

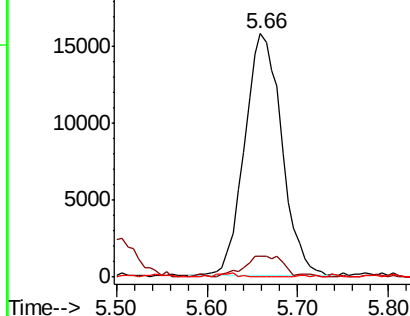


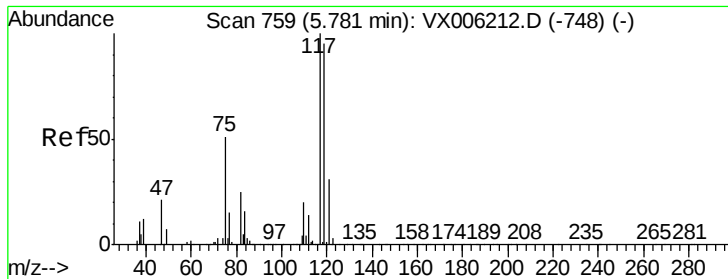




#38  
Carbon Tetrachloride  
Concen: 5.948 ug/l  
RT: 5.67 min Scan# 740  
Delta R.T. -0.12 min  
Lab File: VX006576.D  
Acq: 17 Dec 2018 16:46

Instrument :  
MSVOA\_X  
ClientSampleId :  
EB01-20181211

Tot Ion:117 Resp: 62769  
Ion Ratio Lower Upper  
117 100  
119 4.9 75.8 113.8#  
121 0.0 24.6 37.0#

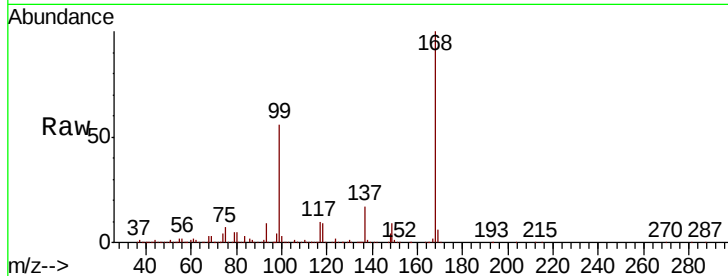


Abundance Ion 116.80 (116.50 to 117.50): V  
Ion 118.80 (118.50 to 119.50): V  
Ion 120.80 (120.50 to 121.50): V

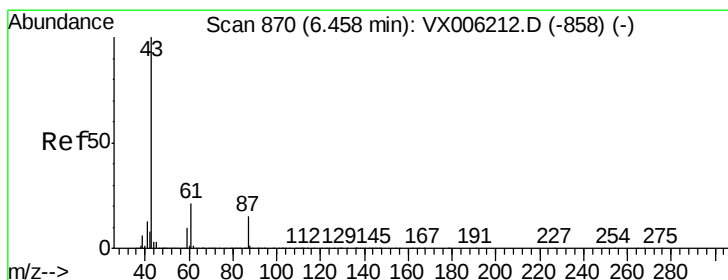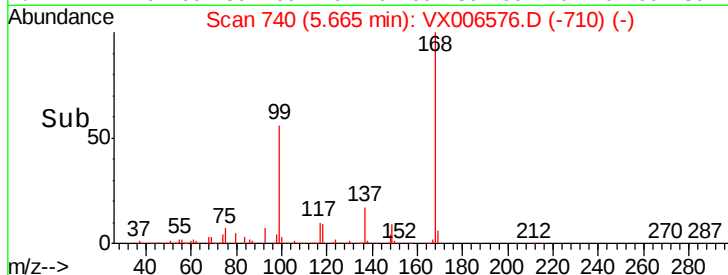
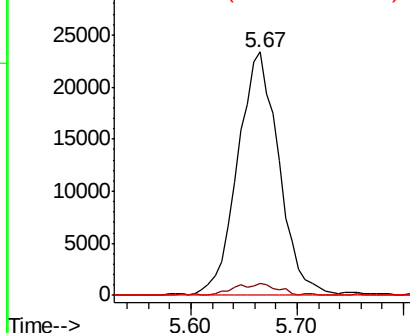



#43  
Isopropyl Acetate  
Concen: 0.460 ug/l  
RT: 6.46 min Scan# 871  
Delta R.T. 0.01 min  
Lab File: VX006576.D  
Acq: 17 Dec 2018 16:46

Tgt Ion: 43 Resp: 7701  
Ion Ratio Lower Upper  
43 100  
61 11.1 16.8 25.2#  
87 17.0 11.9 17.9

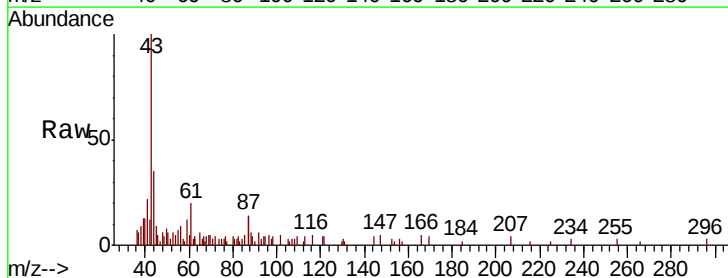

Abundance Ion 43.00 (42.70 to 43.70): VX0  
Ion 61.00 (60.70 to 61.70): VX0  
Ion 87.00 (86.70 to 87.70): VX0

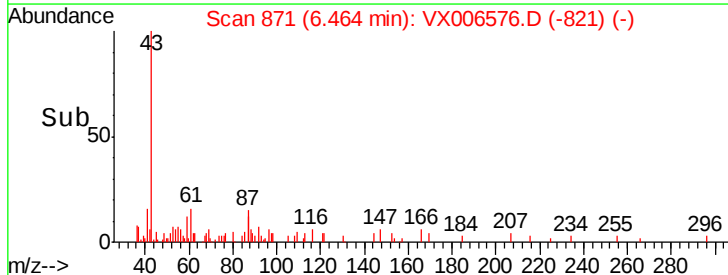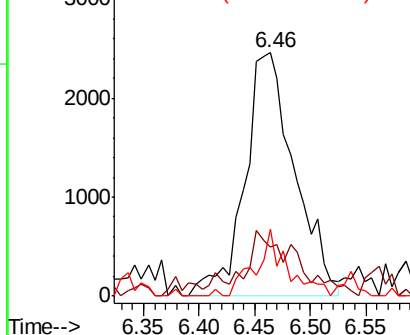

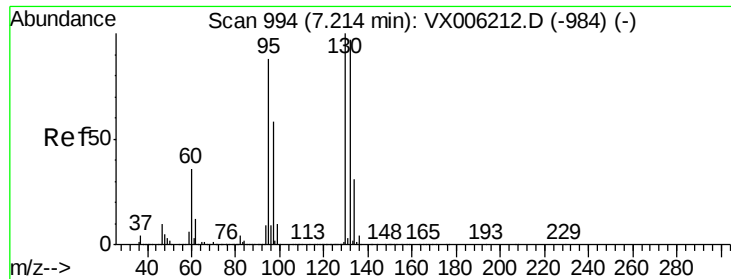

#44

Trichloroethene

Concen: 8.342 ug/l

RT: 7.21 min Scan# 994

Delta R.T. 0.00 min

Lab File: VX006576.D

Acq: 17 Dec 2018 16:46

Instrument :

MSVOA\_X

ClientSampleId :


EB01-20181211

Tot Ion:130 Resp: 67899

Ion Ratio Lower Upper




130 100

95 96.6 0.0 175.8

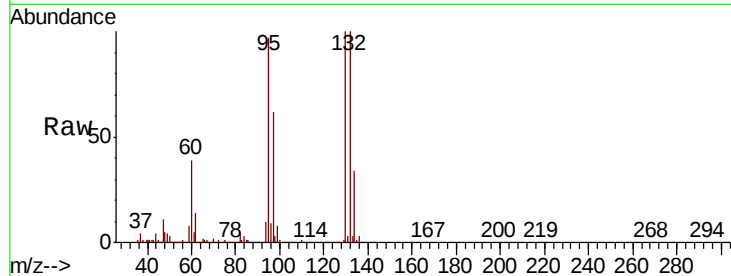

Abundance Ion 129.80 (129.50 to 130.50): V

Ion 94.90 (94.60 to 95.60): VX0

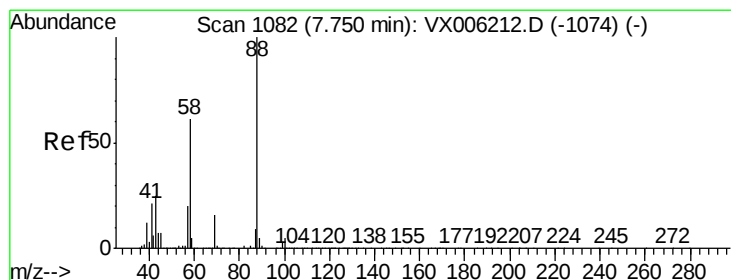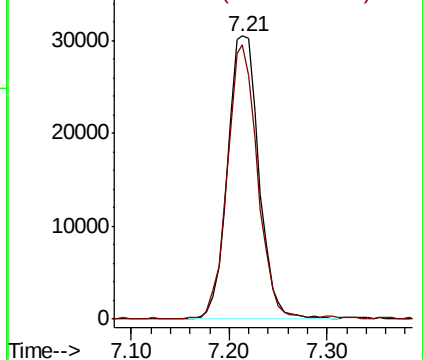

#49

1,4-Dioxane

Concen: 1.399 ug/l

RT: 7.73 min Scan# 1079

Delta R.T. -0.02 min

Lab File: VX006576.D

Acq: 17 Dec 2018 16:46


Tgt Ion: 88 Resp: 281

Ion Ratio Lower Upper

88 100

43 73.0 23.2 34.8#



58 33.5 51.4 77.0#

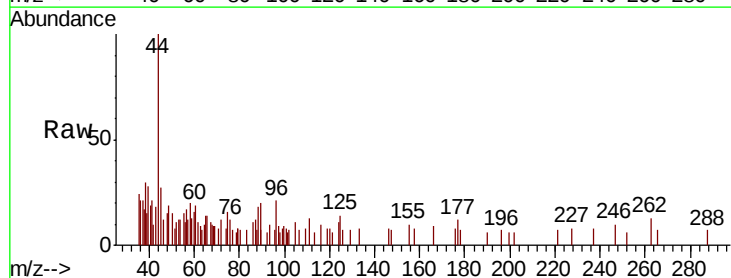


Abundance Ion 88.00 (87.70 to 88.70): VX0

Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

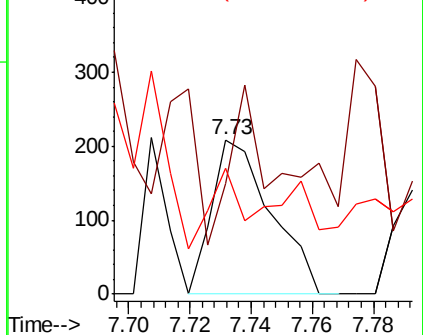

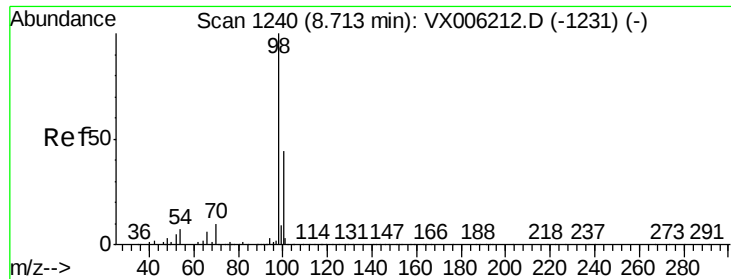

#50

Toluene-d8

Concen: 50.361 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. 0.00 min

Lab File: VX006576.D

Acq: 17 Dec 2018 16:46

Instrument :

MSVOA\_X

ClientSampleId :





EB01-20181211

Tot Ion: 98 Resp: 1263443

Ion Ratio Lower Upper

98 100

100 64.7 52.2 78.2

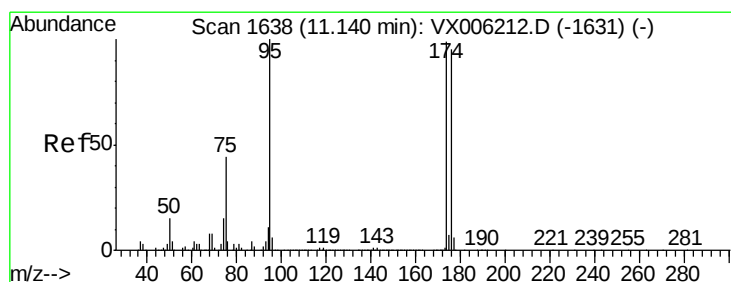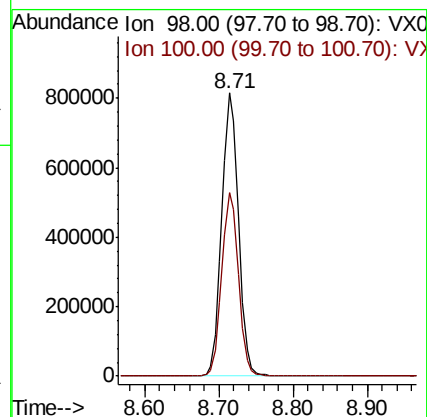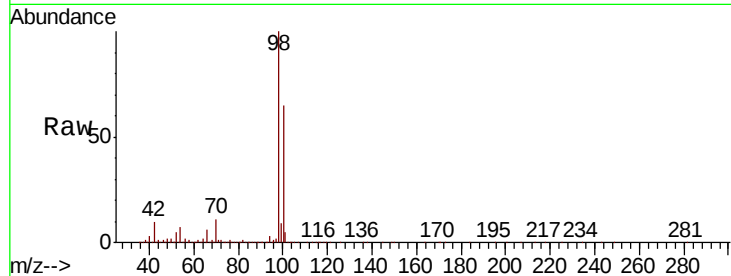

#62

4-Bromofluorobenzene

Concen: 48.827 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. -0.01 min

Lab File: VX006576.D

Acq: 17 Dec 2018 16:46




Tgt Ion: 95 Resp: 461605


Ion Ratio Lower Upper

95 100

174 84.6 0.0 187.0

176 80.9 0.0 181.8


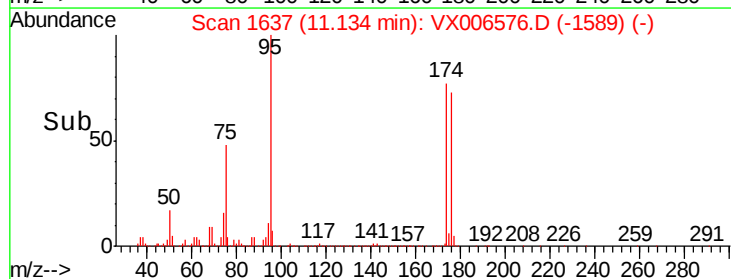
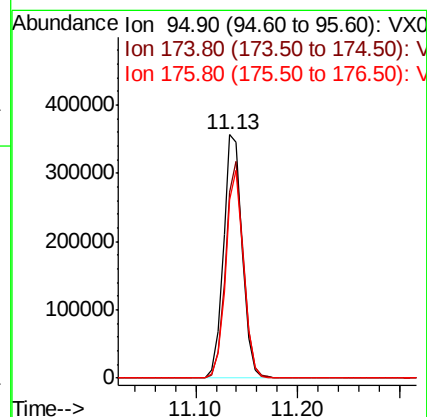
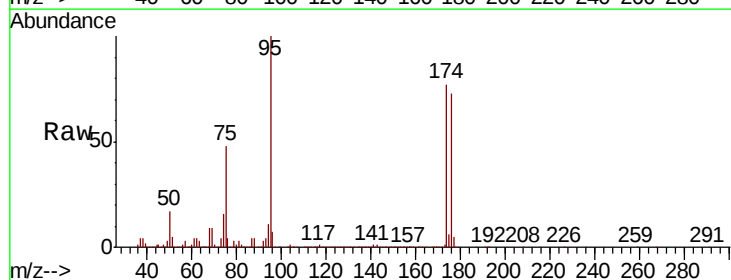


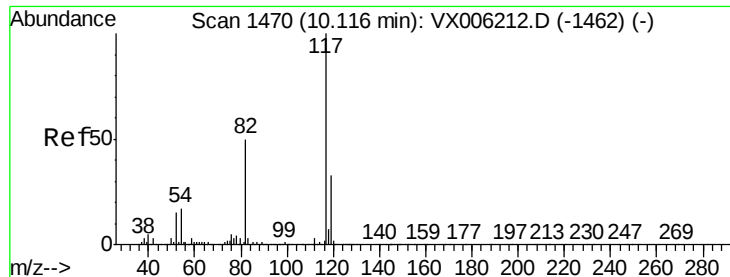

#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 10.12 min Scan# 1470  
Delta R.T. 0.00 min  
Lab File: VX006576.D  
Acq: 17 Dec 2018 16:46




Instrument :  
MSVOA\_X  
ClientSampleId :  
EB01-20181211


| Tot Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 117     | 100   |       |       |
| 82      | 50.6  | 39.6  | 59.4  |
| 119     | 32.8  | 26.3  | 39.5  |

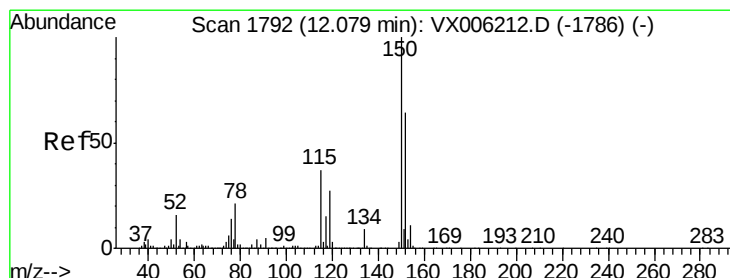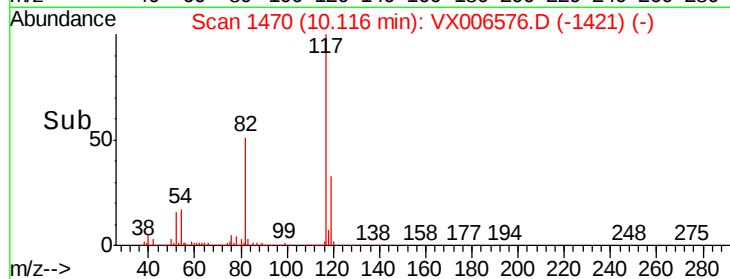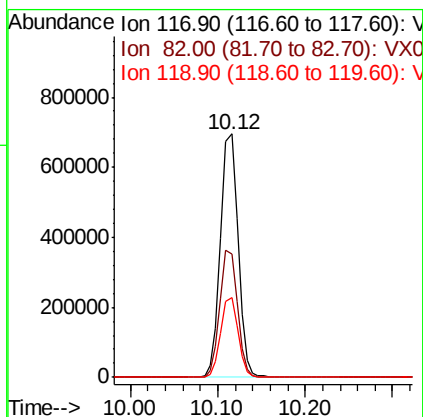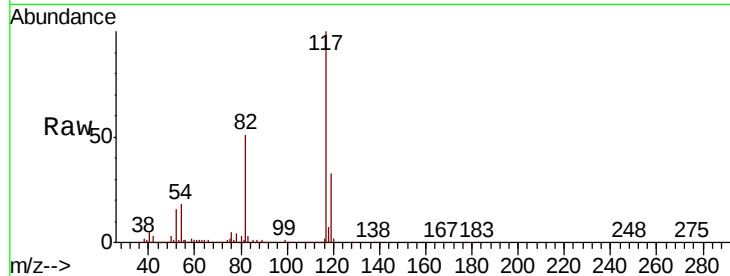

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 12.08 min Scan# 1792  
Delta R.T. 0.00 min  
Lab File: VX006576.D  
Acq: 17 Dec 2018 16:46

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 152     | 100   |       |       |
| 115     | 56.8  | 39.0  | 116.9 |
| 150     | 156.8 | 0.0   | 345.8 |

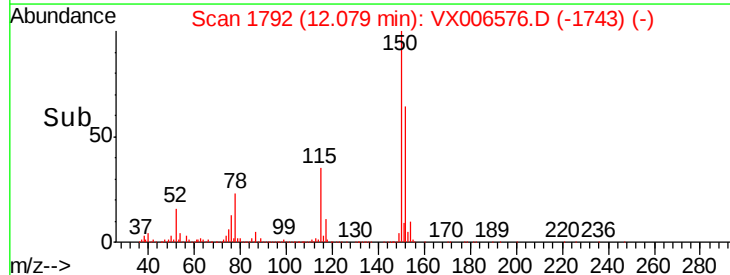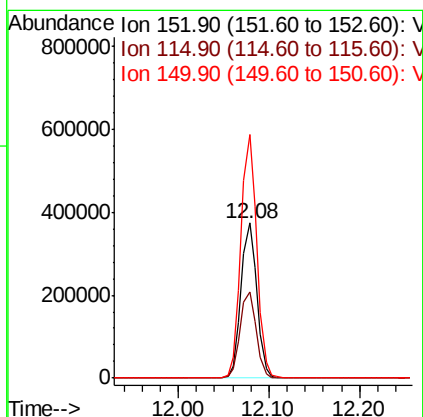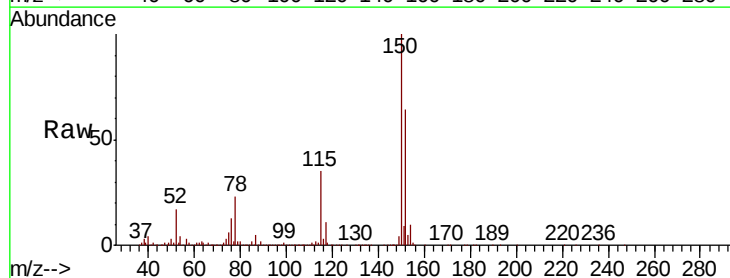



#76

1,2,3-Trichloropropane

Concen: 24.490 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. -0.16 min

Lab File: VX006576.D

Acq: 17 Dec 2018 16:46

Instrument :

MSVOA\_X

ClientSampleId :





EB01-20181211

Tot Ion: 75 Resp: 215706

Ion Ratio Lower Upper

75 100

77 1.1 19.9 59.7#

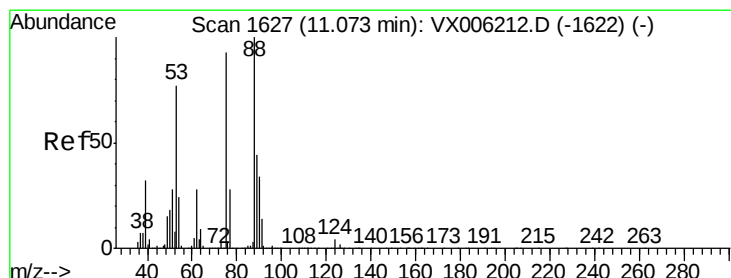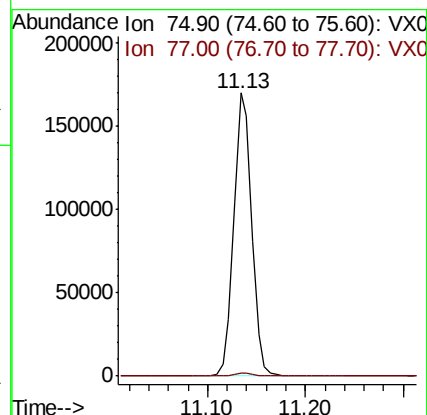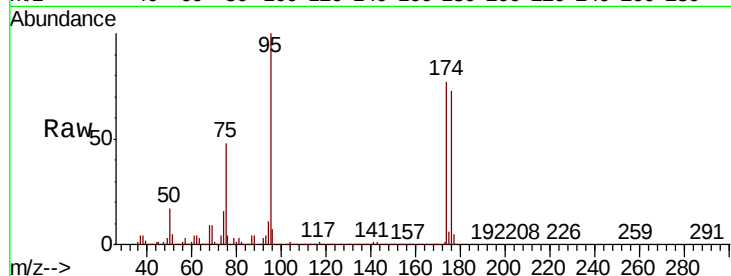

#81

trans-1,4-Dichloro-2-butene

Concen: 57.470 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. 0.06 min

Lab File: VX006576.D

Acq: 17 Dec 2018 16:46

Tgt Ion: 75 Resp: 215706

Ion Ratio Lower Upper

75 100

53 0.1 64.4 96.6#

89 0.0 44.2 66.4#

