


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX121719\
Data File : VX014050.D
Acq On : 17 Dec 2019 10:09
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121319W.M
Title : SW846 8260
Last Update : Tue Dec 17 03:01:07 2019

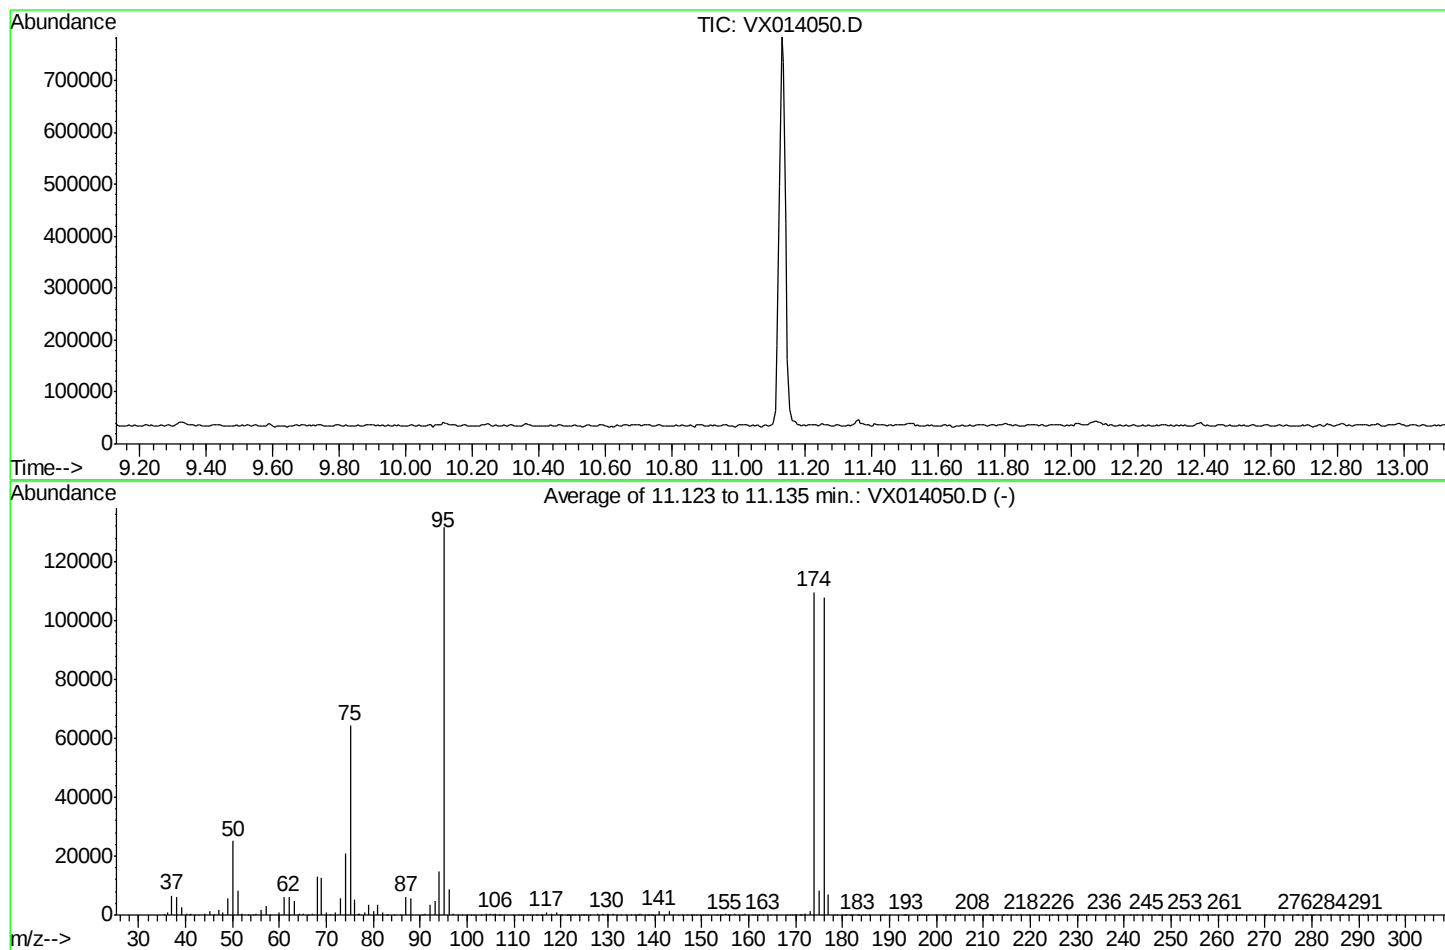

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1672

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	25144	PASS
75	95	30	60	48.8	64271	PASS
95	95	100	100	100.0	131647	PASS
96	95	5	9	6.7	8880	PASS
173	174	0.00	2	1.2	1281	PASS
174	95	50	100	83.3	109720	PASS
175	174	5	9	7.7	8494	PASS
176	174	95	101	98.4	108009	PASS
177	176	5	9	6.3	6807	PASS