


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX121719\
Data File : VX014068.D
Acq On : 17 Dec 2019 22:25
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\624X121219W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Dec 13 01:35:34 2019

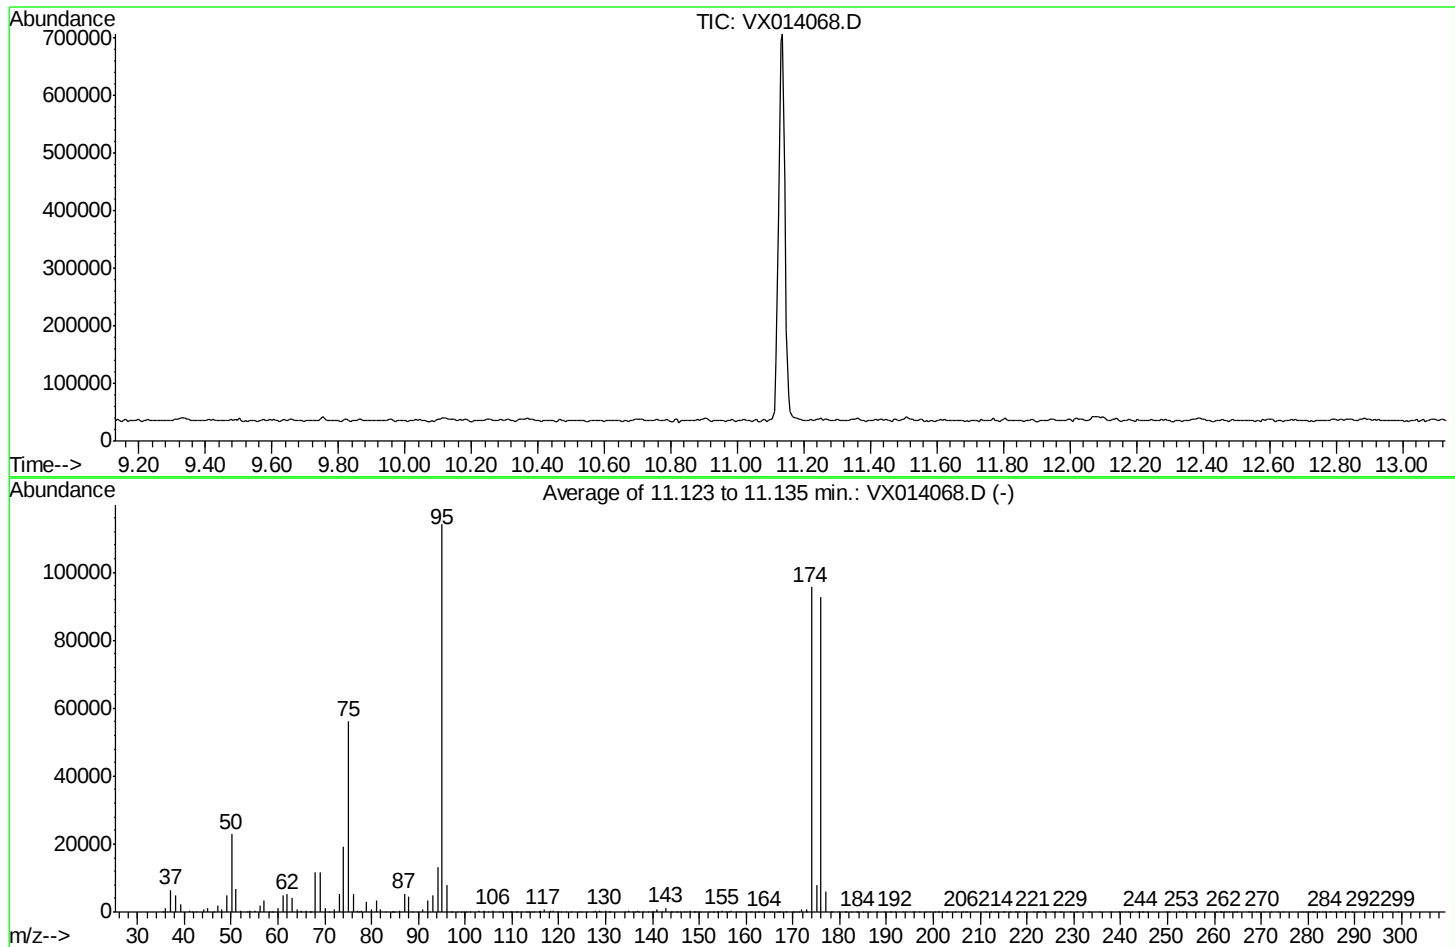

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1674

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	22816	PASS
75	95	30	60	49.1	56052	PASS
95	95	100	100	100.0	114114	PASS
96	95	5	9	6.9	7884	PASS
173	174	0.00	2	1.0	943	PASS
174	95	50	100	83.7	95532	PASS
175	174	5	9	8.1	7758	PASS
176	174	95	101	97.1	92805	PASS
177	176	5	9	6.7	6204	PASS