

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX121720\
 Data File : VX020087.D
 Acq On : 16 Dec 2020 23:42
 Operator : JC/MD
 Sample : L5053-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE122D1-20201209

Quant Time: Dec 17 00:34:48 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X120420W.M
 Quant Title : SW846 8260
 QLast Update : Fri Dec 04 15:32:53 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	293521	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	494218	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.09	117	464792	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	200471	50.00	ug/l	0.00

System Monitoring Compounds		R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4		6.03	65	193935	50.27	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	100.54%	
35) Dibromofluoromethane		5.46	113	154944	48.51	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	97.02%	
50) Toluene-d8		8.70	98	602186	49.38	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	98.76%	
62) 4-Bromofluorobenzene		11.12	95	212880	45.87	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	91.74%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	1.31	50	765	0.242	ug/l #	87
5) Bromomethane	1.64	94	551	0.498	ug/l	92
6) Chloroethane	1.74	64	752	0.376	ug/l #	67
9) 1,1,2-Trichlorotrifluoroet	2.37	101	7621	2.865	ug/l	97
11) Tert butyl alcohol	3.00	59	498	Below Cal	#	73
12) 1,1-Dichloroethene	2.35	96	2249	0.836	ug/l	86
16) Acetone	2.42	43	1879	1.296	ug/l	99
18) Methyl Acetate	2.75	43	763	0.215	ug/l #	84
20) Methylene Chloride	2.84	84	508	Below Cal	#	87
21) trans-1,2-Dichloroethene	3.14	96	1107	0.353	ug/l	98
27) cis-1,2-Dichloroethene	4.56	96	7250	1.976	ug/l	92
29) Tetrahydrofuran	5.10	42	517	0.360	ug/l #	47
30) Chloroform	5.17	83	2256	0.396	ug/l	92
31) Cyclohexane	5.62	56	5629	1.173	ug/l #	1
36) 1,1-Dichloropropene	5.63	75	22560	5.052	ug/l #	48
38) Carbon Tetrachloride	5.74	117	1766	0.404	ug/l #	83
39) Methylcyclohexane	7.18	83	16415	3.129	ug/l #	1
44) Trichloroethene	7.18	130	1397766	390.508	ug/l	98
49) 1,4-Dioxane	7.71	88	1077	12.331	ug/l	94
55) 1,1,2-Trichloroethane	9.20	97	803	0.234	ug/l	94
60) Dibromochloromethane	9.32	129	5152	1.475	ug/l #	11
64) Tetrachloroethene	9.32	164	5580	1.790	ug/l	95
76) 1,2,3-Trichloropropane	11.12	75	104580	23.260	ug/l #	39
81) trans-1,4-Dichloro-2-buten	11.12	75	104580	67.239	ug/l #	12


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX121720\
Data File : VX020087.D
Acq On : 16 Dec 2020 23:42
Operator : JC/MD
Sample : L5053-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE122D1-20201209

Quant Time: Dec 17 00:34:48 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X120420W.M
Quant Title : SW846 8260
QLast Update : Fri Dec 04 15:32:53 2020
Response via : Initial Calibration

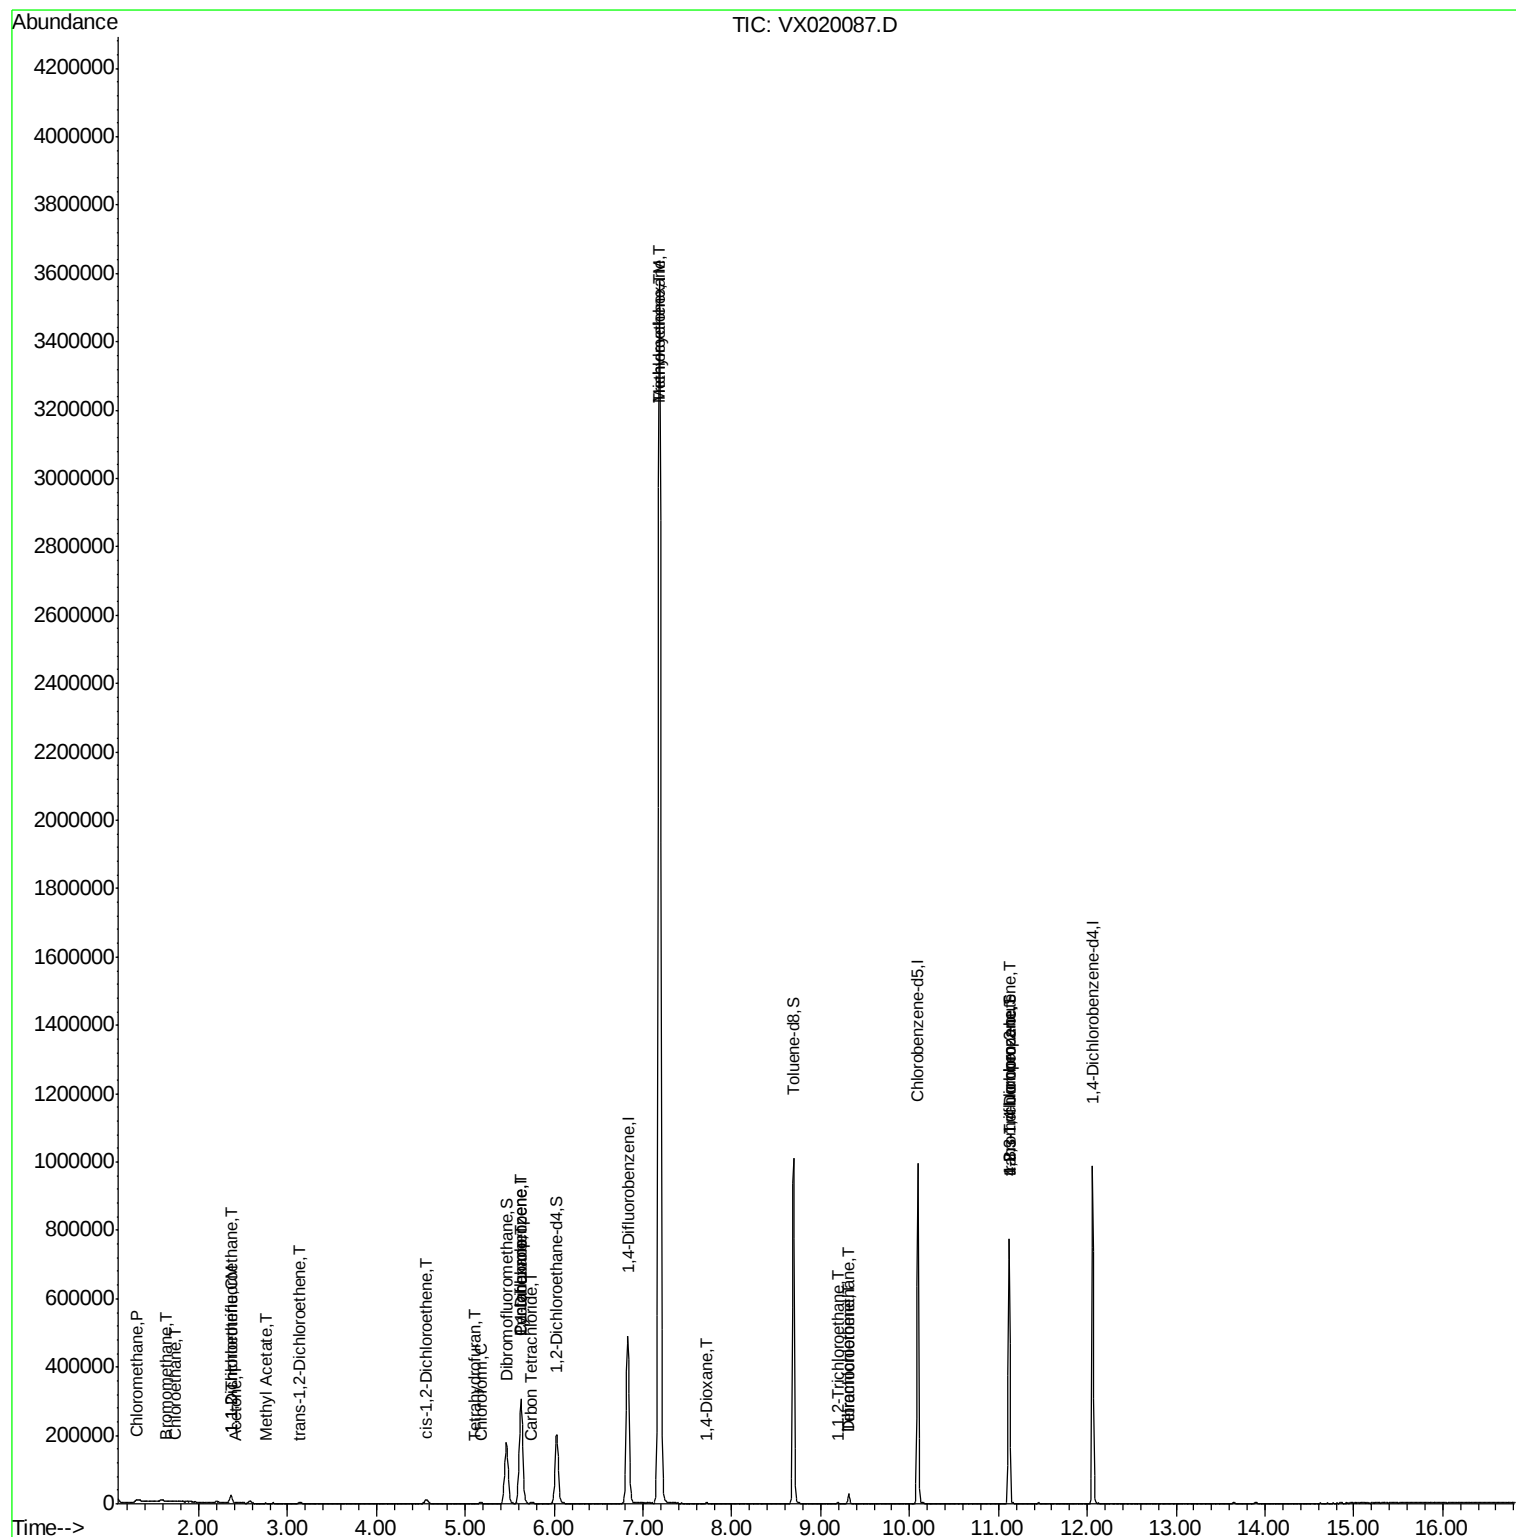

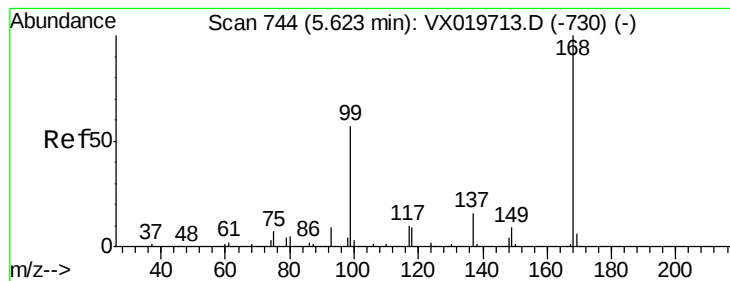

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.63 min Scan# 745

Delta R.T. 0.01 min

Lab File: VX020087.D

Acq: 16 Dec 2020 23:42

Instrument :

MSVOA_X

ClientSampleId :


RE122D1-20201209

Tgt Ion: 168 Resp: 293521

Ion Ratio Lower Upper

168 100

99 57.7 45.8 68.6



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.63

120000

100000

80000



60000

40000

20000

0

Time-->

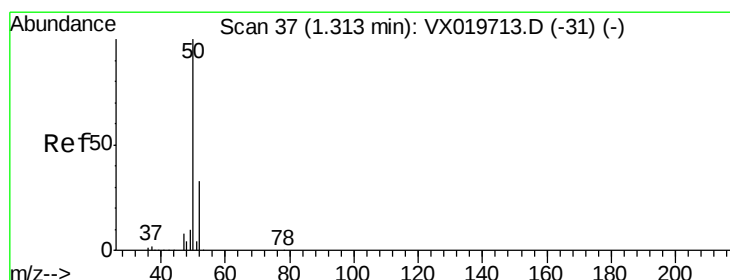

#3

Chloromethane

Concen: 0.242 ug/l

RT: 1.31 min Scan# 37

Delta R.T. -0.00 min

Lab File: VX020087.D


Acq: 16 Dec 2020 23:42

Tgt Ion: 50 Resp: 765

Ion Ratio Lower Upper

50 100

52 25.6 26.4 39.6#

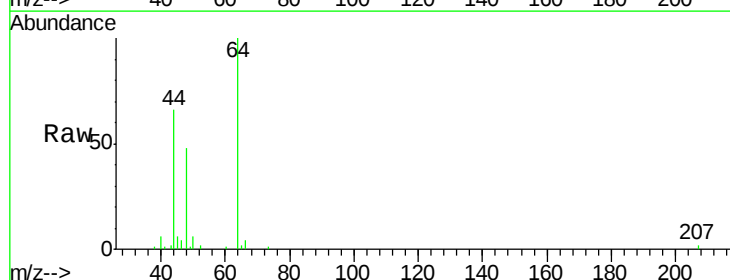

Abundance Ion 49.90 (49.60 to 50.60): VX0

Ion 51.90 (51.60 to 52.60): VX0

1.31


300


200

100

0

Time-->

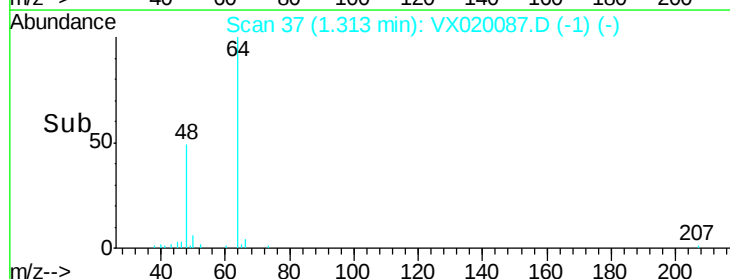



#5

Bromomethane

Concen: 0.498 ug/l

RT: 1.64 min Scan# 90

Delta R.T. 0.01 min

Lab File: VX020087.D

Acq: 16 Dec 2020 23:42

Instrument :

MSVOA_X

ClientSampleId :


RE122D1-20201209

Tgt Ion: 94 Resp: 551

Ion Ratio Lower Upper




94 100

96 87.3 76.4 114.6

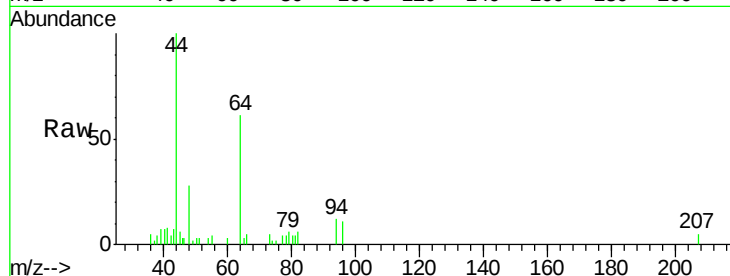

Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0

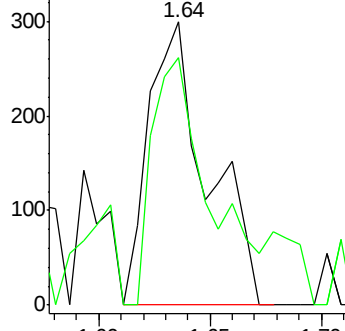

#6

Chloroethane

Concen: 0.376 ug/l

RT: 1.74 min Scan# 107

Delta R.T. 0.04 min

Lab File: VX020087.D


Acq: 16 Dec 2020 23:42

Tgt Ion: 64 Resp: 752

Ion Ratio Lower Upper



64 100


66 13.4 25.4 38.0#



Abundance Ion 63.90 (63.60 to 64.60): VX0

Ion 65.90 (65.60 to 66.60): VX0

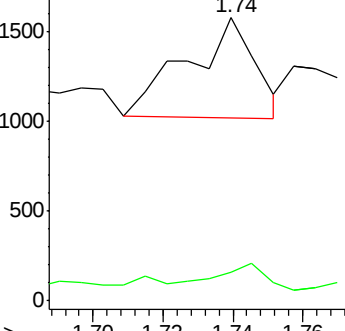



#9

1,1,2-Trichlorotrifluoroethane

Concen: 2.865 ug/l

RT: 2.37 min Scan# 210

Delta R.T. 0.01 min

Lab File: VX020087.D

Acq: 16 Dec 2020 23:42

Instrument :

MSVOA_X

ClientSampleId :

RE122D1-20201209


Tgt Ion:101 Resp: 7621

Ion Ratio Lower Upper

101 100

85 44.4 34.9 52.3




151 73.2 61.4 92.2

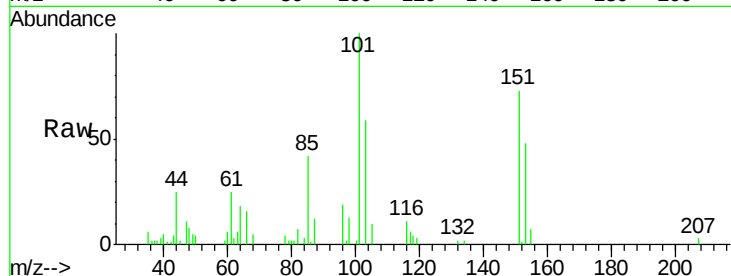

Abundance Ion 100.90 (100.60 to 101.60): V

Ion 84.90 (84.60 to 85.60): VX0

Ion 150.80 (150.50 to 151.50): V

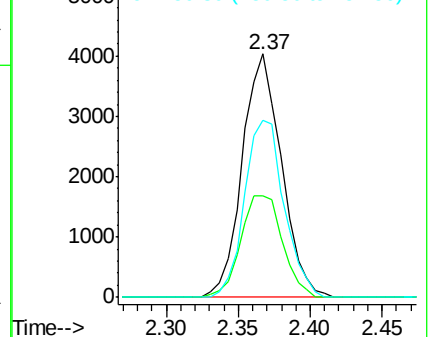

#11

Tert butyl alcohol

Concen: Below Cal

RT: 3.00 min Scan# 314

Delta R.T. -0.01 min

Lab File: VX020087.D


Acq: 16 Dec 2020 23:42

Tgt Ion: 59 Resp: 498

Ion Ratio Lower Upper



59 100


57 0.0 7.8 11.8#



Abundance Ion 59.00 (58.70 to 59.70): VX0

Ion 57.00 (56.70 to 57.70): VX0




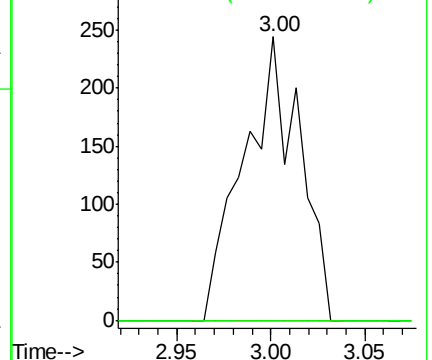




#12
 1,1-Dichloroethene
 Concen: 0.836 ug/l
 RT: 2.35 min Scan# 208
 Delta R.T. -0.00 min
 Lab File: VX020087.D
 Acq: 16 Dec 2020 23:42




Instrument :
 MSVOA_X
 ClientSampleId :
 RE122D1-20201209


Tgt Ion: 96 Resp: 2249
 Ion Ratio Lower Upper
 96 100
 61 133.8 124.6 187.0
 98 57.3 50.6 76.0

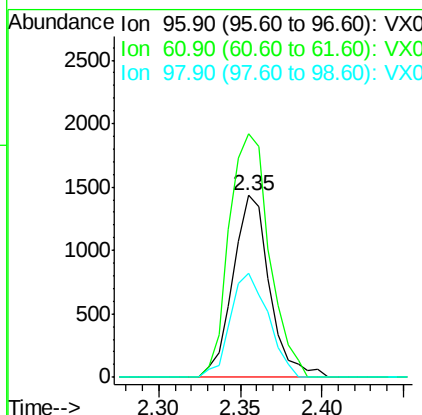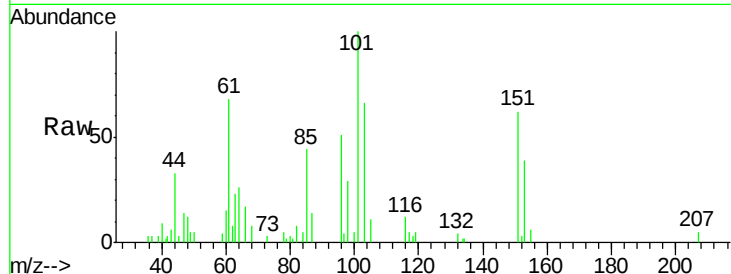

#16
 Acetone
 Concen: 1.296 ug/l
 RT: 2.42 min Scan# 218
 Delta R.T. -0.00 min
 Lab File: VX020087.D
 Acq: 16 Dec 2020 23:42

Tgt Ion: 43 Resp: 1879
 Ion Ratio Lower Upper
 43 100
 58 35.6 27.8 41.8



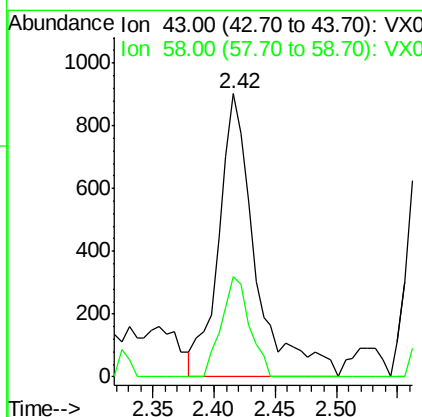
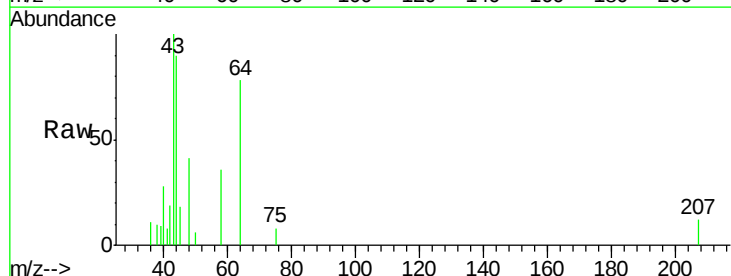




#18
Methyl Acetate
Concen: 0.215 ug/l
RT: 2.75 min Scan# 272
Delta R.T. -0.00 min
Lab File: VX020087.D
Acq: 16 Dec 2020 23:42




Instrument :
MSVOA_X
ClientSampleId :
RE122D1-20201209


Tgt Ion: 43 Resp: 763
Ion Ratio Lower Upper
43 100
74 19.1 21.9 32.9#

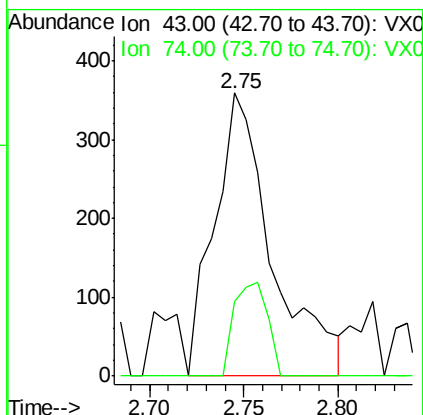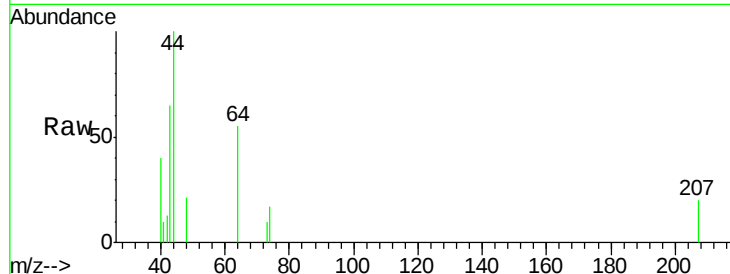

#20
Methylene Chloride
Concen: Below Cal
RT: 2.84 min Scan# 287
Delta R.T. 0.01 min
Lab File: VX020087.D
Acq: 16 Dec 2020 23:42

Tgt Ion: 84 Resp: 508
Ion Ratio Lower Upper
84 100
49 100.7 88.6 132.8
51 39.9 27.0 40.6
86 48.1 50.3 75.5#

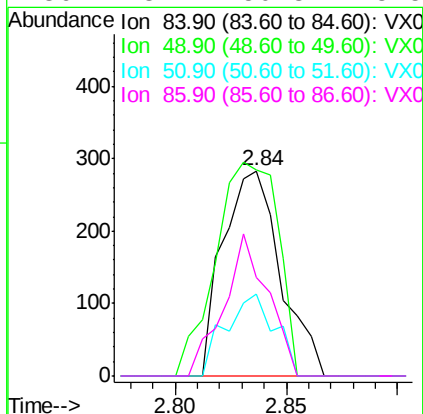

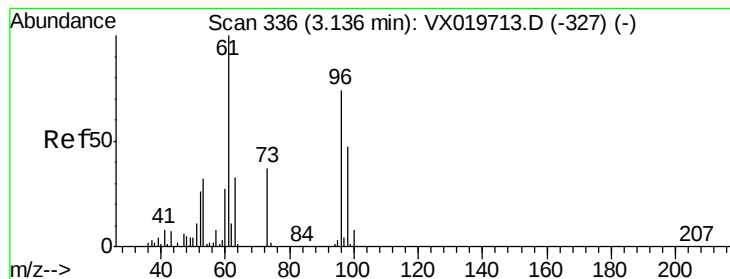

#21

trans-1,2-Dichloroethene

Concen: 0.353 ug/l

RT: 3.14 min Scan# 336

Delta R.T. -0.00 min

Lab File: VX020087.D

Acq: 16 Dec 2020 23:42

Instrument :

MSVOA_X

ClientSampleId :

RE122D1-20201209


Tgt Ion: 96 Resp: 1107

Ion Ratio Lower Upper

96 100

61 137.1 107.7 161.5




98 62.4 50.4 75.6



Abundance Ion 95.90 (95.60 to 96.60): VX0

Ion 60.90 (60.60 to 61.60): VX0

Ion 97.90 (97.60 to 98.60): VX0

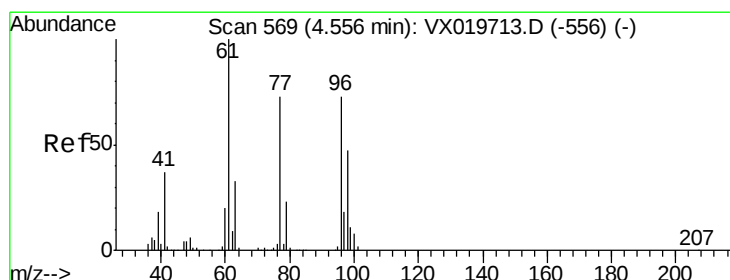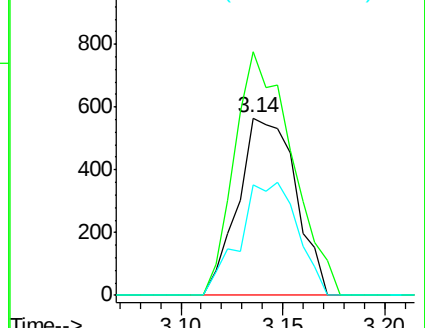

#27

cis-1,2-Dichloroethene

Concen: 1.976 ug/l

RT: 4.56 min Scan# 570

Delta R.T. 0.01 min

Lab File: VX020087.D

Acq: 16 Dec 2020 23:42


Tgt Ion: 96 Resp: 7250

Ion Ratio Lower Upper

96 100

61 131.4 0.0 285.6



98 60.9 0.0 129.6




Abundance Ion 95.90 (95.60 to 96.60): VX0

Ion 60.90 (60.60 to 61.60): VX0

Ion 97.90 (97.60 to 98.60): VX0

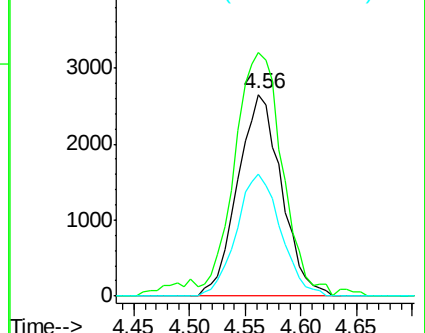

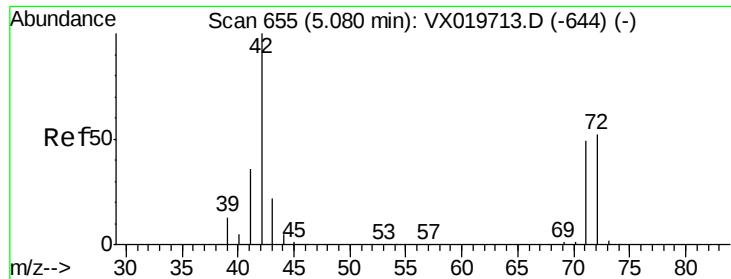

#29

Tetrahydrofuran

Concen: 0.360 ug/l

RT: 5.10 min Scan# 658

Delta R.T. 0.02 min

Lab File: VX020087.D

Acq: 16 Dec 2020 23:42

Instrument :

MSVOA_X

ClientSampleId :

RE122D1-20201209


Tgt Ion: 42 Resp: 517

Ion Ratio Lower Upper

42 100

72 12.8 41.7 62.5#

71 14.5 38.4 57.6#

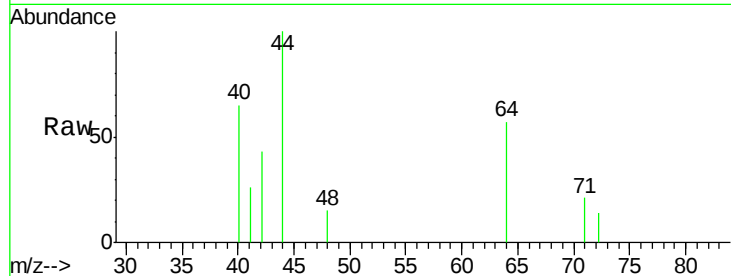


Abundance Ion 42.00 (41.70 to 42.70): VX0

Ion 72.00 (71.70 to 72.70): VX0


Ion 71.00 (70.70 to 71.70): VX0

Time-->

5.05 5.10 5.15



Time-->

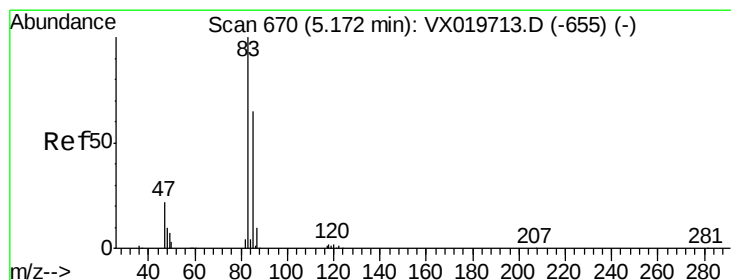

#30

Chloroform

Concen: 0.396 ug/l

RT: 5.17 min Scan# 670

Delta R.T. -0.00 min

Lab File: VX020087.D


Acq: 16 Dec 2020 23:42

Tgt Ion: 83 Resp: 2256

Ion Ratio Lower Upper

83 100

85 58.4 52.0 78.0




Abundance Ion 82.90 (82.60 to 83.60): VX0


Ion 84.90 (84.60 to 85.60): VX0

Time-->

5.10 5.15 5.20 5.25



Time-->

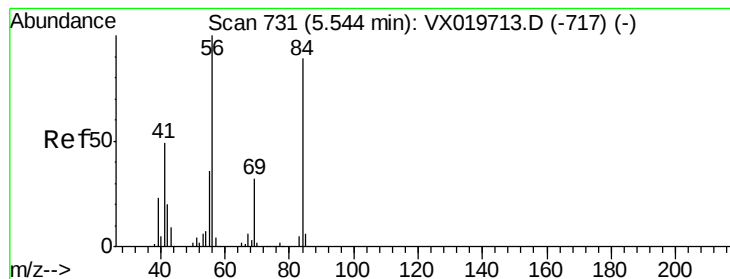

#31

Cyclohexane

Concen: 1.173 ug/l

RT: 5.62 min Scan# 744

Delta R.T. 0.08 min

Lab File: VX020087.D

Acq: 16 Dec 2020 23:42

Instrument :

MSVOA_X

ClientSampleId :

RE122D1-20201209


Tgt Ion: 56 Resp: 5629

Ion Ratio Lower Upper

56 100

69 191.3 25.3 37.9#




84 149.4 71.4 107.0#



Abundance Ion 56.00 (55.70 to 56.70): VX0

Ion 69.00 (68.70 to 69.70): VX0

Ion 84.00 (83.70 to 84.70): VX0

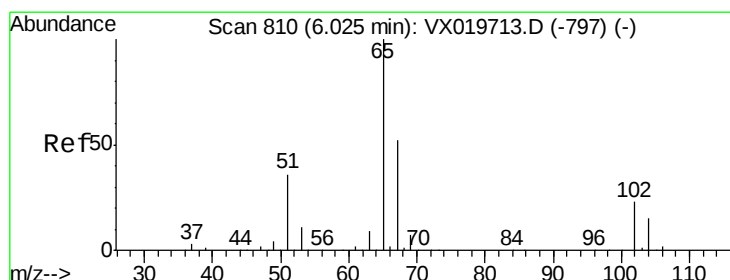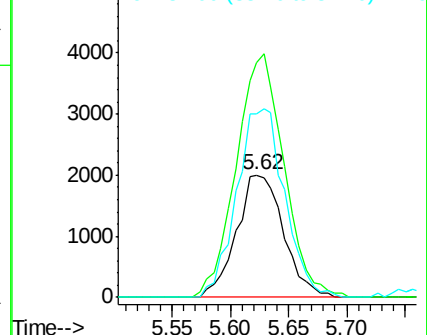

#33

1,2-Dichloroethane-d4

Concen: 50.272 ug/l

RT: 6.03 min Scan# 810

Delta R.T. -0.00 min

Lab File: VX020087.D


Acq: 16 Dec 2020 23:42

Tgt Ion: 65 Resp: 193935

Ion Ratio Lower Upper



65 100


67 52.8 0.0 105.4



Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

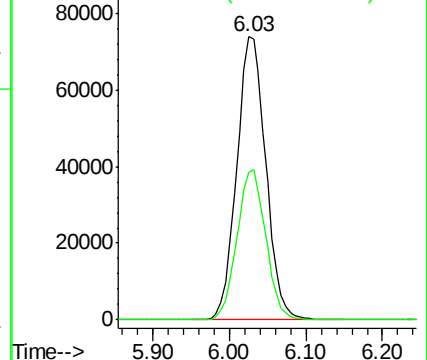

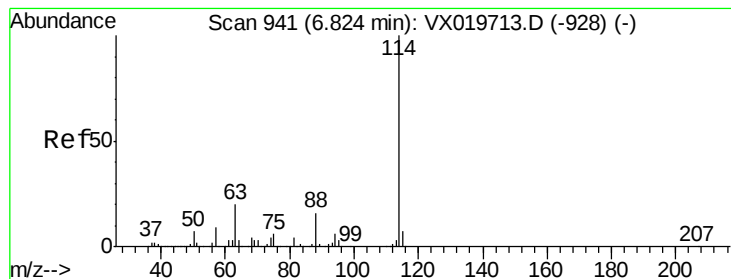

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.83 min Scan# 942

Delta R.T. 0.01 min

Lab File: VX020087.D

Acq: 16 Dec 2020 23:42

Instrument :

MSVOA_X

ClientSampleId :

RE122D1-20201209


Tgt Ion:114 Resp: 494218

Ion Ratio Lower Upper

114 100

63 20.5 0.0 40.8




88 16.3 0.0 32.8



Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

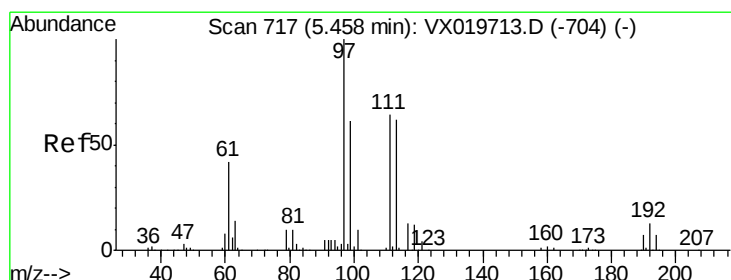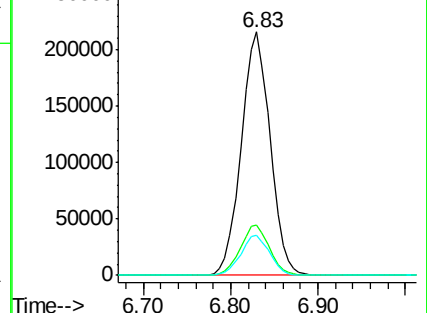

#35

Dibromofluoromethane

Concen: 48.510 ug/l

RT: 5.46 min Scan# 718

Delta R.T. 0.01 min

Lab File: VX020087.D

Acq: 16 Dec 2020 23:42


Tgt Ion:113 Resp: 154944

Ion Ratio Lower Upper

113 100

111 103.4 81.9 122.9



192 20.1 16.7 25.1




Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



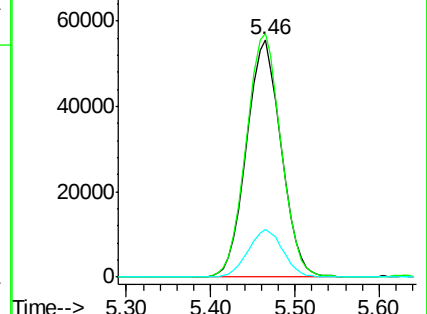





#36
 1,1-Dichloropropene
 Concen: 5.052 ug/l
 RT: 5.63 min Scan# 745
 Delta R.T. -0.13 min
 Lab File: VX020087.D
 Acq: 16 Dec 2020 23:42




Instrument :
 MSVOA_X
 ClientSampleId :
 RE122D1-20201209


Tgt Ion: 75 Resp: 22560
 Ion Ratio Lower Upper
 75 100
 110 8.2 18.1 54.4#
 77 0.0 25.3 37.9#

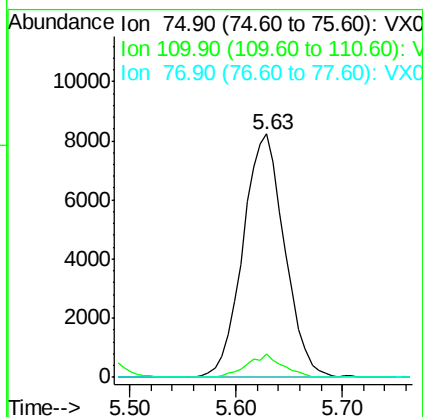

#38
 Carbon Tetrachloride
 Concen: 0.404 ug/l
 RT: 5.74 min Scan# 764
 Delta R.T. -0.01 min
 Lab File: VX020087.D
 Acq: 16 Dec 2020 23:42

Tgt Ion: 117 Resp: 1766
 Ion Ratio Lower Upper
 117 100
 119 81.7 76.2 114.2
 121 16.7 24.8 37.2#



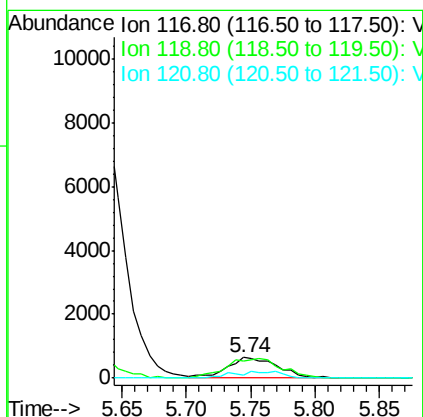





#39
Methylcyclohexane
Concen: 3.129 ug/l
RT: 7.18 min Scan# 1000
Delta R.T. -0.25 min
Lab File: VX020087.D
Acq: 16 Dec 2020 23:42




Instrument :
MSVOA_X
ClientSampleId :
RE122D1-20201209


Tgt Ion: 83 Resp: 16415
Ion Ratio Lower Upper
83 100
55 0.0 58.9 88.3#
98 211.1 38.1 57.1#

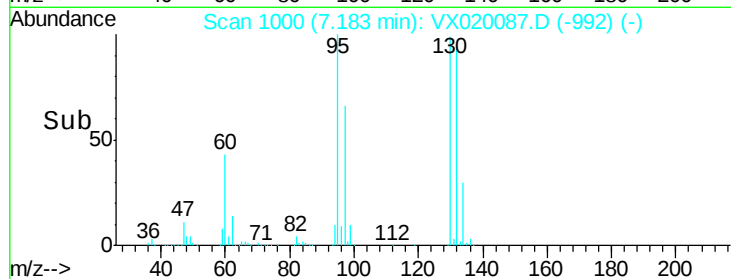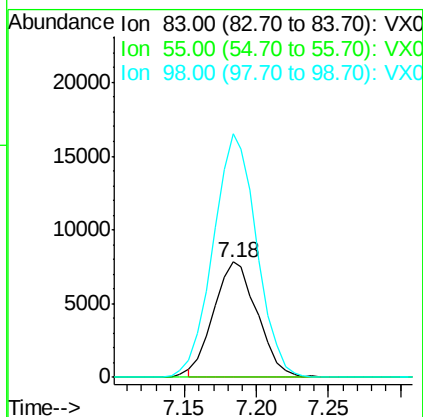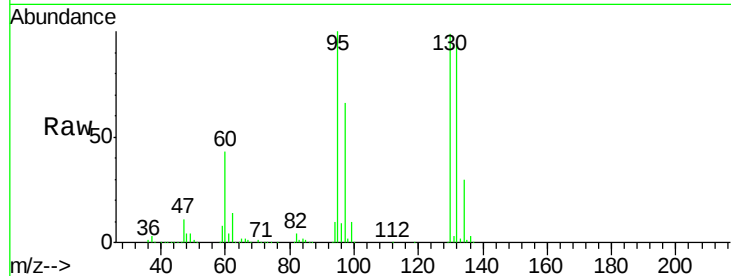

#44
Trichloroethene
Concen: 390.508 ug/l
RT: 7.18 min Scan# 1000
Delta R.T. -0.00 min
Lab File: VX020087.D
Acq: 16 Dec 2020 23:42

Tgt Ion: 130 Resp: 1397766
Ion Ratio Lower Upper
130 100
95 101.4 0.0 198.0


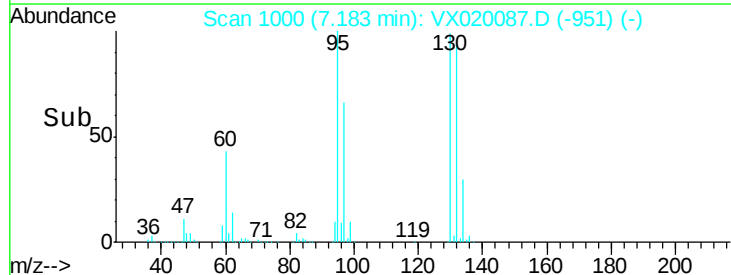
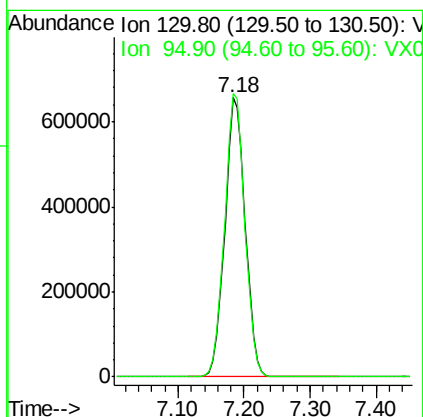





#49
1,4-Dioxane
Concen: 12.331 ug/l
RT: 7.71 min Scan# 1087
Delta R.T. 0.01 min
Lab File: VX020087.D
Acq: 16 Dec 2020 23:42




Instrument :
MSVOA_X
ClientSampleId :
RE122D1-20201209


Tgt Ion: 88 Resp: 1077
Ion Ratio Lower Upper
88 100
43 29.5 23.2 34.8
58 75.7 55.0 82.4

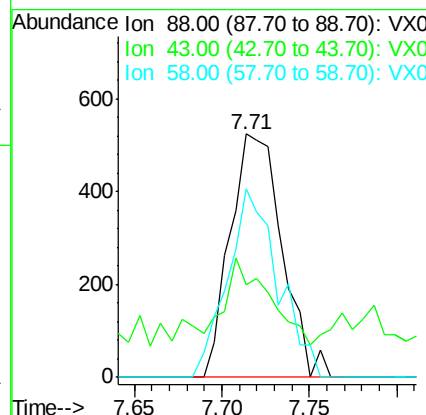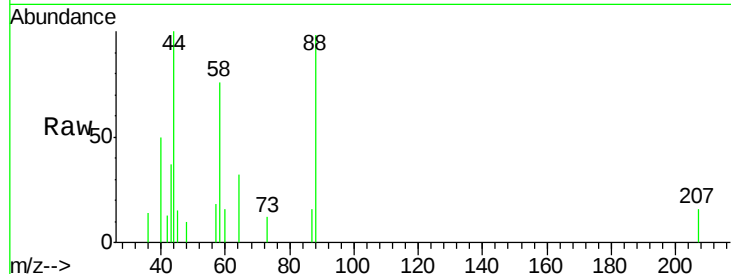

#50
Toluene-d8
Concen: 49.383 ug/l
RT: 8.70 min Scan# 1248
Delta R.T. -0.00 min
Lab File: VX020087.D
Acq: 16 Dec 2020 23:42

Tgt Ion: 98 Resp: 602186
Ion Ratio Lower Upper
98 100
100 65.9 51.9 77.9

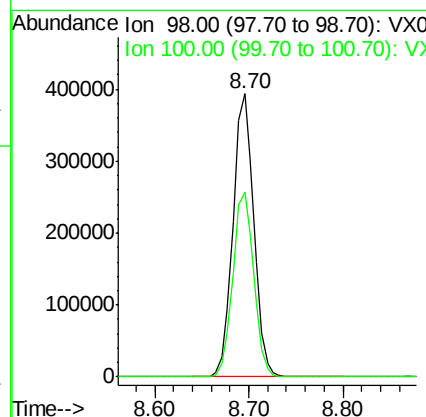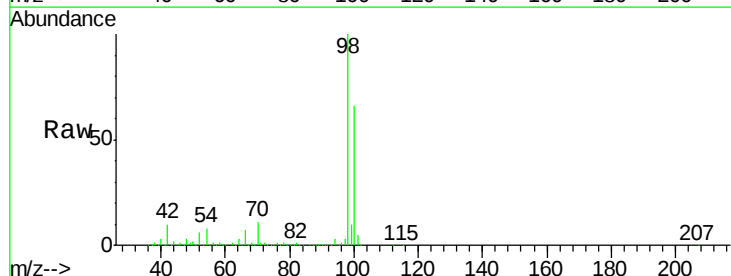


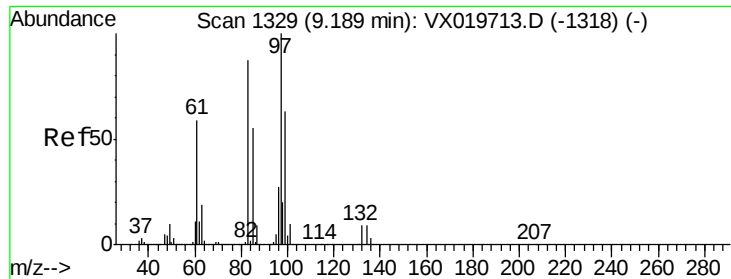




#55
 1,1,2-Trichloroethane
 Concen: 0.234 ug/l
 RT: 9.20 min Scan# 1330
 Delta R.T. 0.01 min
 Lab File: VX020087.D
 Acq: 16 Dec 2020 23:42

Instrument :
 MSVOA_X
 ClientSampleId :
 RE122D1-20201209

Tgt Ion: 97 Resp: 803
 Ion Ratio Lower Upper
 97 100
 83 95.7 69.3 103.9
 85 52.1 44.3 66.5
 99 63.3 50.3 75.5




Abundance Ion 96.90 (96.60 to 97.60): VX0
 Ion 82.90 (82.60 to 83.60): VX0
 Ion 84.90 (84.60 to 85.60): VX0
 Ion 98.90 (98.60 to 99.60): VX0


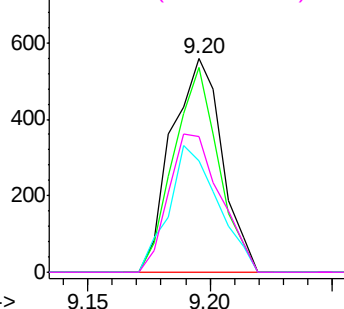



#60
 Dibromochloromethane
 Concen: 1.475 ug/l
 RT: 9.32 min Scan# 1350
 Delta R.T. -0.24 min
 Lab File: VX020087.D
 Acq: 16 Dec 2020 23:42

Tgt Ion: 129 Resp: 5152
 Ion Ratio Lower Upper
 129 100
 127 0.0 38.4 115.2#



Abundance Ion 128.80 (128.50 to 129.50): V
 Ion 126.80 (126.50 to 127.50): V

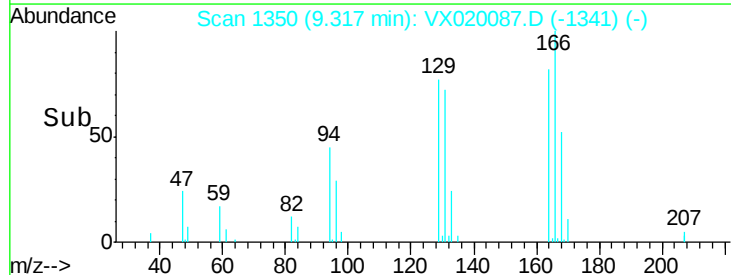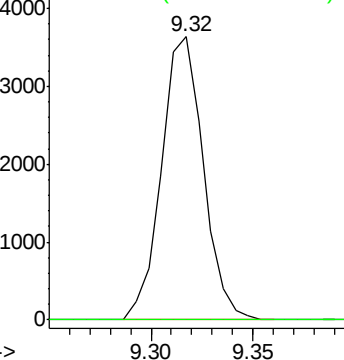



#62

4-Bromofluorobenzene

Concen: 45.867 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.00 min

Lab File: VX020087.D

Acq: 16 Dec 2020 23:42

Instrument :

MSVOA_X

ClientSampleId :

RE122D1-20201209


Tgt Ion: 95 Resp: 212880

Ion Ratio Lower Upper

95 100

174 77.2 0.0 154.6




176 74.1 0.0 155.8



Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): VX0

Ion 175.80 (175.50 to 176.50): VX0

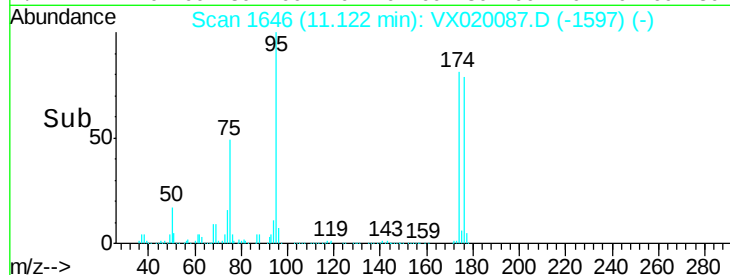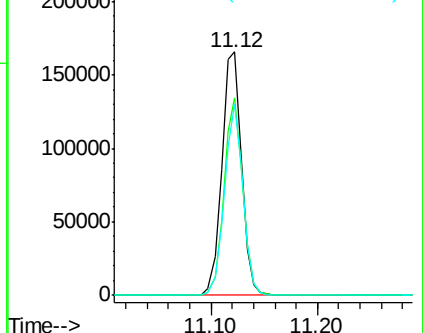

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.09 min Scan# 1477

Delta R.T. -0.00 min

Lab File: VX020087.D

Acq: 16 Dec 2020 23:42


Tgt Ion: 117 Resp: 464792

Ion Ratio Lower Upper

117 100

82 57.2 47.4 71.2



119 31.5 26.6 39.8




Abundance Ion 116.90 (116.60 to 117.60): VX0

Ion 82.00 (81.70 to 82.70): VX0

Ion 118.90 (118.60 to 119.60): VX0




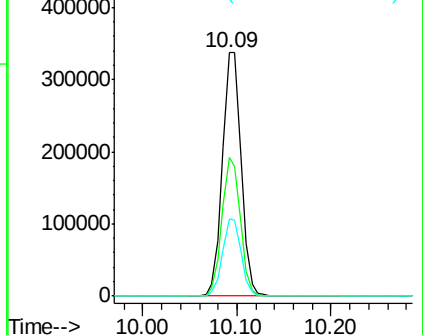




#64
Tetrachloroethene
Concen: 1.790 ug/l
RT: 9.32 min Scan# 1350
Delta R.T. -0.00 min
Lab File: VX020087.D
Acq: 16 Dec 2020 23:42




Instrument :
MSVOA_X
ClientSampleId :
RE122D1-20201209


Tgt Ion:164 Resp: 5580
Ion Ratio Lower Upper
164 100
166 122.6 103.4 155.2
129 94.8 70.8 106.2
131 88.6 72.5 108.7

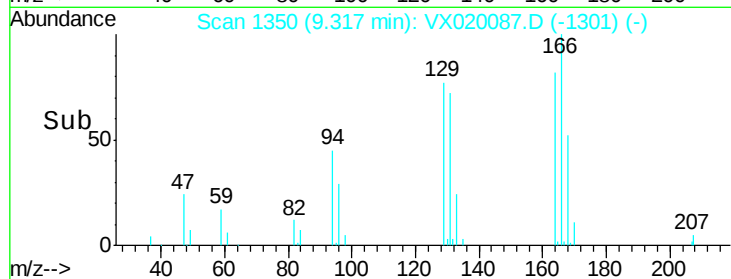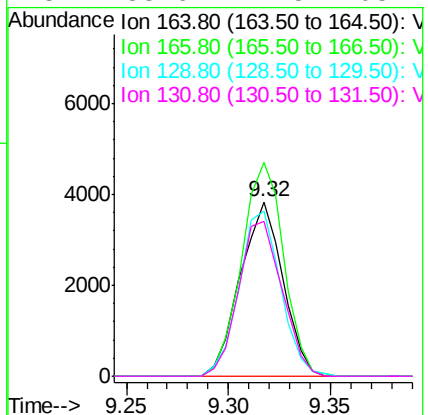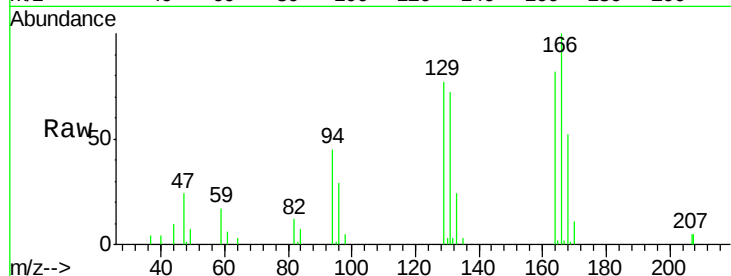

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.06 min Scan# 1800
Delta R.T. -0.00 min
Lab File: VX020087.D
Acq: 16 Dec 2020 23:42

Tgt Ion:152 Resp: 200471
Ion Ratio Lower Upper
152 100
115 60.3 41.1 123.3
150 157.3 0.0 349.0

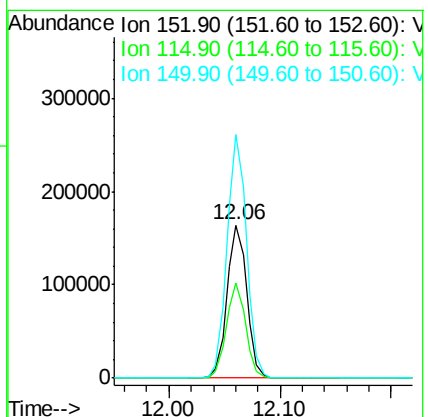



#76

1,2,3-Trichloropropane

Concen: 23.260 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.16 min

Lab File: VX020087.D

Acq: 16 Dec 2020 23:42

Instrument :

MSVOA_X

ClientSampleId :





RE122D1-20201209

Tgt Ion: 75 Resp: 104580

Ion Ratio Lower Upper

75 100

77 1.2 19.1 57.5#

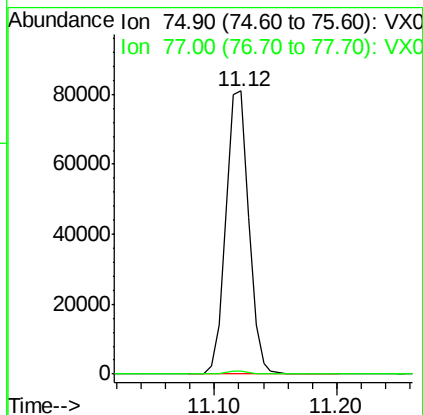

#81

trans-1,4-Dichloro-2-butene

Concen: 67.239 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. 0.07 min

Lab File: VX020087.D

Acq: 16 Dec 2020 23:42

Tgt Ion: 75 Resp: 104580

Ion Ratio Lower Upper

75 100

53 0.1 74.5 111.7#

89 0.0 37.9 56.9#

