

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\WX121720\
 Data File : VX020076.D
 Acq On : 16 Dec 2020 19:27
 Operator : JC/MD
 Sample : L5040-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-2

Integration Parameters: RTEINT.P
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X120420W.M
 Title : Sw846 8260

Signal : TIC: VX020076.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.392	45	50	54	rBV	35760	37160	2.39%	0.386%
2	1.678	92	97	106	rVB	24864	35655	2.29%	0.371%
3	1.947	136	141	147	rBV	12206	17271	1.11%	0.180%
4	2.172	172	178	185	rBV	30879	49629	3.19%	0.516%
5	2.355	200	208	216	rBV	406254	634760	40.86%	6.600%
6	3.672	413	424	438	rVB	61048	149227	9.60%	1.552%
7	4.562	557	570	581	rBV	44275	122597	7.89%	1.275%
8	5.464	704	718	730	rBV	174775	500888	32.24%	5.208%
9	5.623	733	744	764	rVB	303767	861252	55.43%	8.955%
10	6.031	798	811	820	rBV	199785	522586	33.64%	5.434%
11	6.159	828	832	840	rVB	10369	24854	1.60%	0.258%
12	6.300	845	855	868	rBV2	67453	191226	12.31%	1.988%
13	6.830	931	942	955	rBV	473801	1128373	72.63%	11.733%
14	7.226	1003	1007	1016	rVB2	14051	30723	1.98%	0.319%
15	7.708	1078	1086	1096	rBV	59330	114605	7.38%	1.192%
16	8.025	1131	1138	1146	rBV	50743	91436	5.89%	0.951%
17	8.695	1240	1248	1257	rBV	996334	1553668	100.00%	16.155%
18	9.768	1419	1424	1433	rVB	48058	69659	4.48%	0.724%
19	10.098	1471	1478	1487	rBV	953620	1331822	85.72%	13.848%
20	11.122	1640	1646	1657	rBV	775922	993407	63.94%	10.329%
21	12.061	1794	1800	1808	rBV	950172	1156580	74.44%	12.026%




Sum of corrected areas: 9617378

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121720\
Data File : VX020076.D
Acq On : 16 Dec 2020 19:27
Operator : JC/MD
Sample : L5040-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X120420W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

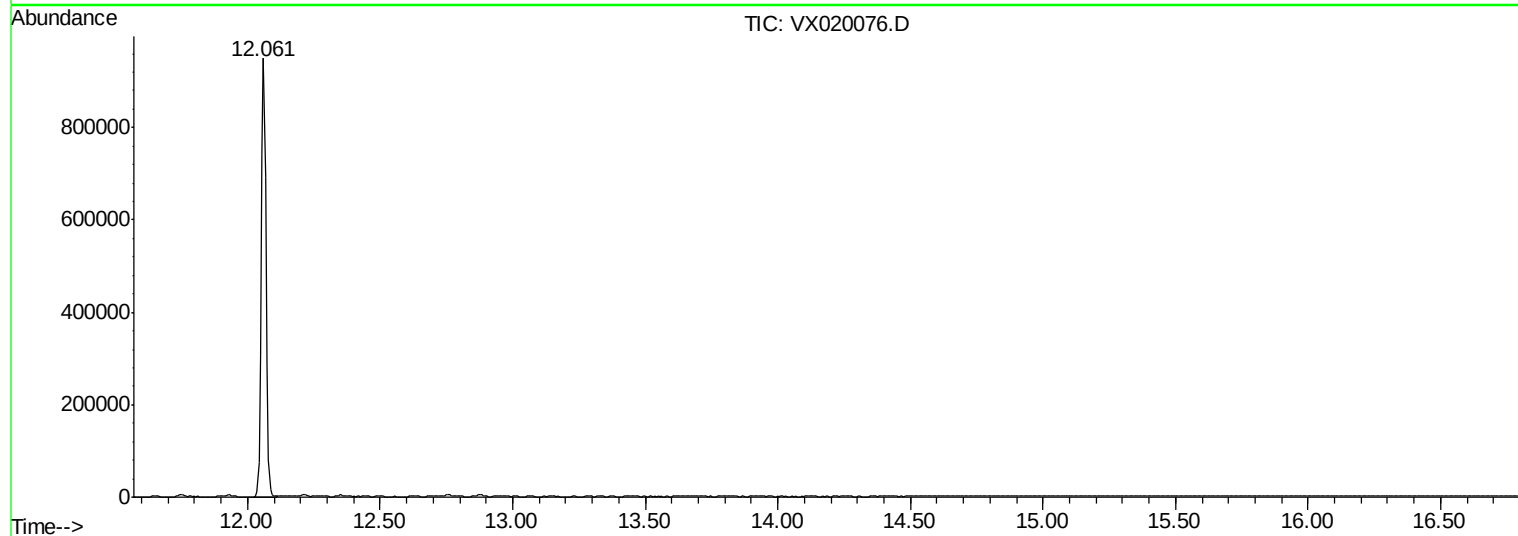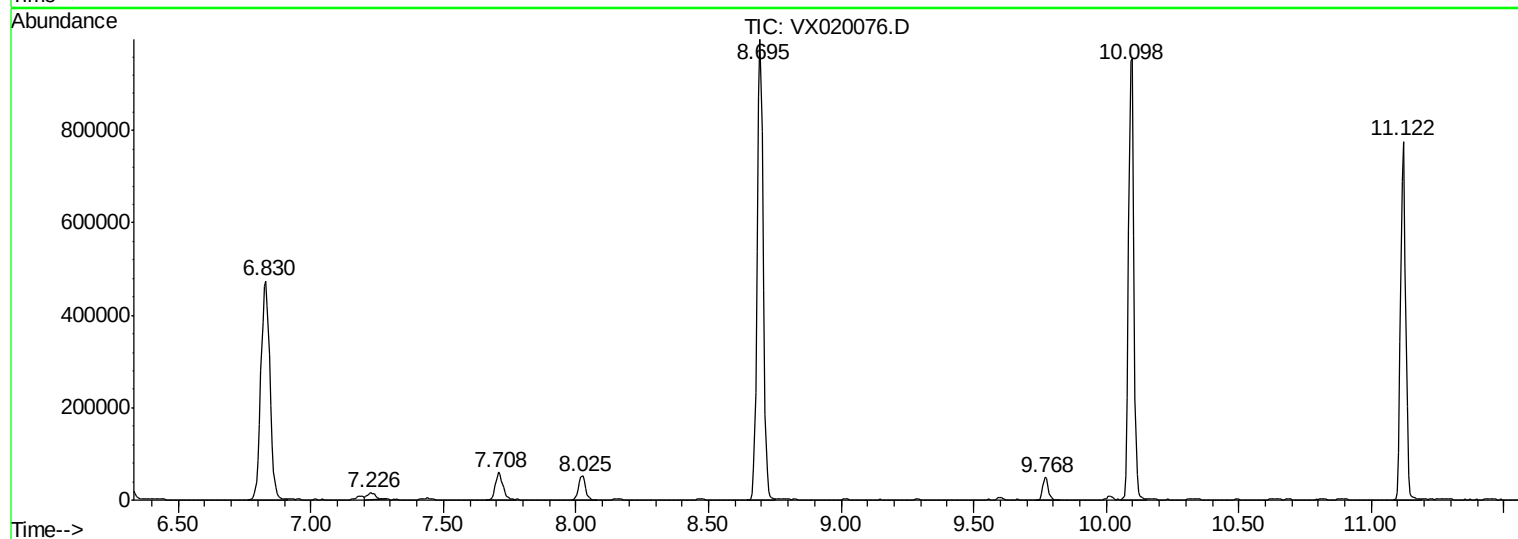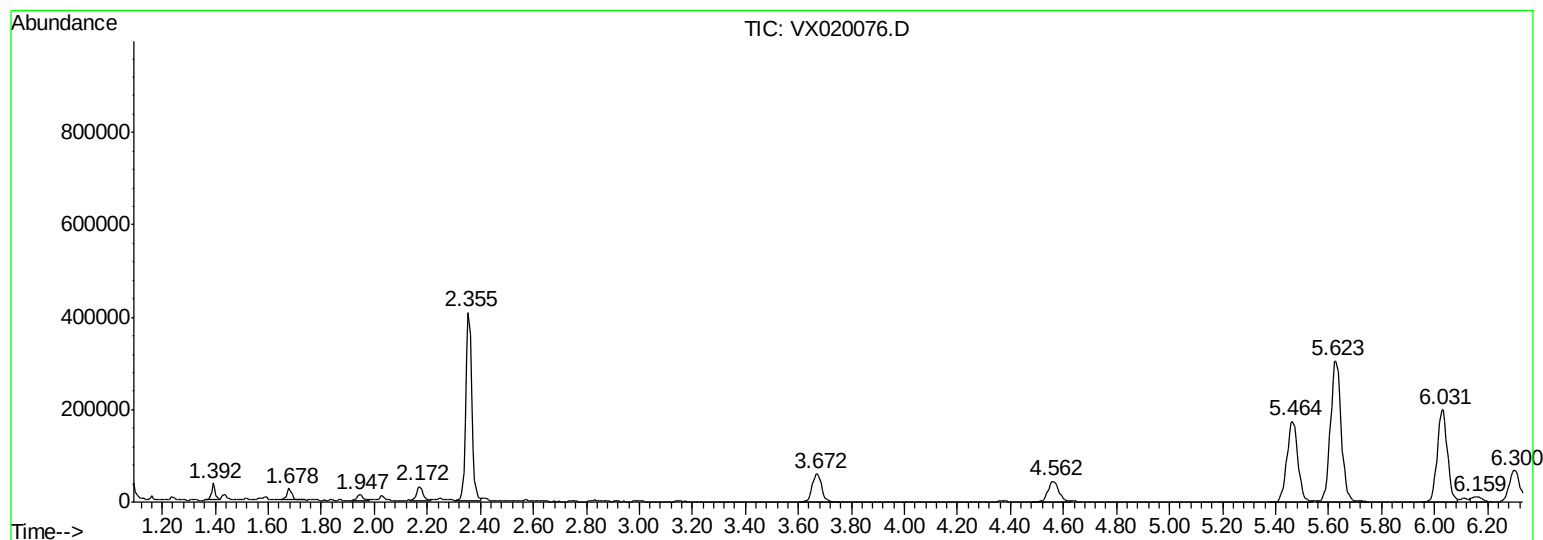

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121720\
Data File : VX020076.D
Acq On : 16 Dec 2020 19:27
Operator : JC/MD
Sample : L5040-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-2










Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X120420W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Amylene hydrate Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.300	8.47 ug/l	191226	1,4-Difluorobenzene	6.830

Hit# of 5	Tentative ID	Mw	MolForm	CAS#	Qual
1	Amylene hydrate	88	C5H12O	000075-85-4	78
2	3-Hexanol	102	C6H14O	000623-37-0	59
3	2-Hexanol, 2,3-dimethyl-	130	C8H18O	019550-03-9	39
4	2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	36
5	1-Butene, 4-ethoxy-	100	C6H12O	044611-46-3	36

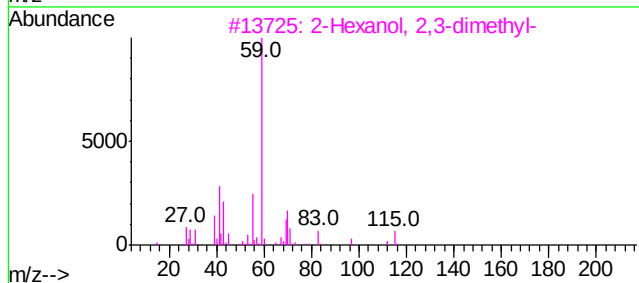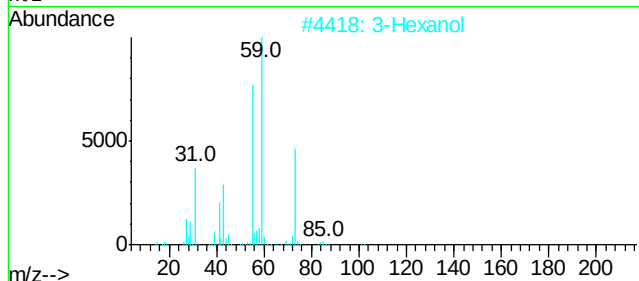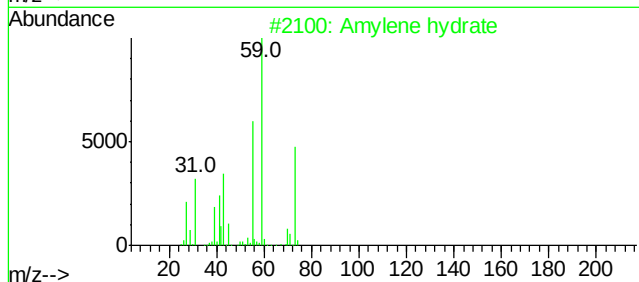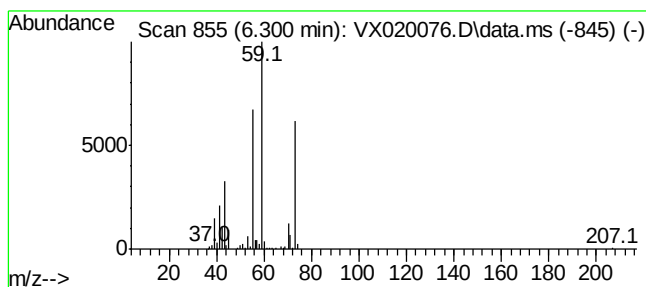

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121720\
Data File : VX020076.D
Acq On : 16 Dec 2020 19:27
Operator : JC/MD
Sample : L5040-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X120420W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Amylene hydrate	6.300	8.5	ug/l	191226	2	6.830	1128370	50.0