


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121720\
Data File : VX020064.D
Acq On : 16 Dec 2020 14:34
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X120420W.M
Title : SW846 8260
Last Update : Fri Dec 04 15:32:53 2020

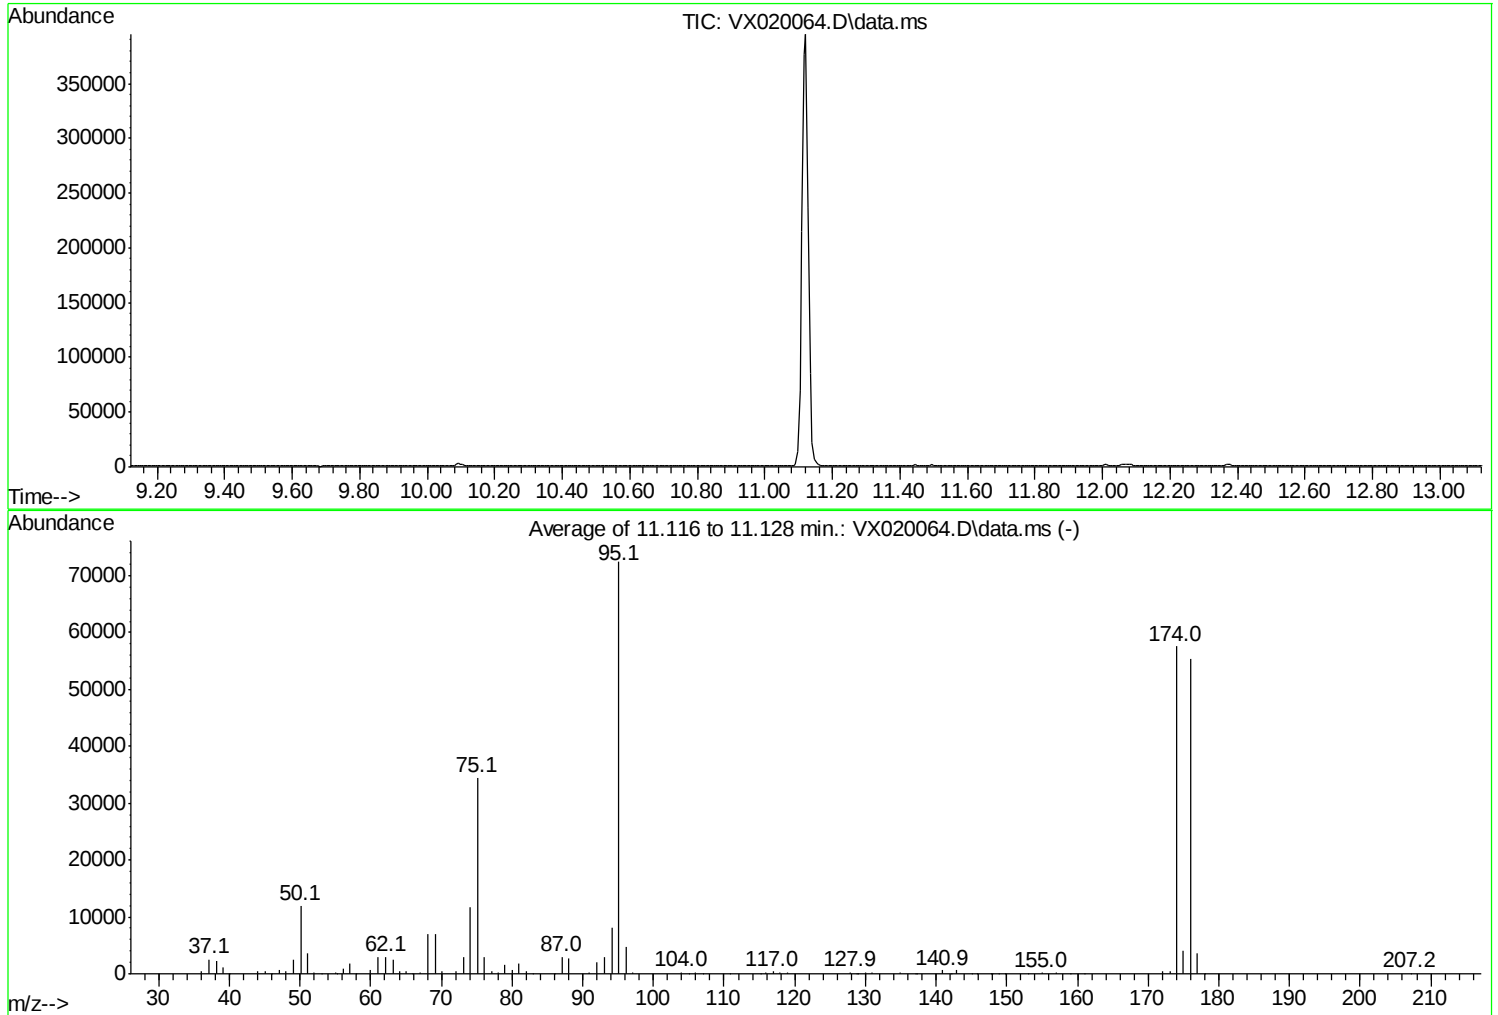

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.6	12045	PASS
75	95	30	60	47.6	34451	PASS
95	95	100	100	100.0	72448	PASS
96	95	5	9	6.5	4712	PASS
173	174	0.00	2	0.9	521	PASS
174	95	50	100	79.5	57595	PASS
175	174	5	9	7.1	4090	PASS
176	174	95	101	96.3	55456	PASS
177	176	5	9	6.4	3540	PASS