

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121721\
 Data File : VX025859.D
 Acq On : 16 Dec 2021 16:42
 Operator : JC/MD
 Sample : PB141455TB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PB141455TB

Quant Time: Dec 17 02:32:26 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121321W.M
 Quant Title : SW846 8260
 QLast Update : Tue Dec 14 07:02:11 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	147431	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	257576	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	242612	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	100549	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	98102	46.247	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	92.500%
35) Dibromofluoromethane	5.391	113	80568	44.851	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	89.700%
50) Toluene-d8	8.653	98	308891	47.194	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	94.380%
62) 4-Bromofluorobenzene	11.085	95	108120	43.487	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	86.980%
Target Compounds						
25) 2-Butanone	4.580	43	5116	3.586	ug/l	96
43) Isopropyl Acetate	6.348	43	13173	3.021	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121721\
Data File : VX025859.D
Acq On : 16 Dec 2021 16:42
Operator : JC/MD
Sample : PB141455TB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PB141455TB

Quant Time: Dec 17 02:32:26 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121321W.M
Quant Title : SW846 8260
QLast Update : Tue Dec 14 07:02:11 2021
Response via : Initial Calibration




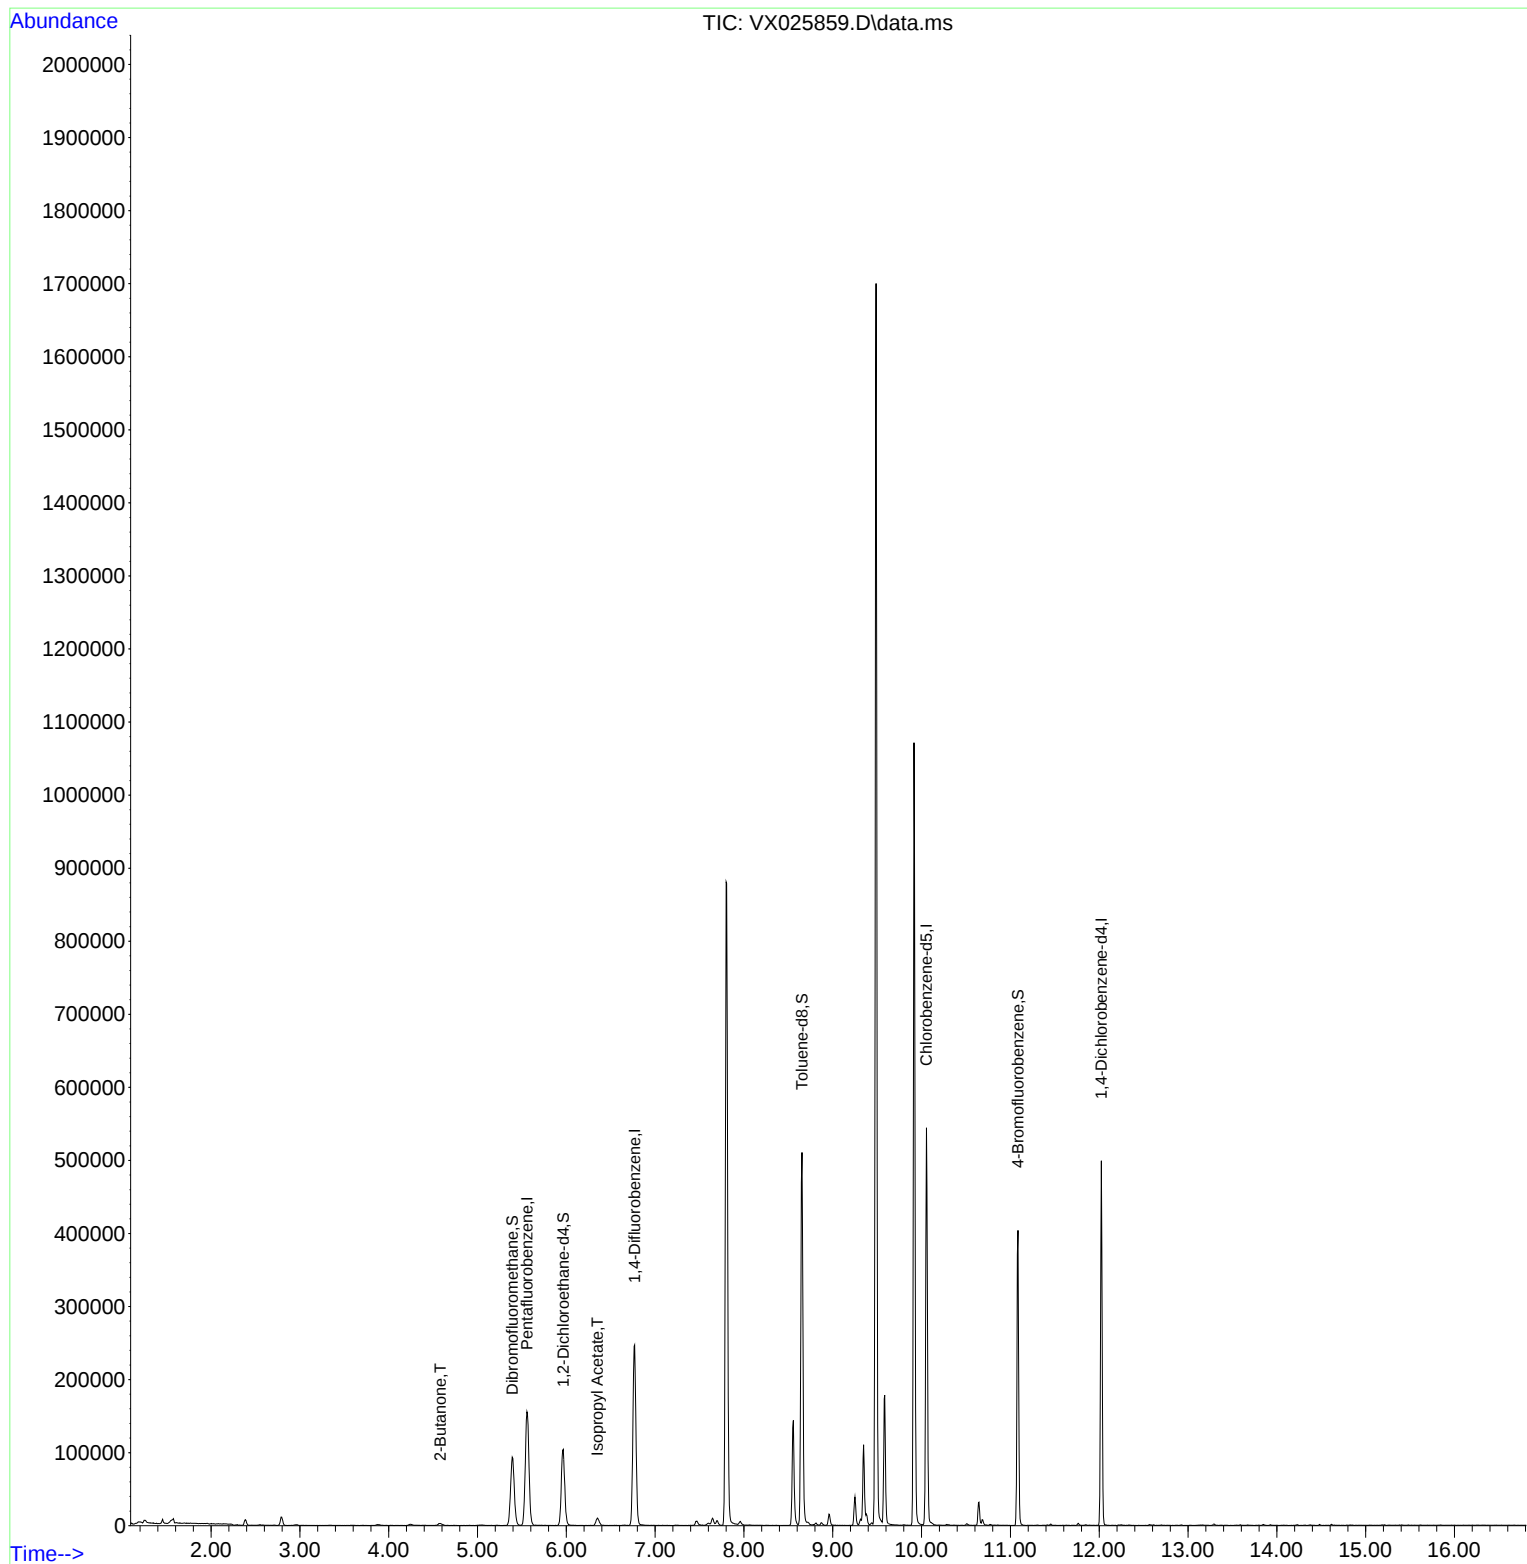


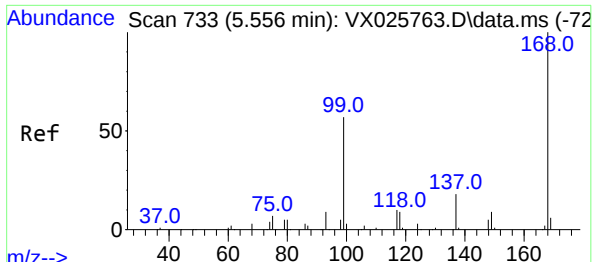

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX025859.D
Acq: 16 Dec 2021 16:42




Instrument :
MSVOA_X
ClientSampleId :
PB141455TB


Tgt Ion:168 Resp: 147431
Ion Ratio Lower Upper
168 100
99 59.5 45.8 68.8

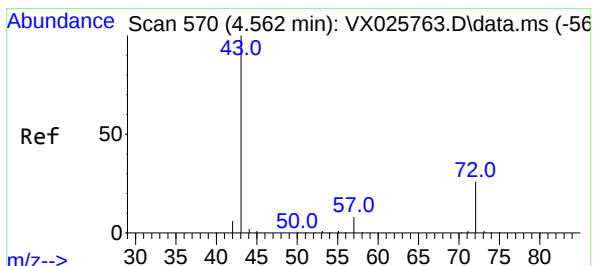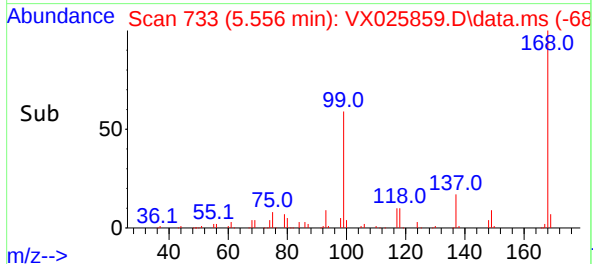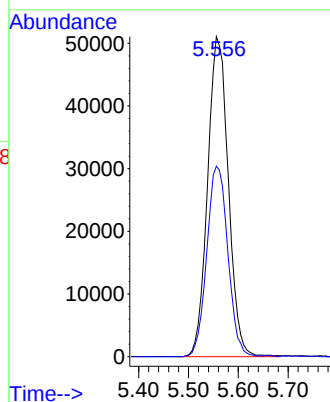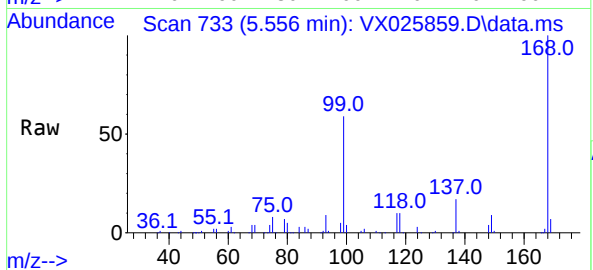

#25
2-Butanone
Concen: 3.586 ug/l
RT: 4.580 min Scan# 573
Delta R.T. 0.018 min
Lab File: VX025859.D
Acq: 16 Dec 2021 16:42

Tgt Ion: 43 Resp: 5116
Ion Ratio Lower Upper
43 100
72 23.9 21.0 31.4

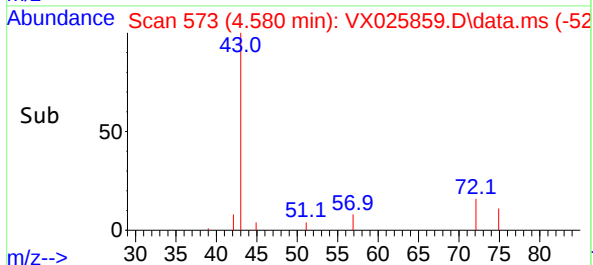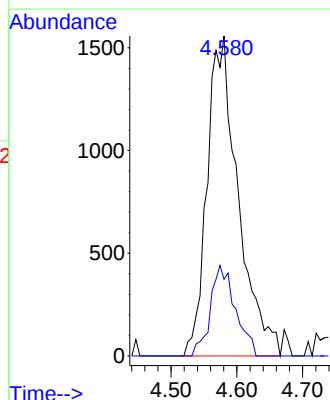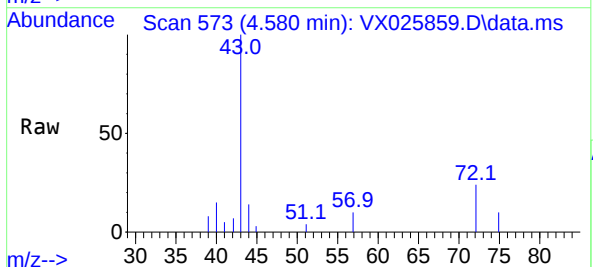

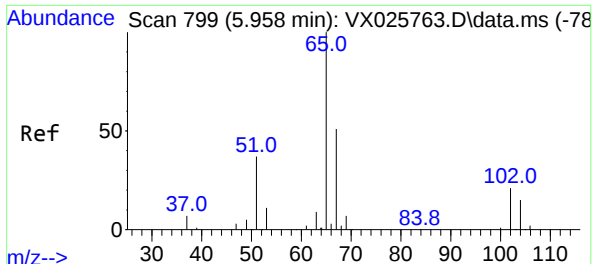

#33

1,2-Dichloroethane-d4

Concen: 46.247 ug/l

RT: 5.964 min Scan# 80

Delta R.T. 0.006 min

Lab File: VX025859.D

Acq: 16 Dec 2021 16:42

Instrument :

MSVOA_X

ClientSampleId :





PB141455TB

Tgt Ion: 65 Resp: 98102

Ion Ratio Lower Upper

65 100

67 50.8 0.0 103.4

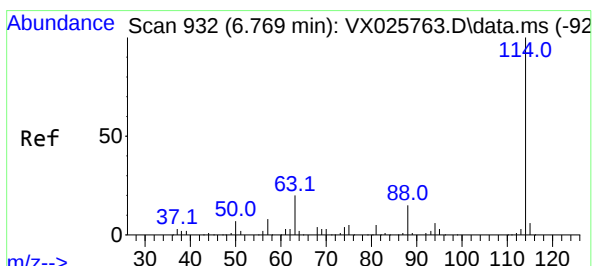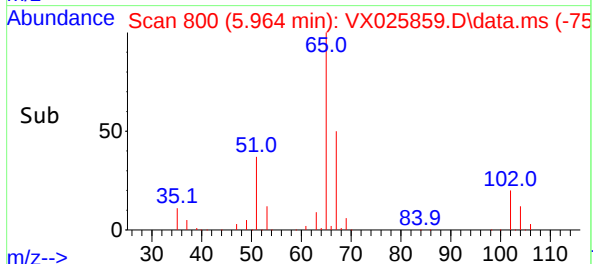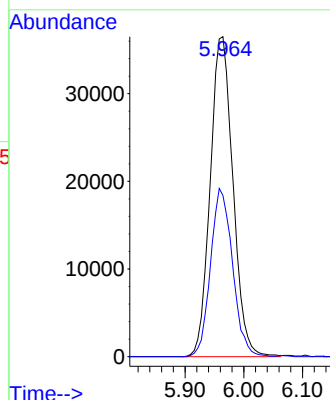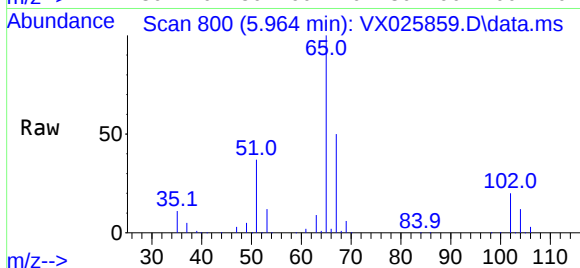

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.769 min Scan# 932

Delta R.T. 0.000 min

Lab File: VX025859.D

Acq: 16 Dec 2021 16:42




Tgt Ion: 114 Resp: 257576


Ion Ratio Lower Upper

114 100

63 20.1 0.0 40.0

88 14.9 0.0 30.6


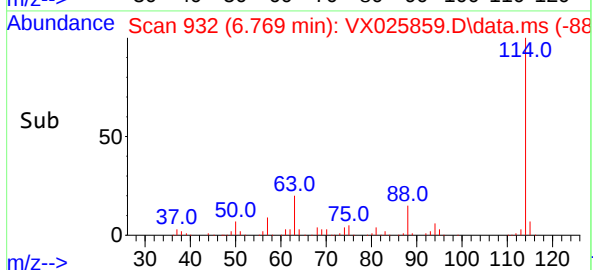
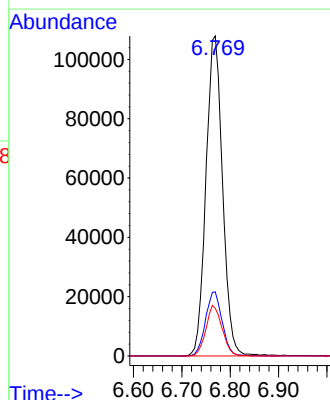
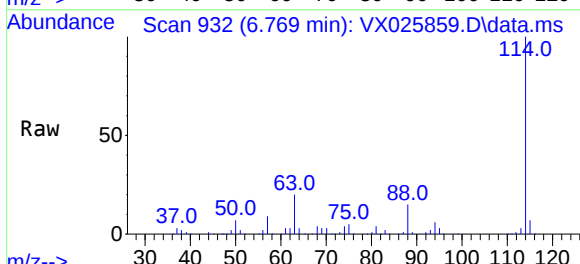


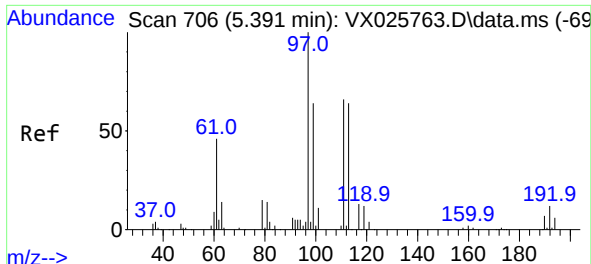

#35
Dibromofluoromethane
Concen: 44.851 ug/l
RT: 5.391 min Scan# 706
Delta R.T. -0.000 min
Lab File: VX025859.D
Acq: 16 Dec 2021 16:42




Instrument :
MSVOA_X
ClientSampleId :
PB141455TB


Tgt Ion:113 Resp: 80568
Ion Ratio Lower Upper
113 100
111 103.7 81.8 122.8
192 18.8 15.0 22.4

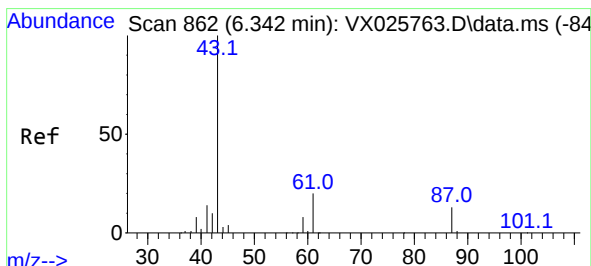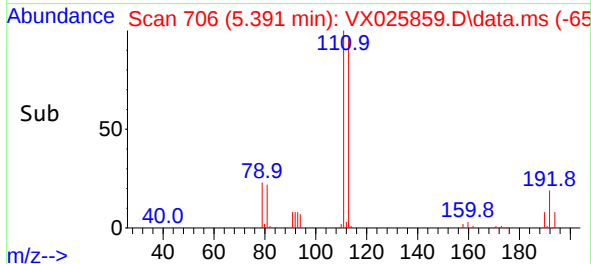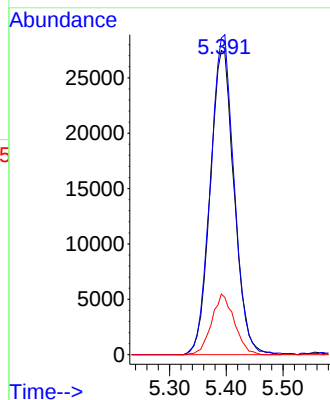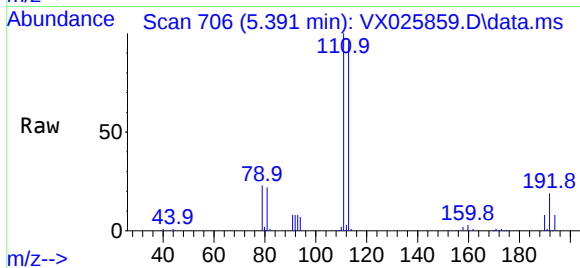

#43
Isopropyl Acetate
Concen: 3.021 ug/l
RT: 6.348 min Scan# 863
Delta R.T. 0.006 min
Lab File: VX025859.D
Acq: 16 Dec 2021 16:42

Tgt Ion: 43 Resp: 13173
Ion Ratio Lower Upper
43 100
61 19.3 15.7 23.5
87 13.1 11.2 16.8


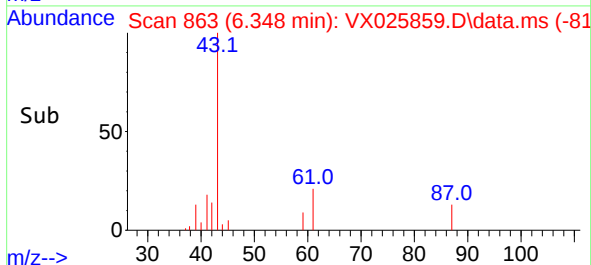
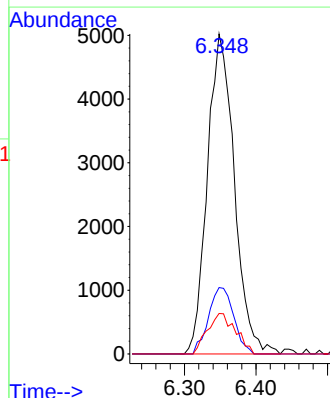
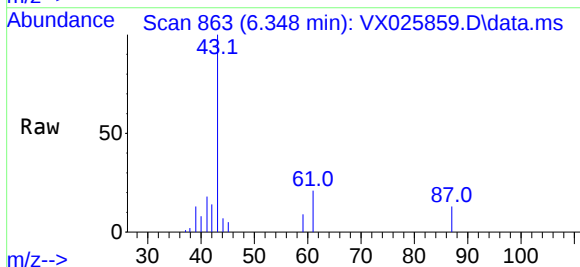


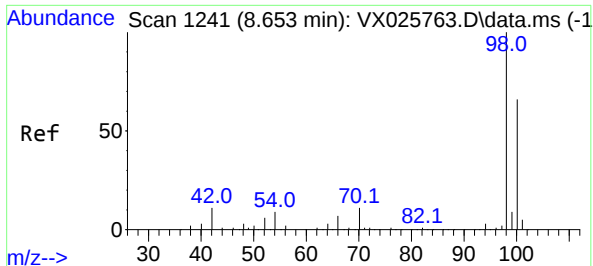

#50
Toluene-d8
Concen: 47.194 ug/l
RT: 8.653 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX025859.D
Acq: 16 Dec 2021 16:42




Instrument :
MSVOA_X
ClientSampleId :
PB141455TB


Tgt Ion: 98 Resp: 308891
Ion Ratio Lower Upper
98 100
100 65.5 52.6 78.8

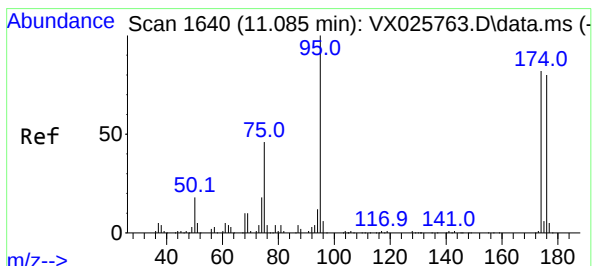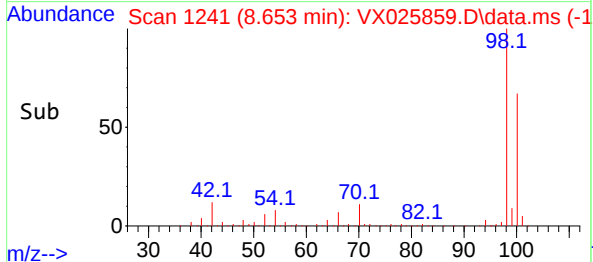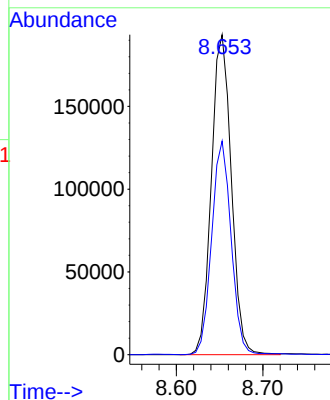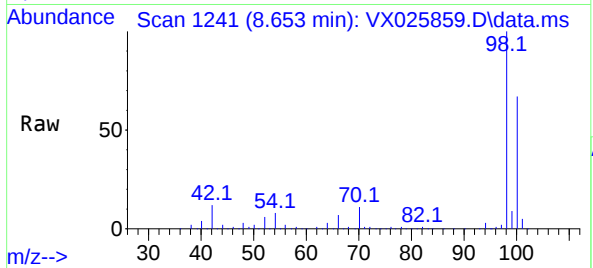

#62
4-Bromofluorobenzene
Concen: 43.487 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.000 min
Lab File: VX025859.D
Acq: 16 Dec 2021 16:42

Tgt Ion: 95 Resp: 108120
Ion Ratio Lower Upper
95 100
174 76.8 0.0 157.4
176 75.8 0.0 154.6


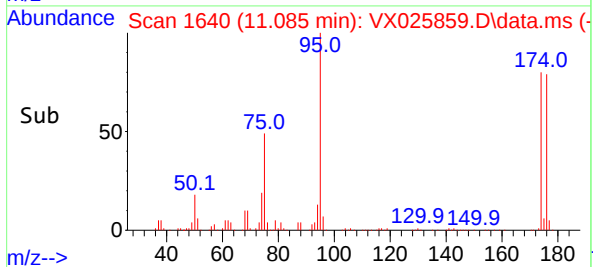
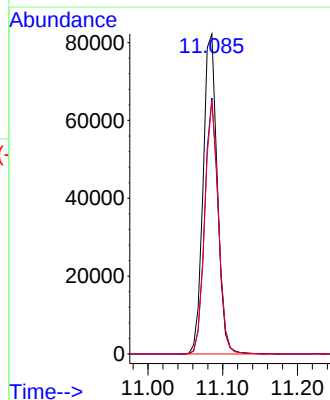
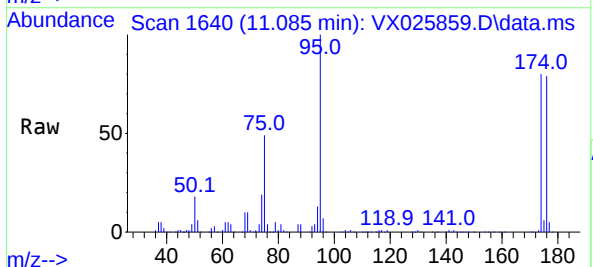


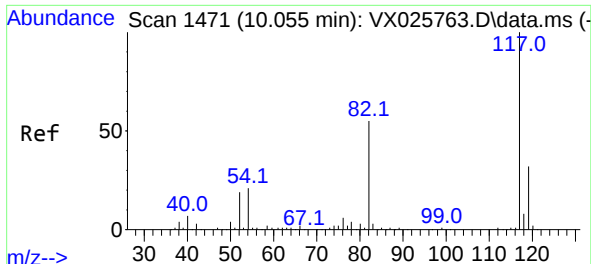

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX025859.D
Acq: 16 Dec 2021 16:42

Instrument :
MSVOA_X
ClientSampleId :
PB141455TB

Tgt Ion:117 Resp: 242612
Ion Ratio Lower Upper
117 100
82 55.0 43.8 65.6
119 32.4 25.2 37.8

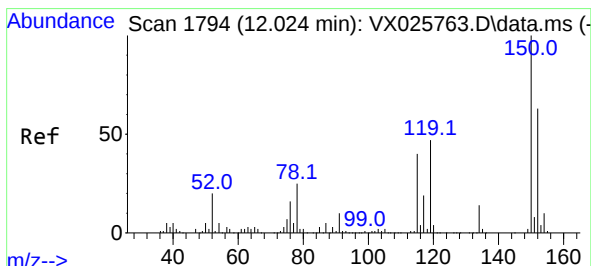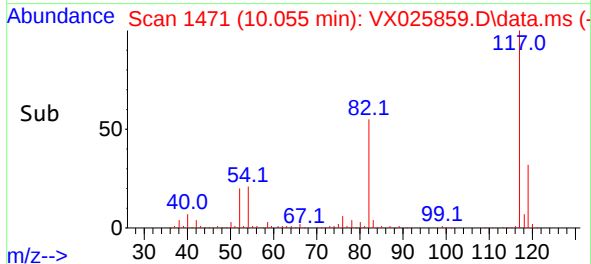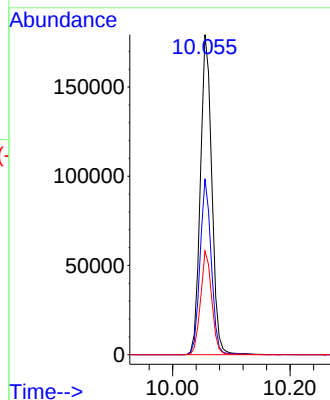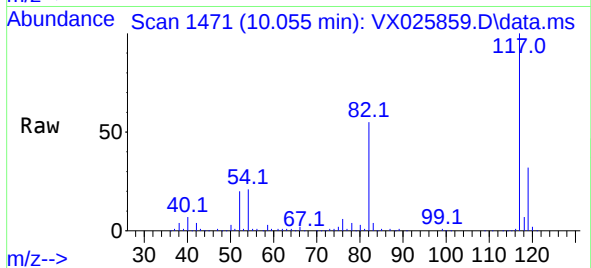

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX025859.D
Acq: 16 Dec 2021 16:42

Tgt Ion:152 Resp: 100549
Ion Ratio Lower Upper
152 100
115 59.8 41.3 123.9
150 158.0 0.0 351.8

