


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121721\
Data File : VX025847.D
Acq On : 16 Dec 2021 09:57
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121321W.M
Title : SW846 8260
Last Update : Tue Dec 14 07:02:11 2021

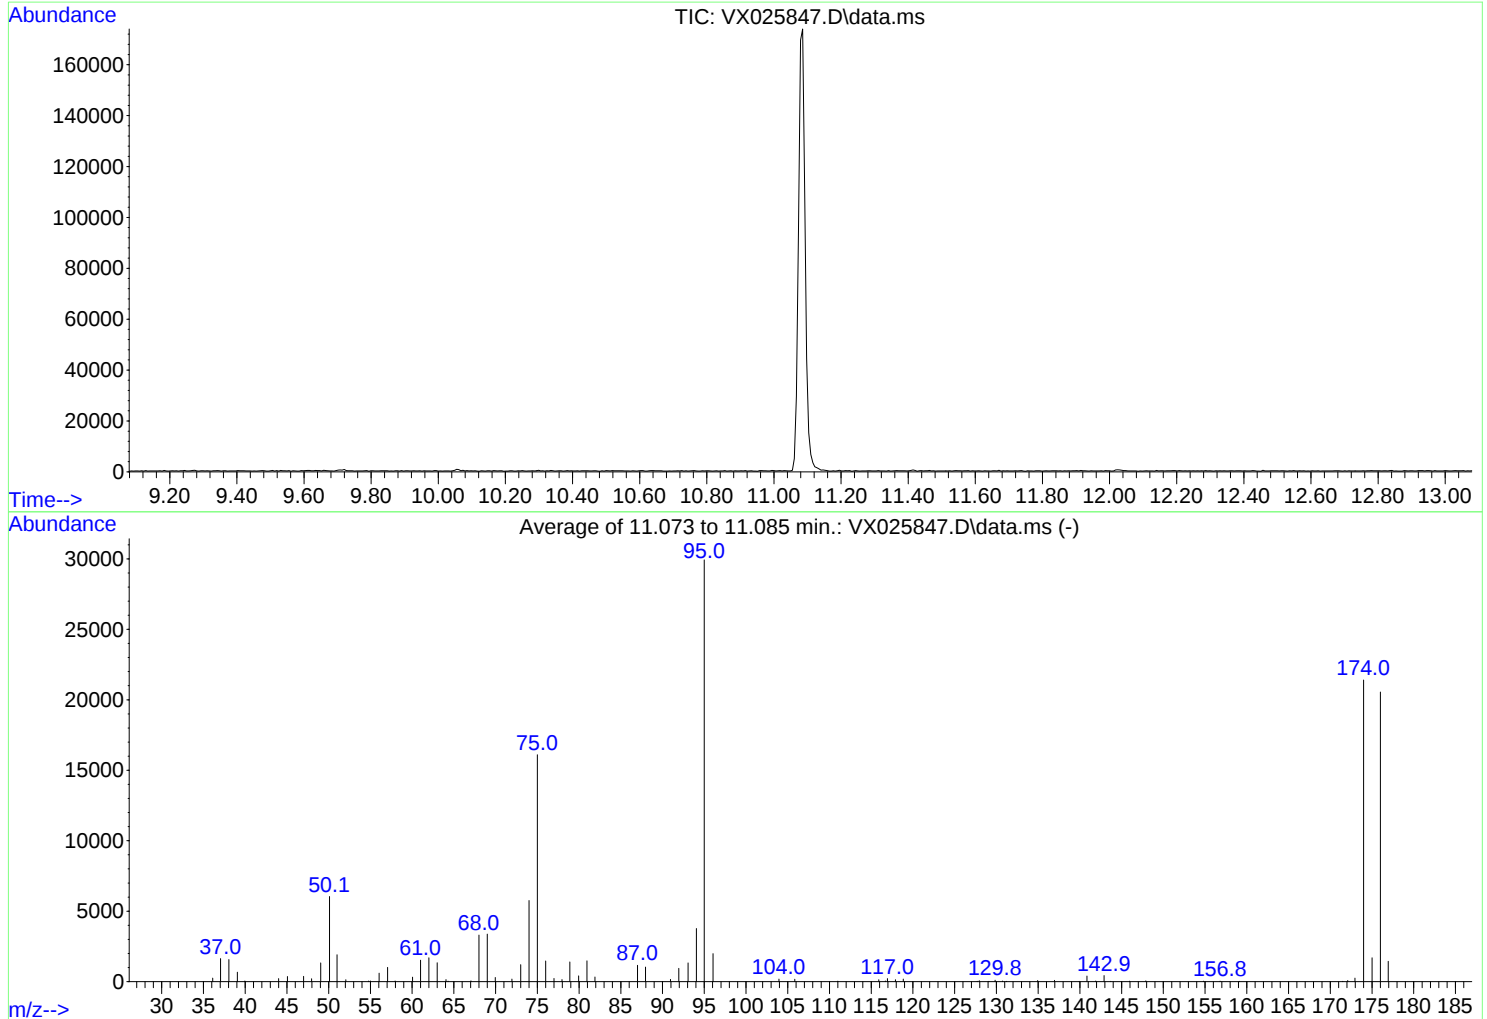

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	6042	PASS
75	95	30	60	53.8	16105	PASS
95	95	100	100	100.0	29931	PASS
96	95	5	9	6.6	1985	PASS
173	174	0.00	2	1.2	252	PASS
174	95	50	100	71.5	21398	PASS
175	174	5	9	7.9	1688	PASS
176	174	95	101	96.1	20554	PASS
177	176	5	9	7.0	1441	PASS