


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121721\
 Data File : VX025871.D
 Acq On : 16 Dec 2021 21:48
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121321W.M
 Title : SW846 8260
 Last Update : Tue Dec 14 07:02:11 2021

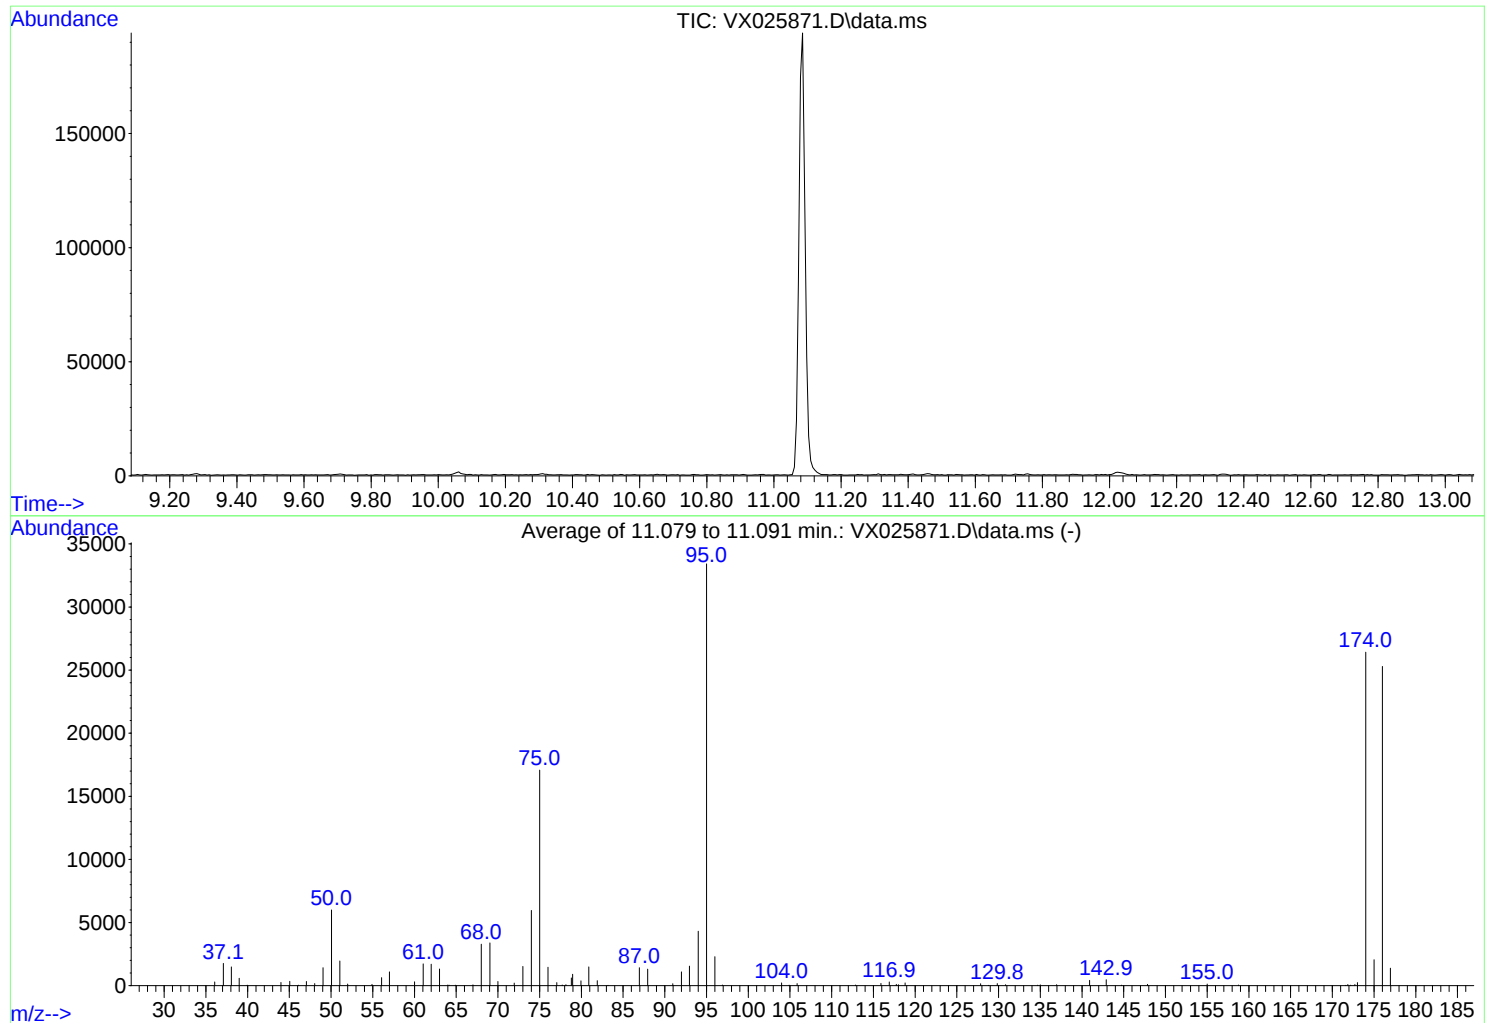

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	5999	PASS
75	95	30	60	51.1	17072	PASS
95	95	100	100	100.0	33419	PASS
96	95	5	9	6.9	2299	PASS
173	174	0.00	2	0.9	244	PASS
174	95	50	100	79.0	26416	PASS
175	174	5	9	7.8	2051	PASS
176	174	95	101	95.7	25293	PASS
177	176	5	9	5.5	1388	PASS