

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121724\
 Data File : VX044356.D
 Acq On : 17 Dec 2024 17:04
 Operator : JC/MD
 Sample : VX1217WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Dec 18 04:41:45 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 18 04:40:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	233416	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	198771	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.018	152	81751	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	86696	40.587	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	81.180%		
7) Chloroethane-d5	1.648	69	81802	49.437	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	98.880%		
11) 1,1-Dichloroethene-d2	2.294	65	37525	41.078	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	82.160%		
21) 2-Butanone-d5	4.458	46	153403	117.300	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	117.300%		
24) Chloroform-d	5.050	84	193064	47.604	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.200%		
26) 1,2-Dichloroethane-d4	5.952	65	136932	47.743	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.480%		
32) Benzene-d6	5.964	84	346865	50.504	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	101.000%		
36) 1,2-Dichloropropane-d6	7.305	67	113958	53.436	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	106.880%		
41) Toluene-d8	8.647	98	296401	46.674	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	93.340%		
43) trans-1,3-Dichloroprop...	8.951	79	45557	44.452	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	88.900%		
47) 2-Hexanone-d5	9.384	63	101850	122.486	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	122.490%		
56) 1,1,2,2-Tetrachloroeth...	11.189	84	160694	56.195	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	112.380%		
66) 1,2-Dichlorobenzene-d4	12.317	152	105371	55.320	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	110.640%		
Target Compounds						Qvalue
44) trans-1,3-Dichloropropene	8.945	75	2655	1.103	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121724\
Data File : VX044356.D
Acq On : 17 Dec 2024 17:04
Operator : JC/MD
Sample : VX1217WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Dec 18 04:41:45 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 18 04:40:20 2024
Response via : Initial Calibration

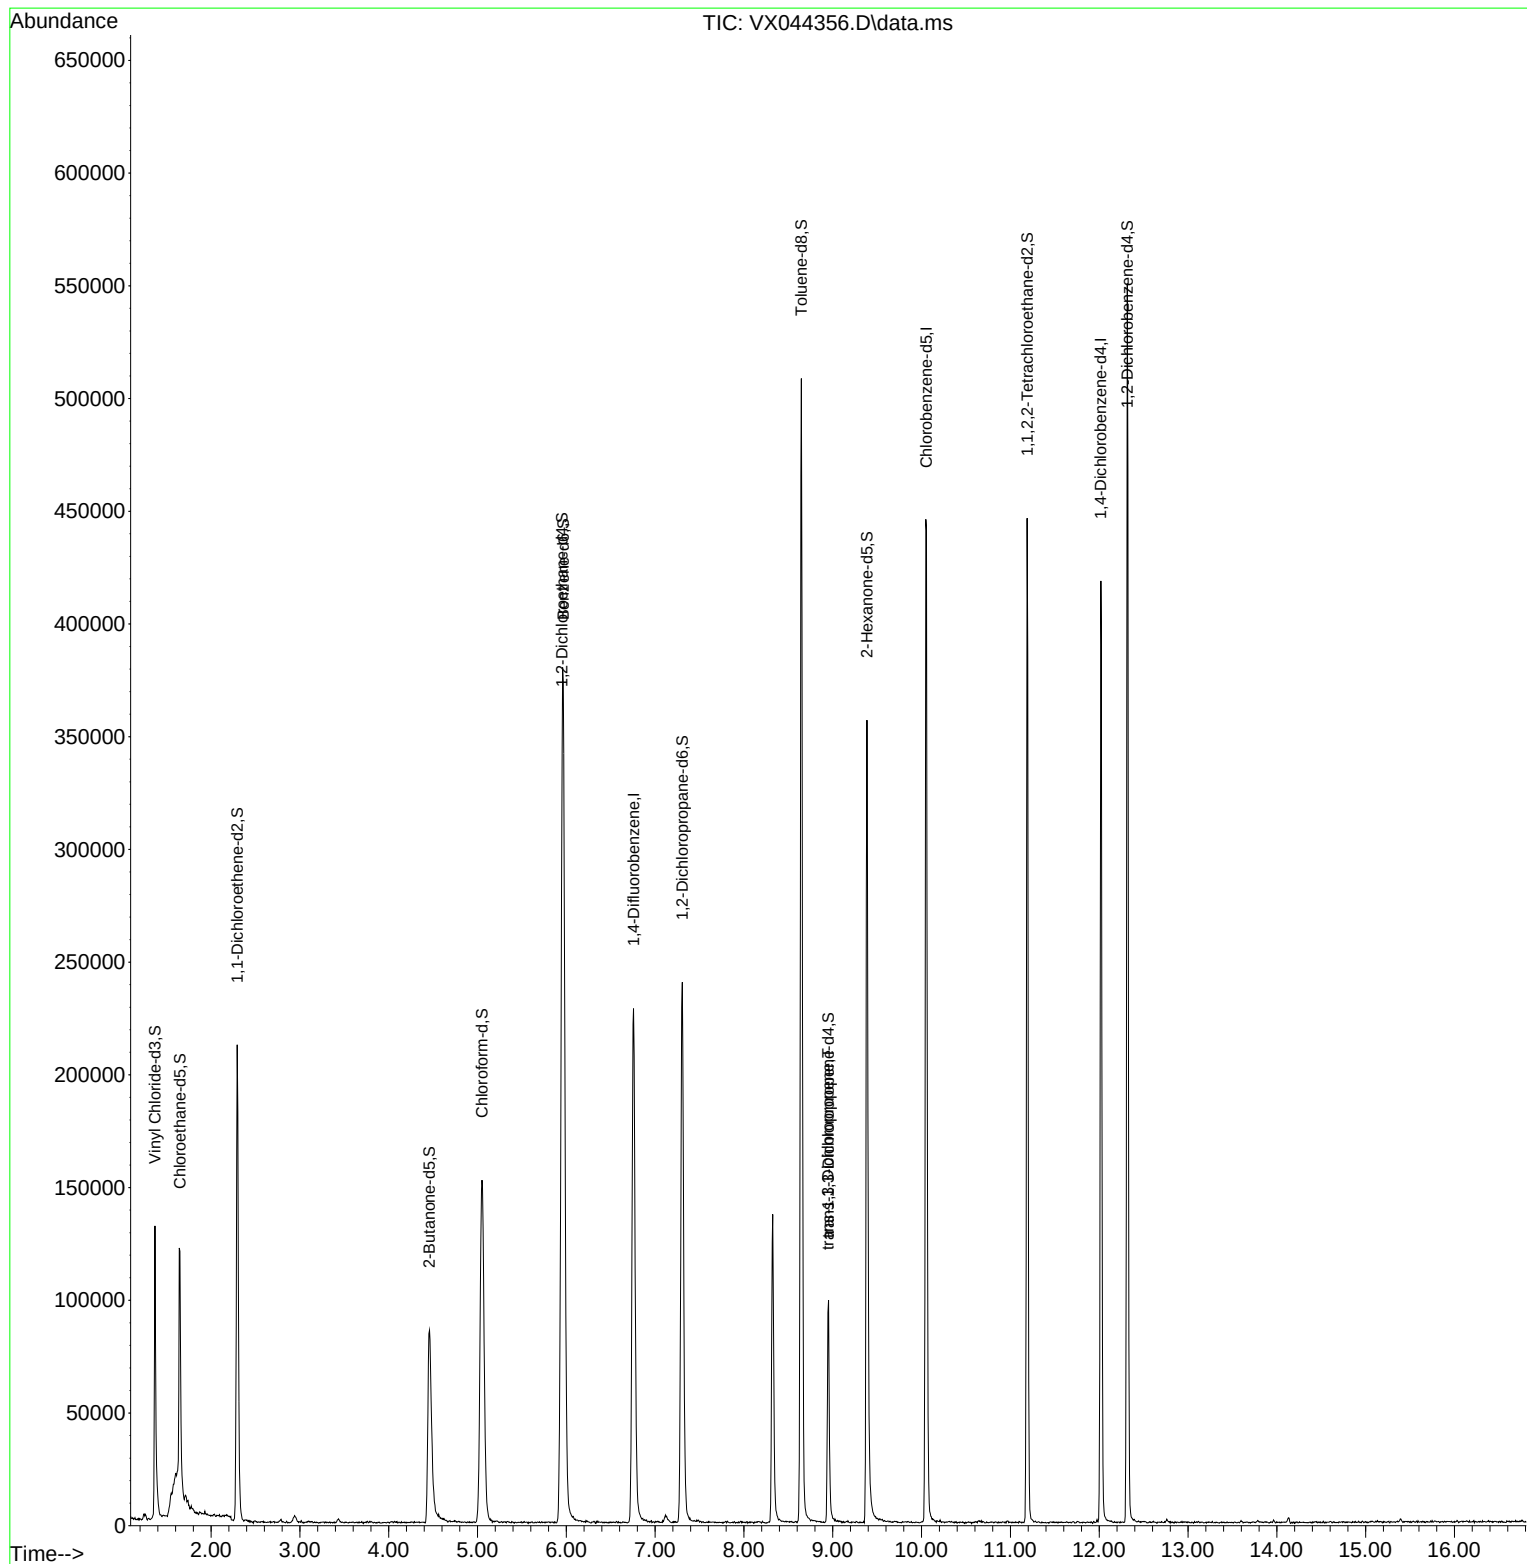

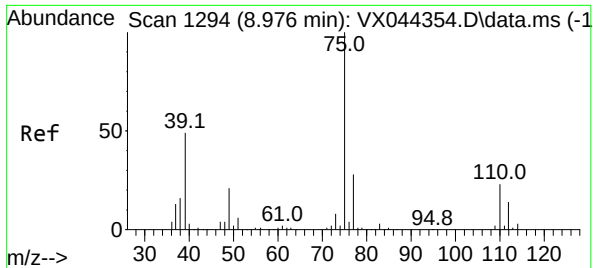

#44
trans-1,3-Dichloropropene
Concen: 1.103 ug/L
RT: 8.945 min Scan# 11
Delta R.T. -0.031 min
Lab File: VX044356.D
Acq: 17 Dec 2024 17:04

Instrument :
MSVOA_X
ClientSampleId :

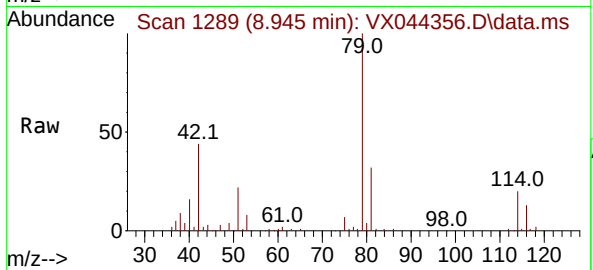

Tgt Ion: 75 Resp: 2655
Ion Ratio Lower Upper
75 100
77 33.6 21.8 40.6

