

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121724\
 Data File : VX044362.D
 Acq On : 17 Dec 2024 19:24
 Operator : JC/MD
 Sample : P5226-02ME
 Misc : 7.41g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Dec 18 04:43:25 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 18 04:40:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	334593	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	307632	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	126765	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	40043	13.078	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	26.160%#
7) Chloroethane-d5	1.642	69	23574	9.939	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	19.880%#
11) 1,1-Dichloroethene-d2	2.270	65	37140	28.362	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	56.720%#
21) 2-Butanone-d5	4.489	46	169215	90.264	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	90.260%
24) Chloroform-d	5.050	84	223359	38.420	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	76.840%
26) 1,2-Dichloroethane-d4	5.952	65	158996	38.673	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	77.340%
32) Benzene-d6	5.958	84	406360	38.229	ug/L	-0.01
Spiked Amount	50.000	Range	70 - 125	Recovery	=	76.460%
36) 1,2-Dichloropropane-d6	7.299	67	135296	40.991	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	81.980%
41) Toluene-d8	8.647	98	363656	37.000	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	74.000%#
43) trans-1,3-Dichloroprop...	8.952	79	53051	33.447	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	66.900%
47) 2-Hexanone-d5	9.391	63	119359	92.747	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	92.750%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	196563	44.414	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	88.820%
66) 1,2-Dichlorobenzene-d4	12.317	152	136014	46.051	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.100%
Target Compounds						
61) 1,2,3-Trichloropropane	12.018	75	17446	5.942	ug/L	Qvalue # 65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121724\
Data File : VX044362.D
Acq On : 17 Dec 2024 19:24
Operator : JC/MD
Sample : P5226-02ME
Misc : 7.41g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Dec 18 04:43:25 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 18 04:40:20 2024
Response via : Initial Calibration

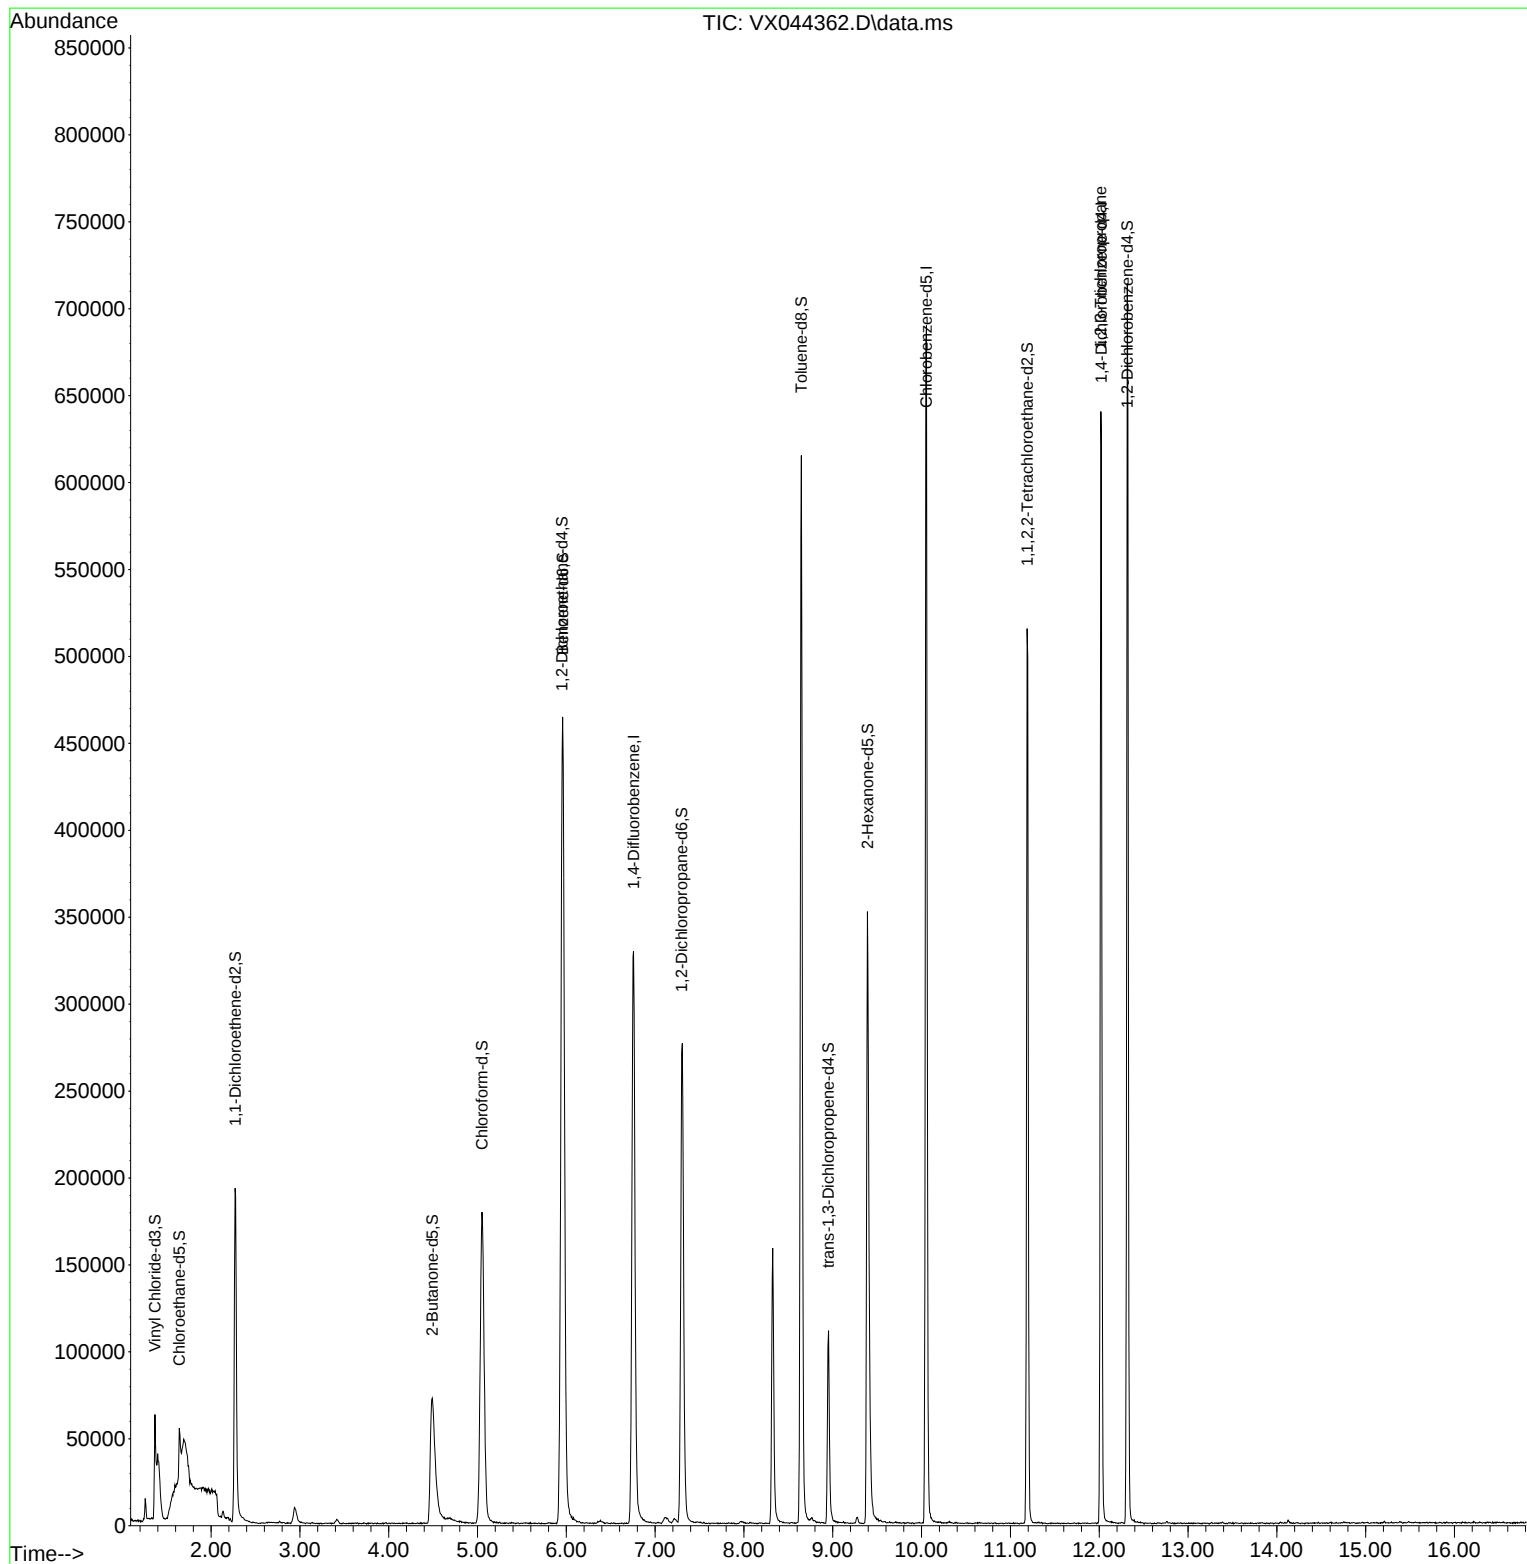

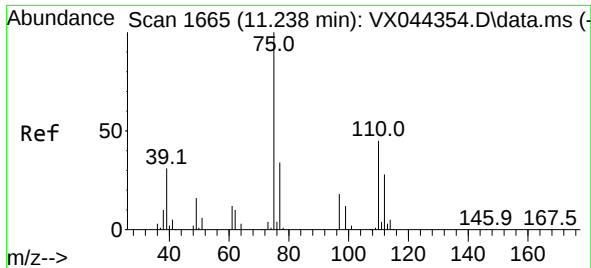

#61
 1,2,3-Trichloropropane
 Concen: 5.942 ug/L
 RT: 12.018 min Scan# 11
 Delta R.T. 0.780 min
 Lab File: VX044362.D
 Acq: 17 Dec 2024 19:24

Instrument :
 MSVOA_X
 ClientSampleId :

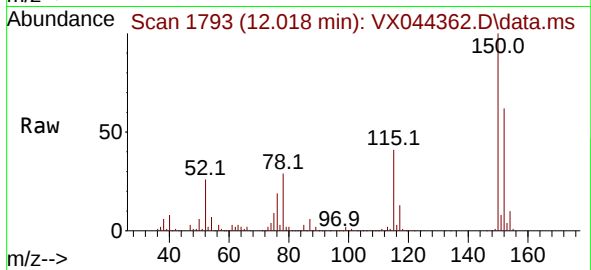

Tgt Ion: 75 Resp: 17446
 Ion Ratio Lower Upper
 75 100
 77 34.5 25.8 38.6
 110 4.0 33.3 49.9#

