

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121724\
 Data File : VX044366.D
 Acq On : 17 Dec 2024 20:56
 Operator : JC/MD
 Sample : P5226-08ME
 Misc : 5.68g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Dec 18 04:44:30 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 18 04:40:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.751	114	207452	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	186858	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	81368	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	20733	10.921	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	21.840%#
7) Chloroethane-d5	1.642	69	13048	8.873	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	17.740%#
11) 1,1-Dichloroethene-d2	2.270	65	19534	24.060	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	48.120%#
21) 2-Butanone-d5	4.489	46	93676	80.594	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	80.590%
24) Chloroform-d	5.056	84	122303	33.930	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	67.860%#
26) 1,2-Dichloroethane-d4	5.952	65	86732	34.025	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	68.060%#
32) Benzene-d6	5.958	84	223759	34.656	ug/L	-0.01
Spiked Amount	50.000	Range	70 - 125	Recovery	=	69.320%#
36) 1,2-Dichloropropane-d6	7.306	67	75412	37.616	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	75.240%
41) Toluene-d8	8.647	98	197902	33.150	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	66.300%#
43) trans-1,3-Dichloroprop...	8.952	79	25930	26.914	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	53.820%#
47) 2-Hexanone-d5	9.391	63	65257	83.482	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	83.480%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	106368	39.568	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	79.140%
66) 1,2-Dichlorobenzene-d4	12.323	152	77733	41.002	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	82.000%
Target Compounds						
					Qvalue	
48) 2-Hexanone	9.397	43	9900	5.330	ug/L #	65
61) 1,2,3-Trichloropropane	12.018	75	10583	5.616	ug/L #	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121724\
Data File : VX044366.D
Acq On : 17 Dec 2024 20:56
Operator : JC/MD
Sample : P5226-08ME
Misc : 5.68g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Dec 18 04:44:30 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 18 04:40:20 2024
Response via : Initial Calibration

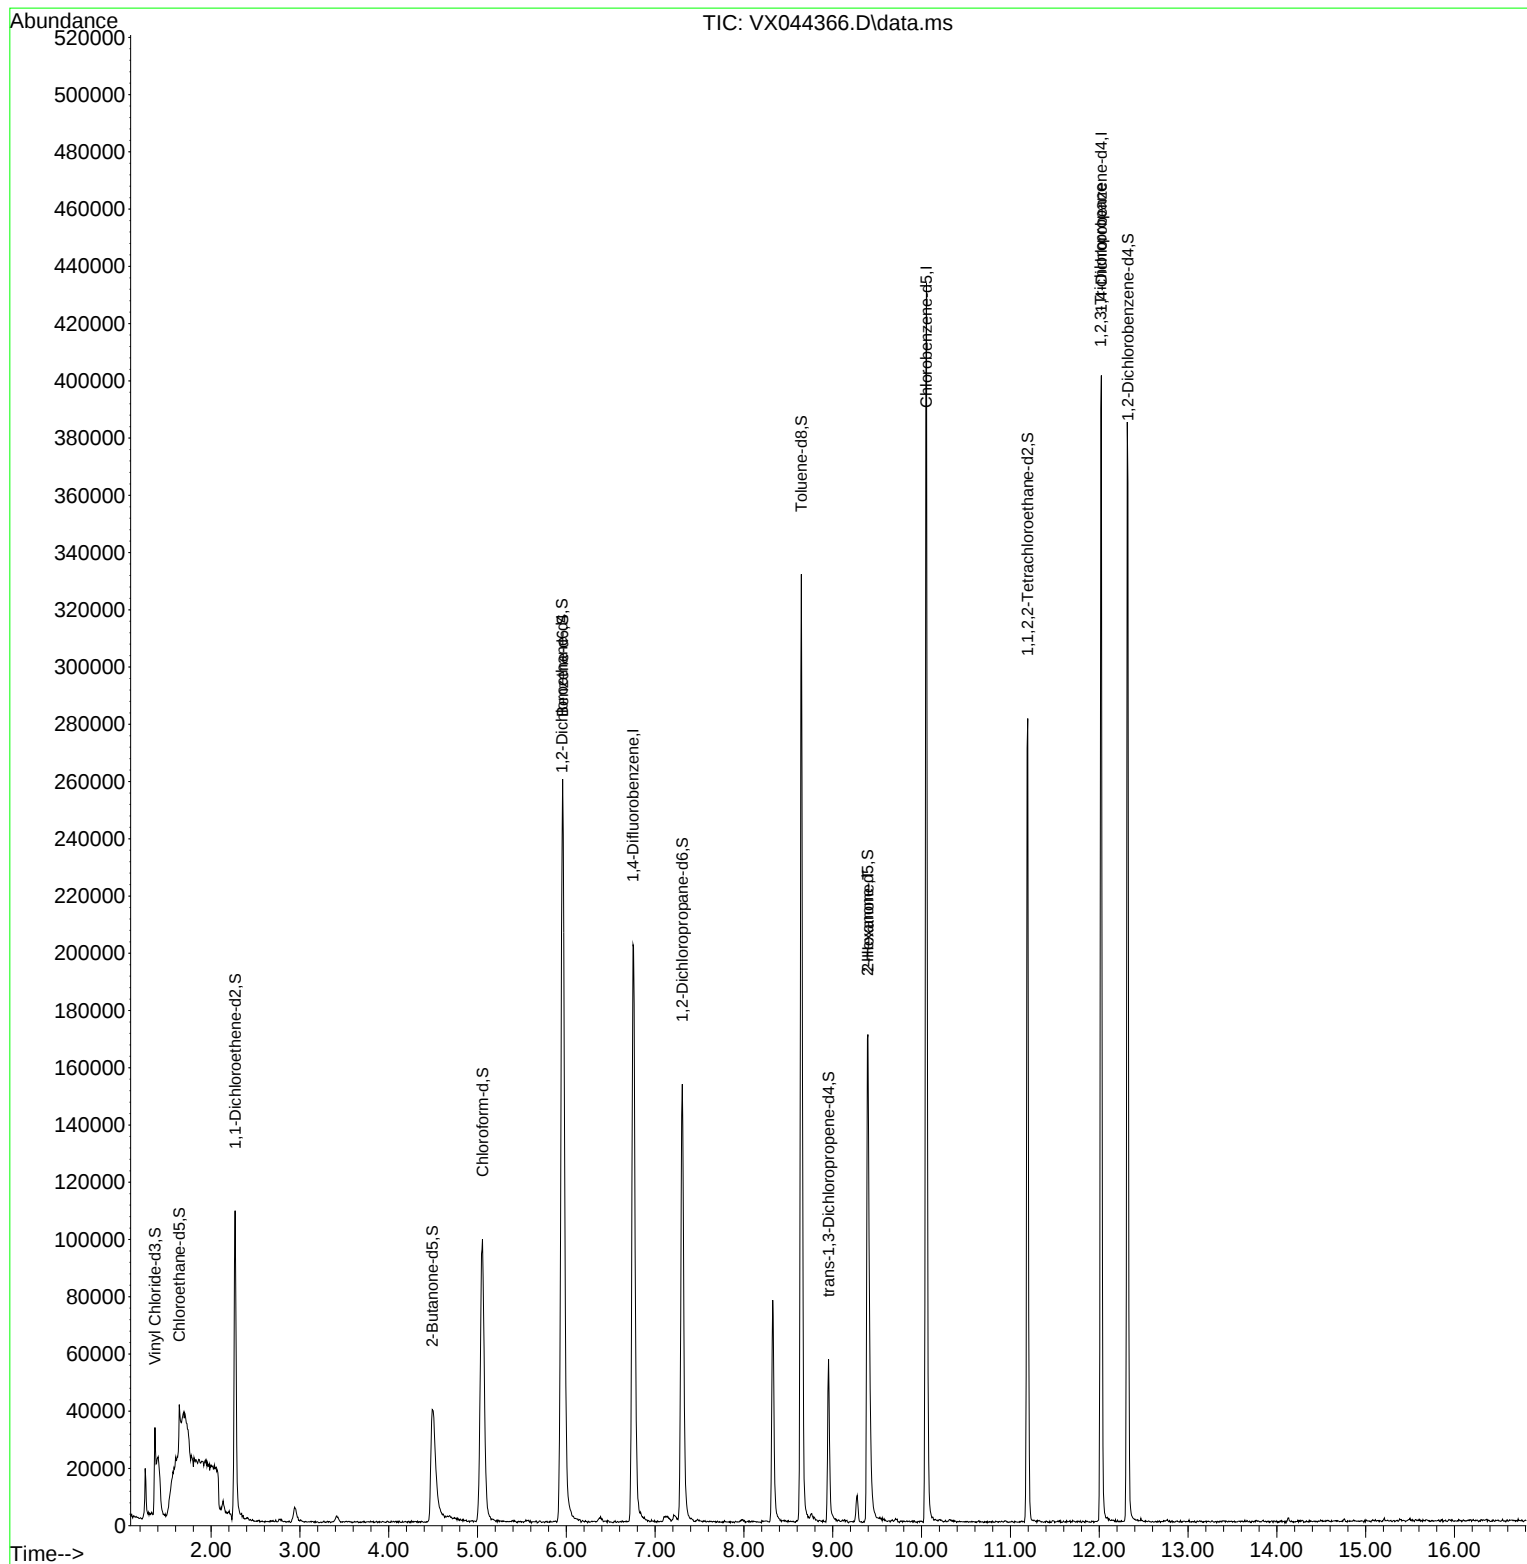

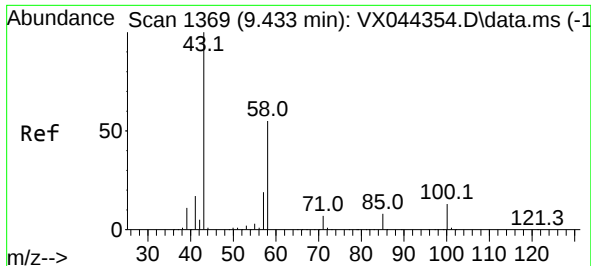




#48
2-Hexanone
Concen: 5.330 ug/L
RT: 9.397 min Scan# 11
Delta R.T. -0.037 min
Lab File: VX044366.D
Acq: 17 Dec 2024 20:56

Instrument :
MSVOA_X
ClientSampleId :

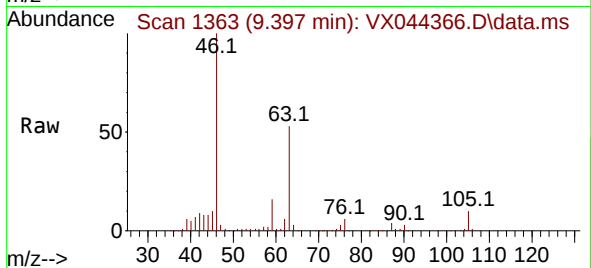

Tgt Ion: 43 Resp: 9900

Ion	Ratio	Lower	Upper
43	100		
58	21.8	45.4	68.2#
57	18.6	15.4	23.0
100	0.0	10.6	15.8#

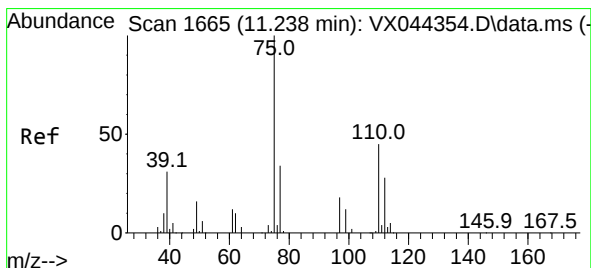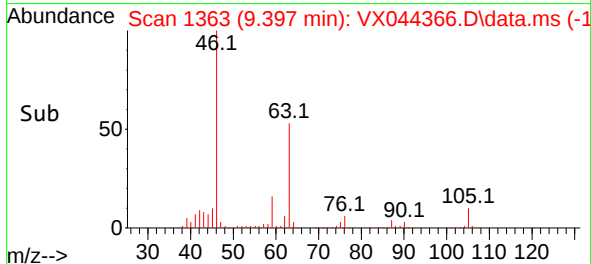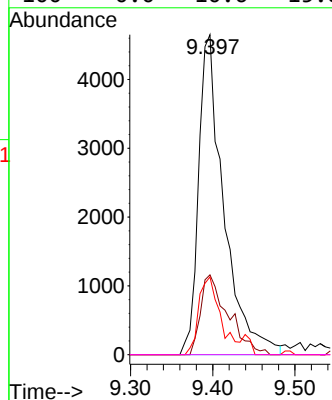

#61
1,2,3-Trichloropropane
Concen: 5.616 ug/L
RT: 12.018 min Scan# 1793
Delta R.T. 0.780 min
Lab File: VX044366.D
Acq: 17 Dec 2024 20:56

Tgt Ion: 75 Resp: 10583

Ion	Ratio	Lower	Upper
75	100		
77	36.4	25.8	38.6
110	5.0	33.3	49.9#

