

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121724\
 Data File : VX044368.D
 Acq On : 17 Dec 2024 21:43
 Operator : JC/MD
 Sample : P5226-17ME
 Misc : 6.37g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Dec 18 04:45:00 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 18 04:40:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	225891	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	200973	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	91138	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	25416	12.295	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	24.600%#
7) Chloroethane-d5	1.642	69	11131	6.951	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	13.900%#
11) 1,1-Dichloroethene-d2	2.270	65	19120	21.627	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	43.260%#
21) 2-Butanone-d5	4.489	46	80723	63.781	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	63.780%
24) Chloroform-d	5.056	84	117042	29.820	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	59.640%#
26) 1,2-Dichloroethane-d4	5.946	65	85271	30.721	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	61.440%#
32) Benzene-d6	5.964	84	210606	30.328	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	60.660%#
36) 1,2-Dichloropropane-d6	7.305	67	70314	32.609	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	65.220%#
41) Toluene-d8	8.647	98	186185	28.997	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	58.000%#
43) trans-1,3-Dichloroprop...	8.951	79	25281	24.398	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	48.800%#
47) 2-Hexanone-d5	9.390	63	58021	69.012	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	69.010%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	99768	34.507	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	69.020%
66) 1,2-Dichlorobenzene-d4	12.317	152	71232	33.545	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	67.100%#
Target Compounds						
13) Acetone	2.416	43	13707	12.171	ug/L	Qvalue 94
61) 1,2,3-Trichloropropane	12.018	75	11928	5.651	ug/L	# 63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121724\
Data File : VX044368.D
Acq On : 17 Dec 2024 21:43
Operator : JC/MD
Sample : P5226-17ME
Misc : 6.37g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Dec 18 04:45:00 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 18 04:40:20 2024
Response via : Initial Calibration

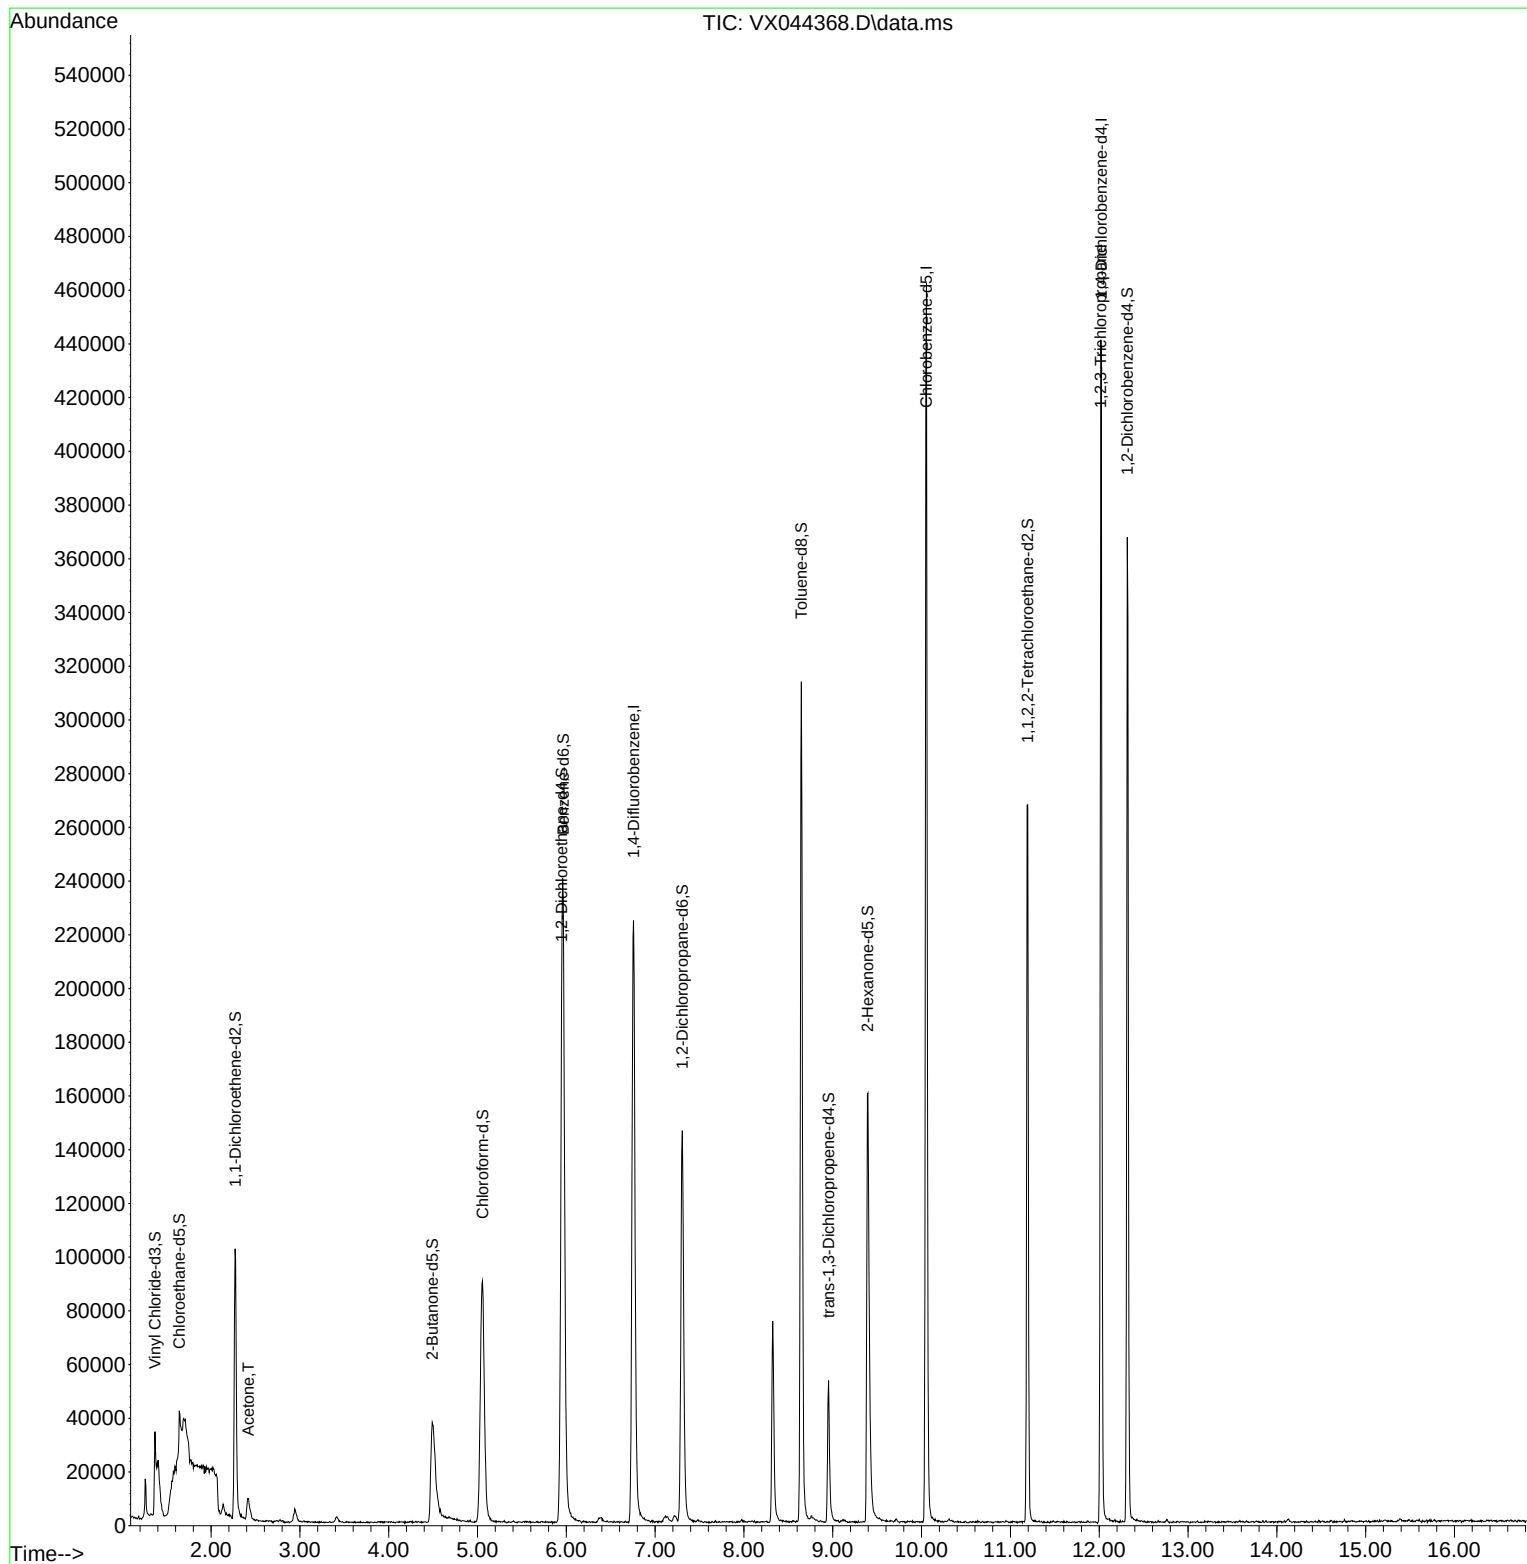

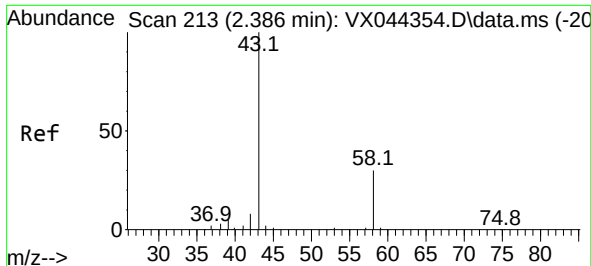

#13

Acetone

Concen: 12.171 ug/L

RT: 2.416 min Scan# 21

Delta R.T. 0.030 min

Lab File: VX044368.D

Acq: 17 Dec 2024 21:43

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 43 Resp: 13707

Ion Ratio Lower Upper

43 100

58 29.5 0.0 66.0

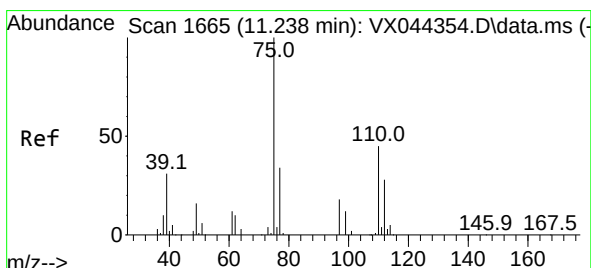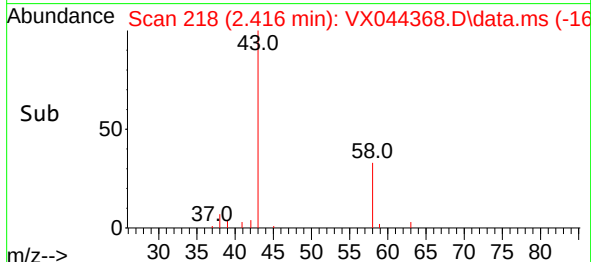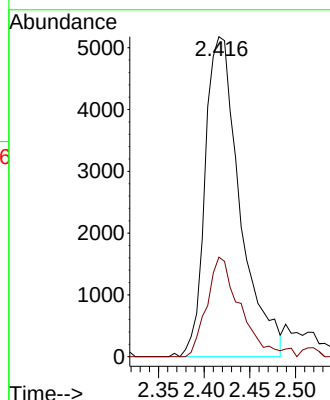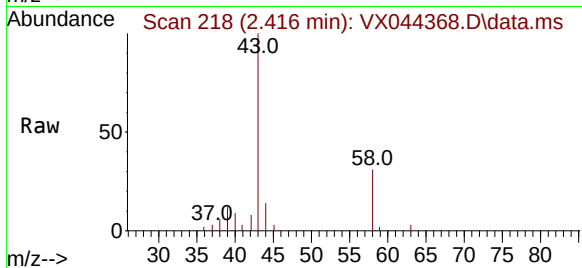

#61

1,2,3-Trichloropropane

Concen: 5.651 ug/L

RT: 12.018 min Scan# 1793

Delta R.T. 0.780 min

Lab File: VX044368.D

Acq: 17 Dec 2024 21:43

Tgt Ion: 75 Resp: 11928

Ion Ratio Lower Upper

75 100

77 36.2 25.8 38.6

110 3.8 33.3 49.9

