

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121724\
 Data File : VX044337.D
 Acq On : 17 Dec 2024 09:39
 Operator : JC/MD
 Sample : VX1217WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK739

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
 Title : VOC Analysis

Signal : TIC: VX044337.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	32	rBV3	4042	6780	0.61%	0.087%
2	1.368	42	46	54	rBV	133766	149477	13.36%	1.917%
3	1.642	88	91	102	rVB	113357	161917	14.47%	2.076%
4	2.294	192	198	210	rBV	210615	329264	29.42%	4.222%
5	2.782	274	278	283	rBV4	1508	2051	0.18%	0.026%
6	2.873	291	293	294	rBV	560	520	0.05%	0.007%
7	2.892	294	296	299	rVB2	722	598	0.05%	0.008%
8	2.916	299	300	301	rBV	959	590	0.05%	0.008%
9	3.026	317	318	320	rBV2	603	525	0.05%	0.007%
10	3.075	324	326	327	rBV	584	579	0.05%	0.007%
11	3.123	330	334	335	rVV3	554	540	0.05%	0.007%
12	3.300	362	363	366	rBV2	593	559	0.05%	0.007%
13	3.428	379	384	392	rVB4	3394	7647	0.68%	0.098%
14	3.508	396	397	402	rVB2	669	713	0.06%	0.009%
15	3.599	411	412	413	rBV	803	478	0.04%	0.006%
16	3.629	416	417	420	rVB2	792	526	0.05%	0.007%
17	3.697	426	428	430	rBV2	506	493	0.04%	0.006%
18	3.800	441	445	448	rBV4	623	988	0.09%	0.013%
19	3.879	456	458	460	rVB2	713	511	0.05%	0.007%
20	3.904	460	462	465	rBV2	589	849	0.08%	0.011%
21	4.392	540	542	545	rVB	570	466	0.04%	0.006%
22	4.459	545	553	571	rBV	79914	247334	22.10%	3.172%
23	5.056	637	651	675	rBV	151636	479868	42.88%	6.154%
24	5.233	678	680	682	rBV3	737	467	0.04%	0.006%
25	5.306	690	692	695	rVB3	558	519	0.05%	0.007%
26	5.336	695	697	701	rBV3	468	697	0.06%	0.009%
27	5.373	701	703	705	rBV2	658	505	0.05%	0.006%
28	5.678	751	753	756	rVB3	654	594	0.05%	0.008%
29	5.702	756	757	761	rBV2	680	736	0.07%	0.009%
30	5.964	788	800	817	rBV2	379506	1119035	100.00%	14.351%
31	6.525	888	892	894	rBV3	540	887	0.08%	0.011%
32	6.641	909	911	914	rBV3	590	667	0.06%	0.009%
33	6.757	921	930	946	rBV	236334	575673	51.44%	7.382%
34	7.031	973	975	977	rBV2	503	473	0.04%	0.006%
35	7.111	984	988	989	rBV3	2743	3658	0.33%	0.047%
36	7.306	1011	1020	1036	rVV	235096	523581	46.79%	6.714%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121724\
 Data File : VX044337.D
 Acq On : 17 Dec 2024 09:39
 Operator : JC/MD
 Sample : VX1217WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK739

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

37	7.909	1116	1119	1121	rBV4	369	493	0.04%	0.006%
38	8.135	1154	1156	1160	rVB3	750	720	0.06%	0.009%
39	8.324	1181	1187	1201	rBV	141549	240344	21.48%	3.082%
40	8.519	1217	1219	1220	rBV	543	483	0.04%	0.006%
41	8.580	1227	1229	1233	rVB5	985	919	0.08%	0.012%
42	8.647	1234	1240	1253	rBV	504845	800921	71.57%	10.271%
43	8.952	1283	1290	1299	rBV	96905	153277	13.70%	1.966%
44	9.275	1341	1343	1345	rVB	956	604	0.05%	0.008%
45	9.385	1356	1361	1375	rBV	340402	515243	46.04%	6.607%
46	9.970	1454	1457	1459	rBV3	654	803	0.07%	0.010%
47	10.049	1465	1470	1482	rVV	459493	667683	59.67%	8.562%
48	10.183	1491	1492	1494	rBV	731	627	0.06%	0.008%
49	10.262	1503	1505	1507	rBV2	551	531	0.05%	0.007%
50	10.305	1510	1512	1515	rBV4	691	834	0.07%	0.011%
51	10.390	1524	1526	1529	rBV3	518	646	0.06%	0.008%
52	10.421	1529	1531	1535	rVB	719	477	0.04%	0.006%
53	10.451	1535	1536	1539	rBV3	459	475	0.04%	0.006%
54	10.579	1555	1557	1559	rBV	593	484	0.04%	0.006%
55	10.695	1574	1576	1582	rBV3	626	1170	0.10%	0.015%
56	10.787	1589	1591	1593	rBV2	647	516	0.05%	0.007%
57	10.957	1617	1619	1621	rBV2	1052	1127	0.10%	0.014%
58	11.189	1652	1657	1670	rVV	419401	543677	48.58%	6.972%
59	11.463	1699	1702	1703	rBB3	601	505	0.05%	0.006%
60	11.756	1747	1750	1754	rBV4	480	563	0.05%	0.007%
61	11.872	1768	1769	1772	rBV2	882	627	0.06%	0.008%
62	11.933	1776	1779	1782	rBV2	847	870	0.08%	0.011%
63	11.976	1784	1786	1788	rBV2	644	643	0.06%	0.008%
64	12.018	1788	1793	1806	rBV	426518	542710	48.50%	6.960%
65	12.158	1814	1816	1819	rBV3	936	909	0.08%	0.012%
66	12.201	1821	1823	1826	rVV3	678	586	0.05%	0.008%
67	12.317	1836	1842	1852	rBV	531958	668112	59.70%	8.568%
68	12.762	1911	1915	1920	rBV3	1990	2689	0.24%	0.034%
69	12.811	1920	1923	1926	rBV2	887	995	0.09%	0.013%
70	12.884	1933	1935	1937	rBV3	657	554	0.05%	0.007%
71	13.128	1973	1975	1978	rVB	519	533	0.05%	0.007%
72	13.225	1990	1991	1994	rVB3	731	560	0.05%	0.007%
73	13.359	2010	2013	2014	rBV3	824	884	0.08%	0.011%
74	13.402	2017	2020	2021	rBV2	575	755	0.07%	0.010%
75	13.542	2041	2043	2047	rVB3	621	721	0.06%	0.009%
76	13.597	2047	2052	2053	rBV3	1216	1764	0.16%	0.023%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121724\
 Data File : VX044337.D
 Acq On : 17 Dec 2024 09:39
 Operator : JC/MD
 Sample : VX1217WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK739

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

77	13.652	2057	2061	2062	rBV3	412	495	0.04%	0.006%
78	13.737	2074	2075	2079	rVB2	447	519	0.05%	0.007%
79	13.786	2079	2083	2084	rBV3	843	1284	0.11%	0.016%
80	13.951	2109	2110	2112	rBV	648	496	0.04%	0.006%
81	14.006	2118	2119	2124	rVB4	438	506	0.05%	0.006%
82	14.060	2124	2128	2130	rVB3	548	765	0.07%	0.010%
83	14.134	2135	2140	2142	rBV	2377	3088	0.28%	0.040%
84	14.201	2149	2151	2153	rBV2	820	861	0.08%	0.011%
85	14.298	2163	2167	2170	rBV4	600	934	0.08%	0.012%
86	14.378	2176	2180	2182	rBV2	745	893	0.08%	0.011%
87	14.414	2184	2186	2188	rVB2	654	523	0.05%	0.007%
88	14.445	2188	2191	2195	rBV3	664	946	0.08%	0.012%
89	14.487	2195	2198	2200	rBV3	519	533	0.05%	0.007%
90	14.634	2218	2222	2223	rBV3	436	596	0.05%	0.008%
91	14.902	2265	2266	2269	rBV2	722	546	0.05%	0.007%
92	15.030	2284	2287	2290	rBV3	630	918	0.08%	0.012%
93	15.243	2320	2322	2327	rVB3	667	568	0.05%	0.007%
94	15.518	2365	2367	2370	rBV3	689	971	0.09%	0.012%
95	16.085	2459	2460	2462	rVB2	776	479	0.04%	0.006%
96	16.103	2462	2463	2465	rBV2	768	479	0.04%	0.006%
97	16.219	2479	2482	2483	rBV3	654	712	0.06%	0.009%
98	16.334	2499	2501	2504	rBV2	519	590	0.05%	0.008%
99	16.414	2511	2514	2516	rBV4	769	986	0.09%	0.013%
100	16.584	2538	2542	2544	rBV4	836	1392	0.12%	0.018%

Sum of corrected areas: 7797879




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121724\
Data File : VX044337.D
Acq On : 17 Dec 2024 09:39
Operator : JC/MD
Sample : VX1217WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK739

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

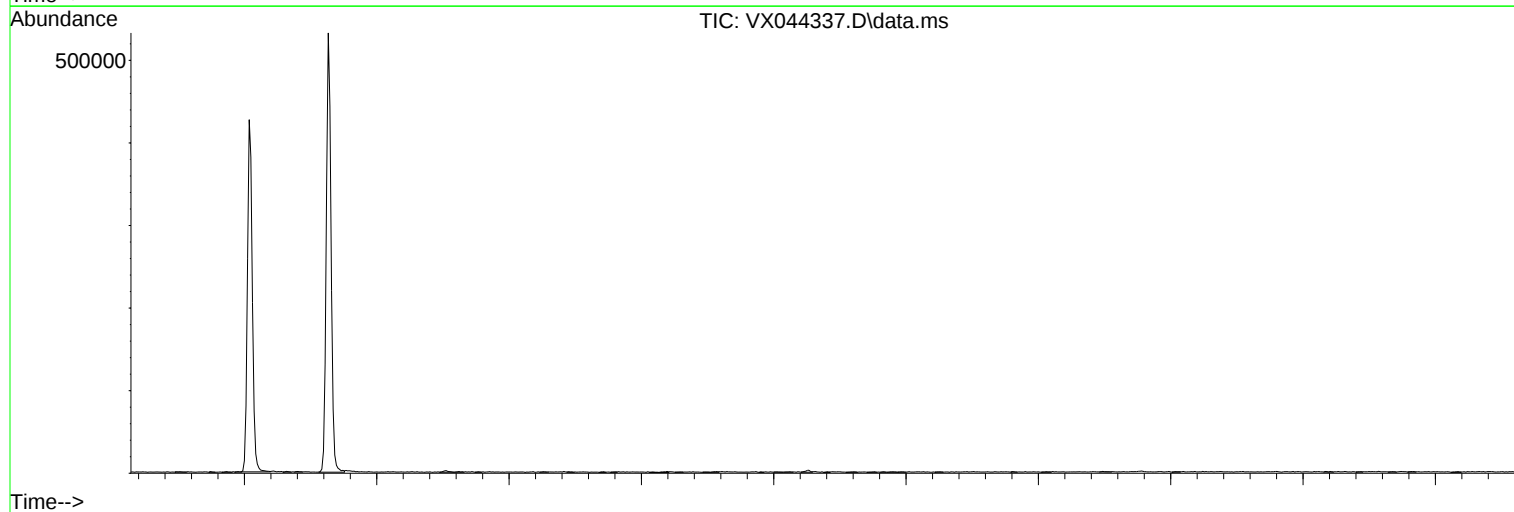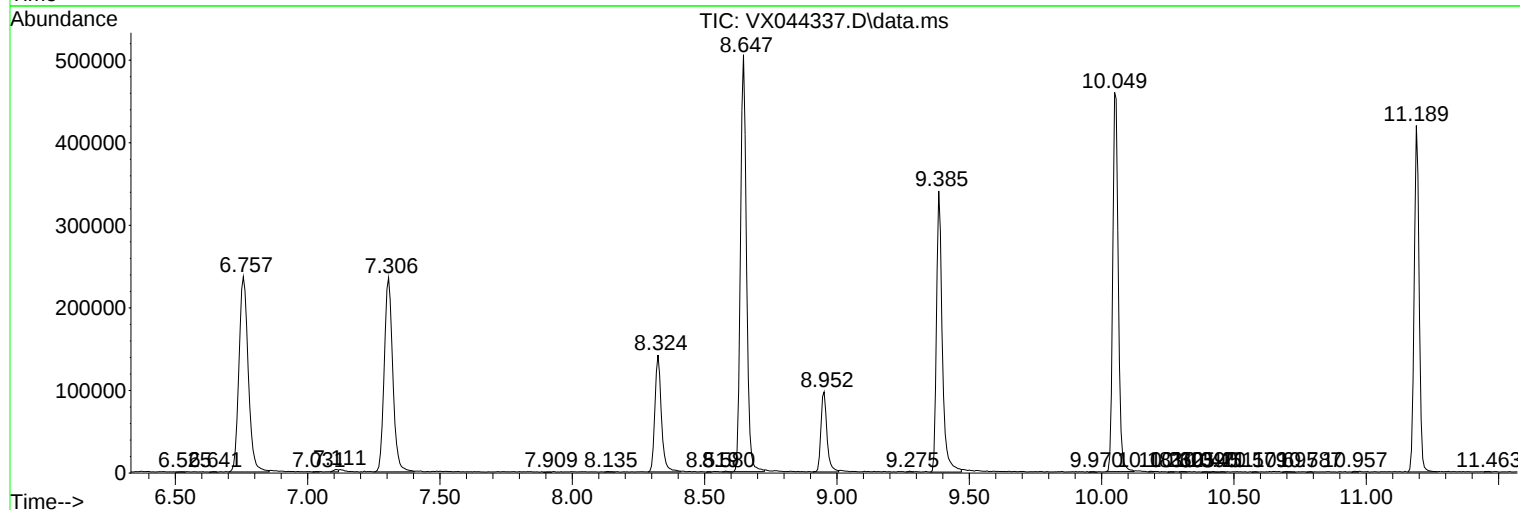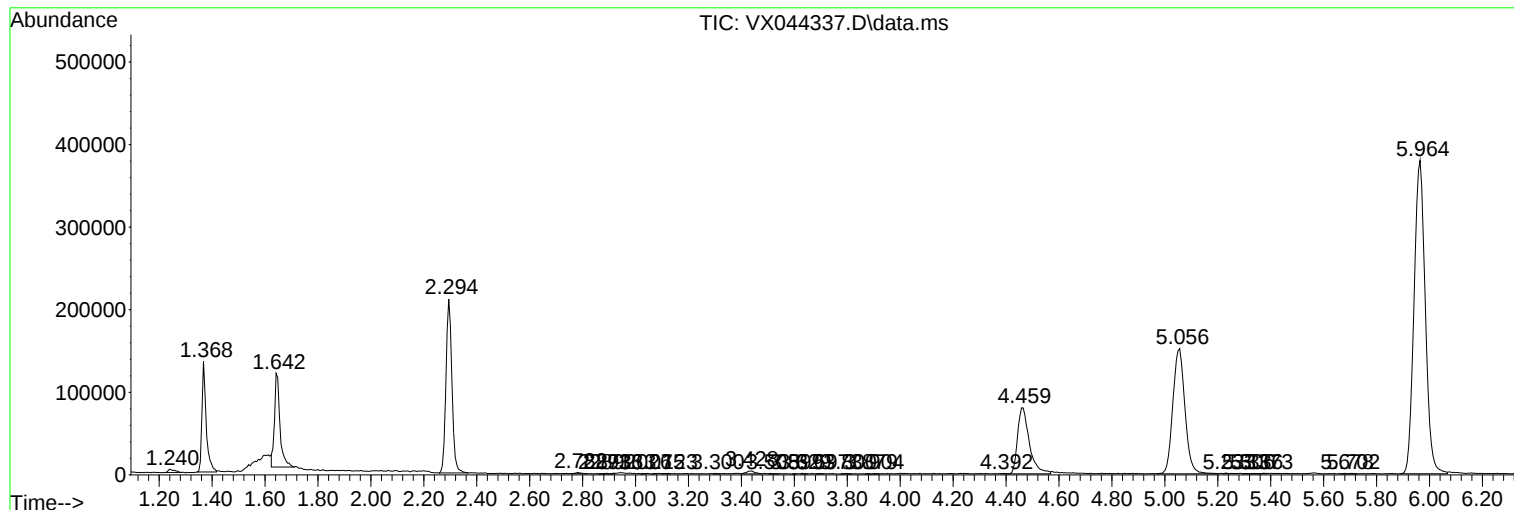

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121724\
Data File : VX044337.D
Acq On : 17 Dec 2024 09:39
Operator : JC/MD
Sample : VX1217WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK739

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121724\
Data File : VX044337.D
Acq On : 17 Dec 2024 09:39
Operator : JC/MD
Sample : VX1217WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK739

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc