

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121724\
 Data File : VX044338.D
 Acq On : 17 Dec 2024 10:02
 Operator : JC/MD
 Sample : P5252-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

Signal : TIC: VX044338.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	27	rBV	4457	4699	0.45%	0.064%
2	1.368	42	46	57	rBV	118412	139009	13.18%	1.900%
3	1.642	88	91	102	rVB	105668	144921	13.74%	1.980%
4	2.294	192	198	209	rVB	194302	301675	28.60%	4.122%
5	2.496	228	231	233	rBV3	561	713	0.07%	0.010%
6	2.563	240	242	245	rVB4	926	986	0.09%	0.013%
7	2.691	261	263	264	rBV	439	416	0.04%	0.006%
8	2.788	274	279	282	rVB4	1470	2126	0.20%	0.029%
9	2.934	298	303	313	rVB2	4467	11130	1.06%	0.152%
10	3.081	326	327	329	rBV	666	475	0.05%	0.006%
11	3.172	339	342	344	rBV2	868	1087	0.10%	0.015%
12	3.428	381	384	394	rVB6	2825	6842	0.65%	0.093%
13	3.599	410	412	417	rVB3	380	741	0.07%	0.010%
14	3.648	418	420	423	rVV3	457	542	0.05%	0.007%
15	3.886	457	459	462	rVB2	524	410	0.04%	0.006%
16	3.922	463	465	468	rVB3	551	497	0.05%	0.007%
17	3.989	472	476	480	rBV3	674	1050	0.10%	0.014%
18	4.318	528	530	531	rBV	630	381	0.04%	0.005%
19	4.465	546	554	569	rBV	79807	238672	22.63%	3.262%
20	4.855	616	618	619	rBV2	565	414	0.04%	0.006%
21	5.050	639	650	666	rBV	140039	438152	41.54%	5.987%
22	5.263	683	685	687	rBV3	630	472	0.04%	0.006%
23	5.635	745	746	748	rBV	673	446	0.04%	0.006%
24	5.794	768	772	774	rBV3	753	939	0.09%	0.013%
25	5.824	774	777	778	rVV3	519	586	0.06%	0.008%
26	5.964	786	800	819	rBV2	353464	1054837	100.00%	14.415%
27	6.306	854	856	857	rVB	746	409	0.04%	0.006%
28	6.330	857	860	861	rBV2	788	719	0.07%	0.010%
29	6.348	861	863	864	rBV2	635	406	0.04%	0.006%
30	6.440	877	878	880	rBV2	584	482	0.05%	0.007%
31	6.605	904	905	907	rBV2	444	433	0.04%	0.006%
32	6.757	921	930	944	rBV2	217497	529483	50.20%	7.236%
33	7.007	967	971	972	rBV3	624	865	0.08%	0.012%
34	7.117	983	989	996	rVV7	3085	7873	0.75%	0.108%
35	7.306	1012	1020	1036	rBV	223644	493228	46.76%	6.740%
36	7.482	1045	1049	1053	rVB3	1143	1234	0.12%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121724\
 Data File : VX044338.D
 Acq On : 17 Dec 2024 10:02
 Operator : JC/MD
 Sample : P5252-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

37	7.806	1099	1102	1104	rBV3	336	377	0.04%	0.005%
38	7.885	1113	1115	1117	rVB2	669	528	0.05%	0.007%
39	7.921	1117	1121	1122	rBV2	557	847	0.08%	0.012%
40	8.104	1150	1151	1154	rVB2	563	405	0.04%	0.006%
41	8.220	1168	1170	1172	rVB2	660	470	0.04%	0.006%
42	8.238	1172	1173	1176	rBV	715	750	0.07%	0.010%
43	8.324	1181	1187	1198	rBV	134489	219171	20.78%	2.995%
44	8.647	1234	1240	1251	rBV	461711	735216	69.70%	10.047%
45	8.860	1273	1275	1279	rBV3	676	923	0.09%	0.013%
46	8.952	1285	1290	1306	rBV	88261	142170	13.48%	1.943%
47	9.165	1323	1325	1328	rBV3	623	564	0.05%	0.008%
48	9.281	1343	1344	1348	rBV2	426	551	0.05%	0.008%
49	9.385	1356	1361	1376	rBV	329637	509514	48.30%	6.963%
50	9.659	1404	1406	1407	rBV	652	426	0.04%	0.006%
51	10.055	1465	1471	1485	rBV	428903	621341	58.90%	8.491%
52	10.244	1500	1502	1507	rVB3	775	1080	0.10%	0.015%
53	10.305	1509	1512	1516	rVV4	812	1388	0.13%	0.019%
54	10.390	1524	1526	1527	rVB2	740	413	0.04%	0.006%
55	10.439	1533	1534	1539	rVB4	614	814	0.08%	0.011%
56	10.506	1539	1545	1549	rBV4	914	1929	0.18%	0.026%
57	10.805	1592	1594	1596	rBV2	678	429	0.04%	0.006%
58	10.878	1603	1606	1611	rBV4	574	831	0.08%	0.011%
59	10.933	1611	1615	1616	rBV3	720	784	0.07%	0.011%
60	11.024	1627	1630	1631	rBV3	806	871	0.08%	0.012%
61	11.092	1639	1641	1642	rBV	740	493	0.05%	0.007%
62	11.140	1647	1649	1651	rVB2	714	676	0.06%	0.009%
63	11.189	1651	1657	1669	rBV	415143	536501	50.86%	7.331%
64	11.579	1719	1721	1722	rBV2	488	385	0.04%	0.005%
65	11.896	1770	1773	1774	rBV2	412	478	0.05%	0.007%
66	11.976	1783	1786	1788	rBV2	886	802	0.08%	0.011%
67	12.018	1788	1793	1805	rBV	382994	503460	47.73%	6.880%
68	12.317	1837	1842	1852	rBV	488317	621049	58.88%	8.487%
69	12.414	1857	1858	1860	rVB	927	456	0.04%	0.006%
70	12.469	1866	1867	1869	rBV2	944	629	0.06%	0.009%
71	12.549	1878	1880	1883	rBV3	682	680	0.06%	0.009%
72	12.579	1883	1885	1887	rVV2	425	467	0.04%	0.006%
73	12.603	1887	1889	1890	rVV	695	447	0.04%	0.006%
74	12.622	1890	1892	1896	rVB3	565	549	0.05%	0.008%
75	12.762	1912	1915	1917	rVV2	1655	1848	0.18%	0.025%
76	12.805	1920	1922	1924	rBV3	444	517	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121724\
 Data File : VX044338.D
 Acq On : 17 Dec 2024 10:02
 Operator : JC/MD
 Sample : P5252-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

77	12.914	1938	1940	1941	rBV2	846	716	0.07%	0.010%
78	13.237	1990	1993	1995	rVB3	545	669	0.06%	0.009%
79	13.353	2011	2012	2016	rBV2	554	438	0.04%	0.006%
80	13.457	2027	2029	2030	rBV	473	440	0.04%	0.006%
81	13.646	2058	2060	2063	rVV2	468	497	0.05%	0.007%
82	13.670	2063	2064	2067	rVB2	995	839	0.08%	0.011%
83	13.774	2079	2081	2083	rBV2	641	625	0.06%	0.009%
84	13.890	2098	2100	2102	rVB3	579	422	0.04%	0.006%
85	13.914	2102	2104	2107	rBV3	853	779	0.07%	0.011%
86	13.975	2111	2114	2117	rBV3	682	1039	0.10%	0.014%
87	14.128	2134	2139	2144	rBV3	2880	3918	0.37%	0.054%
88	14.268	2160	2162	2163	rBV	991	699	0.07%	0.010%
89	14.298	2166	2167	2169	rVV	667	404	0.04%	0.006%
90	14.329	2170	2172	2175	rVV2	875	818	0.08%	0.011%
91	14.420	2185	2187	2188	rBV2	550	395	0.04%	0.005%
92	14.548	2206	2208	2211	rVB2	497	529	0.05%	0.007%
93	14.670	2226	2228	2229	rBV	729	461	0.04%	0.006%
94	14.749	2239	2241	2242	rBV	609	391	0.04%	0.005%
95	14.890	2262	2264	2265	rVB	686	377	0.04%	0.005%
96	15.042	2283	2289	2291	rBV4	686	964	0.09%	0.013%
97	15.225	2317	2319	2321	rBV3	501	510	0.05%	0.007%
98	16.255	2484	2488	2489	rBV2	1187	952	0.09%	0.013%
99	16.621	2546	2548	2549	rBV	887	631	0.06%	0.009%
100	16.652	2549	2553	2557	rVV3	956	1722	0.16%	0.024%

Sum of corrected areas: 7317814




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121724\
Data File : VX044338.D
Acq On : 17 Dec 2024 10:02
Operator : JC/MD
Sample : P5252-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

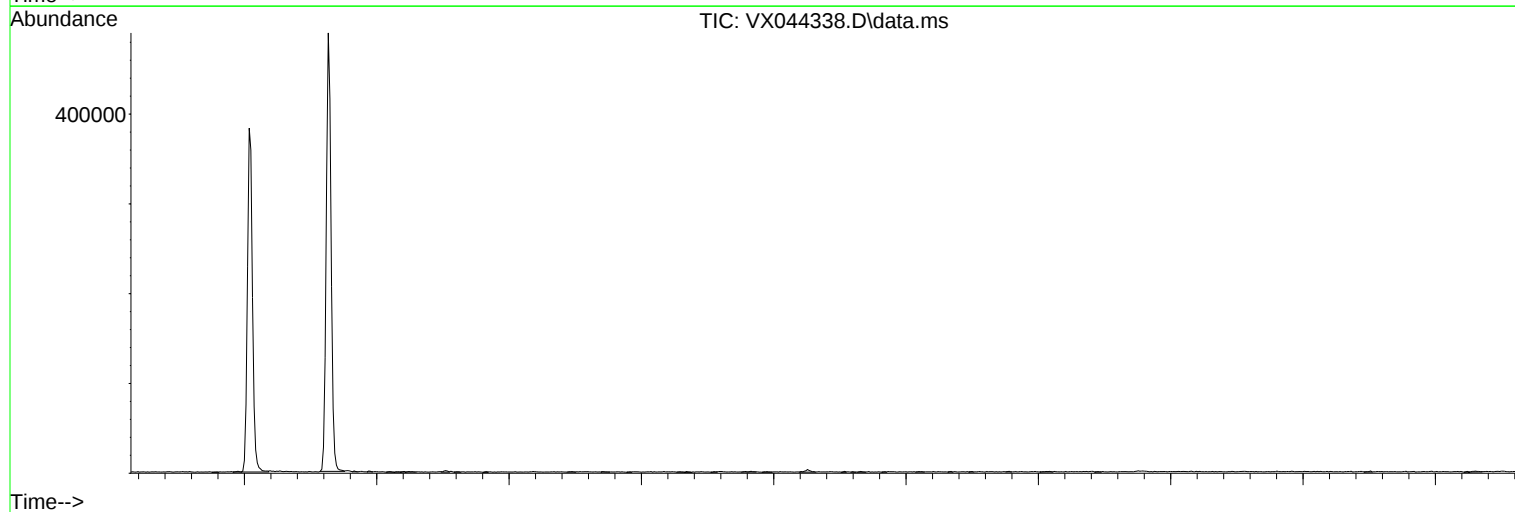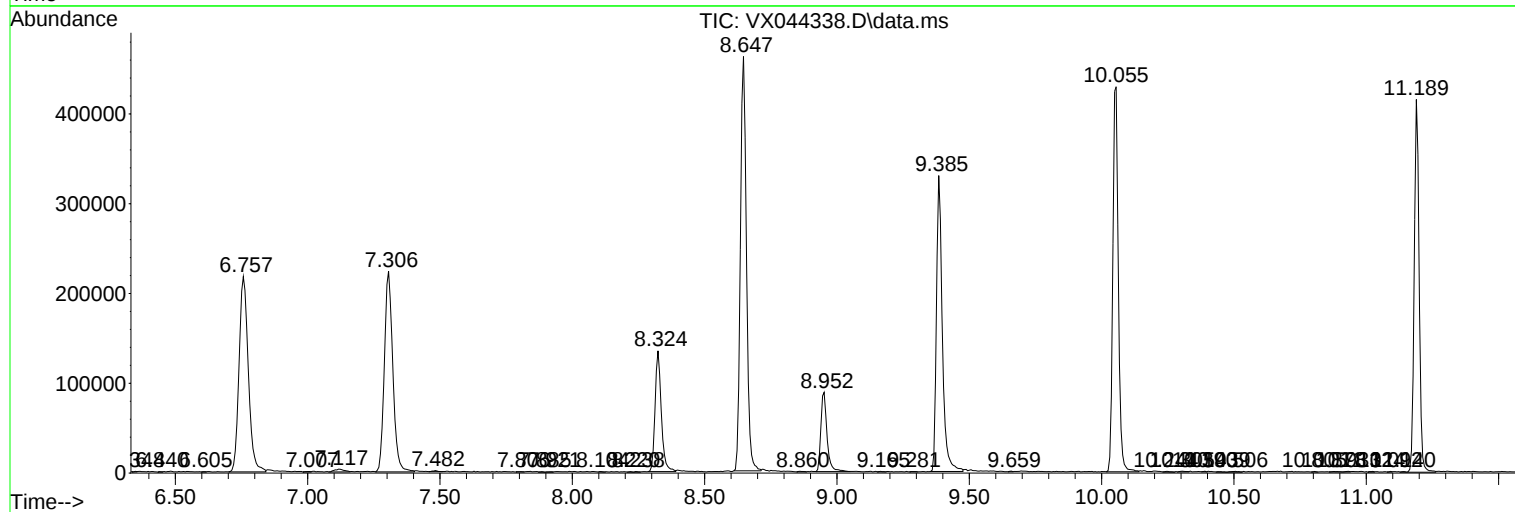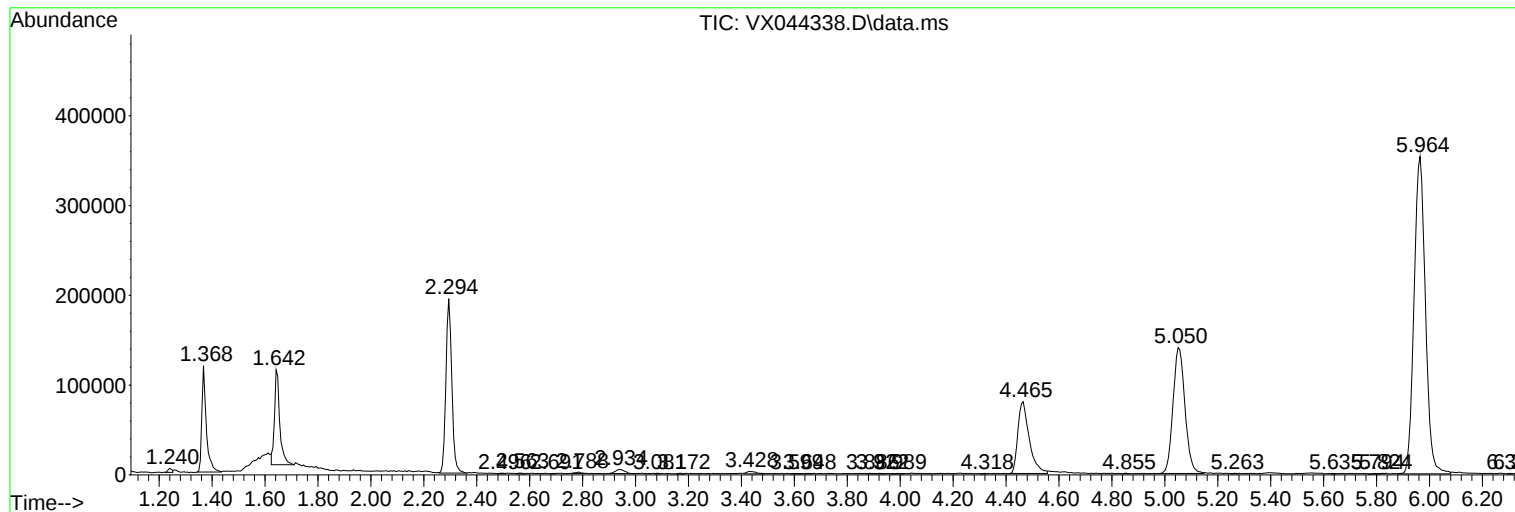

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121724\
Data File : VX044338.D
Acq On : 17 Dec 2024 10:02
Operator : JC/MD
Sample : P5252-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121724\
Data File : VX044338.D
Acq On : 17 Dec 2024 10:02
Operator : JC/MD
Sample : P5252-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
